

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120615\
 Data File : BM003392.D
 Acq On : 06 Dec 2015 16:57
 Operator : UM/IZ
 Sample : G4664-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5E84

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	22	rVB	2745	3664	0.20%	0.022%
2	6.887	640	646	654	rVB	59032	84632	4.61%	0.497%
3	7.057	669	675	685	rBV	261324	393391	21.42%	2.312%
4	7.251	702	708	717	rVB	250186	392932	21.40%	2.309%
5	7.722	782	788	795	rVB	253610	394326	21.47%	2.317%
6	8.422	902	907	916	rBV	191830	298032	16.23%	1.751%
7	8.881	978	985	993	rVB	293424	462341	25.18%	2.717%
8	9.298	1050	1056	1060	rBV2	2492	4091	0.22%	0.024%
9	9.598	1101	1107	1114	rVB	243805	376046	20.48%	2.210%
10	10.133	1191	1198	1207	rBV	373328	596004	32.45%	3.502%
11	10.516	1255	1263	1273	rBB	377927	626200	34.10%	3.679%
12	10.651	1281	1286	1292	rVB	3716	5990	0.33%	0.035%
13	12.110	1530	1534	1539	rVB	4831	7059	0.38%	0.041%
14	13.780	1812	1818	1826	rBV	790271	1085176	59.09%	6.376%
15	14.063	1860	1866	1883	rBV	903533	1316266	71.68%	7.734%
16	14.374	1913	1919	1928	rVB2	585593	875872	47.69%	5.147%
17	14.568	1947	1952	1961	rVB	26890	40510	2.21%	0.238%
18	15.368	2082	2088	2100	rVB	1186395	1694861	92.29%	9.959%
19	15.486	2103	2108	2118	rBV	259300	332545	18.11%	1.954%
20	15.610	2124	2129	2134	rVB	9418	12179	0.66%	0.072%
21	16.268	2238	2241	2245	rBV	2731	2693	0.15%	0.016%
22	16.904	2346	2349	2354	rBV	1479	2029	0.11%	0.012%
23	17.121	2380	2386	2393	rBV	698616	989561	53.88%	5.815%
24	17.221	2396	2403	2416	rBV	1233176	1730555	94.23%	10.169%
25	19.156	2728	2732	2736	rVB	8485	10924	0.59%	0.064%
26	19.409	2771	2775	2782	rVB	7719	10842	0.59%	0.064%
27	19.521	2788	2794	2806	rBV	1378884	1836432	100.00%	10.791%
28	19.756	2830	2834	2838	rBV	4273	4858	0.26%	0.029%
29	20.839	3015	3018	3021	rBV4	1753	2316	0.13%	0.014%
30	21.321	3094	3100	3109	rBV	738647	958816	52.21%	5.634%
31	22.839	3353	3358	3362	rBV3	6653	11336	0.62%	0.067%
32	23.433	3451	3459	3475	rBV	834022	1565862	85.27%	9.201%
33	23.574	3476	3483	3496	rVB	485070	890276	48.48%	5.231%

LSC Area Percent Report

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120615\
Data File : BM003392.D
Acq On : 06 Dec 2015 16:57
Operator : UM/IZ
Sample : G4664-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5E84

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION


Sum of corrected areas: 17018617

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120615\
Data File : BM003392.D
Acq On : 06 Dec 2015 16:57
Operator : UM/IZ
Sample : G4664-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5E84

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

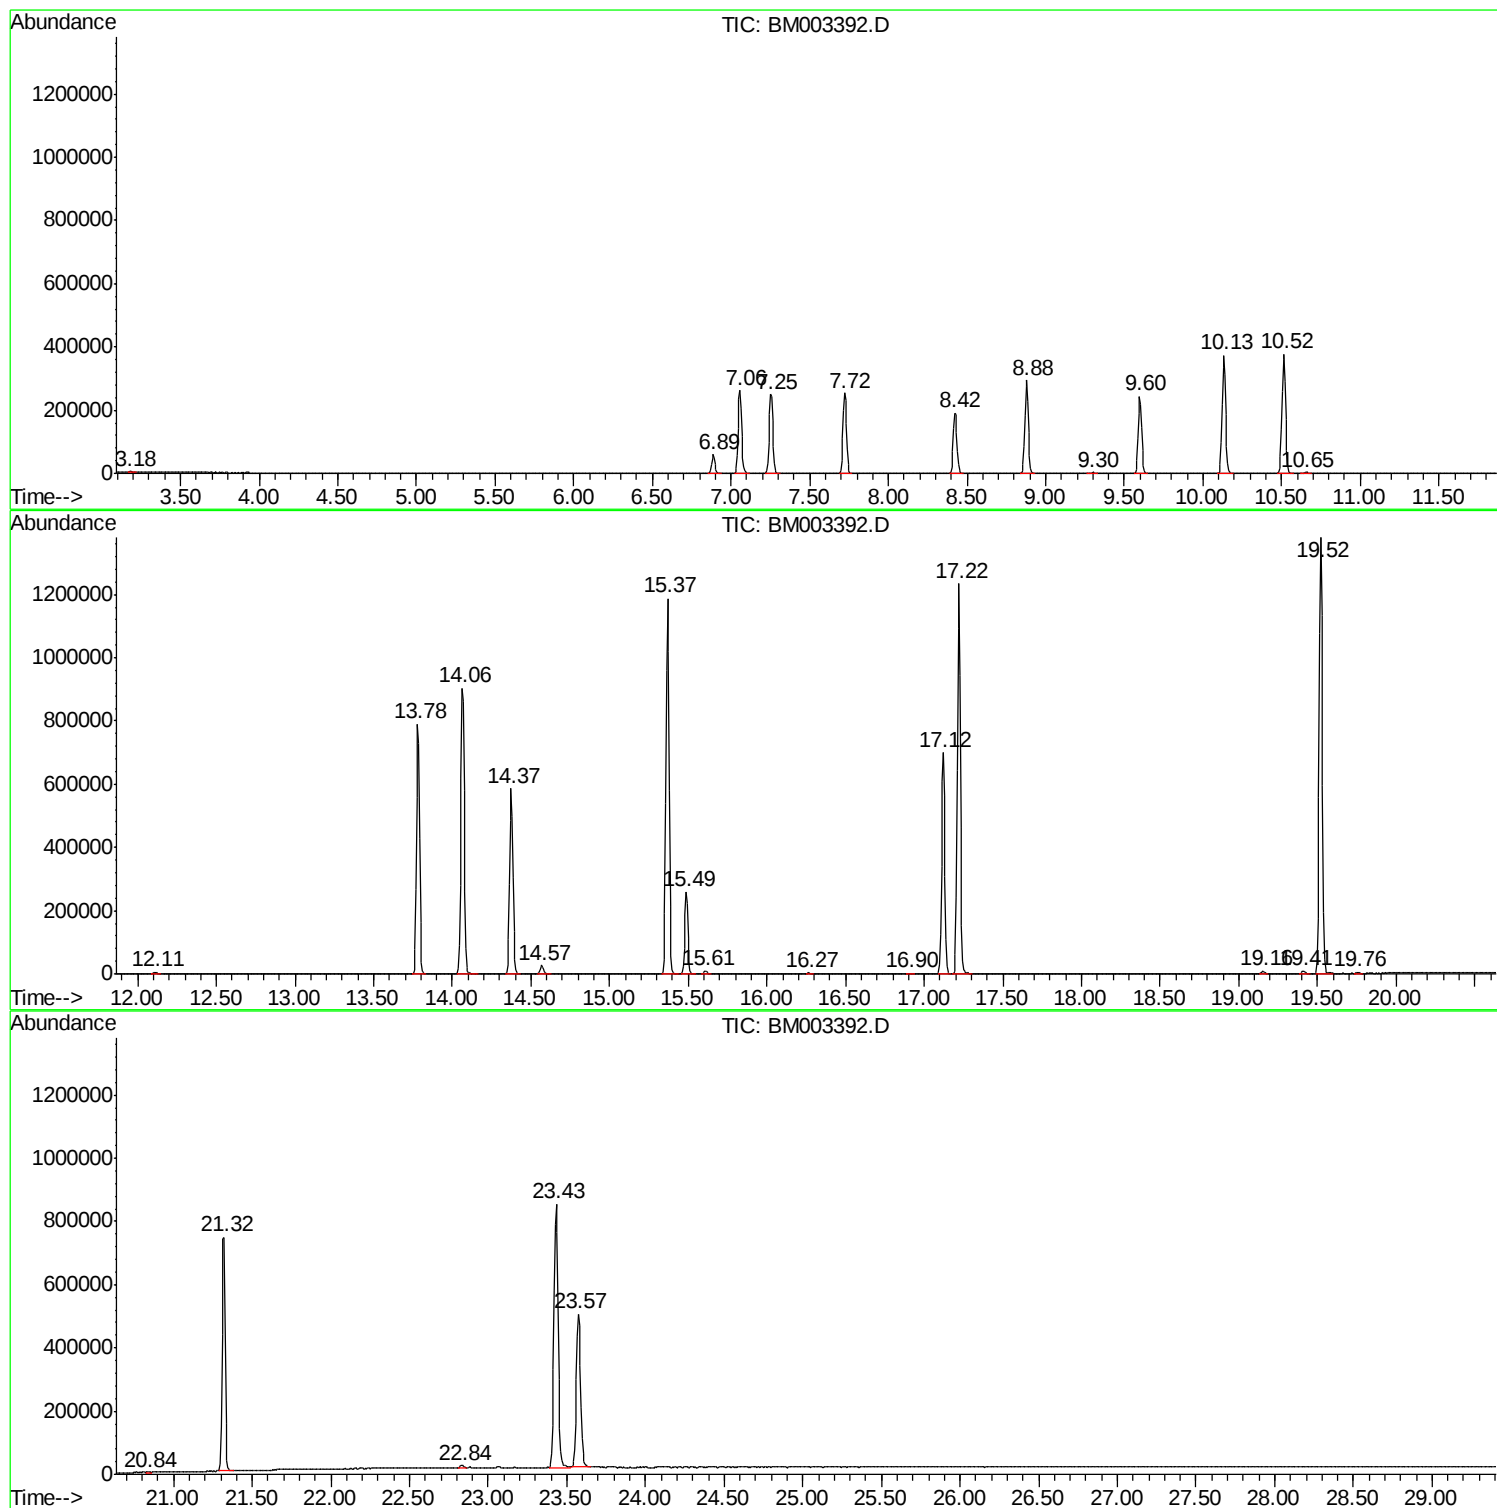

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120615\
Data File : BM003392.D
Acq On : 06 Dec 2015 16:57
Operator : UM/IZ
Sample : G4664-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5E84

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120615\
Data File : BM003392.D
Acq On : 06 Dec 2015 16:57
Operator : UM/IZ
Sample : G4664-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5E84

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc