


Data Path : Z:\HPCHEM1\BNA_M\Data\BM120616\
Data File : BM008182.D
Acq On : 06 Dec 2016 13:30
Operator : UM/SJ
Sample : PB95036BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK36

Manual Integrations
APPROVED

sohil
12/7/2016 4:39:04 PM

Quant Time: Dec 06 14:15:08 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 13:48:59 2016
Response via : Initial Calibration

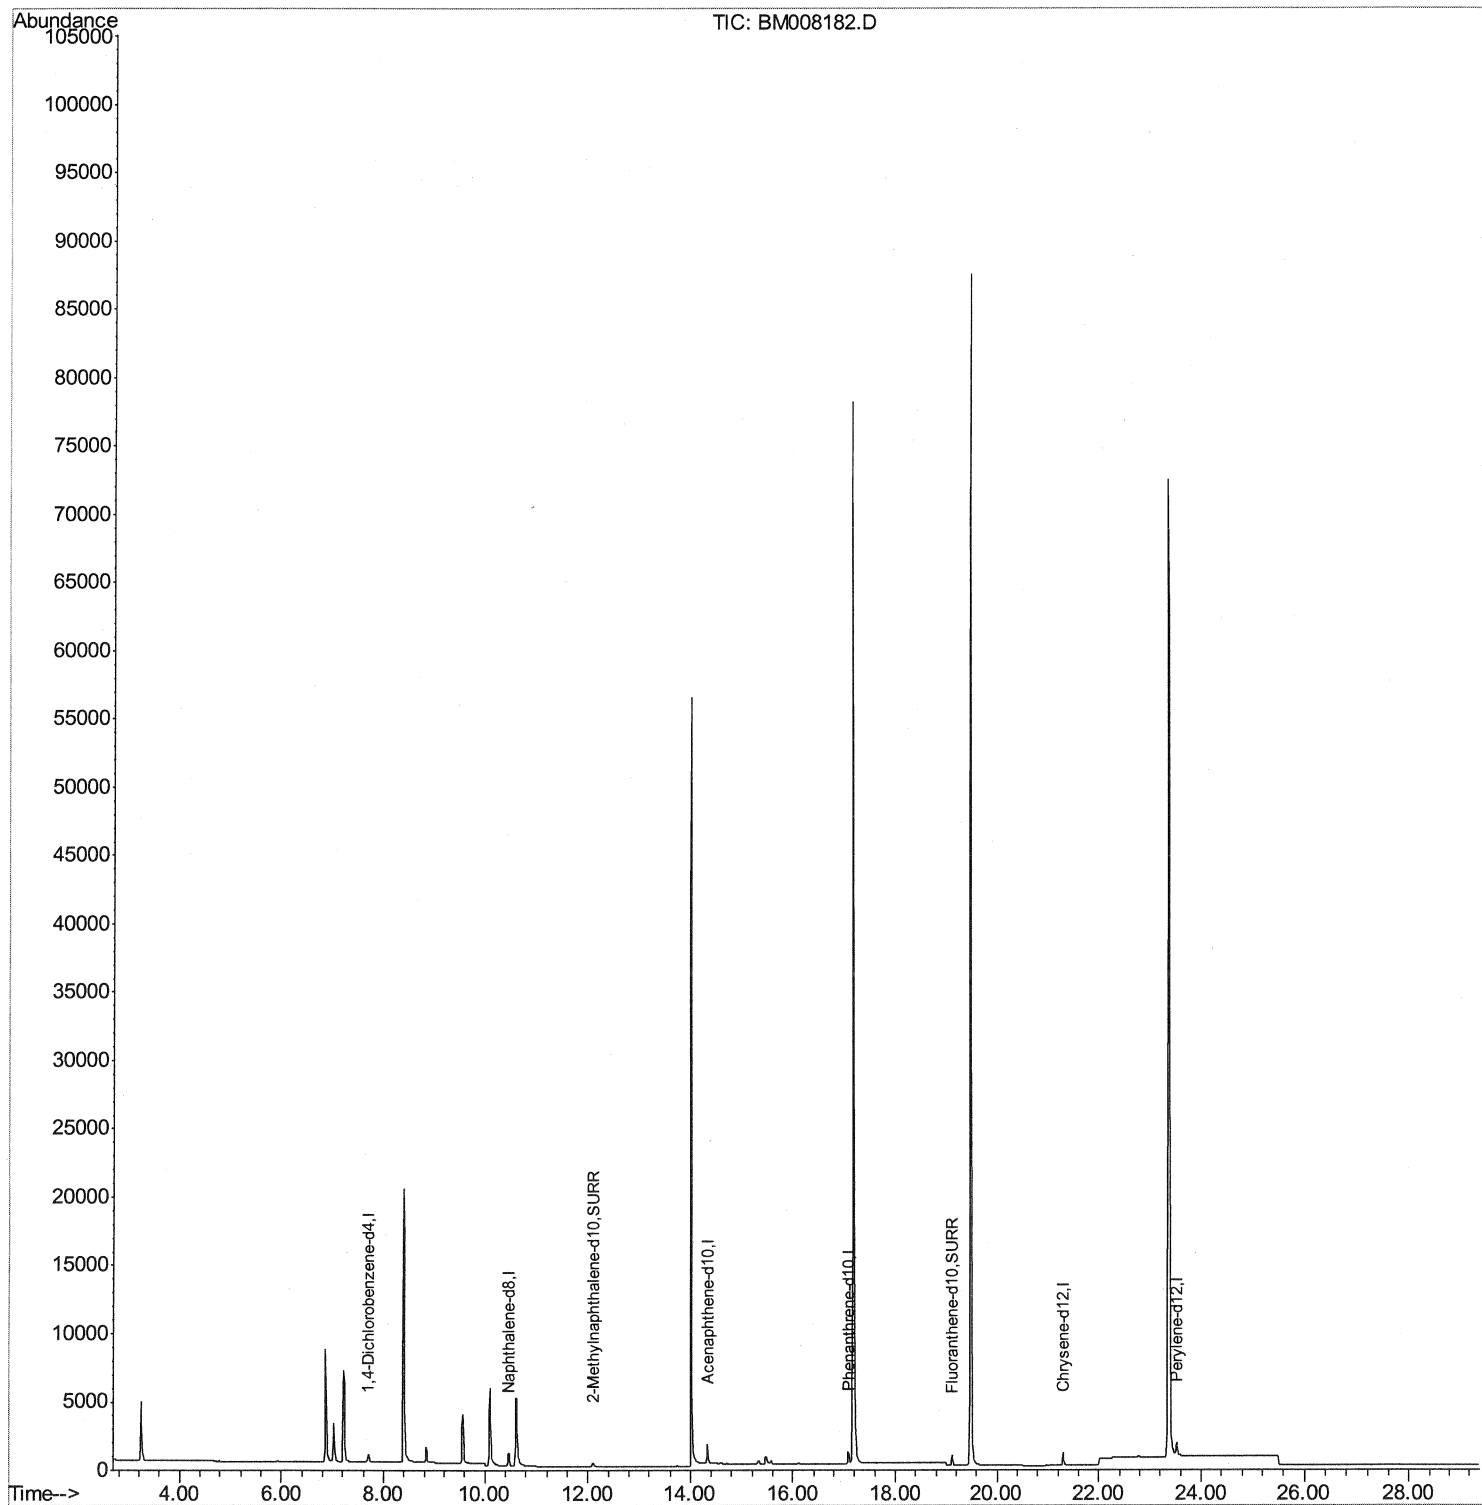




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120616\
Data File : BM008182.D
Acq On : 06 Dec 2016 13:30
Operator : UM/SJ
Sample : PB95036BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK36

Manual Integrations
APPROVED

sohil
12/7/2016 4:39:04 PM

Quant Time: Dec 06 14:13:22 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 13:48:59 2016
Response via : Initial Calibration

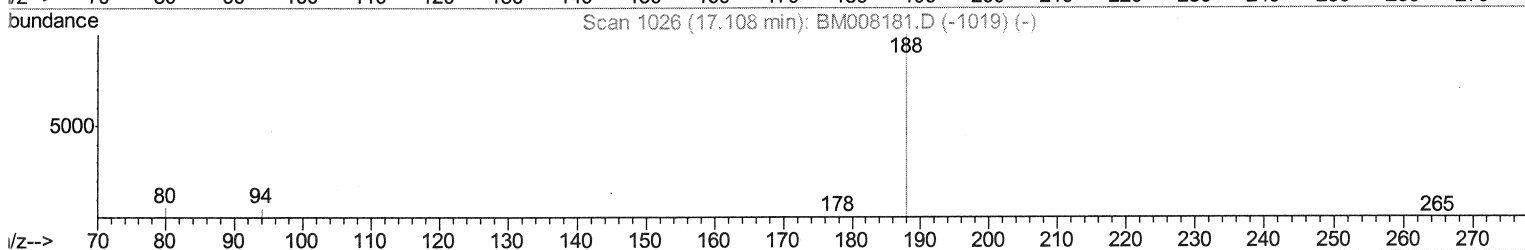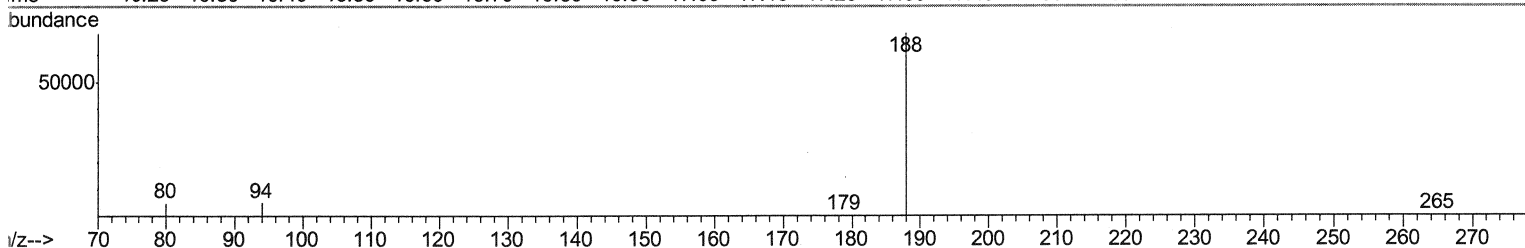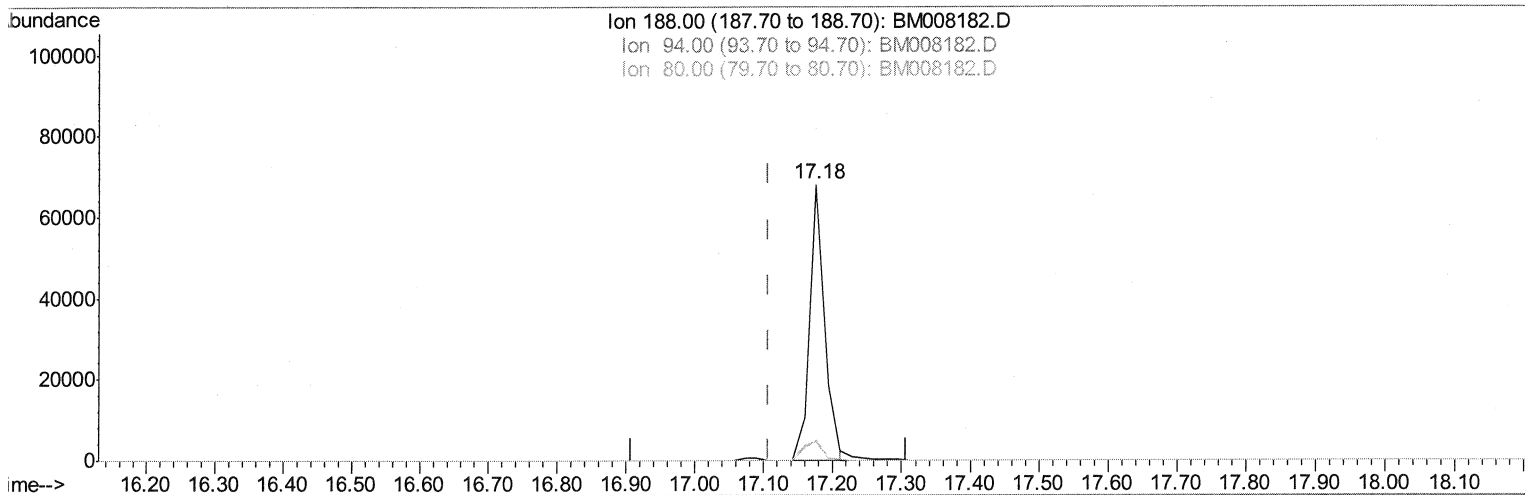

TIC: BM008182.D

(10) Phenanthrene-d10 (I)

17.176min (+0.068) 0.40ng/ul

response 102016

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.37#
80.00	11.80	6.95#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM120616\
Data File : BM008182.D
Acq On : 06 Dec 2016 13:30
Operator : UM/SJ
Sample : PB95036BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK36

Manual Integrations
APPROVED

sohil
12/7/2016 4:39:04 PM

Quant Time: Dec 06 14:13:22 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 13:48:59 2016
Response via : Initial Calibration

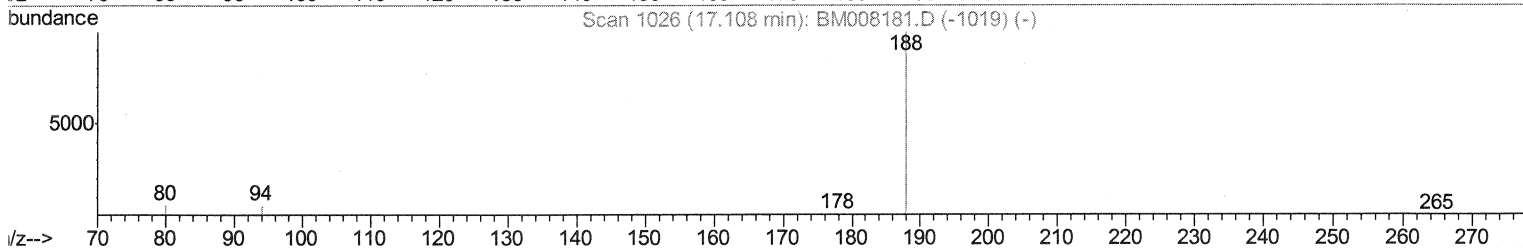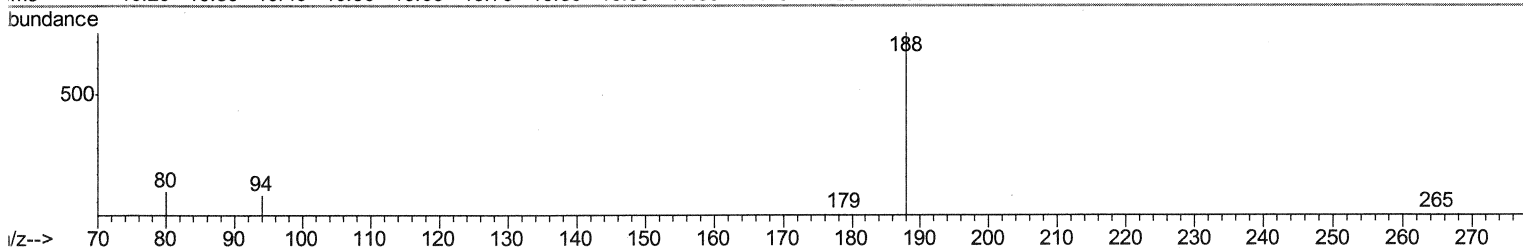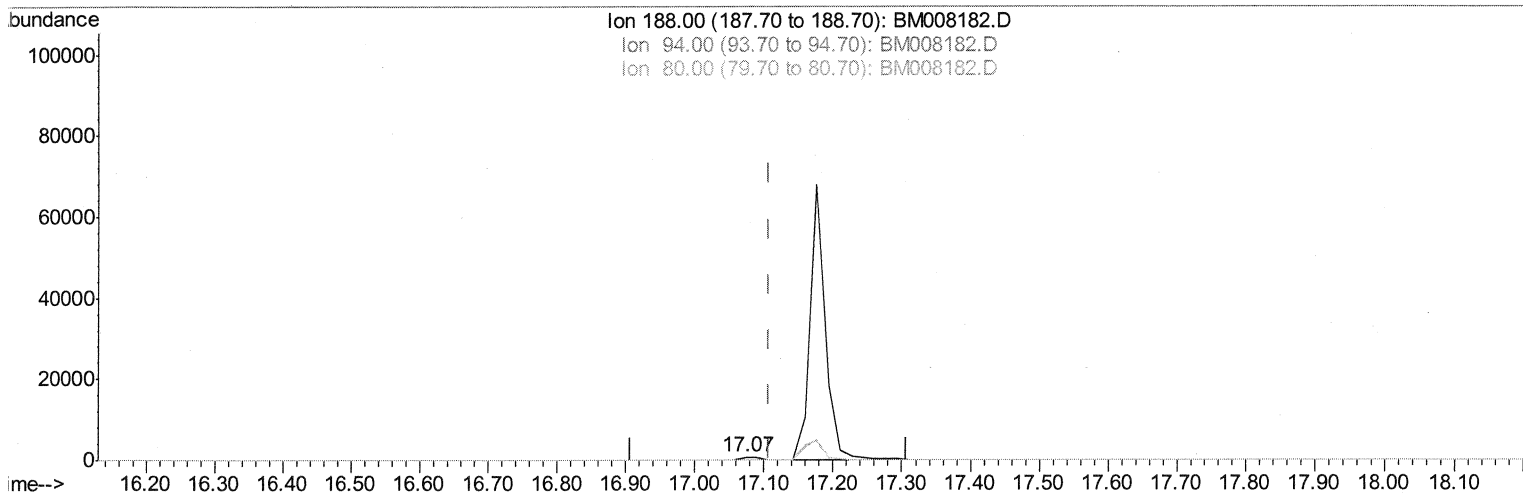

TIC: BM008182.D

(10) Phenanthrene-d10 (I)

17.073min (-0.035) 0.40ng/ul m

SJ 12/8/16

response 1591

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	16.55#
80.00	11.80	18.47#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM120616\
Data File : BM008182.D
Acq On : 06 Dec 2016 13:30
Operator : UM/SJ
Sample : PB95036BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK36

Manual Integrations
APPROVED

sohil
12/7/2016 4:39:04 PM

Quant Time: Dec 06 14:15:08 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 13:48:59 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	442	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.48	136	1433	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.33	164	819	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.07	188	1591m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.30	240	1362	0.40	ng/ul	0.01
20) Perylene-d12	23.52	264	1828	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.10	152	601	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	1153	0.26	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed