



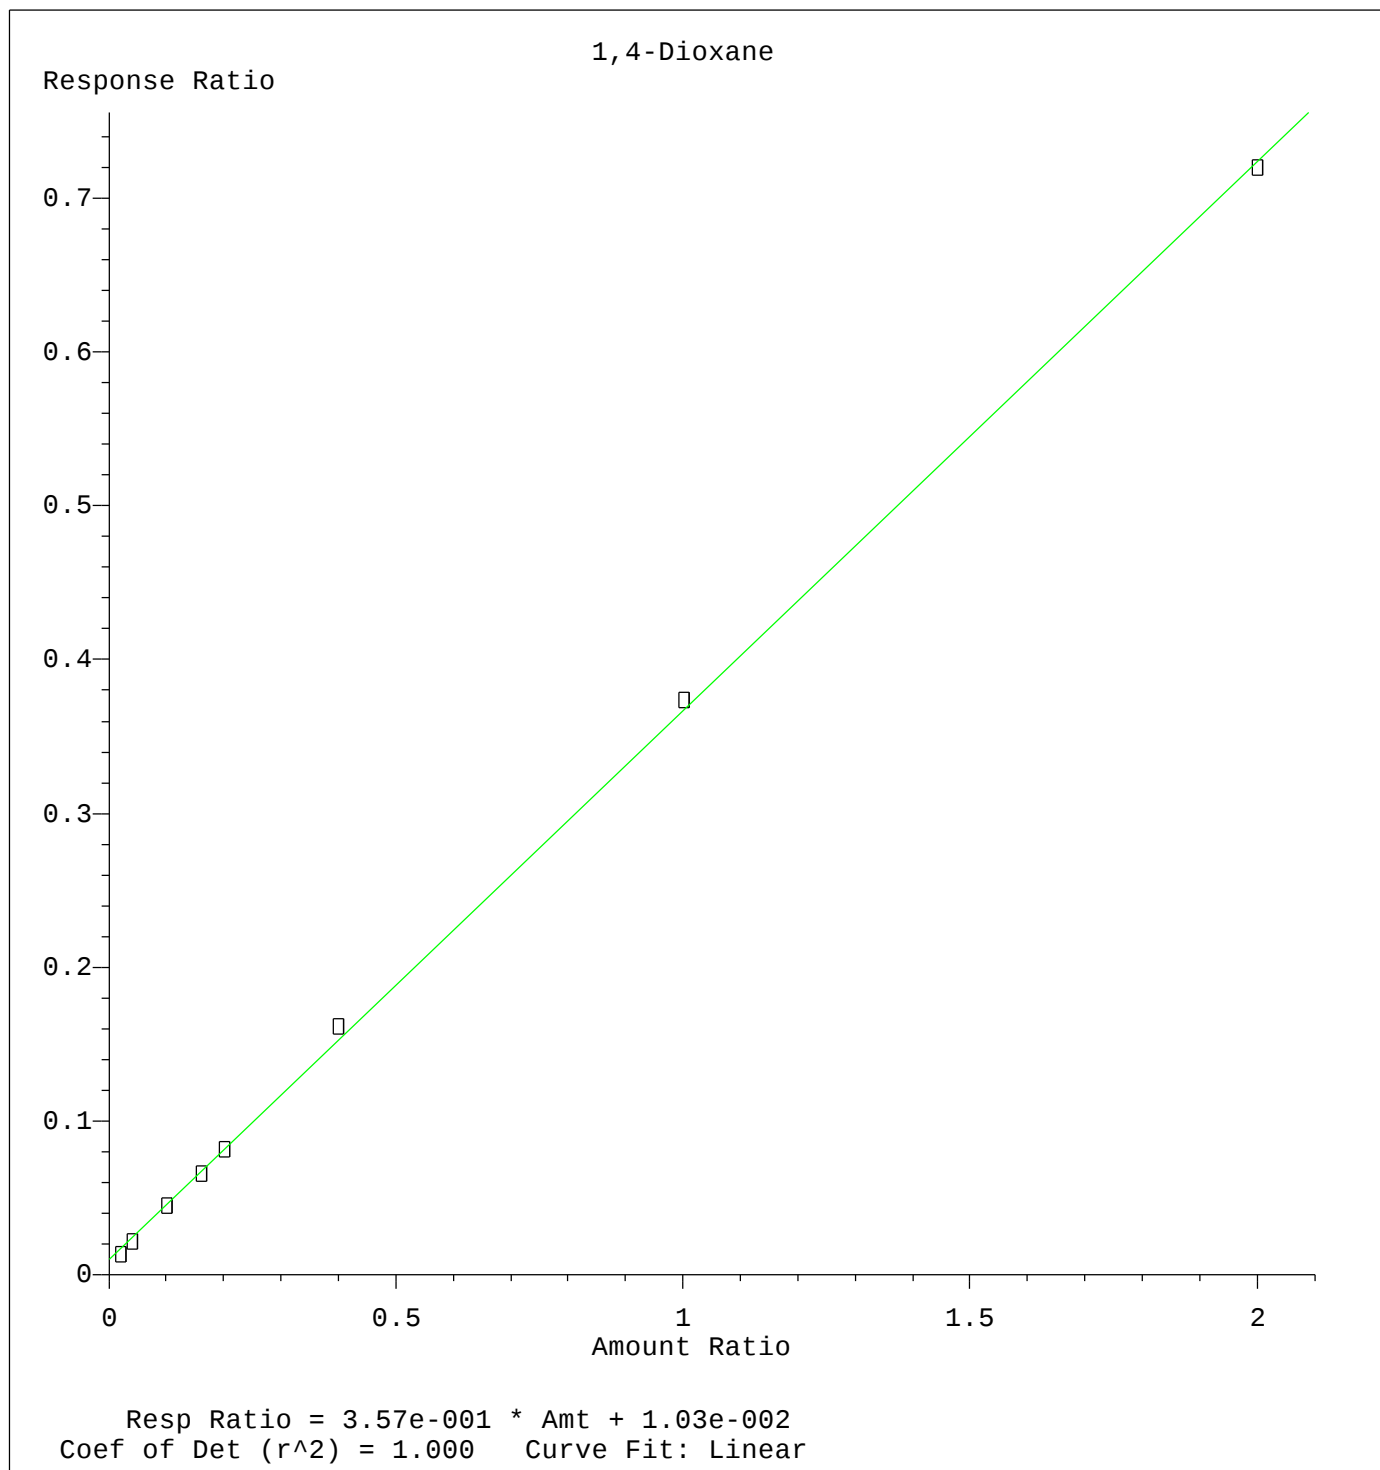


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Calibration Table Last Updated: Mon Dec 07 15:08:30 2015

4-Chloro-3-methylphenol

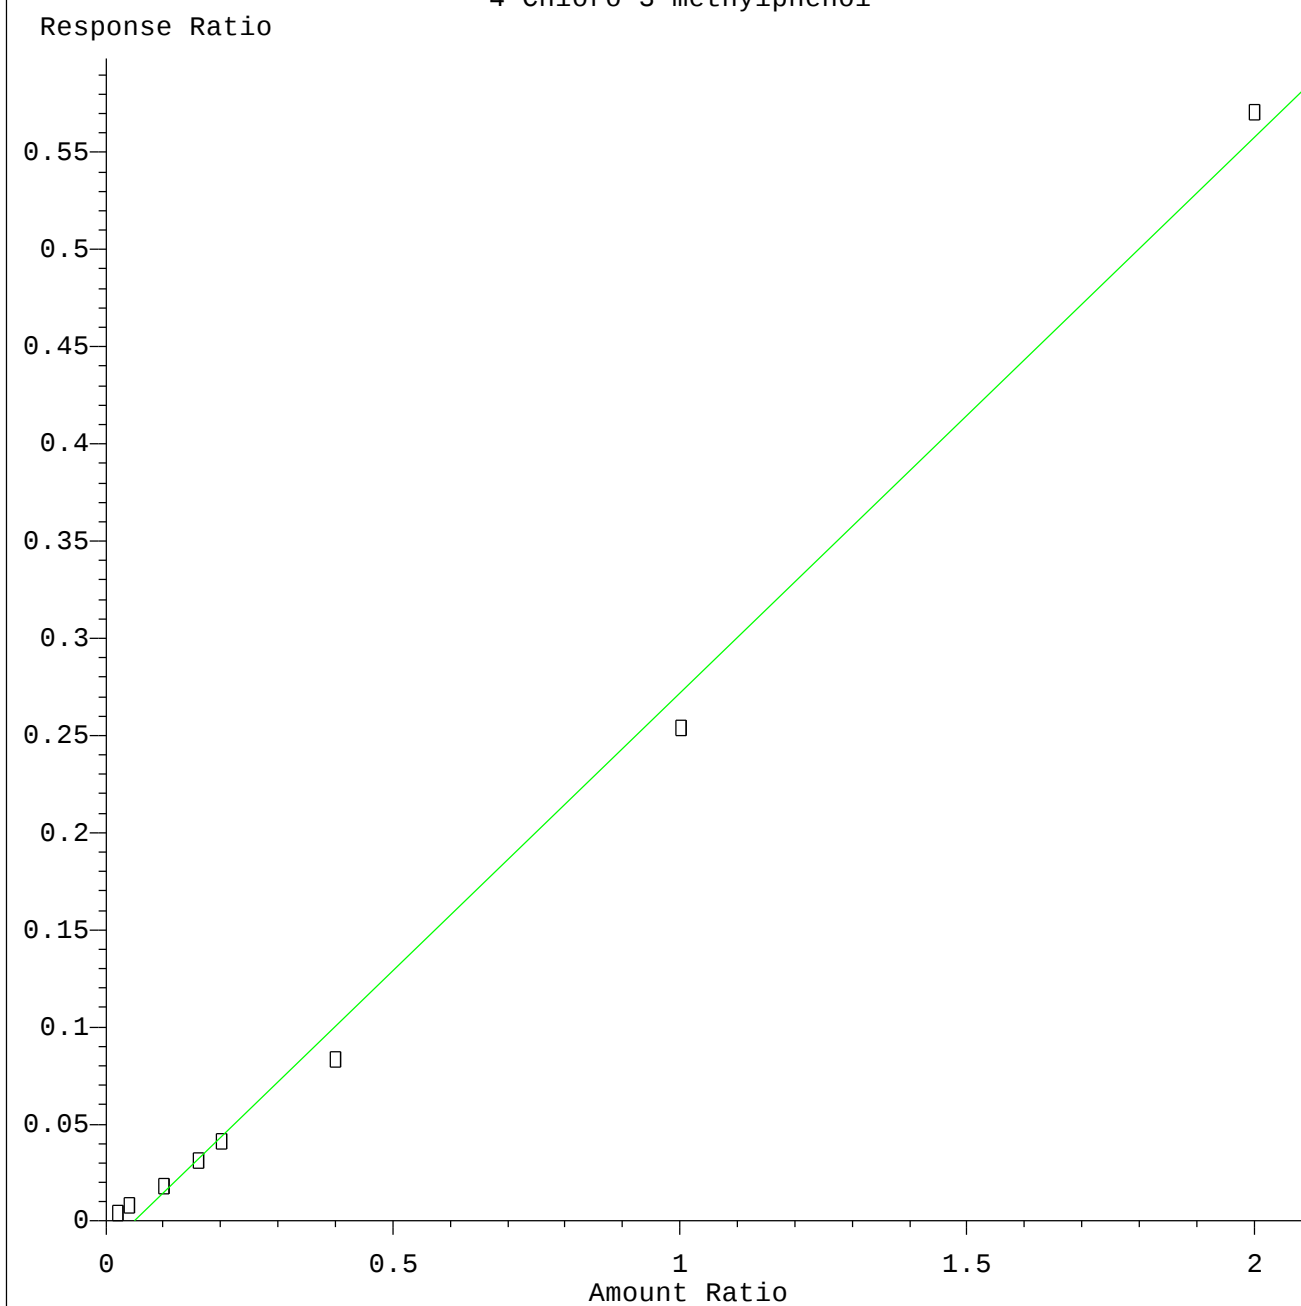

Resp Ratio = $2.86 \times 10^{-1} \times \text{Amt} - 1.41 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Calibration Table Last Updated: Mon Dec 07 15:08:30 2015

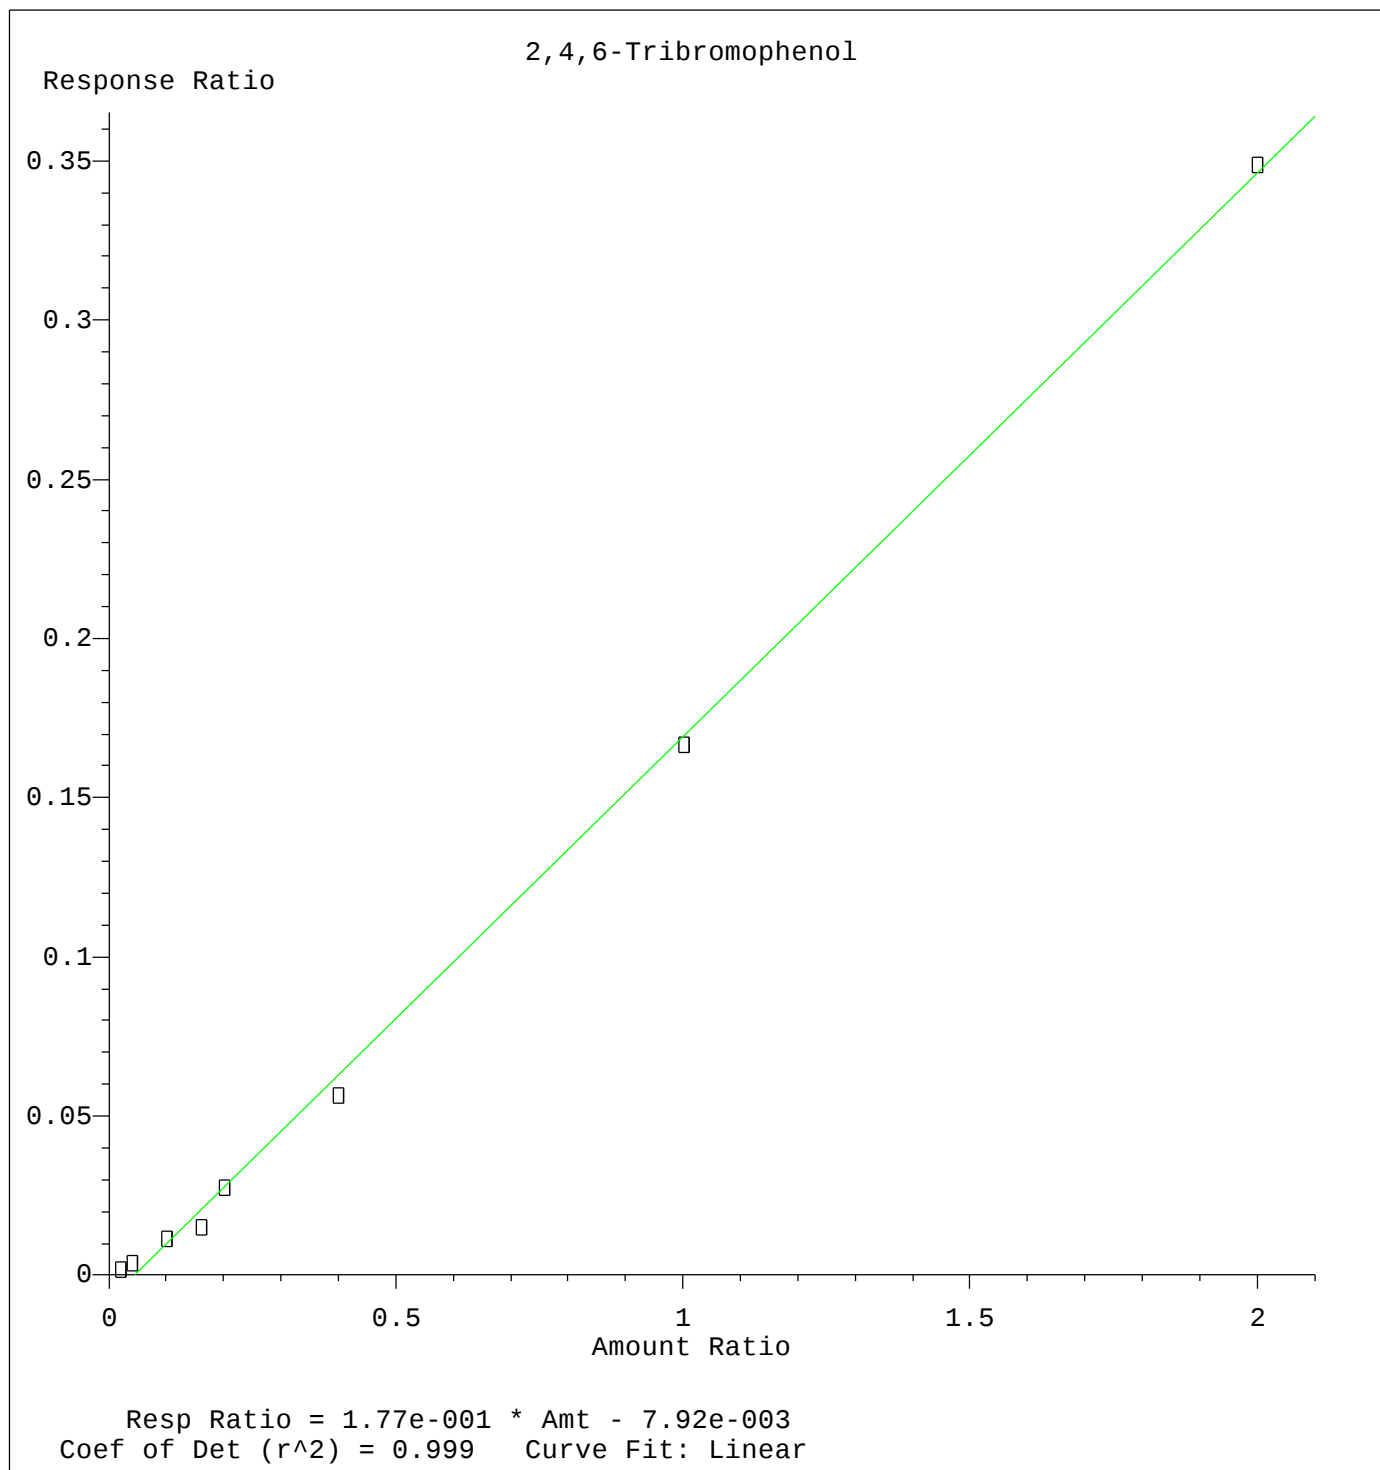

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Calibration Table Last Updated: Mon Dec 07 15:08:30 2015


2,4,5-Trichlorophenol

Response Ratio

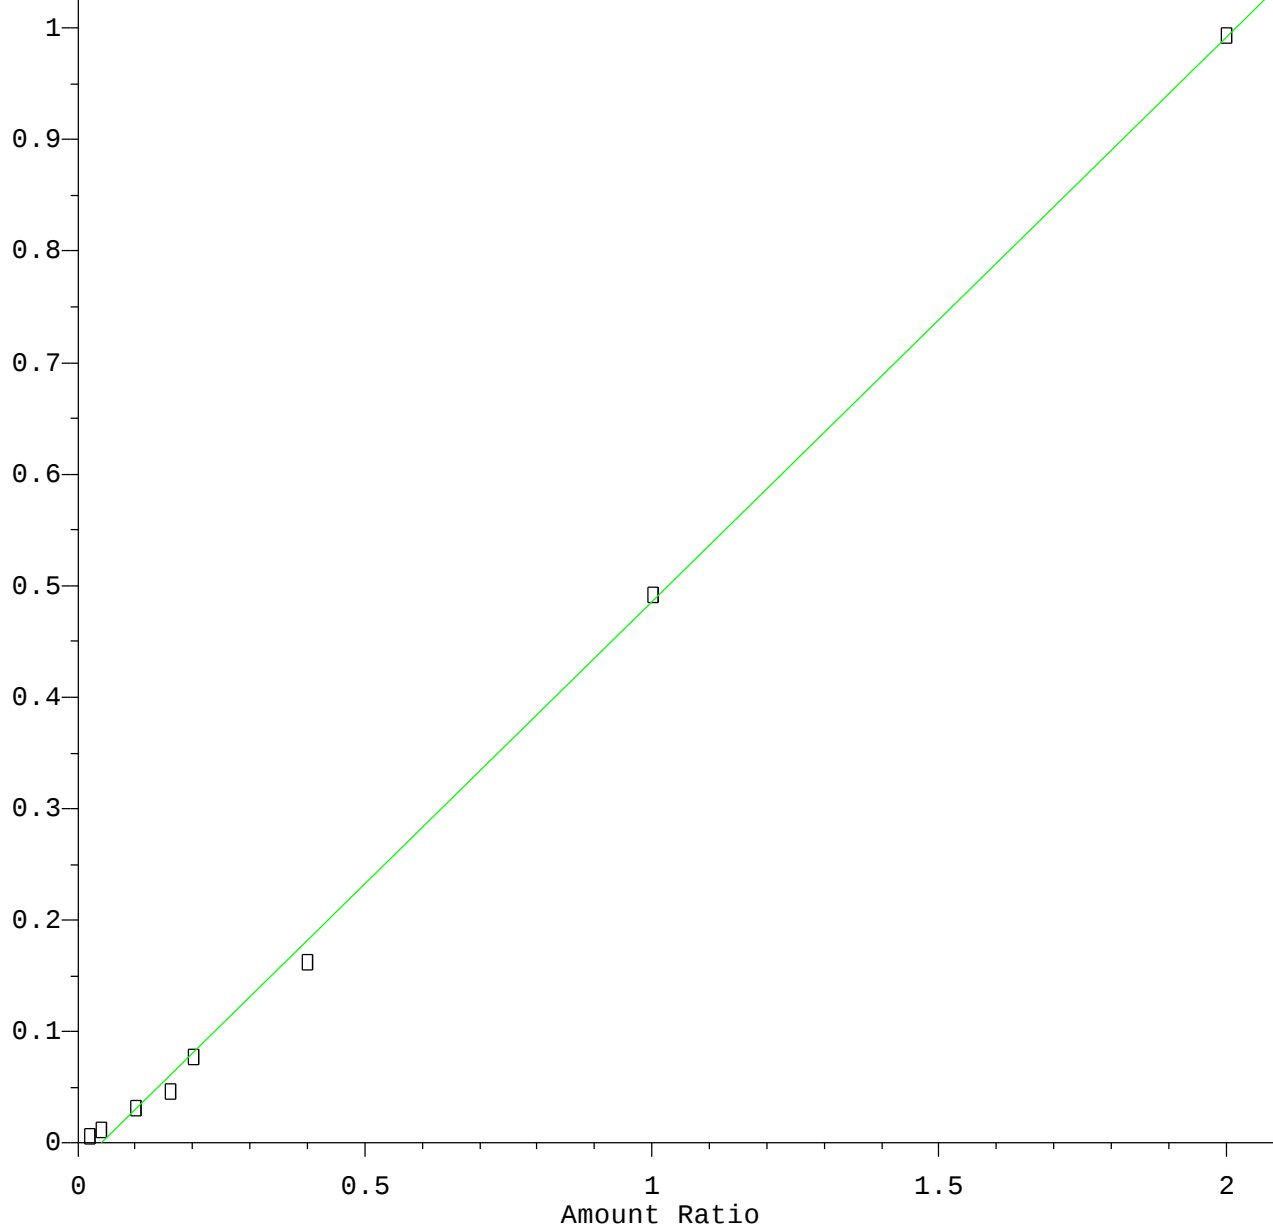


Resp Ratio = $5.06 \times 10^{-1} \times \text{Amt} - 2.06 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Calibration Table Last Updated: Mon Dec 07 15:08:30 2015

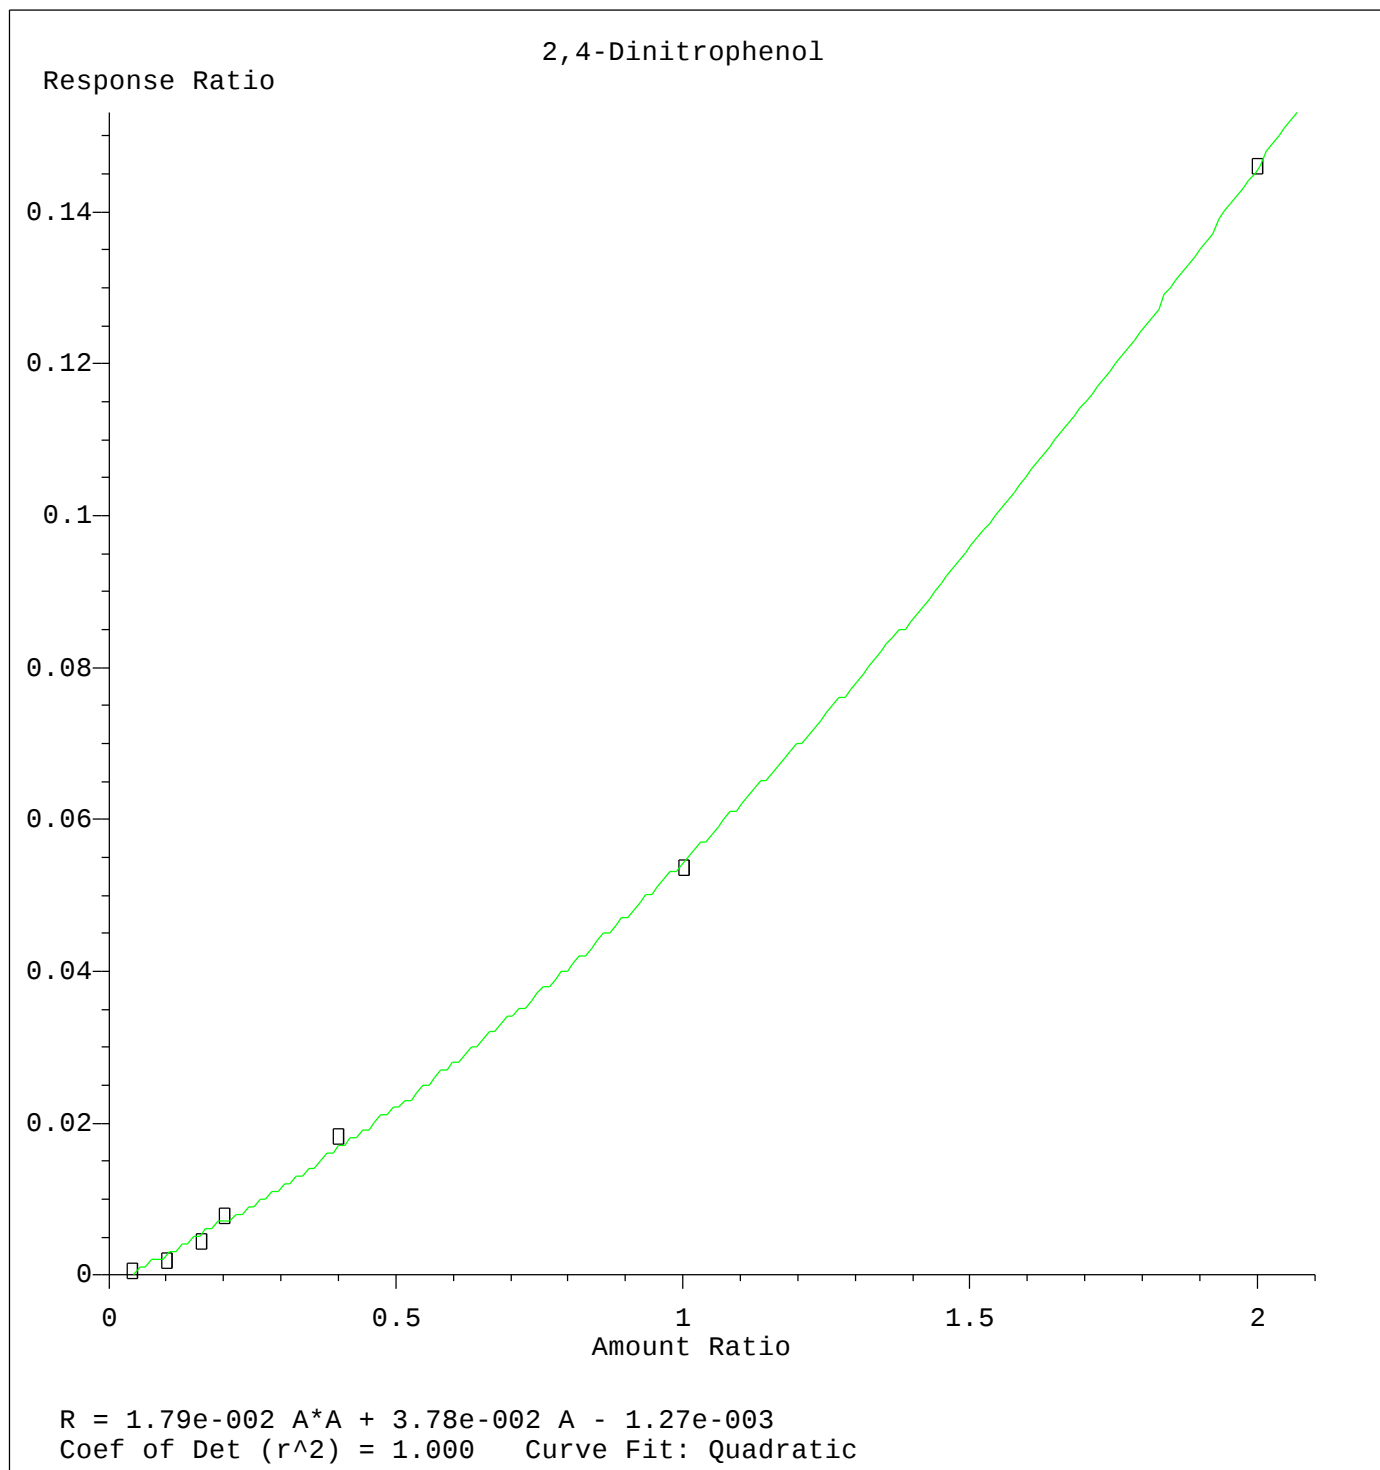


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Calibration Table Last Updated: Mon Dec 07 15:08:30 2015

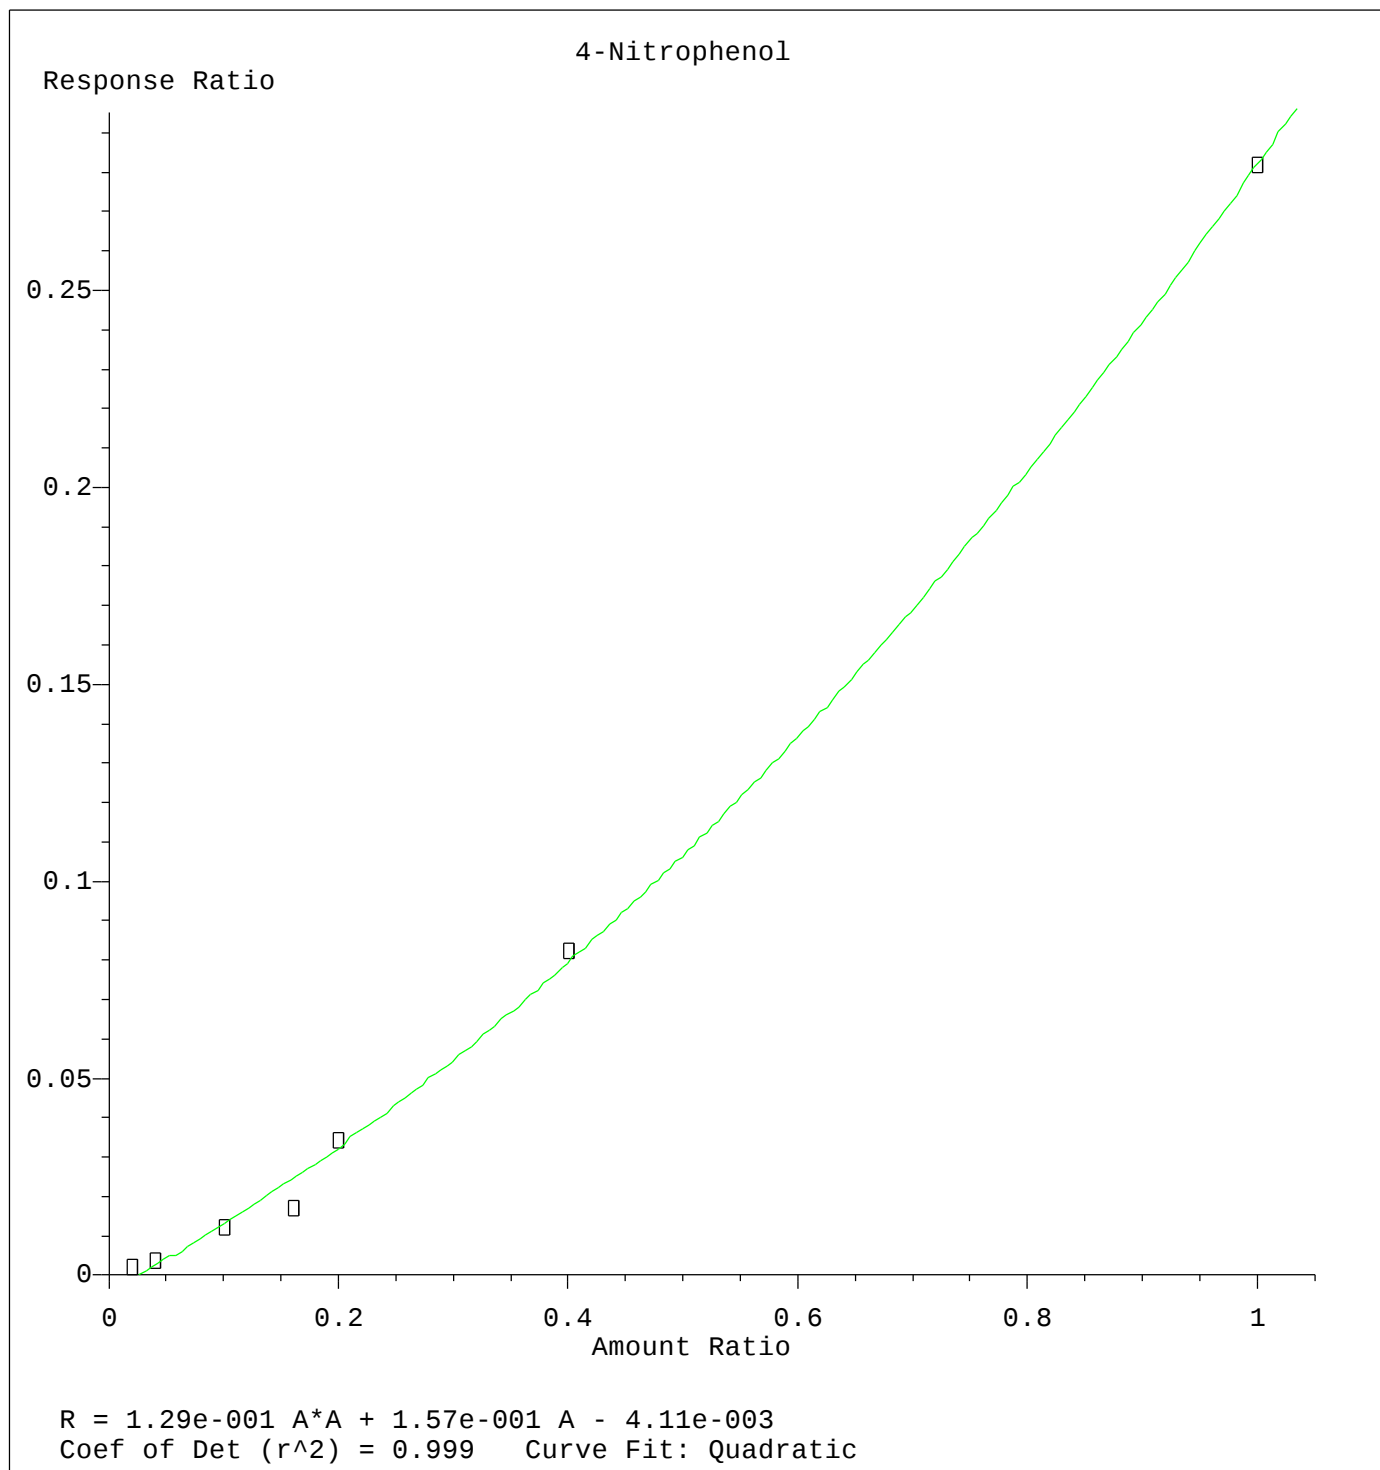

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Calibration Table Last Updated: Mon Dec 07 15:08:30 2015


4,6-Dinitro-2-methylphenol

Response Ratio

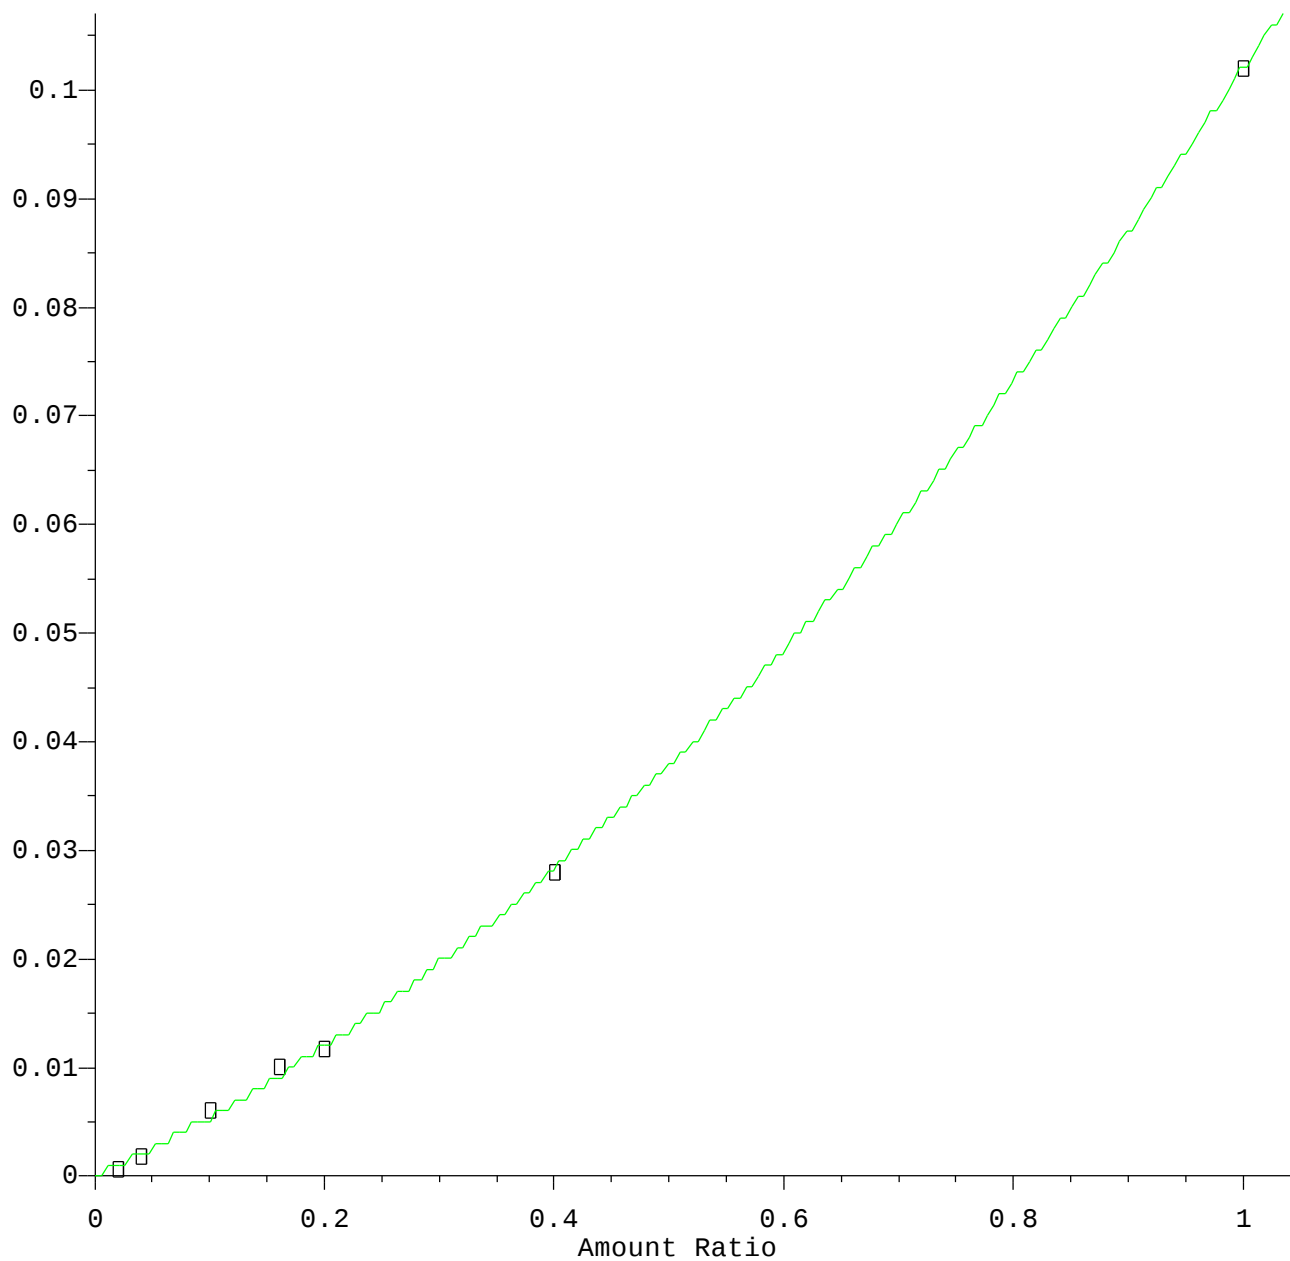


$R = 5.25e-002 A^2 + 4.94e-002 A + 9.32e-006$
Coef of Det (r^2) = 1.000 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Calibration Table Last Updated: Mon Dec 07 15:08:30 2015

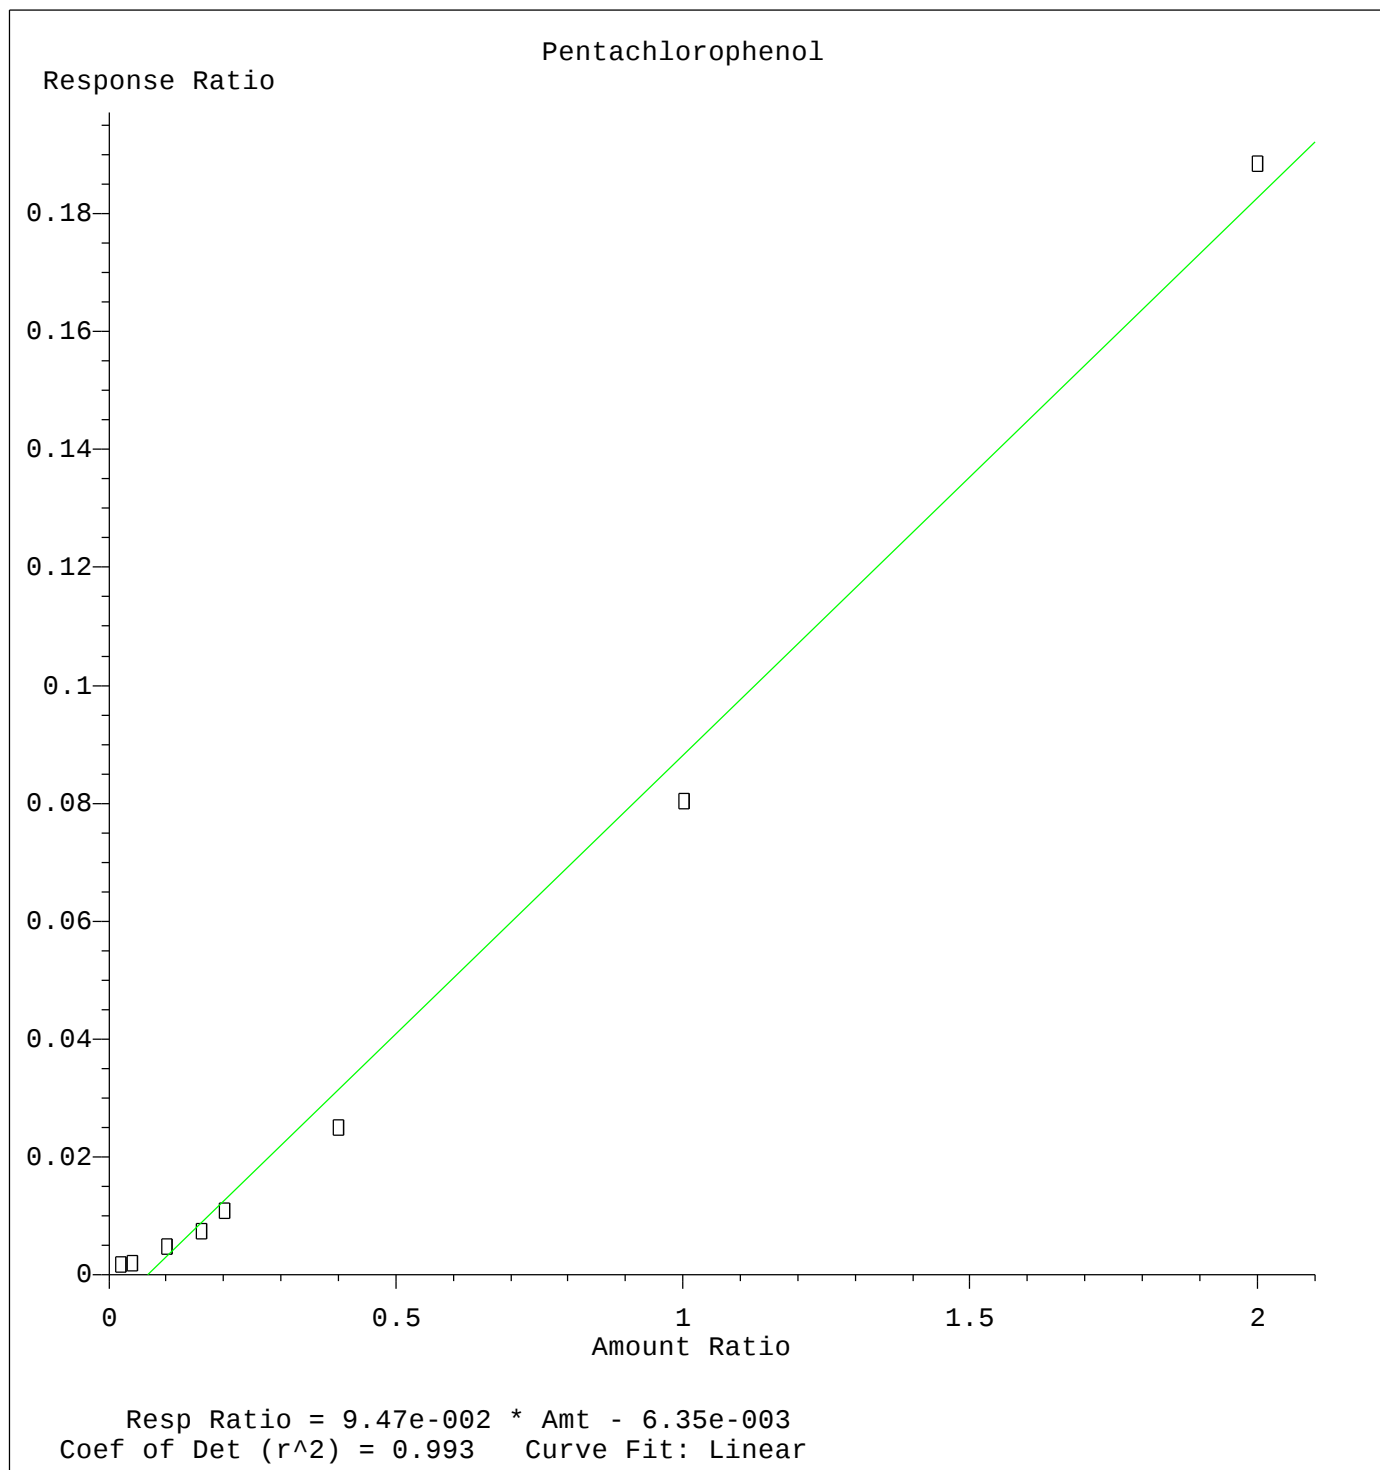


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Calibration Table Last Updated: Mon Dec 07 15:08:30 2015

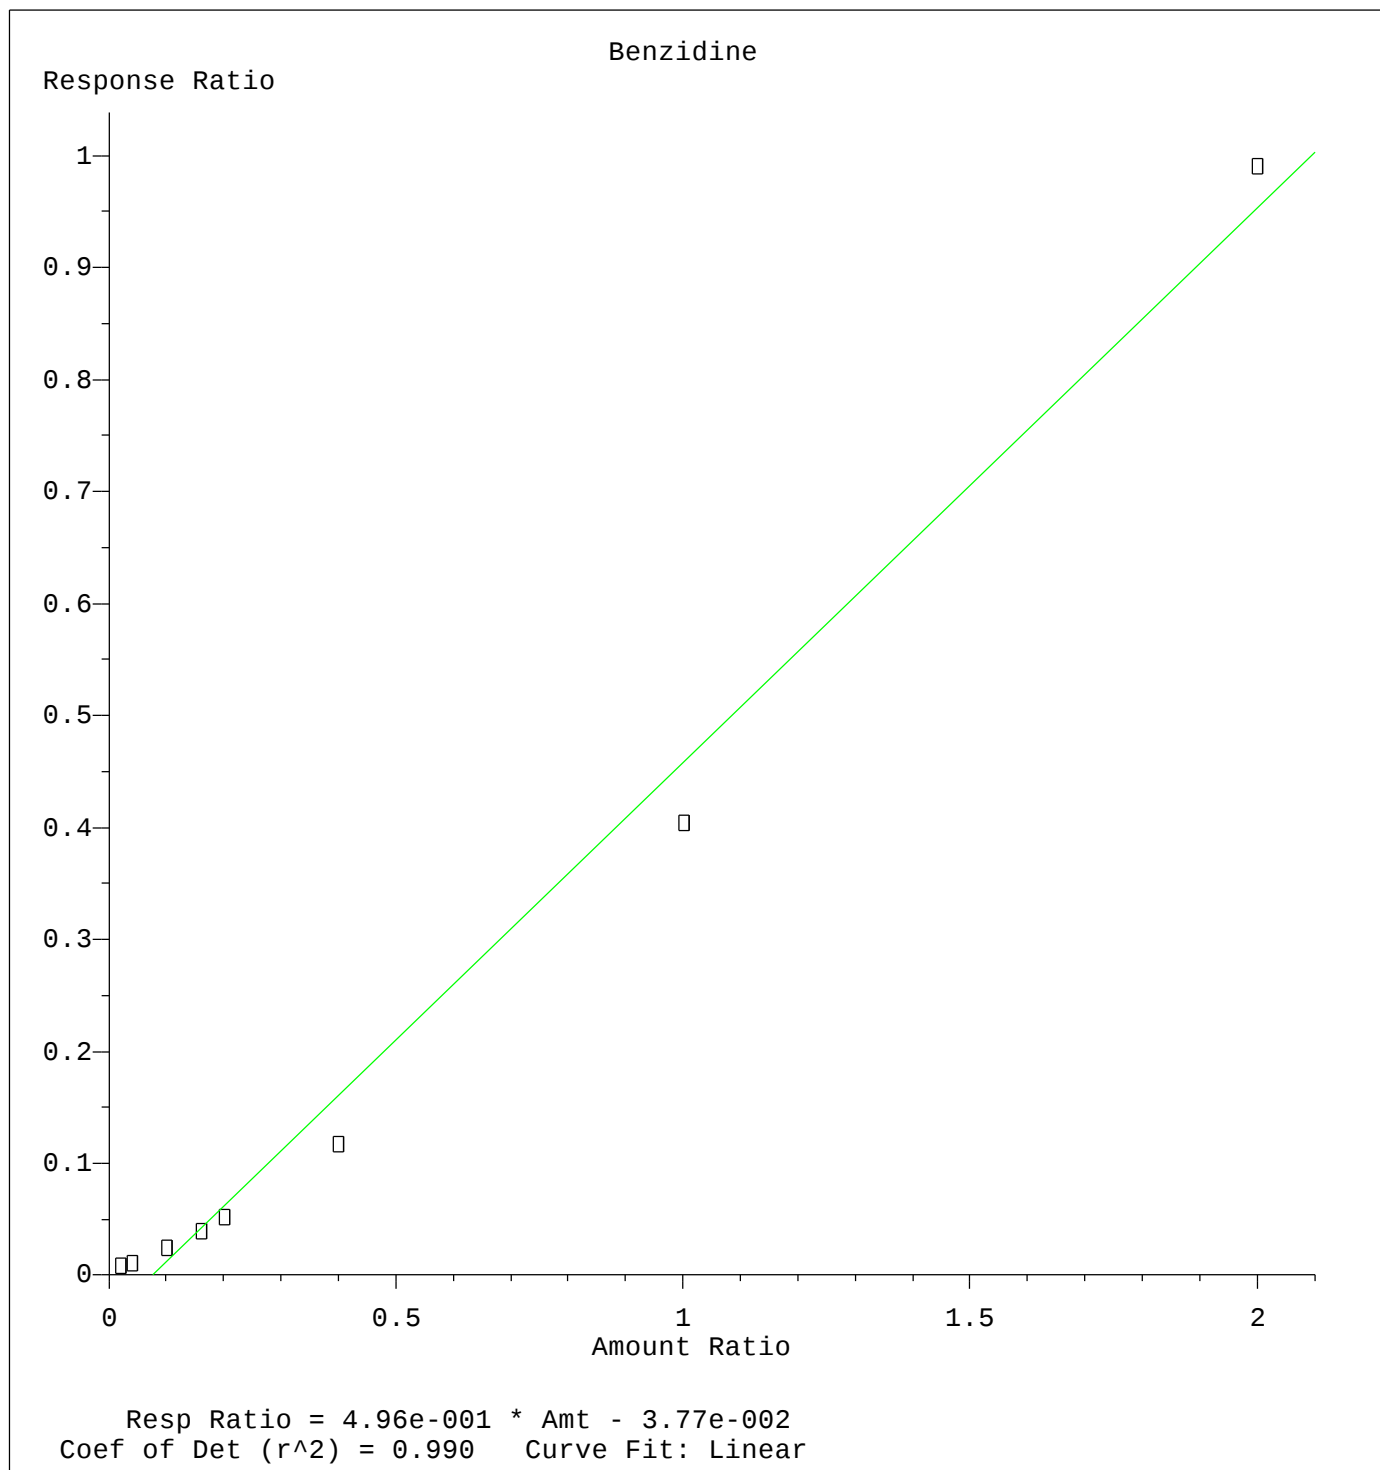

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Calibration Table Last Updated: Mon Dec 07 15:08:30 2015

3,3'-Dichlorobenzidine

Response Ratio

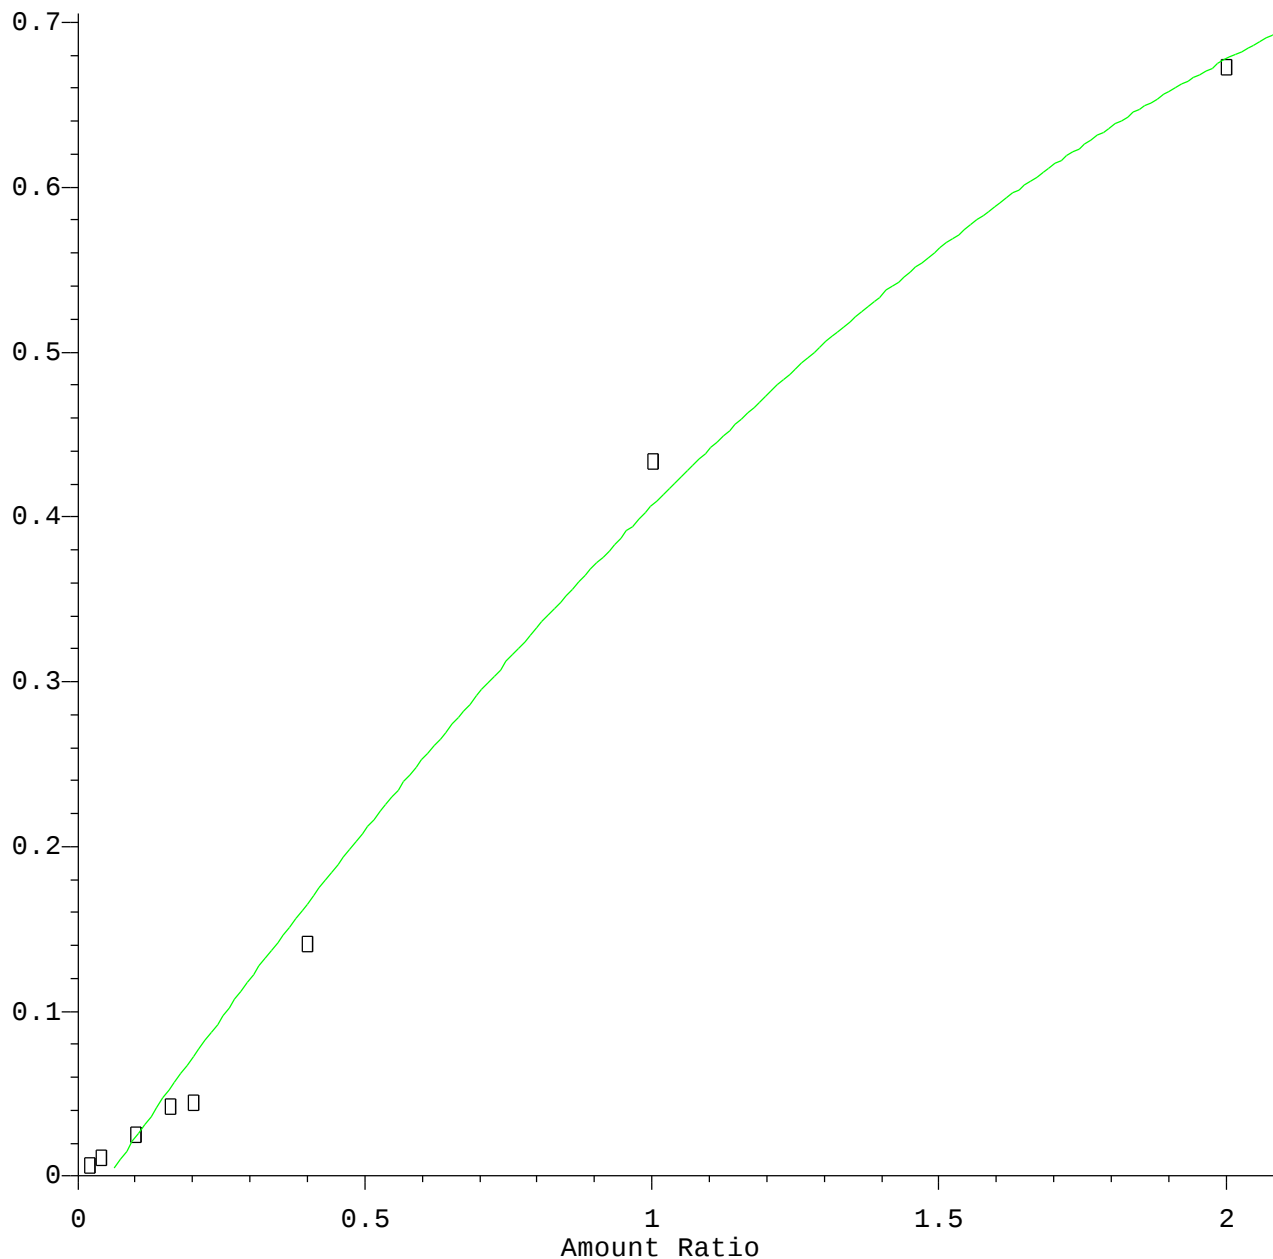

$R = -8.16e-002 A^2 + 5.16e-001 A - 2.75e-002$
Coef of Det (r^2) = 0.993 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Calibration Table Last Updated: Mon Dec 07 15:08:30 2015