
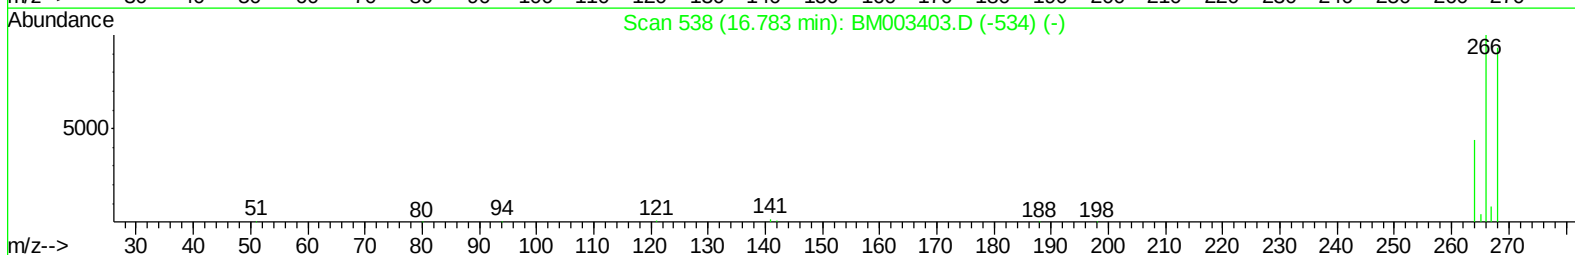
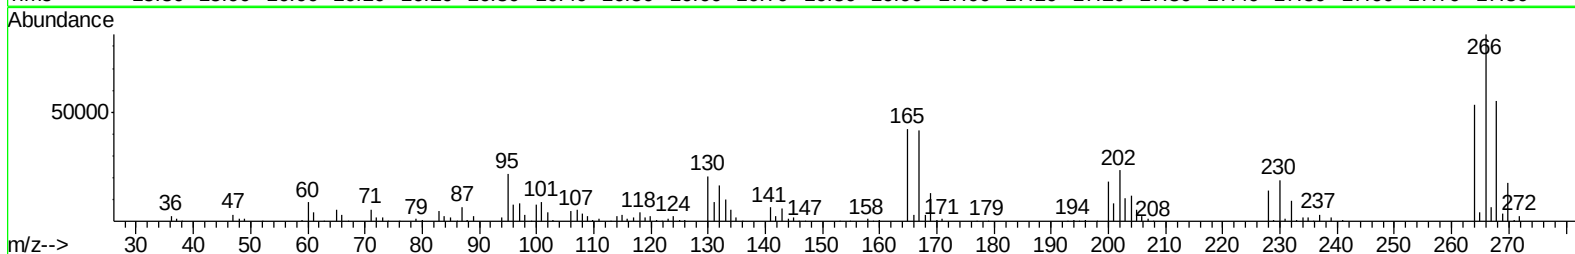


Data Path : Z:\HPCHEM1\BNA M\Data\BM120715\
Data File : BM003398.D
Acq On : 07 Dec 2015 08:46
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 13:07:22 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SIM-BM120715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 15:08:30 2015
Response via : Initial Calibration

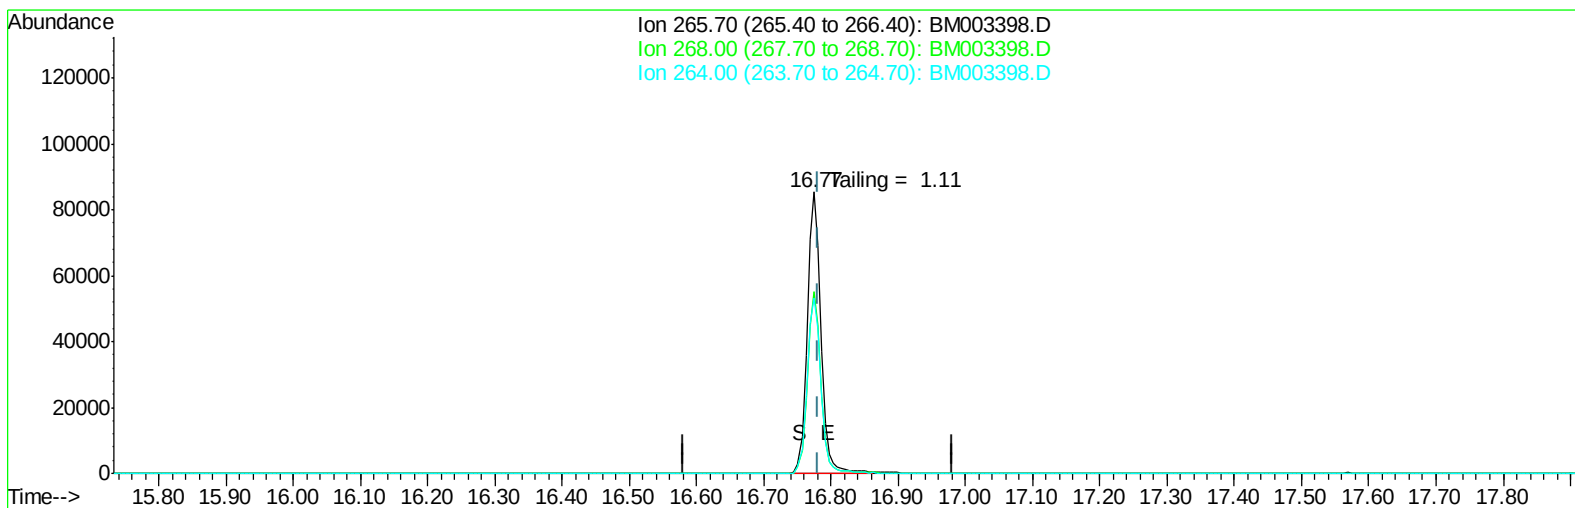

TIC: BM003398.D

(30) Pentachlorophenol (C)




16.774min (-0.008) 0.00ng

response 123076

Ion	Exp%	Act%
265.70	100	100
268.00	78.30	64.38
264.00	59.90	62.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM120715\
Data File : BM003398.D
Acq On : 07 Dec 2015 08:46
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 13:07:22 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SIM-BM120715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 15:08:30 2015
Response via : Initial Calibration

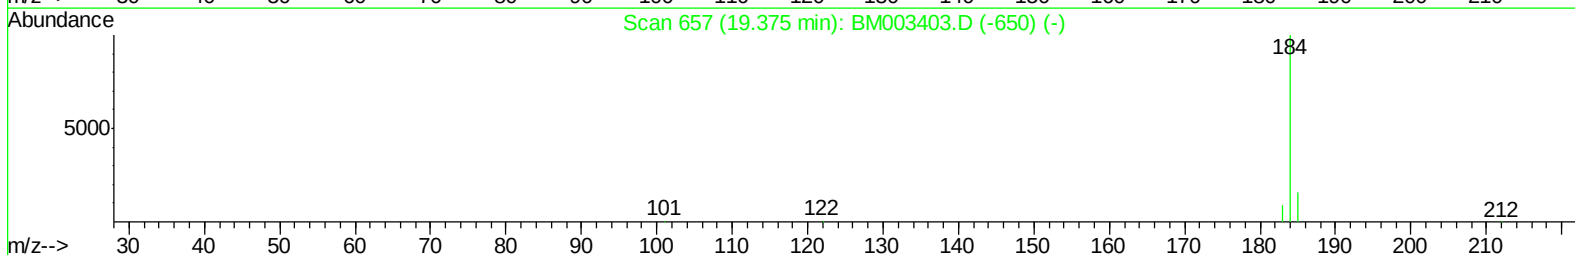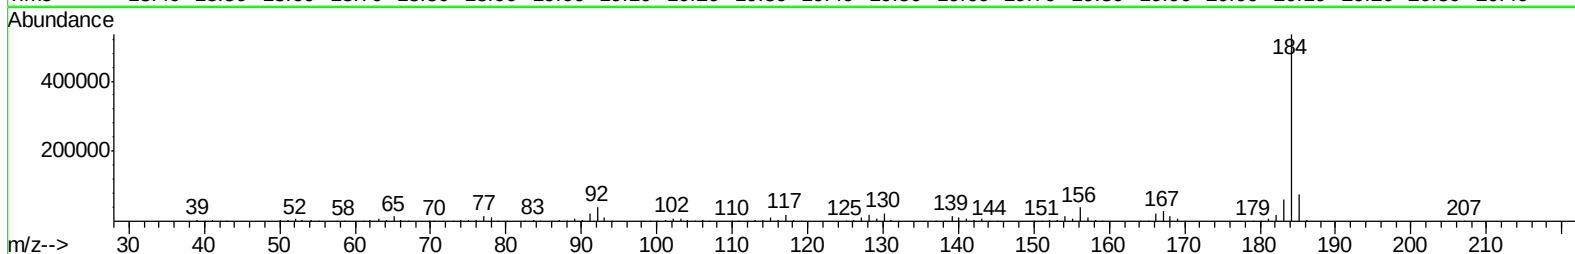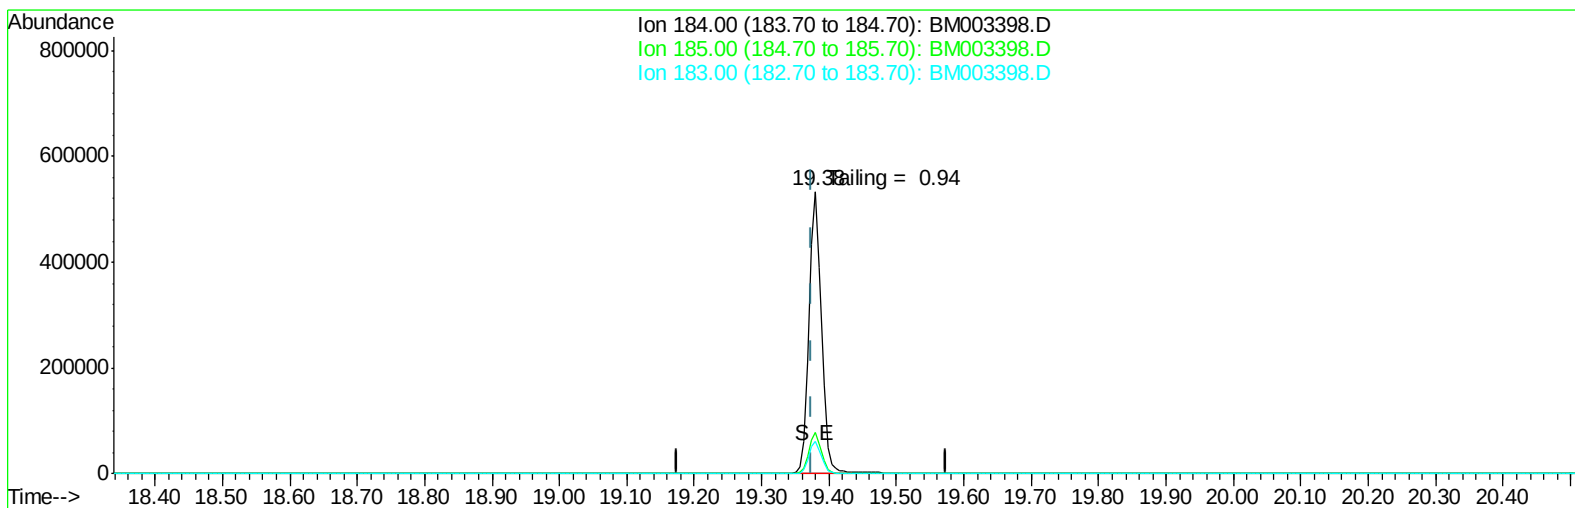

TIC: BM003398.D

(32) Benzidine

19.380min (+0.005) 7615.49ng

response 676434

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.60
183.00	10.80	11.38
0.00	0.00	0.00