


Data Path : Z:\HPCHEM1\BNA M\DATA\BM120715\
Data File : BM003398.D
Acq On : 07 Dec 2015 08:46
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM120715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 07 15:08:30 2015

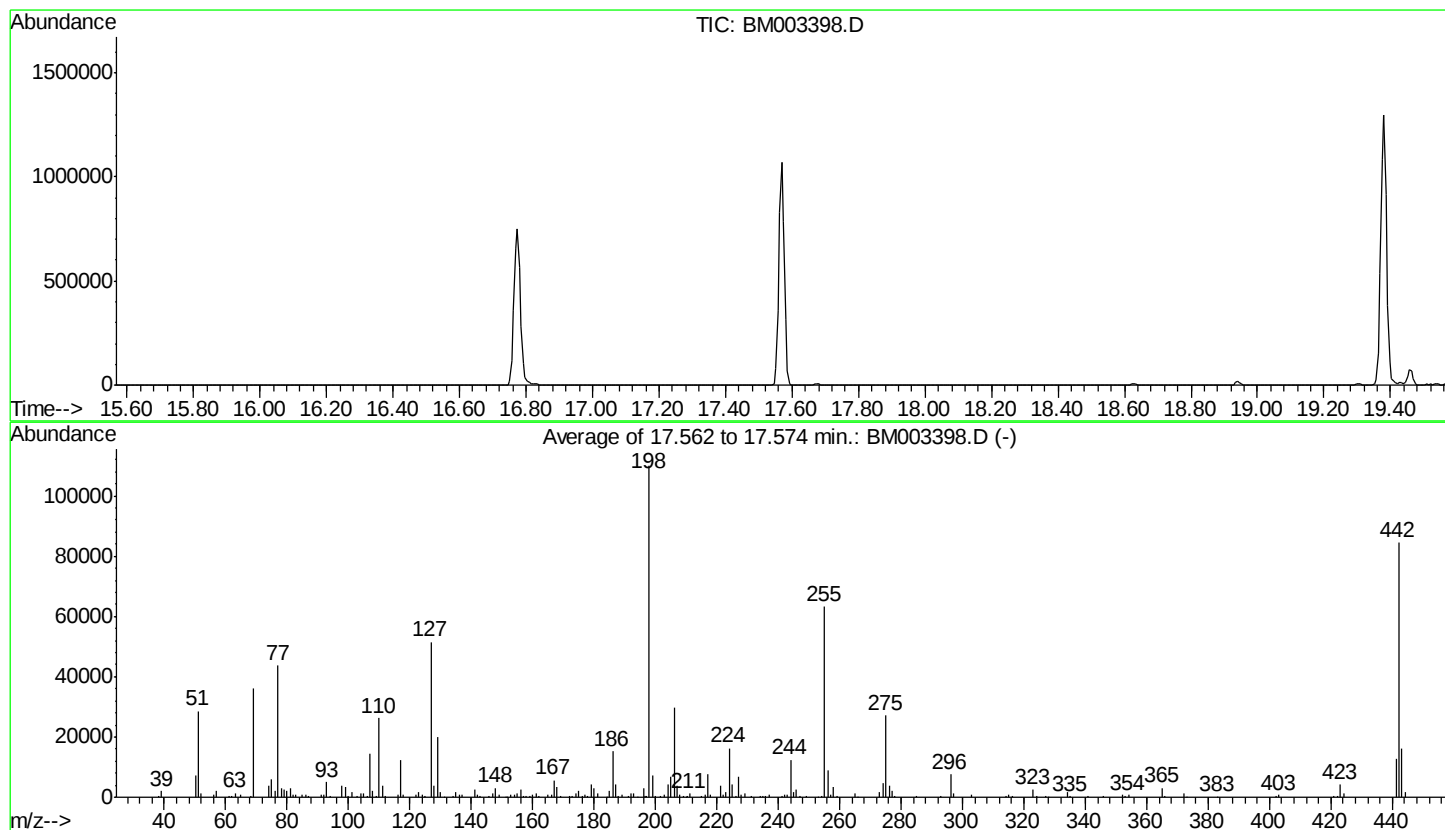

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.9	28501	PASS
68	69	0.00	2	1.7	607	PASS
69	198	0.00	100	32.8	36064	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.9	51613	PASS
197	198	0.00	2	0.3	378	PASS
198	198	100	100	100.0	110061	PASS
199	198	5	9	6.8	7442	PASS
275	198	10	60	24.6	27109	PASS
365	198	1	100	2.9	3160	PASS
441	442	0.01	24	15.2	12845	PASS
442	198	50	100	76.8	84517	PASS
443	442	15	24	18.9	15987	PASS