

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM120717\
 Data File : BM013241.D
 Acq On : 07 Dec 2017 13:53
 Operator : SJ/JU
 Sample : I6647-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0279

Manual Integrations
 APPROVED

Sohil
 12/8/2017 11:15:19 AM

Quant Time: Dec 08 03:03:31 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 08 01:54:15 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	198163	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	766838	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.35	164	406857	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.10	188	798147	20.00	ng/ul	0.01
75) Chrysene-d12	21.29	240	841219	20.00	ng/ul	0.01
83) Perylene-d12	23.53	264	898431	20.00	ng/ul	0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	17166m	4.29	ng/uL	0.00
5) Phenol-d5	6.89	99	381339	22.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	220247	22.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	326773	24.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	308662	21.07	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	158597	26.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	173826	26.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	322909	24.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	320785	26.02	ng/ul	0.01
43) Dimethylphthalate-d6	13.76	166	892824	24.66	ng/ul	0.00
46) Acenaphthylene-d8	14.04	160	1154463	25.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	135466	21.54	ng/ul	0.00
57) Fluorene-d10	15.35	176	739810	23.76	ng/ul	0.01
62) 4,6-Dinitro-2-methylphenol	15.47	200	90924	18.11	ng/ul	0.01
70) Anthracene-d10	17.19	188	1045539	26.16	ng/ul	0.00
76) Pyrene-d10	19.49	212	1090823	26.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.39	264	1163021	25.41	ng/ul	0.02

Target Compounds

					Ovalue	
6) Phenol	6.92	94	42353	2.499	ng/ul#	77
34) 2-Methylnaphthalene	12.15	142	60338	2.034	ng/ul	83
44) Dimethylphthalate	13.80	163	209065	6.037	ng/ul#	98
49) Acenaphthene	14.41	153	226822	8.053	ng/ul	97
53) Dibenzofuran	14.75	168	83646	2.012	ng/ul#	85
58) Fluorene	15.40	166	316221	9.193	ng/ul#	99
69) Phenanthrene	17.14	178	2756073	60.781	ng/ul	99
71) Anthracene	17.23	178	276768	5.971	ng/ul	95
72) Carbazole	17.50	167	199744	5.010	ng/ul#	97
74) Fluoranthene	19.16	202	3180370	57.234	ng/ul#	94
77) Pyrene	19.53	202	2951146	57.745	ng/ul#	95
80) Benzo(a)anthracene	21.27	228	1095854	20.532	ng/ul	97
82) Chrysene	21.32	228	1481976	29.929	ng/ul	97
85) Benzo(b)fluoranthene	22.86	252	1870679	30.887	ng/ul#	95
86) Benzo(k)fluoranthene	22.90	252	567028m	9.949	ng/ul	
88) Benzo(a)pyrene	23.43	252	1097253	20.168	ng/ul#	96
89) Indeno(1,2,3-cd)pyrene	25.78	276	872371	16.160	ng/ul#	96
90) Dibenzo(a,h)anthracene	25.78	278	229088m	4.984	ng/ul	
91) Benzo(g,h,i)perylene	26.48	276	870718	20.449	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM120717\
Data File : BM013241.D
Acq On : 07 Dec 2017 13:53
Operator : SJ/JU
Sample : I6647-11
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0279

Quant Time: Dec 08 03:03:31 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 08 01:54:15 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/8/2017 11:15:19 AM

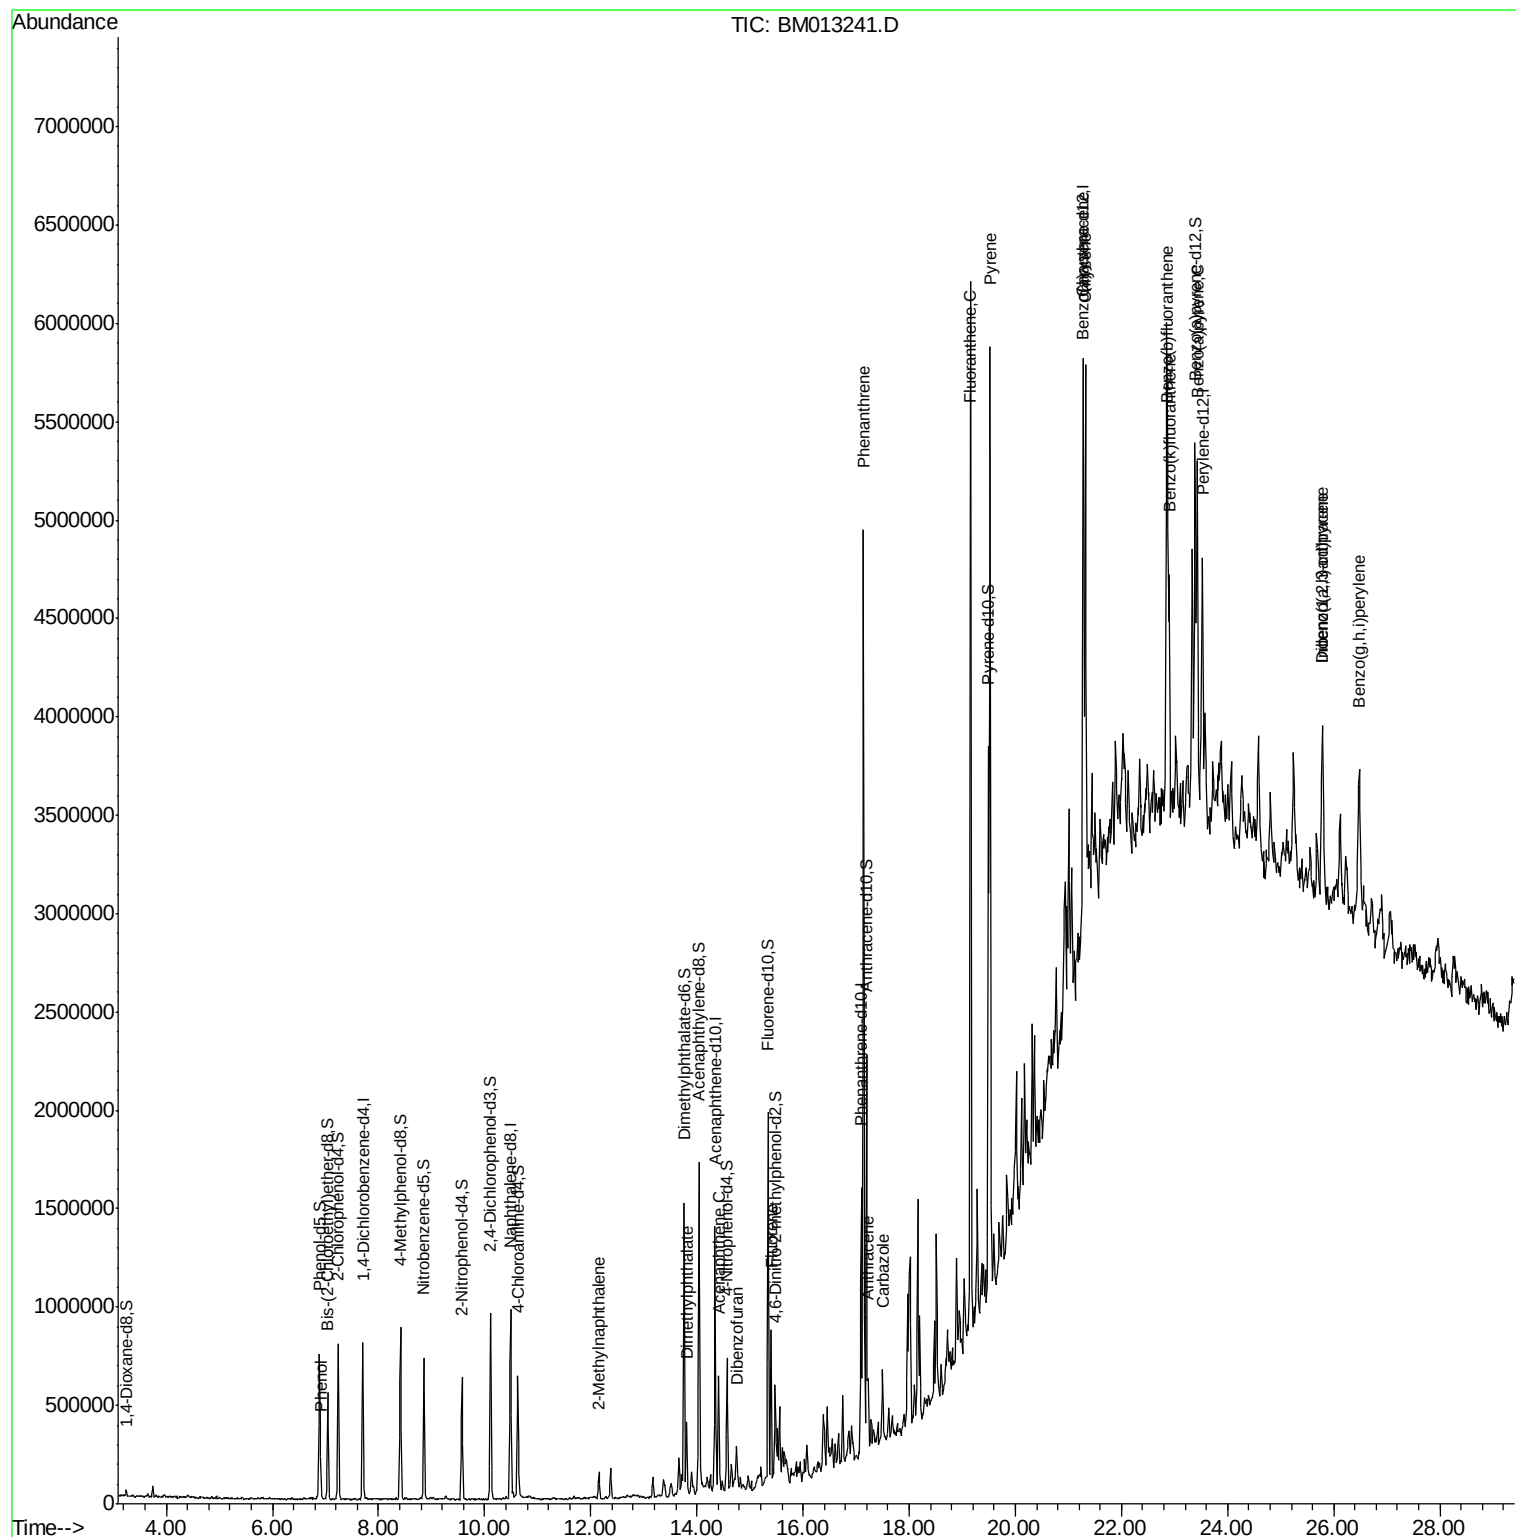

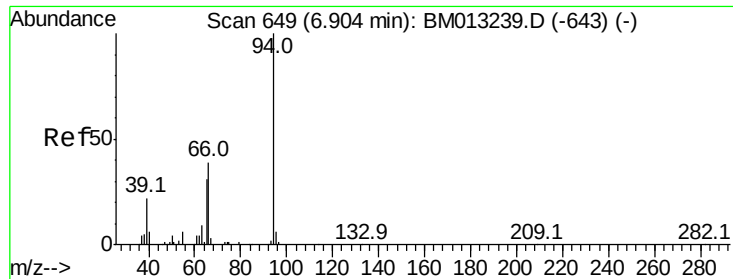

#6

Phenol





Concen: 2.499 ng/ul
 RT: 6.92 min Scan# 651
 Delta R.T. 0.01 min
 Lab File: BM013241.D
 Acq: 07 Dec 2017 13:53

Instrument :
 BNA_M
 ClientSampled :
 C0279

Tot Ion	Ratio	Lower	Upper
94	100		
65	24.6	28.2	42.4#
66	39.6	47.2	70.8#

Manual Integrations
 APPROVED

Sohil
 12/8/2017 11:15:19 AM

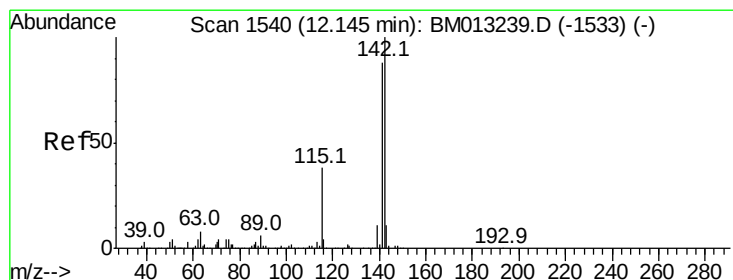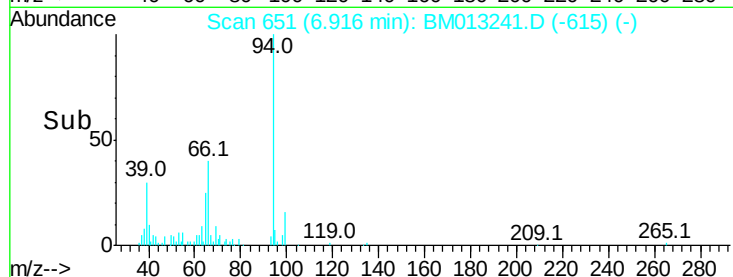
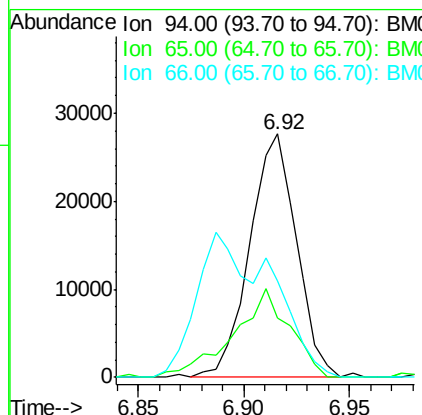
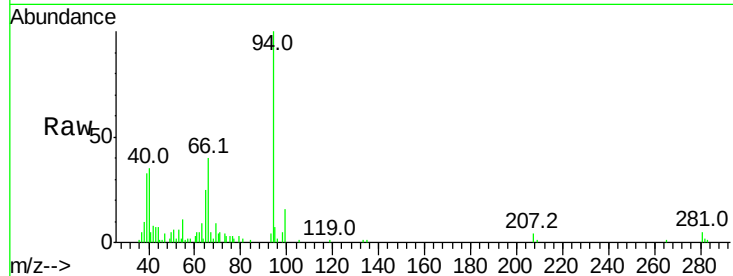



#34

2-Methylnaphthalene

Concen: 2.034 ng/ul
 RT: 12.15 min Scan# 1541
 Delta R.T. 0.01 min
 Lab File: BM013241.D
 Acq: 07 Dec 2017 13:53

Tgt Ion	Ratio	Lower	Upper
142	100		
141	76.6	74.1	111.1

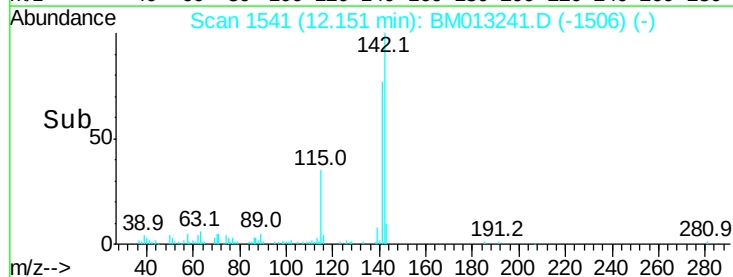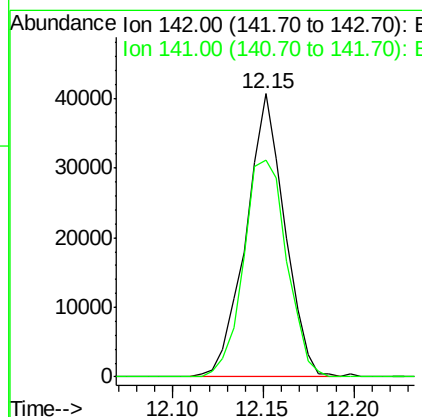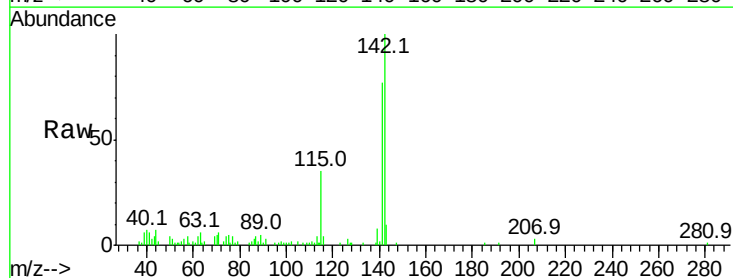

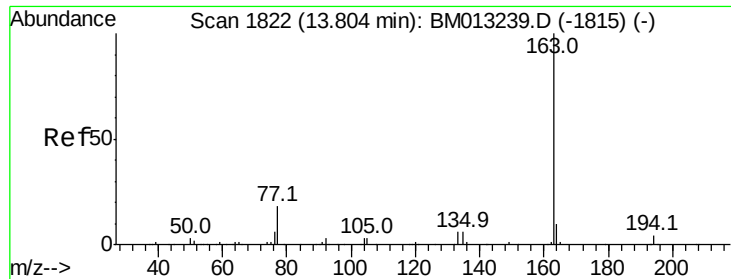





#44
Dimethylphthalate
Concen: 6.037 ng/ul
RT: 13.80 min Scan# 1822
Delta R.T. 0.00 min
Lab File: BM013241.D
Acq: 07 Dec 2017 13:53

Instrument :
BNA_M
ClientSampleId :
C0279

Tot Ion	Ratio	Resp	Lower	Upper
163	100	209065		
194	3.2		3.5	5.3#
164	11.0		8.2	12.4




Manual Integrations
APPROVED


Sohil
12/8/2017 11:15:19 AM

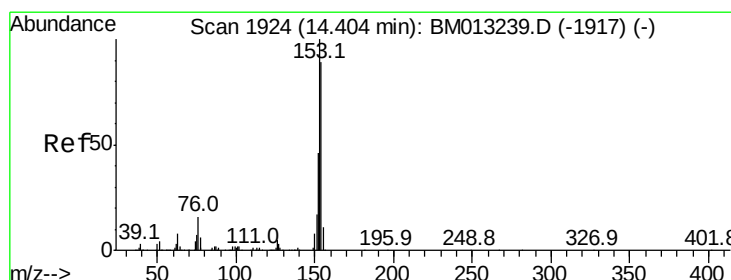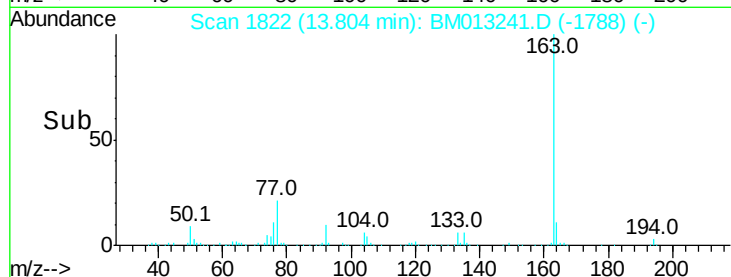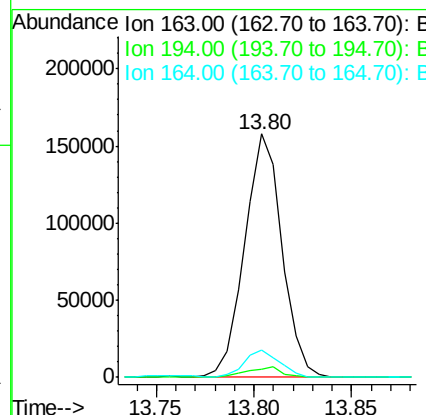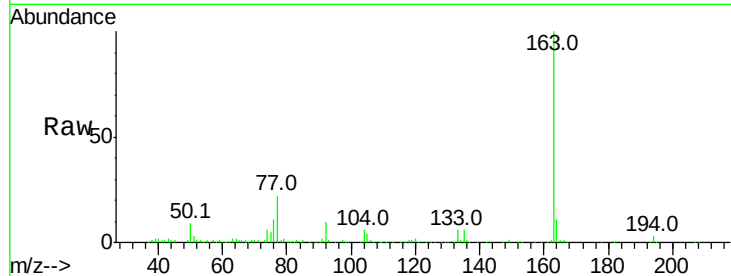

#49
Acenaphthene
Concen: 8.053 ng/ul
RT: 14.41 min Scan# 1925
Delta R.T. 0.01 min
Lab File: BM013241.D
Acq: 07 Dec 2017 13:53

Tgt Ion	Ratio	Resp	Lower	Upper
153	100	226822		
152	42.2		37.6	56.4
154	87.6		70.4	105.6

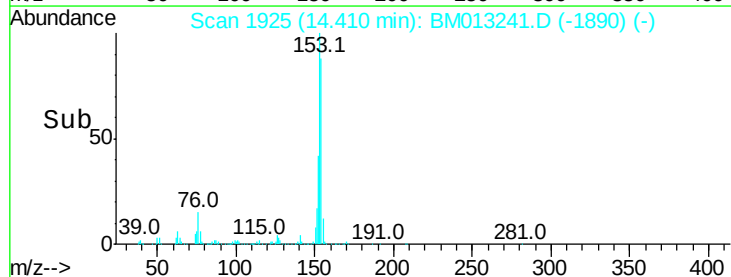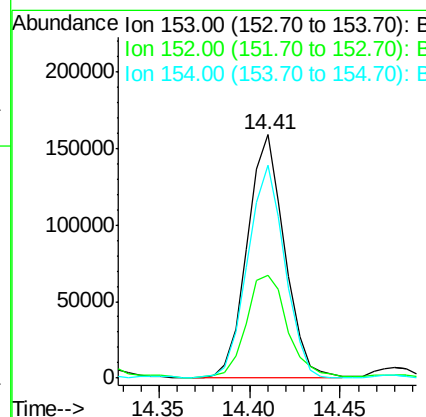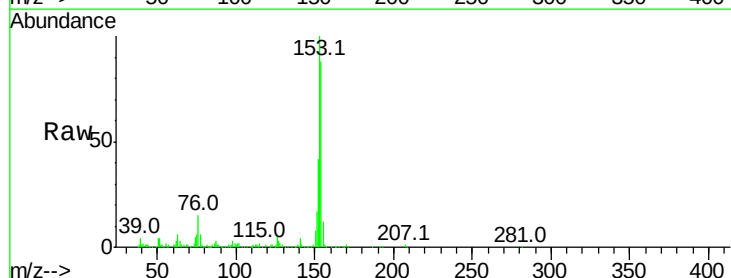

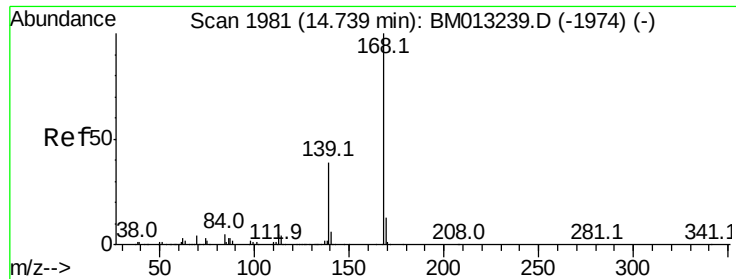

#53

Dibenzofuran

Concen: 2.012 ng/ul

RT: 14.75 min Scan# 1982

Delta R.T. 0.01 min

Lab File: BM013241.D

Acq: 07 Dec 2017 13:53

Instrument :

BNA_M

ClientSampled :

C0279

Tot Ion:168 Resp: 83646

Ion Ratio Lower Upper





168 100

139 47.7 30.8 46.2#

Manual Integrations
APPROVED

Sohil

12/8/2017 11:15:19 AM

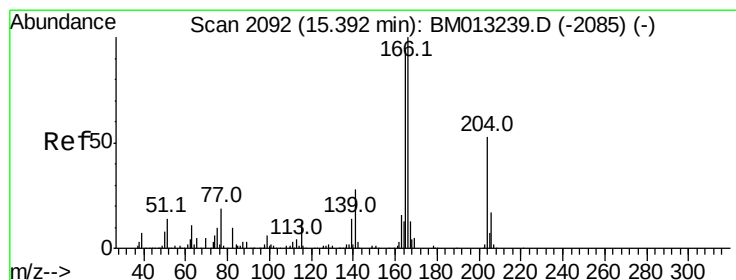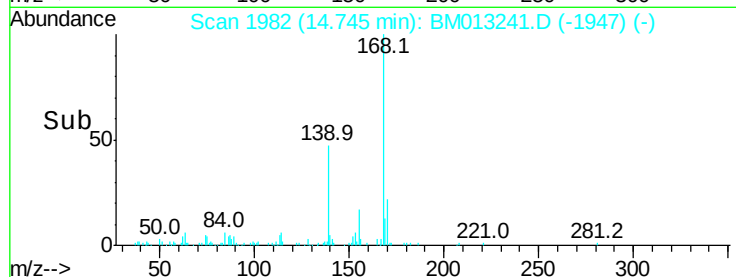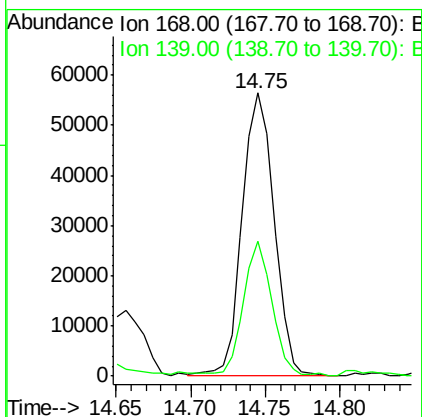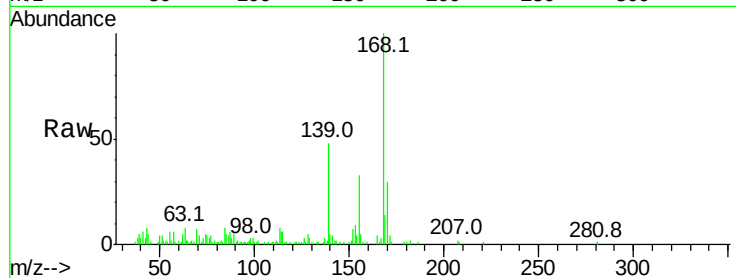

#58

Fluorene

Concen: 9.193 ng/ul

RT: 15.40 min Scan# 2093

Delta R.T. 0.01 min

Lab File: BM013241.D

Acq: 07 Dec 2017 13:53




Tgt Ion:166 Resp: 316221


Ion Ratio Lower Upper

166 100

165 97.3 77.9 116.9

167 16.3 10.6 16.0#

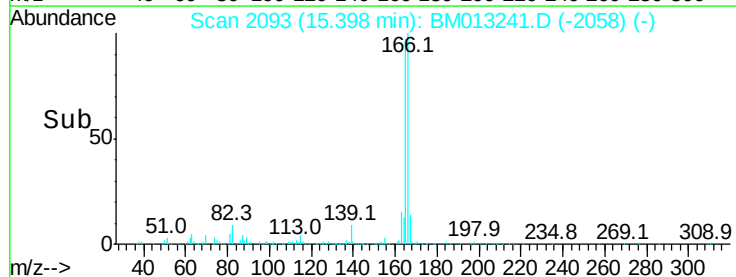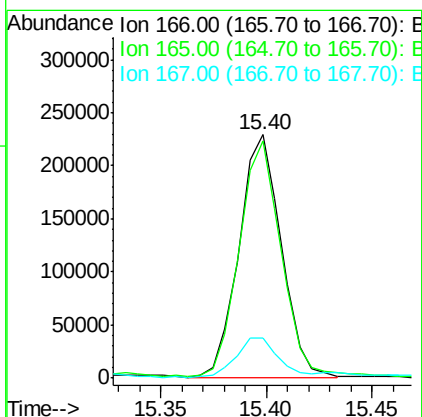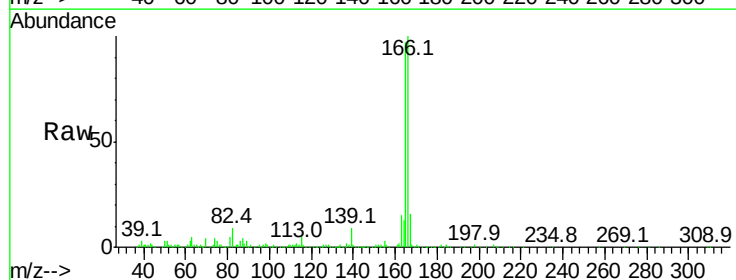

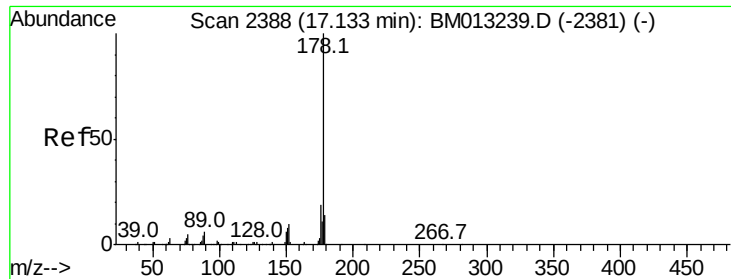

#69

Phenanthrene

Concen: 60.781 ng/ul

RT: 17.14 min Scan# 2389

Delta R.T. 0.01 min

Lab File: BM013241.D

Acq: 07 Dec 2017 13:53

Instrument :

BNA_M

ClientSampled :

C0279

Tot Ion:178 Resp: 2756073

Ion Ratio Lower Upper

178 100


179 15.3 12.6 19.0

176 18.4 14.9 22.3

Manual Integrations
APPROVED

Sohil




12/8/2017 11:15:19 AM

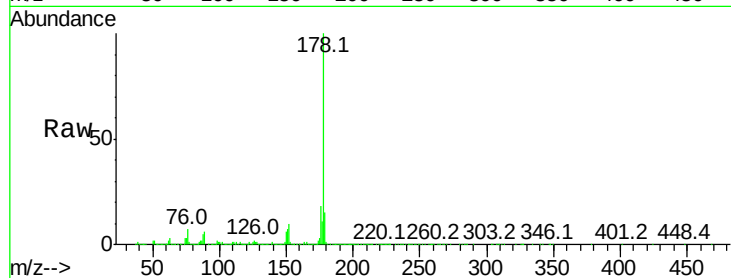

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

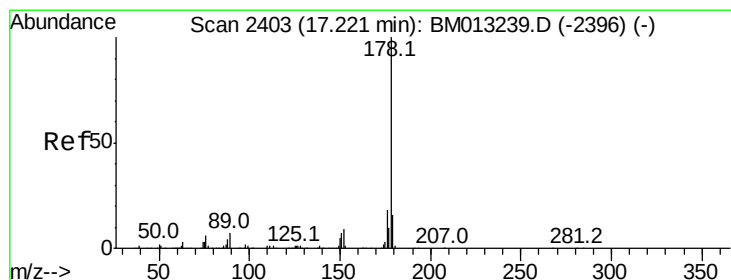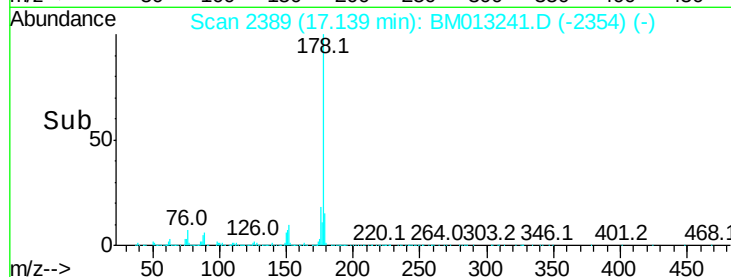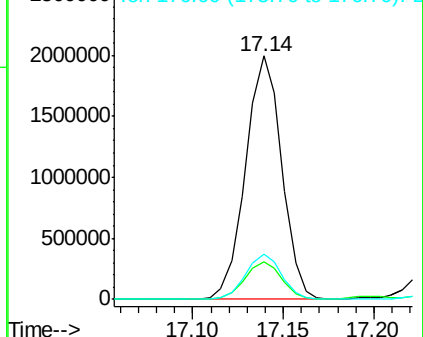

#71

Anthracene

Concen: 5.971 ng/ul

RT: 17.23 min Scan# 2404

Delta R.T. 0.01 min

Lab File: BM013241.D

Acq: 07 Dec 2017 13:53

Tgt Ion:178 Resp: 276768

Ion Ratio Lower Upper

178 100




179 17.4 11.7 17.5


176 16.7 14.6 21.8

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

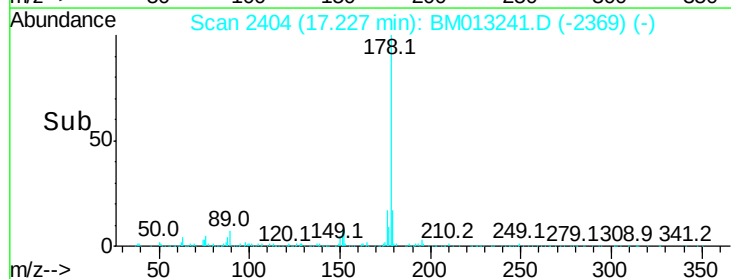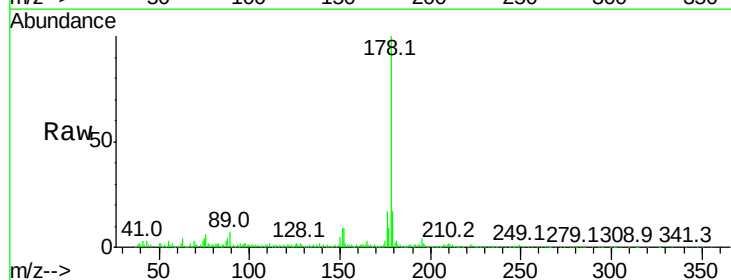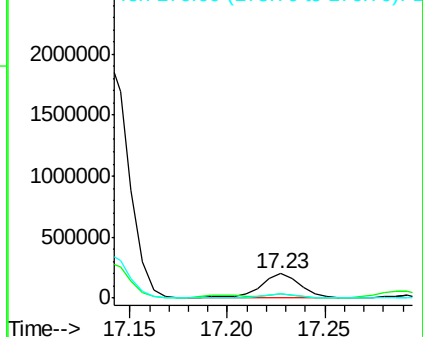

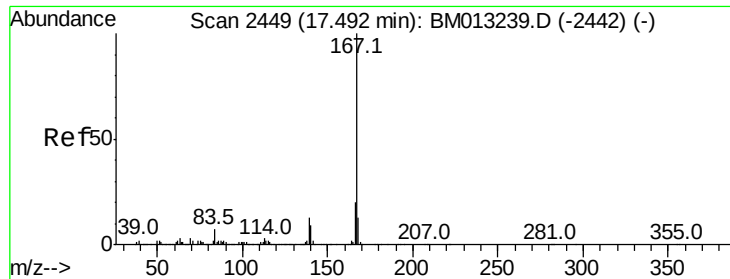

#72

Carbazole

Concen: 5.010 ng/ul

RT: 17.50 min Scan# 2450

Delta R.T. 0.01 min

Lab File: BM013241.D

Acq: 07 Dec 2017 13:53

Instrument :

BNA_M





ClientSampleId :

C0279

Tot Ion:	167	Resp:	199744
Ion Ratio	Lower	Upper	
167	100		
166	21.6	17.1	25.7
139	15.2	10.0	15.0#

Manual Integrations
APPROVED

Sohil
12/8/2017 11:15:19 AM

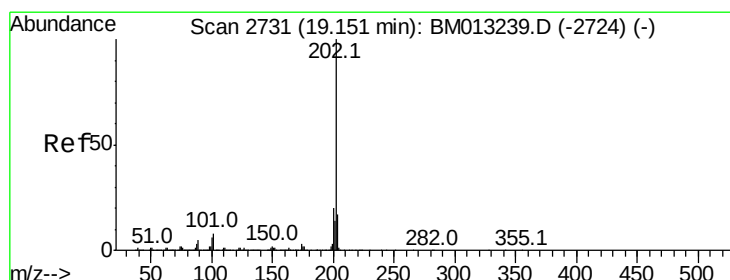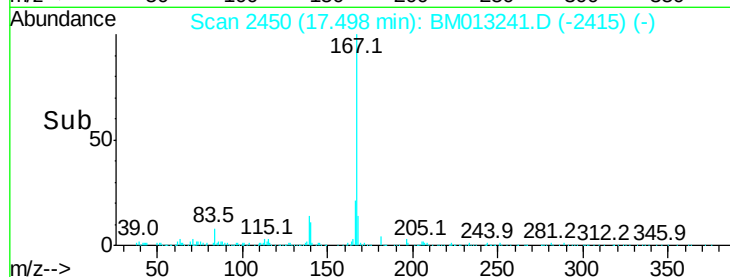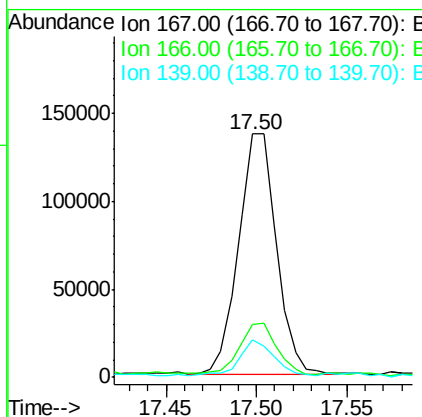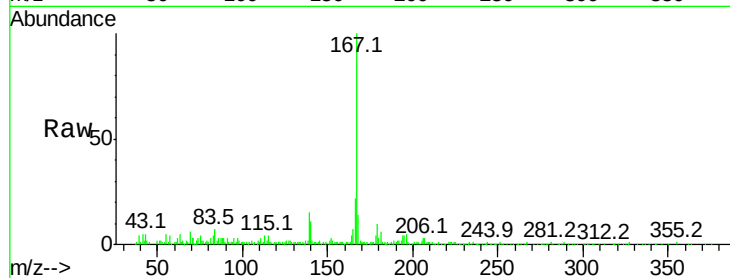

#74

Fluoranthene

Concen: 57.234 ng/ul




RT: 19.16 min Scan# 2733


Delta R.T. 0.01 min

Lab File: BM013241.D

Acq: 07 Dec 2017 13:53

Tgt Ion:	202	Resp:	3180370
Ion Ratio	Lower	Upper	
202	100		
101	7.9	4.6	7.0#
100	6.1	3.4	5.2#

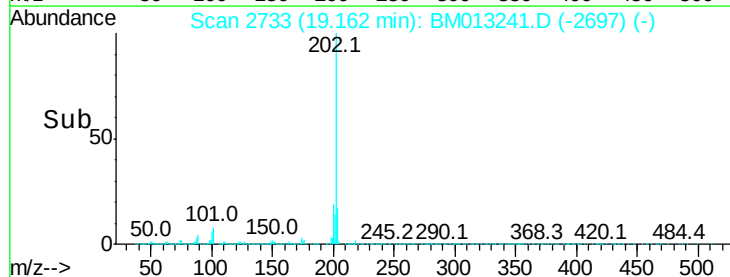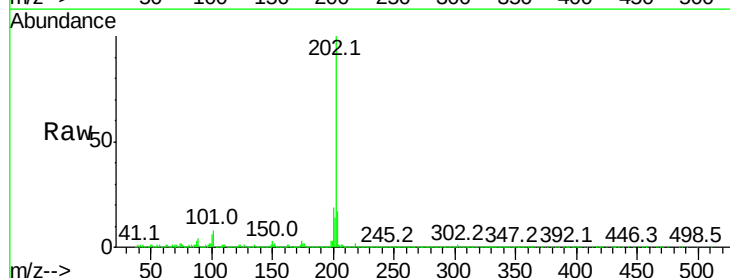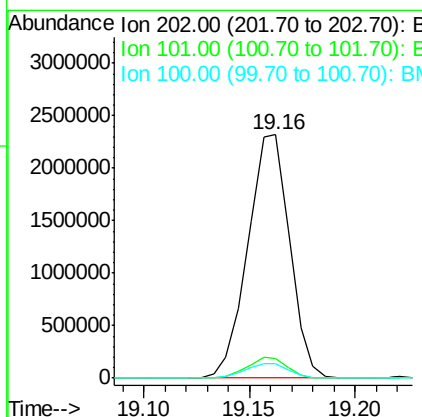

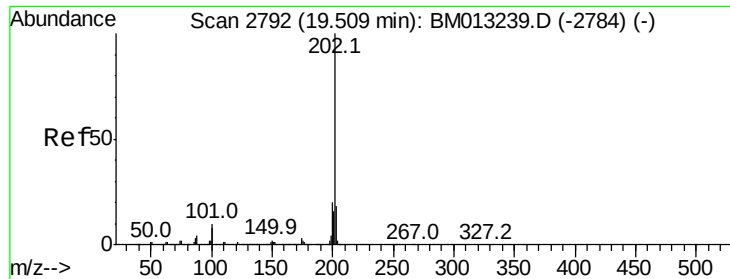





#77
Pvrene
Concen: 57.745 ng/ul
RT: 19.53 min Scan# 2795
Delta R.T. 0.02 min
Lab File: BM013241.D
Acq: 07 Dec 2017 13:53

Instrument :
BNA_M
ClientSampled :
C0279

Tot Ion	Ratio	Lower	Upper
202	100		
101	8.8	5.1	7.7#
100	7.4	4.9	7.3#




Manual Integrations
APPROVED


Sohil
12/8/2017 11:15:19 AM

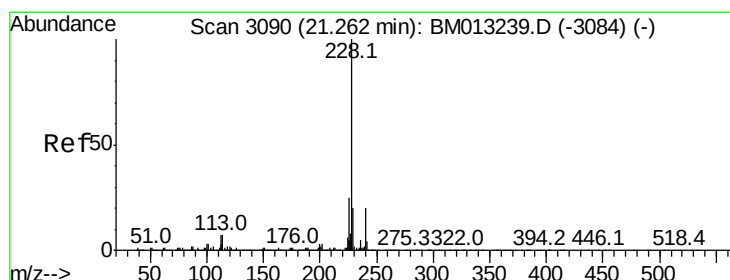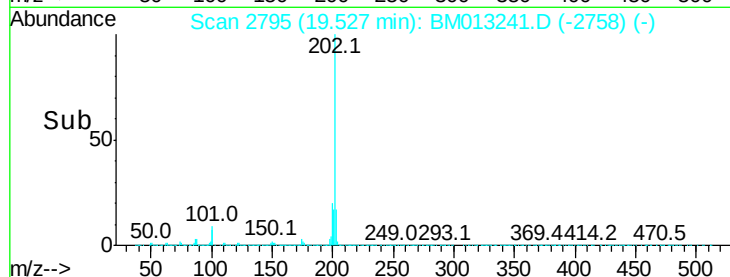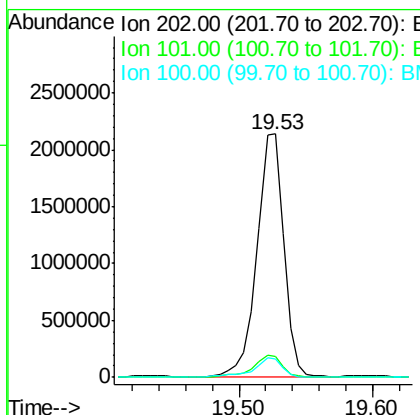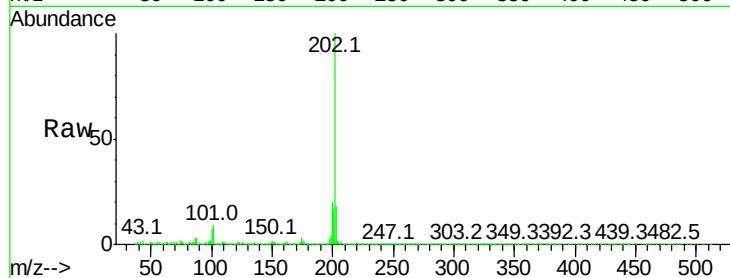

#80
Benzo(a)anthracene
Concen: 20.532 ng/ul
RT: 21.27 min Scan# 3091
Delta R.T. 0.01 min
Lab File: BM013241.D
Acq: 07 Dec 2017 13:53

Tgt Ion	Ratio	Lower	Upper
228	100		
229	22.3	15.4	23.0
226	26.6	21.4	32.0

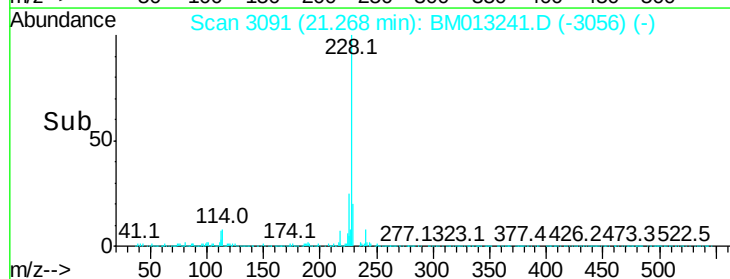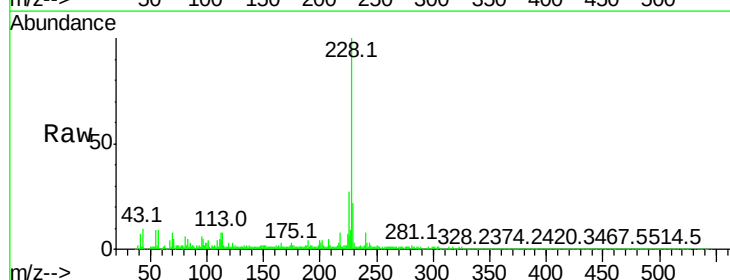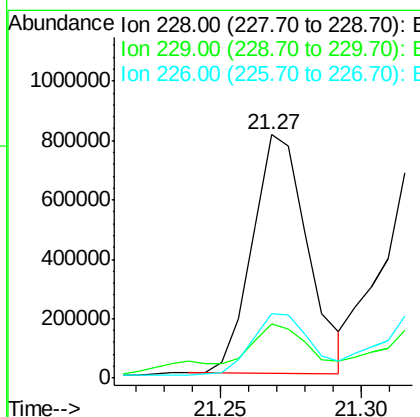

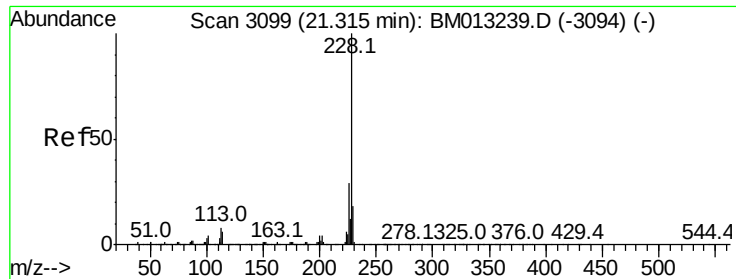

#82

Chrysene

Concen: 29.929 ng/ul

RT: 21.32 min Scan# 3100

Delta R.T. 0.01 min

Lab File: BM013241.D

Acq: 07 Dec 2017 13:53

Instrument :

BNA_M

ClientSampled :

C0279

Tot Ion:228 Resp: 1481976

Ion Ratio Lower Upper

228 100





226 29.7 23.4 35.2

229 22.0 15.5 23.3

Manual Integrations
APPROVED

Sohil

12/8/2017 11:15:19 AM

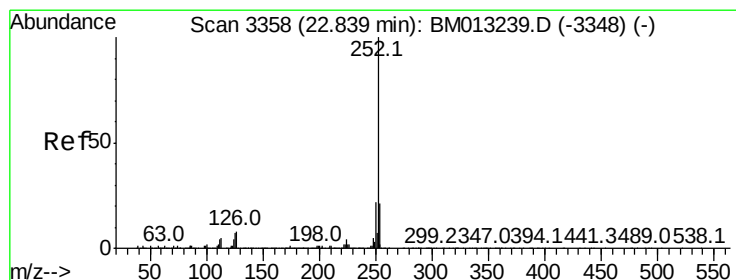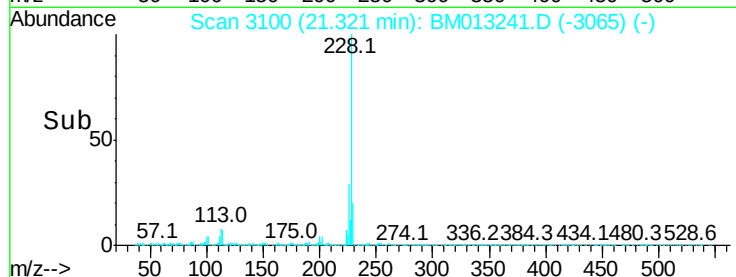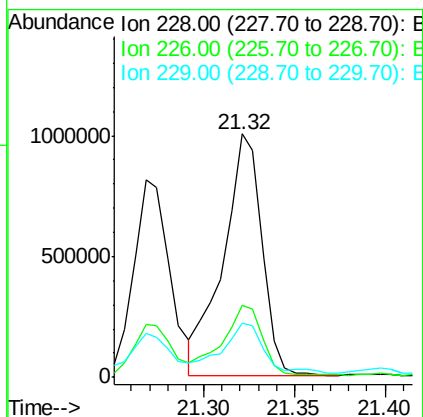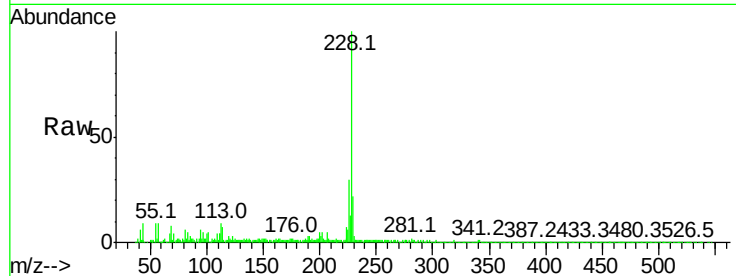

#85

Benzo(b)fluoranthene

Concen: 30.887 ng/ul

RT: 22.86 min Scan# 3361

Delta R.T. 0.02 min

Lab File: BM013241.D

Acq: 07 Dec 2017 13:53




Tgt Ion:252 Resp: 1870679


Ion Ratio Lower Upper

252 100

253 23.5 17.9 26.9

125 9.7 3.6 5.4#

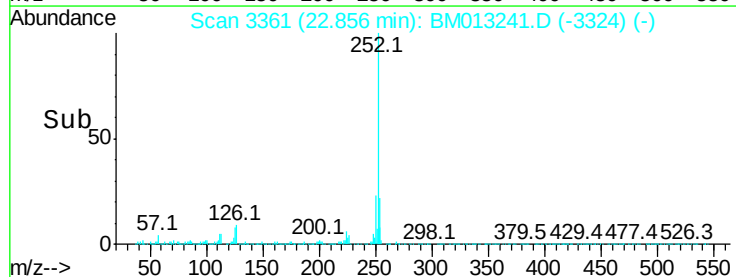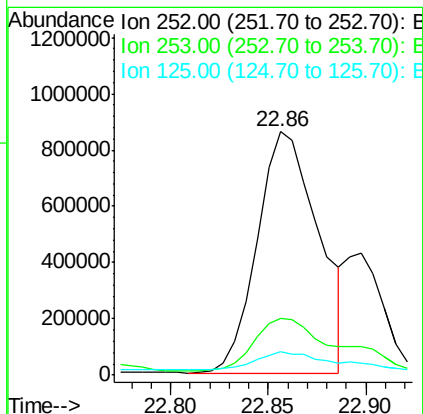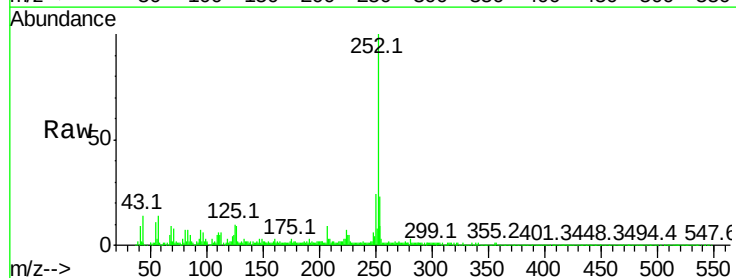

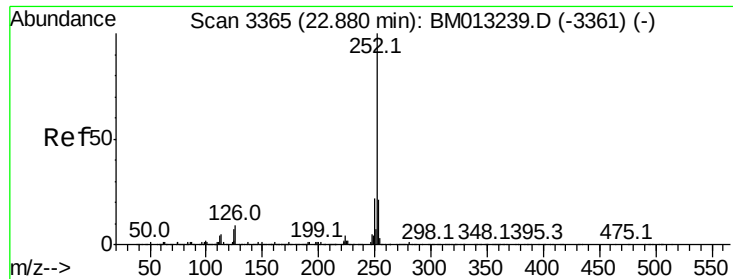





#86
Benzo(k)fluoranthene
Concen: 9.949 ng/ul m
RT: 22.90 min Scan# 3368
Delta R.T. 0.02 min
Lab File: BM013241.D
Acq: 07 Dec 2017 13:53

Instrument :
BNA_M
ClientSampled :
C0279

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.7	17.1	25.7
125	9.9	3.4	5.2#




Manual Integrations
APPROVED


Sohil
12/8/2017 11:15:19 AM

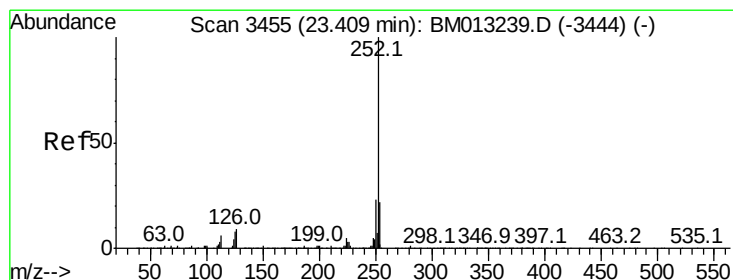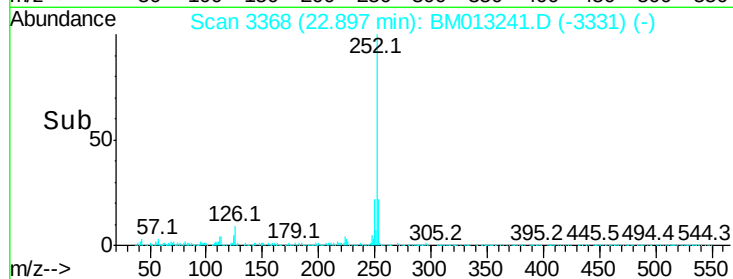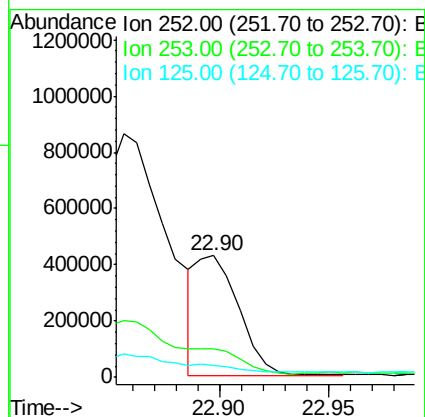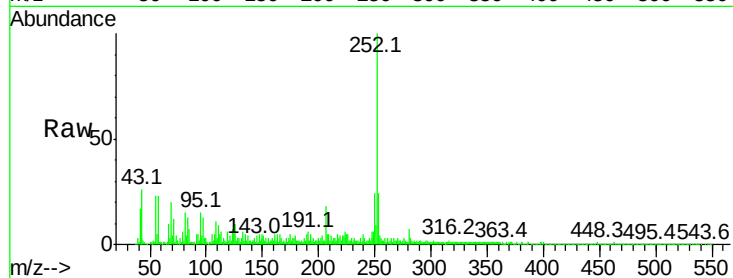

#88
Benzo(a)pyrene
Concen: 20.168 ng/ul
RT: 23.43 min Scan# 3459
Delta R.T. 0.02 min
Lab File: BM013241.D
Acq: 07 Dec 2017 13:53

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.5	18.2	27.2
125	10.0	4.0	6.0#

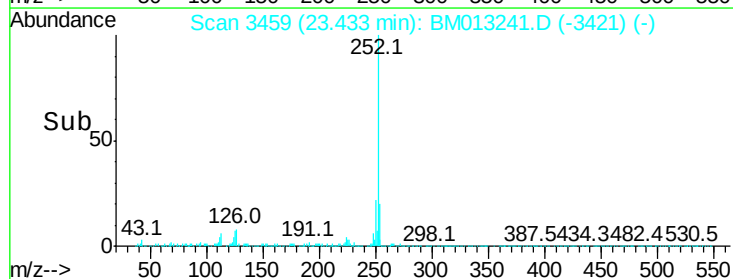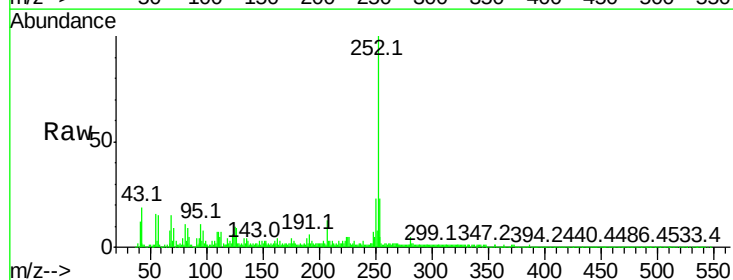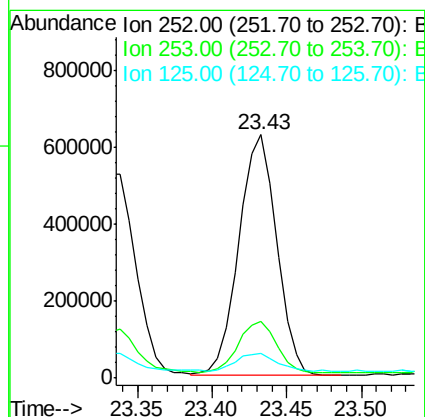

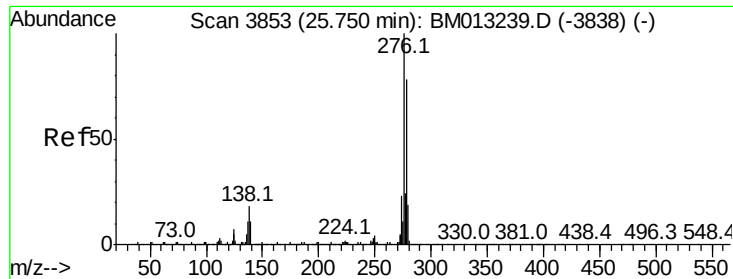

#89

Indeno(1,2,3-cd)pyrene

Concen: 16.160 ng/ul

RT: 25.78 min Scan# 3858

Delta R.T. 0.03 min

Lab File: BM013241.D

Acq: 07 Dec 2017 13:53

Instrument :

BNA_M





ClientSampleId :

C0279

Tot Ion:	276	Resp:	872371
Ion Ratio	Lower	Upper	
276	100		
138	14.8	9.3	13.9#
277	25.8	19.9	29.9

Manual Integrations
APPROVED

Sohil
12/8/2017 11:15:19 AM

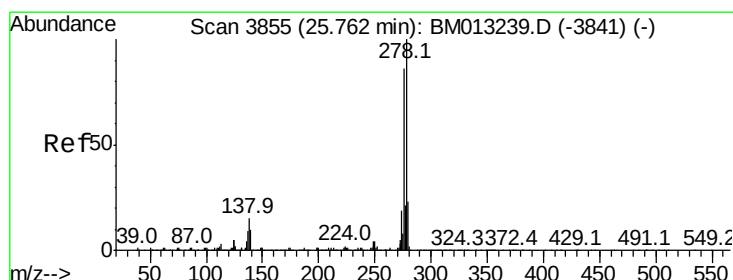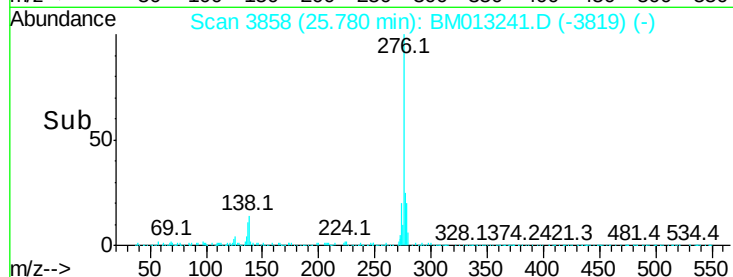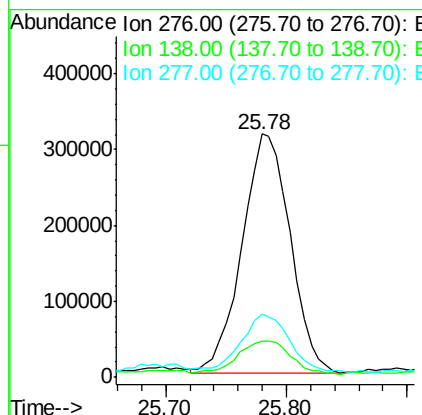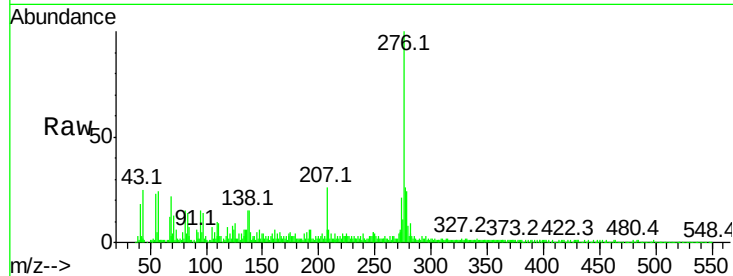

#90

Dibenzo(a,h)anthracene

Concen: 4.984 ng/ul m




RT: 25.78 min Scan# 3858


Delta R.T. 0.02 min

Lab File: BM013241.D

Acq: 07 Dec 2017 13:53

Tgt Ion:	278	Resp:	229088
Ion Ratio	Lower	Upper	
278	100		
139	20.4	5.8	8.8#
279	35.5	18.6	27.8#

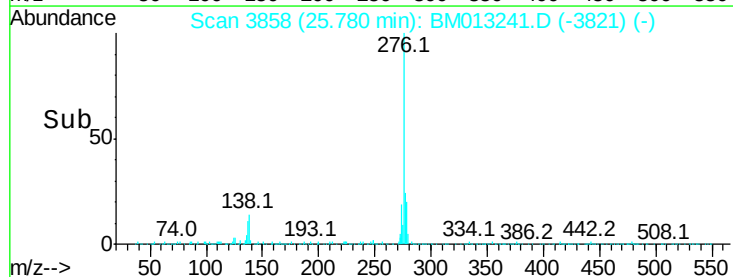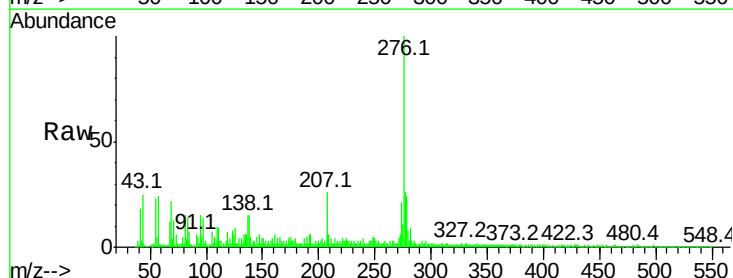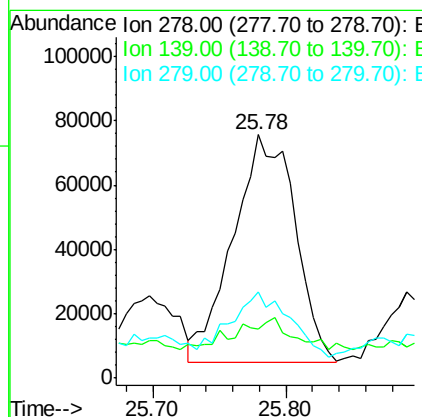

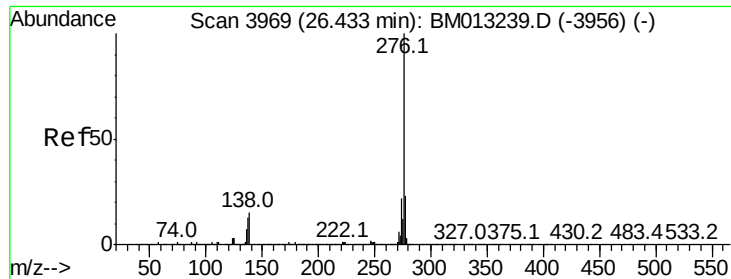

#91
 Benzo(a,h,i)perylene
 Concen: 20.449 ng/ul
 RT: 26.48 min Scan# 3977
 Delta R.T. 0.05 min
 Lab File: BM013241.D
 Acq: 07 Dec 2017 13:53

Instrument :
 BNA_M
 ClientSampleId :
 C0279

Tot Ion	Ratio	Lower	Upper
276	100		
138	14.4	8.5	12.7#
277	27.5	18.6	28.0

Manual Integrations
 APPROVED

Sohil
 12/8/2017 11:15:19 AM

