

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120722\
 Data File : BM037873.D
 Acq On : 07 Dec 2022 15:59
 Operator : CG/JU
 Sample : SSTD16008
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160010

Quant Time: Dec 08 01:03:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 08 00:59:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.092	152	223443	20.000	ng/u1	0.00
20) Naphthalene-d8	10.916	136	889840	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.721	164	488966	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.462	188	933487	20.000	ng/u1	0.00
79) Chrysene-d12	21.633	240	737545	20.000	ng/u1	0.00
88) Perylene-d12	24.115	264	865736	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	317919	66.755	ng/uL	0.00
4) Pyridine-d5	3.863	84	2431629	157.864	ng/u1	0.00
7) Phenol-d5	7.263	99	3118828	154.927	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.422	67	1807443	153.894	ng/u1	0.01
11) 2-Chlorophenol-d4	7.628	132	2647596	173.949	ng/u1	0.01
15) 4-Methylphenol-d8	8.822	113	2388171	149.175	ng/u1	0.02
21) Nitrobenzene-d5	9.275	128	1286001	181.933	ng/u1	0.01
24) 2-Nitrophenol-d4	9.998	143	1433739	196.016	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.539	165	2449592	180.584	ng/u1	0.01
31) 4-Chloroaniline-d4	11.063	131	3275266	157.414	ng/u1	0.02
46) Dimethylphthalate-d6	14.139	166	5783064	172.235	ng/u1	0.01
49) Acenaphthylene-d8	14.421	160	7119605	174.351	ng/u1	0.00
54) 4-Nitrophenol-d4	14.933	143	1114184	159.872	ng/u1	0.02
60) Fluorene-d10	15.715	176	4858101	159.483	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.839	200	1008350	205.058	ng/u1	0.02
73) Anthracene-d10	17.562	188	6779830	157.931	ng/u1	0.00
81) Pyrene-d10	19.845	212	6999858	183.223	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.968	264	6972517	160.765	ng/u1	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.463	88	339844	66.584	ng/uL	94
5) Pyridine	3.881	79	2374730	157.235	ng/u1	96
6) Benzaldehyde	7.228	77	1108424	114.327	ng/u1	99
8) Phenol	7.292	94	3111229	151.230	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.522	93	2488918	151.651	ng/u1	97
12) 2-Chlorophenol	7.663	128	2691050	164.265	ng/u1	98
13) 2-Methylphenol	8.545	108	2375213	144.770	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.634	45	4211631	138.103	ng/u1	98
16) Acetophenone	8.939	105	3607899	142.870	ng/u1	95
17) N-Nitroso-di-n-propyla...	8.945	70	1707165	134.213	ng/u1	93
18) 4-Methylphenol	8.898	108	2520173	142.366	ng/u1	97
19) Hexachloroethane	9.181	117	1083889	173.216	ng/u1	94
22) Nitrobenzene	9.322	77	2613794	176.445	ng/u1	94
23) Isophorone	9.863	82	4852954	152.268	ng/u1	99
25) 2-Nitrophenol	10.033	139	1447805	182.655	ng/u1	99
26) 2,4-Dimethylphenol	10.092	107	2621979	172.084	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.328	93	3170804	164.757	ng/u1	99
29) 2,4-Dichlorophenol	10.569	162	2369513	172.696	ng/u1	98
30) Naphthalene	10.969	128	8105088	167.828	ng/u1	100
32) 4-Chloroaniline	11.086	127	3220167	152.939	ng/u1	99
33) Hexachlorobutadiene	11.245	225	1485937	174.837	ng/u1	99
34) Caprolactam	11.927	113	367144	73.688	ng/u1	89
35) 4-Chloro-3-methylphenol	12.204	107	2235497	156.126	ng/u1	95
36) 2-Methylnaphthalene	12.569	142	5147194	154.055	ng/u1	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120722\
 Data File : BM037873.D
 Acq On : 07 Dec 2022 15:59
 Operator : CG/JU
 Sample : SSTD16008
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160010

Quant Time: Dec 08 01:03:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 08 00:59:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.786	142	5162646	154.382	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.933	216	2528549	180.564	ng/ul	97
40) Hexachlorocyclopentadiene	12.904	237	1733264	225.078	ng/ul	100
41) 2,4,6-Trichlorophenol	13.169	196	1725300	188.721	ng/ul	98
42) 2,4,5-Trichlorophenol	13.245	196	1824784	187.413	ng/ul	99
43) 1,1'-Biphenyl	13.569	154	6369669	179.214	ng/ul	98
44) 2-Chloronaphthalene	13.610	162	4985449	178.748	ng/ul	97
45) 2-Nitroaniline	13.821	65	1382640	175.200	ng/ul	94
47) Dimethylphthalate	14.186	163	5669545	162.118	ng/ul	100
48) 2,6-Dinitrotoluene	14.310	165	1255206	175.792	ng/ul	98
50) Acenaphthylene	14.451	152	7679068	169.611	ng/ul	97
51) 3-Nitroaniline	14.639	138	1273229	149.396	ng/ul	98
52) Acenaphthene	14.792	153	5168362	164.744	ng/ul	99
53) 2,4-Dinitrophenol	14.839	184	744337	178.489	ng/ul	96
55) 4-Nitrophenol	14.951	109	717821	167.100	ng/ul	95
56) Dibenzofuran	15.121	168	6851247	162.205	ng/ul	95
57) 2,4-Dinitrotoluene	15.092	165	1665647	167.031	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.345	232	1446927	168.949	ng/ul	90
59) Diethylphthalate	15.539	149	5536338	154.366	ng/ul	98
61) Fluorene	15.774	166	5117890	143.928	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.757	204	2448822	144.454	ng/ul	91
63) 4-Nitroaniline	15.810	138	1112926	129.804	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.857	198	945935	186.606	ng/ul#	96
67) N-Nitrosodiphenylamine	15.974	169	4497362	167.182	ng/ul	100
68) 4-Bromophenyl-phenylether	16.651	248	1601165	167.147	ng/ul	96
69) Hexachlorobenzene	16.768	284	1820493	162.742	ng/ul#	93
70) Atrazine	16.927	200	1574426	169.945	ng/ul	98
71) Pentachlorophenol	17.109	266	1197530	174.056	ng/ul	98
72) Phenanthrene	17.509	178	7834415	154.854	ng/ul	99
74) Anthracene	17.604	178	7815087	151.422	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.533	216	2495264	198.251	ng/ul	99
76) Pentachlorobenzene	15.045	250	2282200	166.666	ng/ul	98
77) Carbazole	17.868	167	7264128	152.943	ng/ul	98
78) Di-n-butylphthalate	18.415	149	8933826	149.609	ng/ul	99
80) Fluoranthene	19.509	202	8195940	175.634	ng/ul	98
82) Pyrene	19.874	202	8163210	169.422	ng/ul	97
83) Butylbenzylphthalate	20.750	149	3821800	181.921	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.544	252	2208837	142.958	ng/ul	98
85) Benzo(a)anthracene	21.615	228	7627465	161.638	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.521	149	5219030	164.411	ng/ul	97
87) Chrysene	21.674	228	7054257	160.595	ng/ul	99
89) Di-n-octyl phthalate	22.474	149	9122418	146.420	ng/ul	100
90) Benzo(b)fluoranthene	23.362	252	8340449	150.015	ng/ul	99
91) Benzo(k)fluoranthene	23.415	252	8018770	149.509	ng/ul	99
93) Benzo(a)pyrene	24.027	252	7540815	156.405	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.738	276	9969585	183.927	ng/ul	100
95) Dibenzo(a,h)anthracene	26.768	278	8153225	165.266	ng/ul	99
96) Benzo(g,h,i)perylene	27.556	276	8557726	180.914	ng/ul	98





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 66.584 ng/uL
RT: 3.463 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion: 88 Resp: 339844
Ion Ratio Lower Upper
88 100
43 36.0 32.8 49.2
58 84.7 64.6 97.0

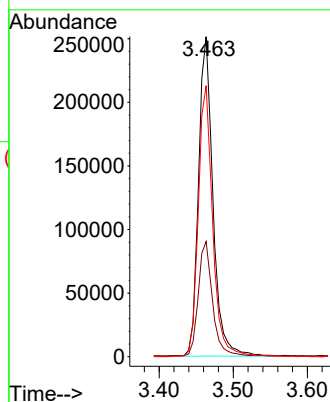

#5
Pyridine
Concen: 157.235 ng/uL
RT: 3.881 min Scan# 84
Delta R.T. -0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion: 79 Resp: 2374730
Ion Ratio Lower Upper
79 100
52 94.3 78.1 117.1
51 41.9 37.2 55.8









#6
Benzaldehyde
Concen: 114.327 ng/ul
RT: 7.228 min Scan# 611
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion: 77 Resp: 1108424
Ion Ratio Lower Upper
77 100
105 105.1 82.5 123.7
106 102.8 81.8 122.6

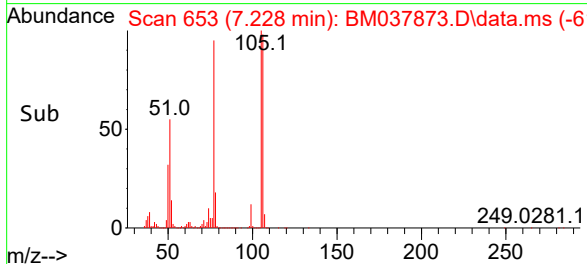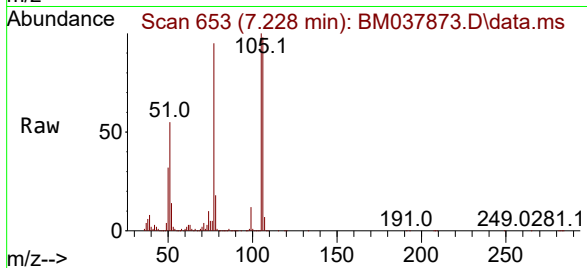

#8
Phenol
Concen: 151.230 ng/ul
RT: 7.292 min Scan# 664
Delta R.T. 0.023 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion: 94 Resp: 3111229
Ion Ratio Lower Upper
94 100
65 26.9 22.2 33.4
66 33.2 27.3 40.9




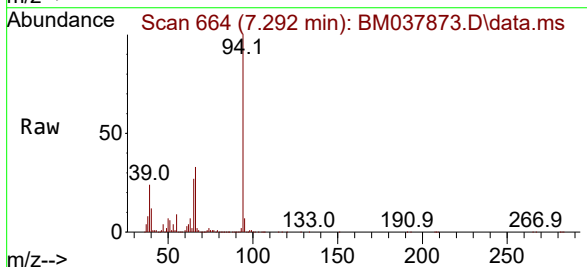




#10
Bis(2-Chloroethyl)ether
Concen: 151.651 ng/ul
RT: 7.522 min Scan# 703
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion: 93 Resp: 2488918
Ion Ratio Lower Upper
93 100
63 79.2 66.3 99.5
95 33.1 25.7 38.5



#12
2-Chlorophenol
Concen: 164.265 ng/ul
RT: 7.663 min Scan# 727
Delta R.T. 0.012 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion: 128 Resp: 2691050
Ion Ratio Lower Upper
128 100
64 42.6 35.2 52.8
130 33.1 25.9 38.9





#13

2-Methylphenol

Concen: 144.770 ng/ul

RT: 8.545 min Scan# 81

Delta R.T. 0.012 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :





SSTD160010

Tgt Ion:108 Resp: 2375213

Ion Ratio Lower Upper

108 100

107 87.3 71.9 107.9



#14

2,2'-oxybis(1-Chloropropane)

Concen: 138.103 ng/ul

RT: 8.634 min Scan# 892

Delta R.T. 0.006 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion: 45 Resp: 4211631


Ion Ratio Lower Upper

45 100

77 10.6 9.0 13.4

79 8.9 6.2 9.4









#16
Acetophenone
Concen: 142.870 ng/ul
RT: 8.939 min Scan# 941
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:105 Resp: 3607899
Ion Ratio Lower Upper
105 100
77 71.8 59.7 89.5
51 29.3 27.2 40.8

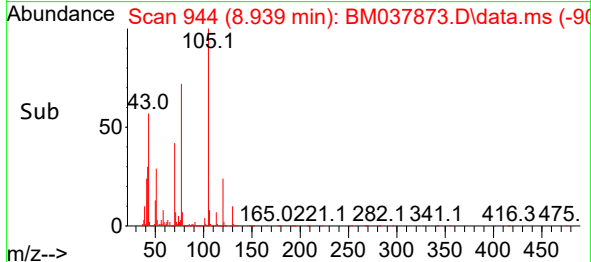

#17
N-Nitroso-di-n-propylamine
Concen: 134.213 ng/ul
RT: 8.945 min Scan# 945
Delta R.T. 0.041 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion: 70 Resp: 1707165
Ion Ratio Lower Upper
70 100
42 70.6 62.3 93.5
101 10.2 8.0 12.0
130 23.9 17.6 26.4









#18
4-Methylphenol
Concen: 142.366 ng/ul
RT: 8.898 min Scan# 91
Delta R.T. 0.035 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:108 Resp: 2520173
Ion Ratio Lower Upper
108 100
107 107.3 88.1 132.1

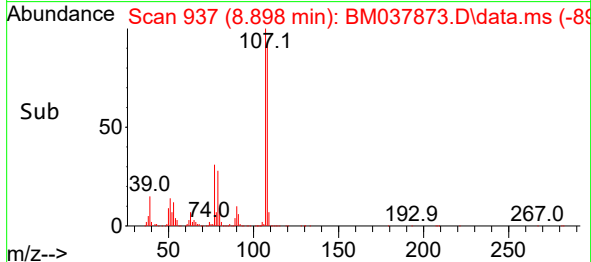

#19
Hexachloroethane
Concen: 173.216 ng/ul
RT: 9.181 min Scan# 985
Delta R.T. -0.000 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:117 Resp: 1083889
Ion Ratio Lower Upper
117 100
201 100.5 87.3 130.9
199 62.8 50.9 76.3




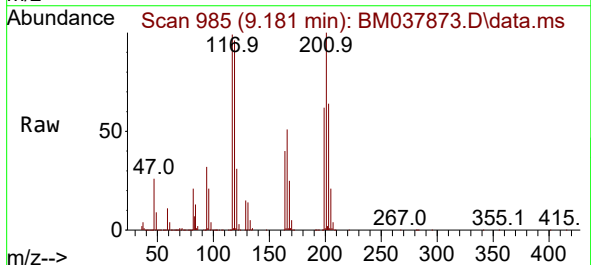




#22
Nitrobenzene
Concen: 176.445 ng/ul
RT: 9.322 min Scan# 1101
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion: 77 Resp: 2613794
Ion Ratio Lower Upper
77 100
123 51.9 37.8 56.6
65 13.6 11.1 16.7



#23
Isophorone
Concen: 152.268 ng/ul
RT: 9.863 min Scan# 1101
Delta R.T. 0.029 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion: 82 Resp: 4852954
Ion Ratio Lower Upper
82 100
95 6.6 5.2 7.8
138 18.9 14.9 22.3









#25
2-Nitrophenol
Concen: 182.655 ng/ul
RT: 10.033 min Scan# 1110
Delta R.T. 0.012 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:139 Resp: 1447805
Ion Ratio Lower Upper
139 100
65 44.6 36.2 54.4
109 25.2 19.7 29.5

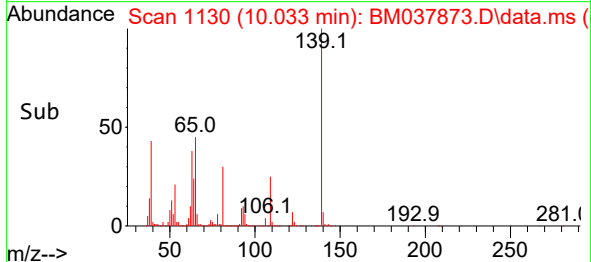

#26
2,4-Dimethylphenol
Concen: 172.084 ng/ul
RT: 10.092 min Scan# 1140
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:107 Resp: 2621979
Ion Ratio Lower Upper
107 100
121 52.2 42.0 63.0
122 92.5 71.4 107.2

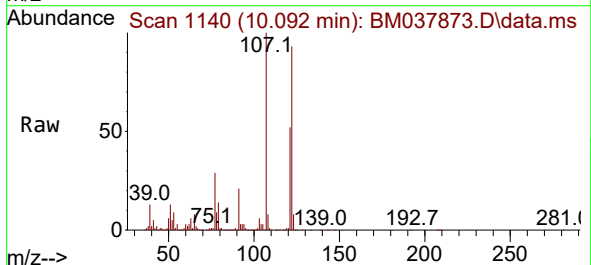

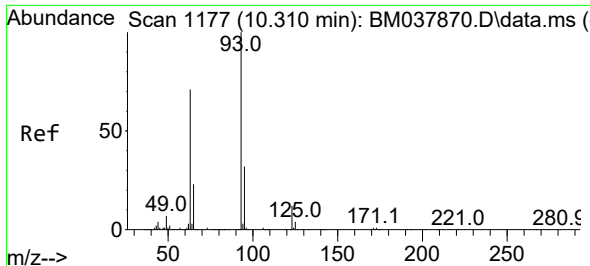

#27

Bis(2-Chloroethoxy)methane

Concen: 164.757 ng/ul

RT: 10.328 min Scan# 1177

Delta R.T. 0.018 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion: 93 Resp: 3170804

Ion Ratio Lower Upper

93 100

95 32.9 25.5 38.3

123 11.9 9.4 14.2

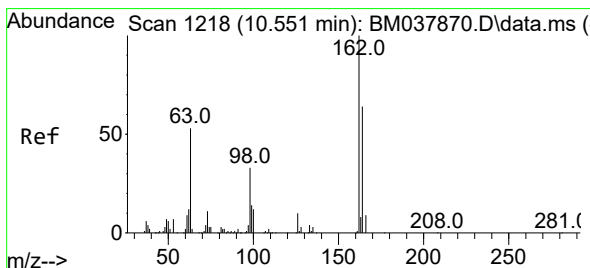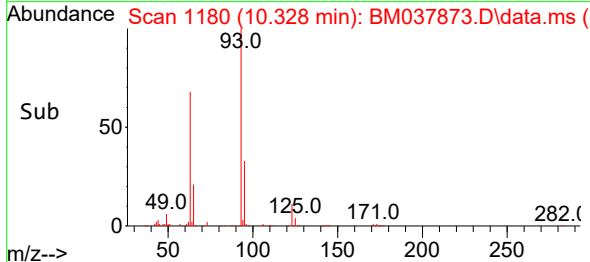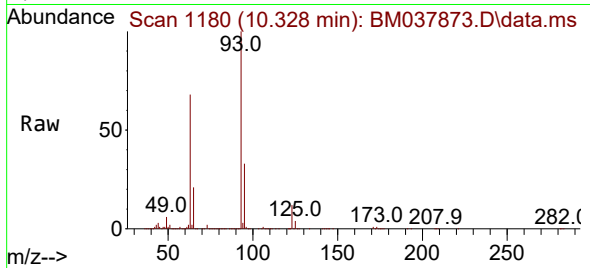

#29

2,4-Dichlorophenol

Concen: 172.696 ng/ul

RT: 10.569 min Scan# 1221

Delta R.T. 0.018 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion:162 Resp: 2369513


Ion Ratio Lower Upper

162 100

164 65.4 51.4 77.2

98 33.7 26.1 39.1


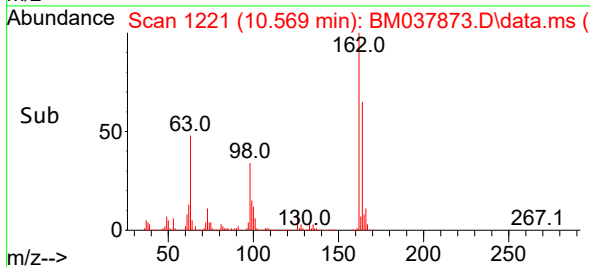

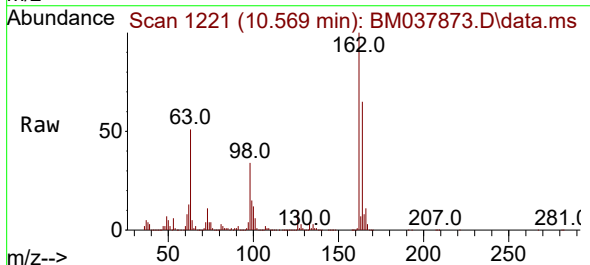




#30
Naphthalene
Concen: 167.828 ng/ul
RT: 10.969 min Scan# 1288
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:128 Resp: 8105088
Ion Ratio Lower Upper
128 100
129 11.3 9.0 13.4
127 13.2 10.4 15.6



#32
4-Chloroaniline
Concen: 152.939 ng/ul
RT: 11.086 min Scan# 1309
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:127 Resp: 3220167
Ion Ratio Lower Upper
127 100
129 32.4 25.3 37.9


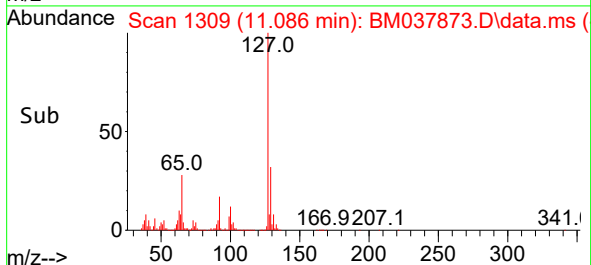






#33
Hexachlorobutadiene
Concen: 174.837 ng/ul
RT: 11.245 min Scan# 11
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:225 Resp: 1485937
Ion Ratio Lower Upper
225 100
223 62.7 50.8 76.2
227 64.2 50.5 75.7

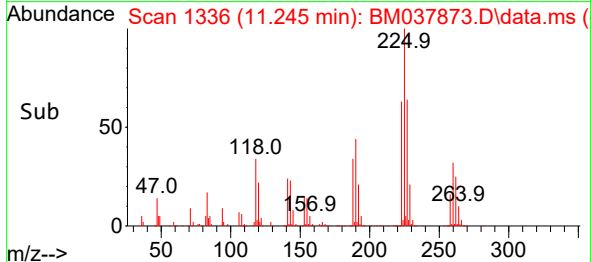

#34
Caprolactam
Concen: 73.688 ng/ul
RT: 11.927 min Scan# 1452
Delta R.T. 0.076 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:113 Resp: 367144
Ion Ratio Lower Upper
113 100
55 195.7 172.2 258.2
56 137.7 120.7 181.1




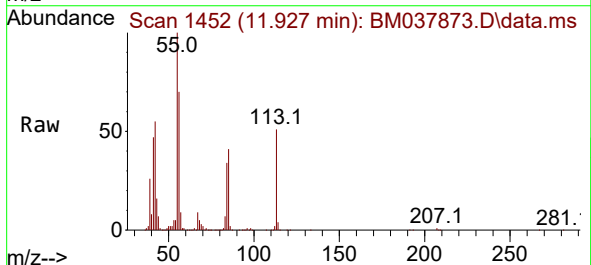




#35
4-Chloro-3-methylphenol
Concen: 156.126 ng/ul
RT: 12.204 min Scan# 1499
Delta R.T. 0.023 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:107 Resp: 2235497
Ion Ratio Lower Upper
107 100
144 27.3 23.4 35.0
142 83.4 71.0 106.4

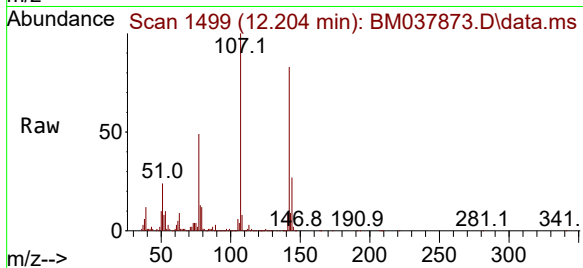

#36
2-Methylnaphthalene
Concen: 154.055 ng/ul
RT: 12.569 min Scan# 1561
Delta R.T. 0.012 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:142 Resp: 5147194
Ion Ratio Lower Upper
142 100
141 87.6 69.4 104.0

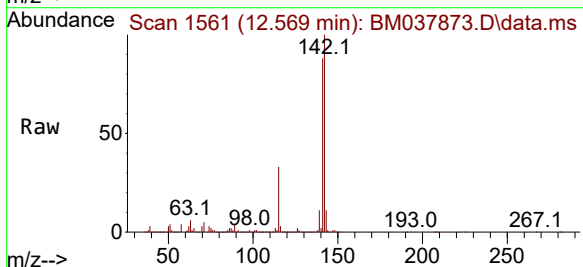



#37

1-Methylnaphthalene

Concen: 154.382 ng/ul

RT: 12.786 min Scan# 1

Delta R.T. 0.012 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:142 Resp: 5162646

Ion Ratio Lower Upper

142 100

141 91.8 72.4 108.6

116 3.5 2.9 4.3

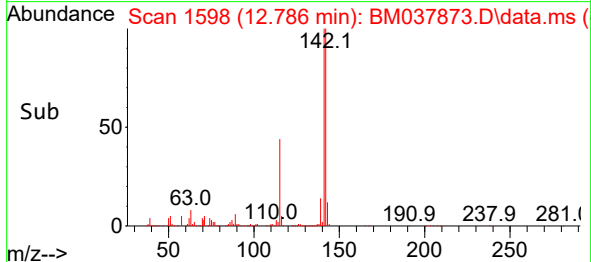

#39

1,2,4,5-Tetrachlorobenzene

Concen: 180.564 ng/ul

RT: 12.933 min Scan# 1623

Delta R.T. 0.012 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Tgt Ion:216 Resp: 2528549




Ion Ratio Lower Upper


216 100

214 78.1 64.2 96.4

179 20.4 15.4 23.2

108 16.9 12.7 19.1




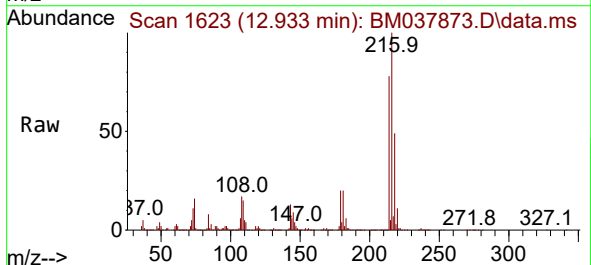




#40
Hexachlorocyclopentadiene
Concen: 225.078 ng/ul
RT: 12.904 min Scan# 1
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:237 Resp: 1733264
Ion Ratio Lower Upper
237 100
235 62.7 50.4 75.6
272 13.2 10.6 16.0

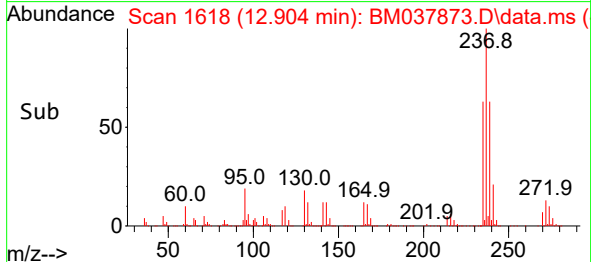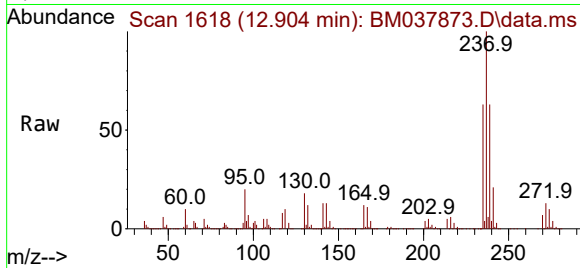

#41
2,4,6-Trichlorophenol
Concen: 188.721 ng/ul
RT: 13.169 min Scan# 1663
Delta R.T. 0.012 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:196 Resp: 1725300
Ion Ratio Lower Upper
196 100
198 96.2 75.0 112.6
200 30.7 24.5 36.7

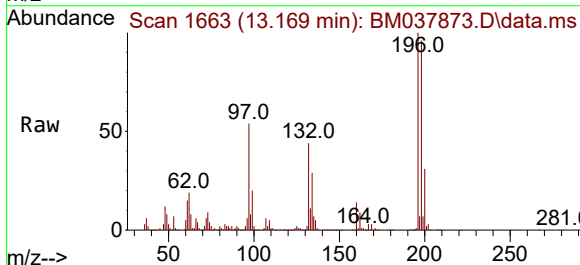



#42

2,4,5-Trichlorophenol

Concen: 187.413 ng/ul

RT: 13.245 min Scan# 1

Delta R.T. 0.018 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:196 Resp: 1824784

Ion Ratio Lower Upper

196 100

198 94.8 76.5 114.7

200 31.0 24.9 37.3

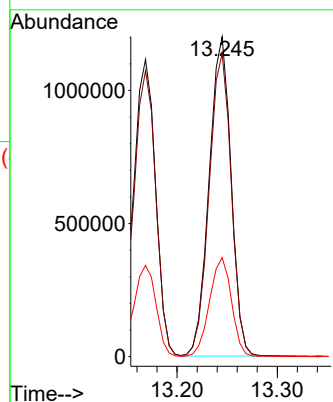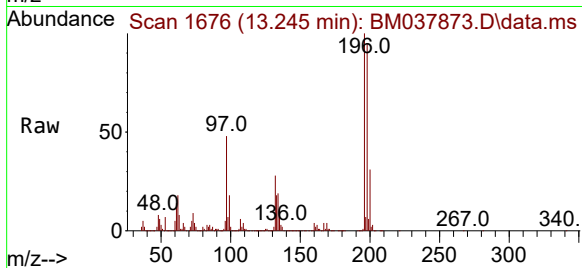

#43

1,1'-Biphenyl

Concen: 179.214 ng/ul

RT: 13.569 min Scan# 1731

Delta R.T. 0.012 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion:154 Resp: 6369669


Ion Ratio Lower Upper

154 100

153 40.4 31.2 46.8

76 12.1 9.3 13.9



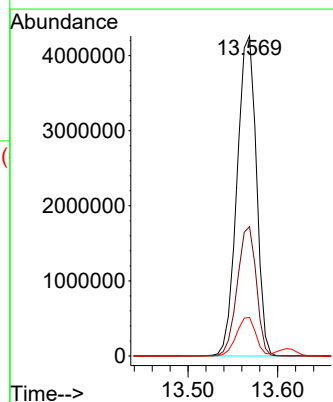
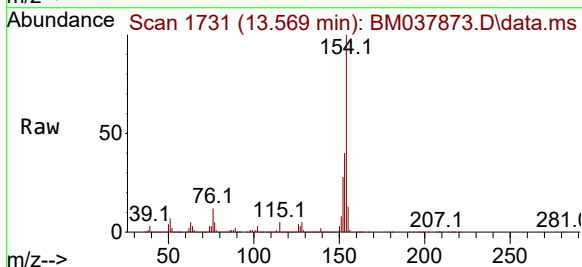




#44
2-Chloronaphthalene
Concen: 178.748 ng/ul
RT: 13.610 min Scan# 1738
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:162 Resp: 4985449
Ion Ratio Lower Upper
162 100
164 33.4 27.3 40.9
127 39.4 29.4 44.0

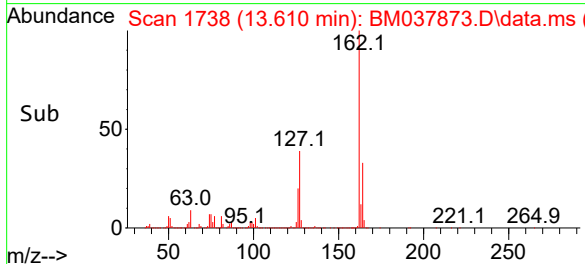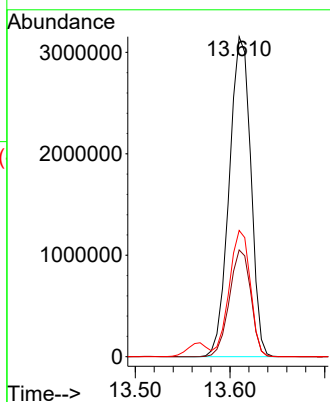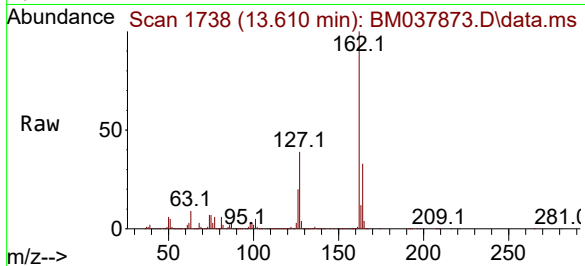

#45
2-Nitroaniline
Concen: 175.200 ng/ul
RT: 13.821 min Scan# 1774
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion: 65 Resp: 1382640
Ion Ratio Lower Upper
65 100
92 69.5 53.5 80.3
138 122.3 91.3 136.9


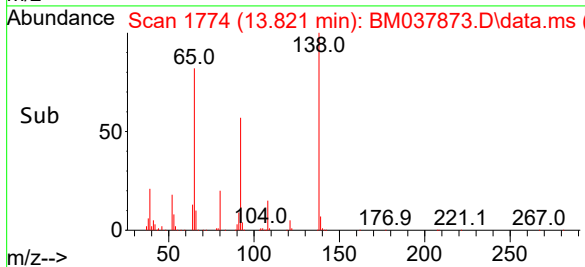

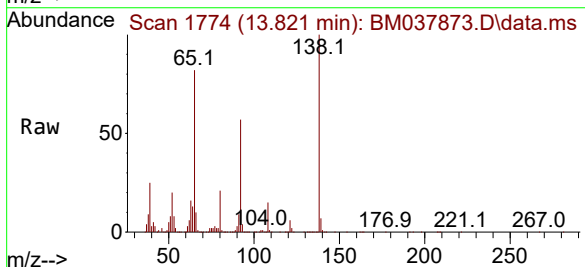




#47
Dimethylphthalate
Concen: 162.118 ng/ul
RT: 14.186 min Scan# 1836
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:163 Resp: 5669545
Ion Ratio Lower Upper
163 100
194 4.0 3.0 4.6
164 10.3 8.2 12.4

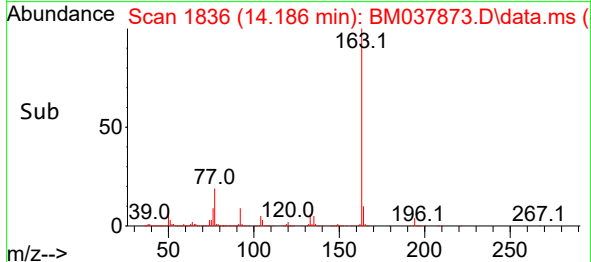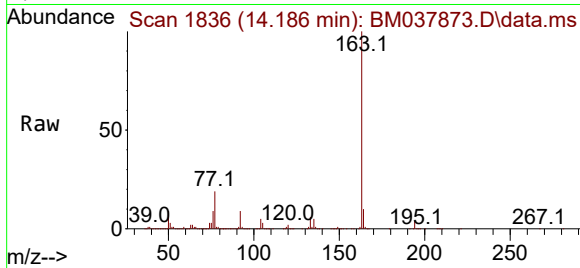

#48
2,6-Dinitrotoluene
Concen: 175.792 ng/ul
RT: 14.310 min Scan# 1857
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:165 Resp: 1255206
Ion Ratio Lower Upper
165 100
89 52.7 41.1 61.7
121 20.3 17.4 26.2




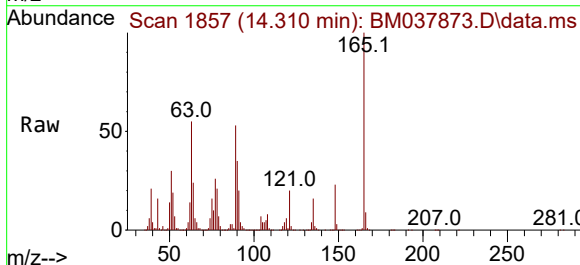


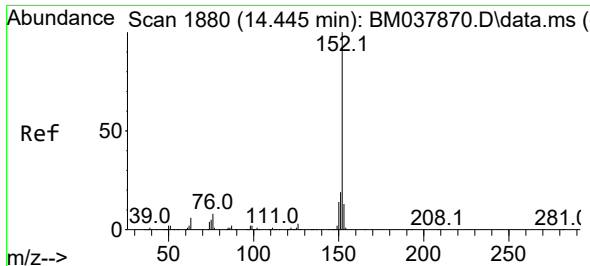

#50
Acenaphthylene
Concen: 169.611 ng/ul
RT: 14.451 min Scan# 1880
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:152 Resp: 7679068
Ion Ratio Lower Upper
152 100
151 20.4 15.3 22.9
153 13.8 10.2 15.4

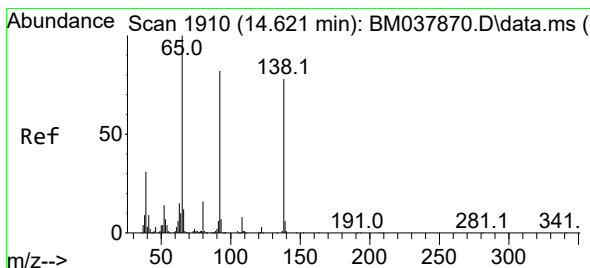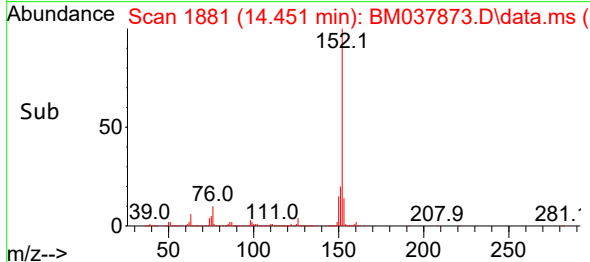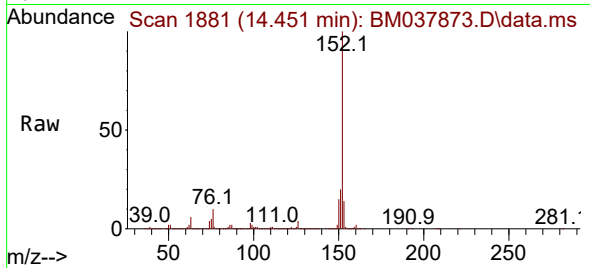

#51
3-Nitroaniline
Concen: 149.396 ng/ul
RT: 14.639 min Scan# 1913
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:138 Resp: 1273229
Ion Ratio Lower Upper
138 100
108 9.1 7.9 11.9
92 106.6 83.4 125.0


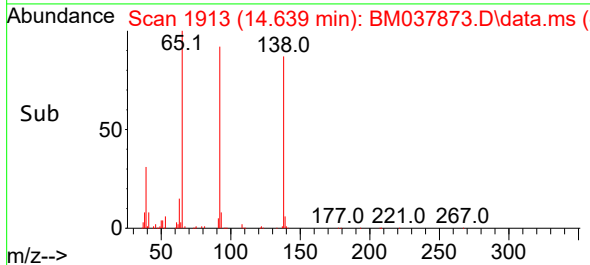

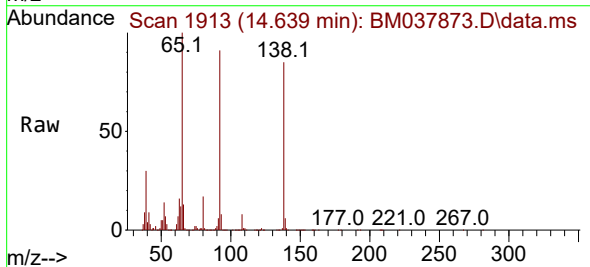




#52
Acenaphthene
Concen: 164.744 ng/ul
RT: 14.792 min Scan# 1939
Delta R.T. 0.012 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:153 Resp: 5168362
Ion Ratio Lower Upper
153 100
152 48.1 38.2 57.4
154 90.7 71.4 107.0

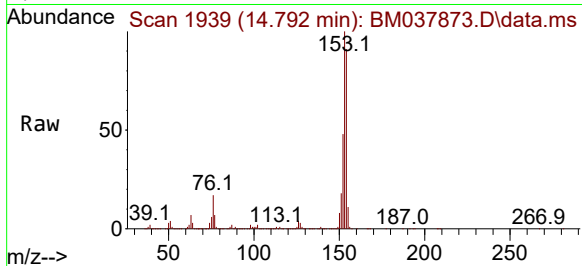

#53
2,4-Dinitrophenol
Concen: 178.489 ng/ul
RT: 14.839 min Scan# 1947
Delta R.T. 0.012 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:184 Resp: 744337
Ion Ratio Lower Upper
184 100
63 62.0 46.2 69.4
154 55.8 45.5 68.3




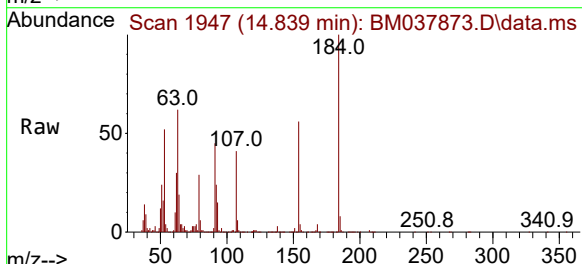




#55
4-Nitrophenol
Concen: 167.100 ng/ul
RT: 14.951 min Scan# 1966
Delta R.T. 0.029 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:109 Resp: 717821
Ion Ratio Lower Upper
109 100
139 157.5 119.2 178.8
65 139.3 108.7 163.1

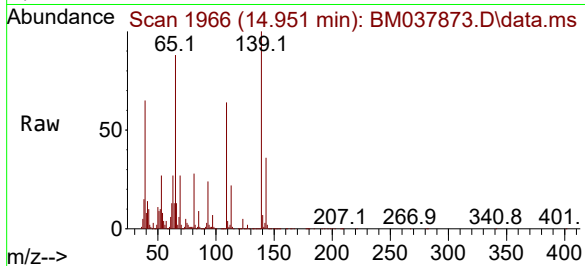

#56
Dibenzofuran
Concen: 162.205 ng/ul
RT: 15.121 min Scan# 1995
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:168 Resp: 6851247
Ion Ratio Lower Upper
168 100
139 38.1 28.1 42.1

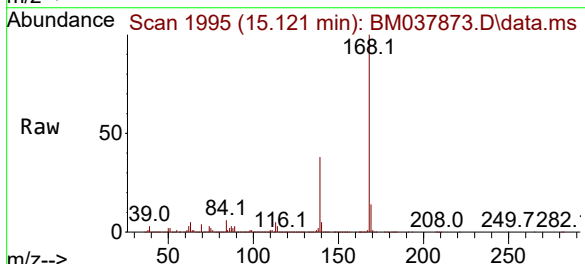

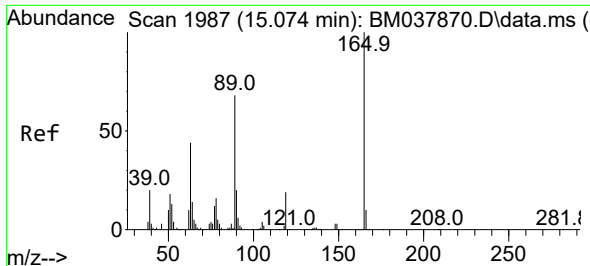

#57

2,4-Dinitrotoluene

Concen: 167.031 ng/ul

RT: 15.092 min Scan# 1987

Delta R.T. 0.018 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:165 Resp: 1665647

Ion Ratio Lower Upper

165 100

63 42.1 34.9 52.3

182 2.4 2.2 3.2

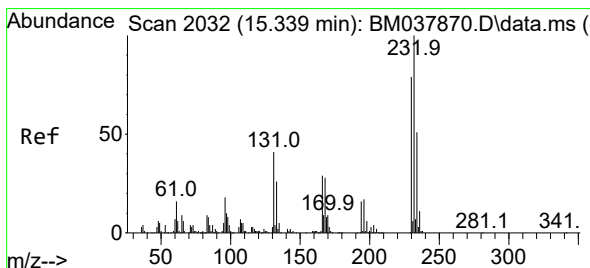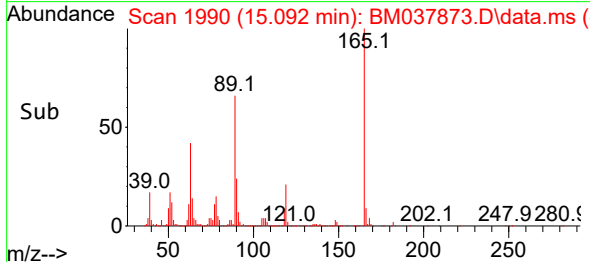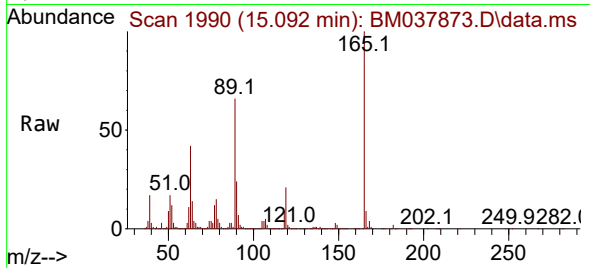

#58

2,3,4,6-Tetrachlorophenol

Concen: 168.949 ng/ul

RT: 15.345 min Scan# 2033

Delta R.T. 0.006 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Tgt Ion:232 Resp: 1446927




Ion Ratio Lower Upper


232 100

131 48.7 32.8 49.2

130 2.4 2.0 3.0

166 32.5 23.2 34.8

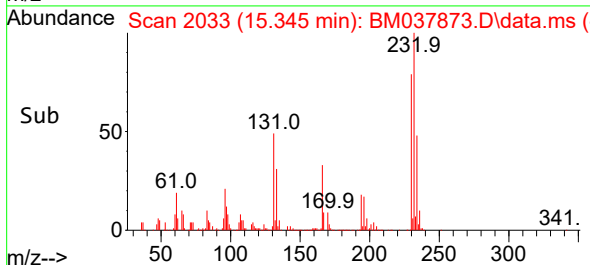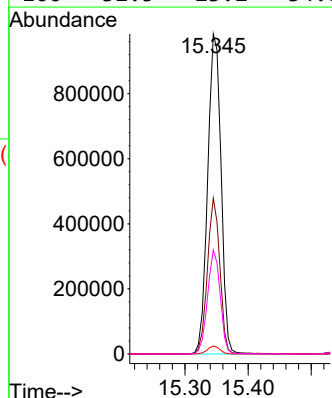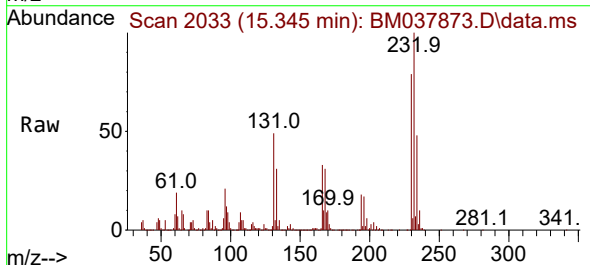



#59

Diethylphthalate

Concen: 154.366 ng/ul

RT: 15.539 min Scan# 2066

Delta R.T. 0.012 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:149 Resp: 5536338

Ion Ratio Lower Upper

149 100

177 22.3 18.5 27.7

150 12.7 9.5 14.3



#61

Fluorene

Concen: 143.928 ng/ul

RT: 15.774 min Scan# 2106

Delta R.T. 0.012 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion:166 Resp: 5117890


Ion Ratio Lower Upper

166 100

165 96.5 77.2 115.8

167 13.4 10.4 15.6









#62
4-Chlorophenyl-phenylether
Concen: 144.454 ng/ul
RT: 15.757 min Scan# 2103
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:204 Resp: 2448822
Ion Ratio Lower Upper
204 100
206 33.0 25.5 38.3
141 63.0 42.8 64.2

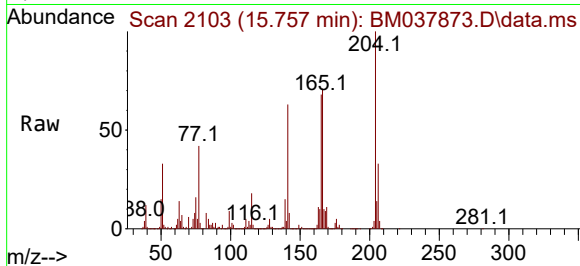

#63
4-Nitroaniline
Concen: 129.804 ng/ul
RT: 15.810 min Scan# 2112
Delta R.T. 0.029 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:138 Resp: 1112926
Ion Ratio Lower Upper
138 100
92 44.3 36.1 54.1
108 65.3 51.6 77.4









#66
 4,6-Dinitro-2-methylphenol
 Concen: 186.606 ng/ul
 RT: 15.857 min Scan# 2116
 Delta R.T. 0.023 min
 Lab File: BM037873.D
 Acq: 07 Dec 2022 15:59




Instrument :
 BNA_M
 ClientSampleId :
 SSTD160010


Tgt Ion:198 Resp: 945935
 Ion Ratio Lower Upper
 198 100
 182 2.9 3.8 5.8#
 77 22.1 19.3 28.9

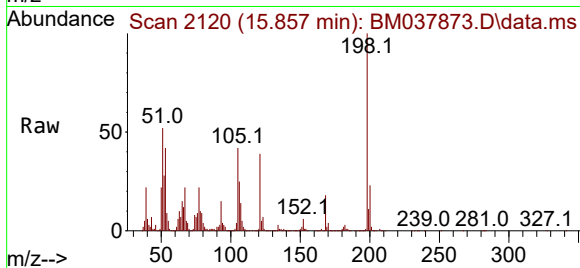

#67
 N-Nitrosodiphenylamine
 Concen: 167.182 ng/ul
 RT: 15.974 min Scan# 2140
 Delta R.T. 0.012 min
 Lab File: BM037873.D
 Acq: 07 Dec 2022 15:59

Tgt Ion:169 Resp: 4497362
 Ion Ratio Lower Upper
 169 100
 168 67.2 53.8 80.8
 167 37.1 29.3 43.9




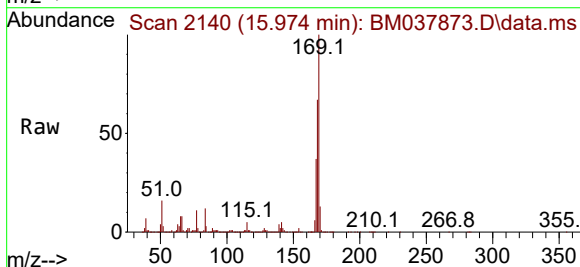




#68
4-Bromophenyl-phenylether
Concen: 167.147 ng/ul
RT: 16.651 min Scan# 21
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:248 Resp: 1601165
Ion Ratio Lower Upper
248 100
250 97.4 78.7 118.1
141 72.8 52.7 79.1

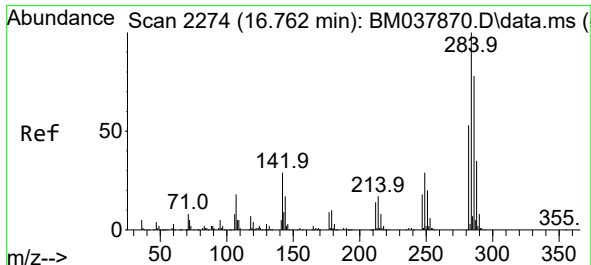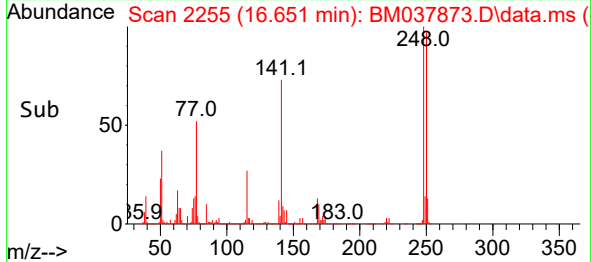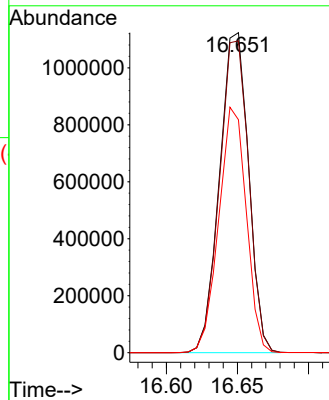

#69
Hexachlorobenzene
Concen: 162.742 ng/ul
RT: 16.768 min Scan# 2275
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:284 Resp: 1820493
Ion Ratio Lower Upper
284 100
142 35.4 23.1 34.7#
249 30.1 23.3 34.9

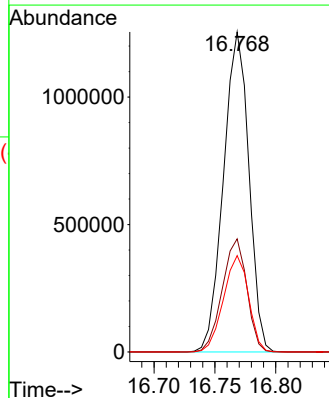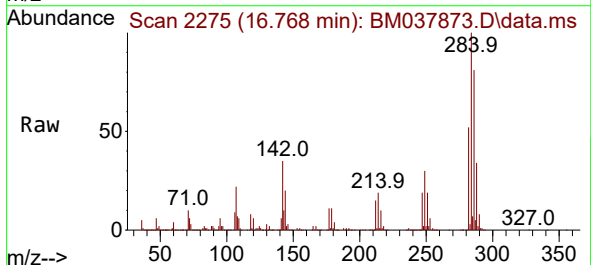



#70

Atrazine

Concen: 169.945 ng/ul

RT: 16.927 min Scan# 21

Delta R.T. 0.018 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:200 Resp: 1574426

Ion Ratio Lower Upper

200 100

173 26.8 20.5 30.7

215 48.7 40.1 60.1

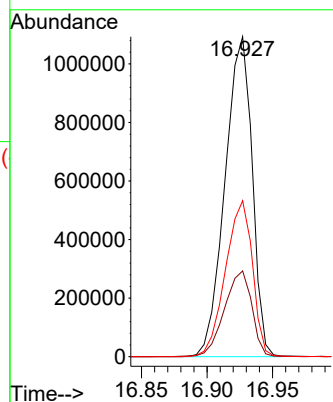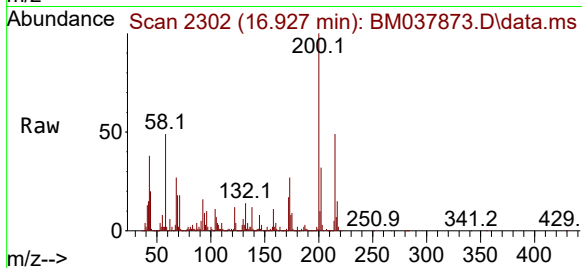

#71

Pentachlorophenol

Concen: 174.056 ng/ul

RT: 17.109 min Scan# 2333

Delta R.T. 0.006 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion:266 Resp: 1197530


Ion Ratio Lower Upper

266 100

264 63.9 50.1 75.1

268 64.8 50.6 75.8

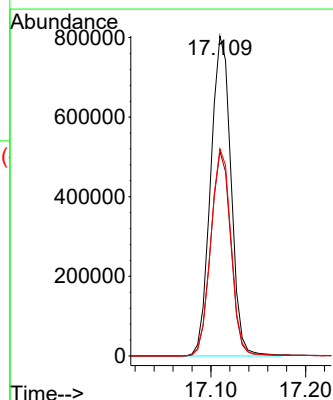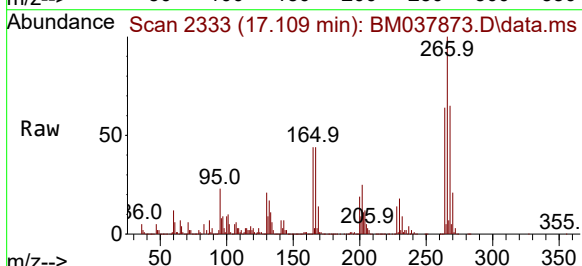



#72

Phenanthrene

Concen: 154.854 ng/ul

RT: 17.509 min Scan# 2410

Delta R.T. 0.012 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:178 Resp: 7834415

Ion Ratio Lower Upper

178 100

179 15.8 12.2 18.2

176 19.7 15.4 23.0

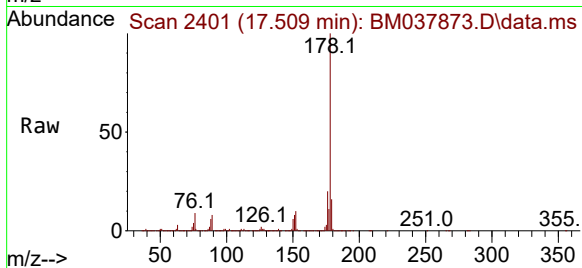

#74

Anthracene

Concen: 151.422 ng/ul

RT: 17.604 min Scan# 2417

Delta R.T. 0.012 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion:178 Resp: 7815087


Ion Ratio Lower Upper

178 100

179 15.9 11.8 17.8

176 19.3 15.0 22.6




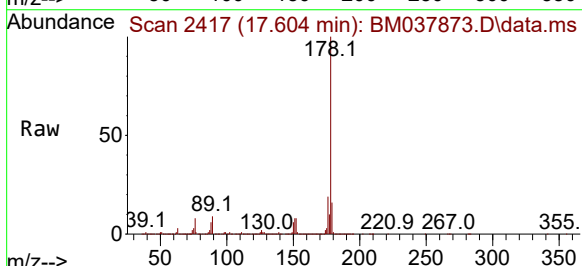




#75
1,2,3,4-Tetrachlorobenzene
Concen: 198.251 ng/uL
RT: 13.533 min Scan# 1725
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:216 Resp: 2495264
Ion Ratio Lower Upper
216 100
214 79.8 62.6 93.8
218 48.2 38.3 57.5



#76
Pentachlorobenzene
Concen: 166.666 ng/uL
RT: 15.045 min Scan# 1982
Delta R.T. 0.012 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:250 Resp: 2282200
Ion Ratio Lower Upper
250 100
248 62.1 51.0 76.4
252 63.9 51.8 77.6





#77

Carbazole

Concen: 152.943 ng/ul

RT: 17.868 min Scan# 2460

Delta R.T. 0.012 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:167 Resp: 7264128

Ion Ratio Lower Upper

167 100

166 21.8 16.7 25.1

139 13.2 9.8 14.6



#78

Di-n-butylphthalate

Concen: 149.609 ng/ul

RT: 18.415 min Scan# 2555

Delta R.T. 0.006 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion:149 Resp: 8933826


Ion Ratio Lower Upper

149 100

150 9.5 7.3 10.9

104 4.9 3.4 5.2





#80

Fluoranthene

Concen: 175.634 ng/ul

RT: 19.509 min Scan# 21

Delta R.T. 0.006 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:202 Resp: 8195940

Ion Ratio Lower Upper

202 100

101 11.5 8.6 13.0

100 8.8 6.6 10.0



#82

Pyrene

Concen: 169.422 ng/ul

RT: 19.874 min Scan# 2803

Delta R.T. 0.006 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion:202 Resp: 8163210


Ion Ratio Lower Upper

202 100

101 13.5 10.0 15.0

100 11.3 7.9 11.9





#83

Butylbenzylphthalate

Concen: 181.921 ng/ul

RT: 20.750 min Scan# 2951

Delta R.T. 0.006 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:149 Resp: 3821800

Ion Ratio Lower Upper

149 100

91 68.9 54.5 81.7

206 20.0 15.8 23.8

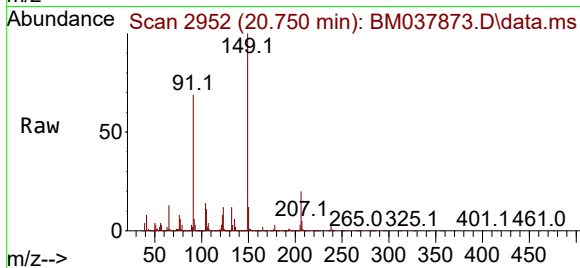

#84

3,3'-Dichlorobenzidine

Concen: 142.958 ng/ul

RT: 21.544 min Scan# 3087

Delta R.T. 0.006 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion:252 Resp: 2208837


Ion Ratio Lower Upper

252 100

254 65.3 53.2 79.8

126 11.0 7.8 11.8

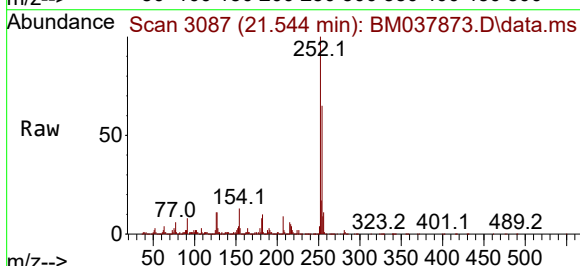



#85

Benzo(a)anthracene

Concen: 161.638 ng/ul

RT: 21.615 min Scan# 3099

Delta R.T. 0.006 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:228 Resp: 7627465

Ion Ratio Lower Upper

228 100

229 20.3 15.5 23.3

226 27.4 21.8 32.8

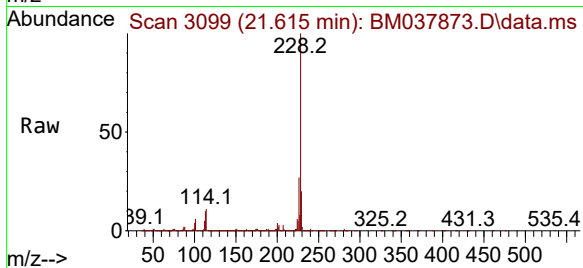

#86

Bis(2-ethylhexyl)phthalate

Concen: 164.411 ng/ul

RT: 21.521 min Scan# 3083

Delta R.T. 0.006 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion:149 Resp: 5219030


Ion Ratio Lower Upper

149 100

167 28.4 21.5 32.3

279 4.2 3.2 4.8




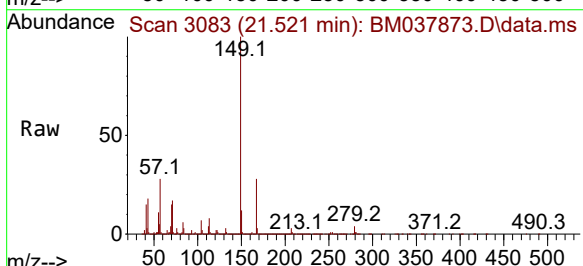




#87
Chrysene
Concen: 160.595 ng/ul
RT: 21.674 min Scan# 3109
Delta R.T. 0.012 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:228 Resp: 7054257
Ion Ratio Lower Upper
228 100
226 30.5 24.3 36.5
229 20.3 15.6 23.4



#89
Di-n-octyl phthalate
Concen: 146.420 ng/ul
RT: 22.474 min Scan# 3245
Delta R.T. 0.006 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:149 Resp: 9122418




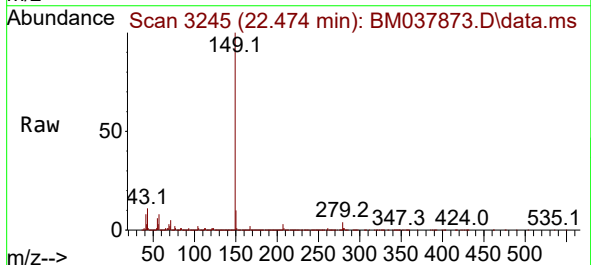




#90
Benzo(b)fluoranthene
Concen: 150.015 ng/ul
RT: 23.362 min Scan# 31
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59




Instrument :
BNA_M
ClientSampleId :
SSTD160010


Tgt Ion:252 Resp: 8340449
Ion Ratio Lower Upper
252 100
253 22.5 17.6 26.4
125 10.4 8.0 12.0

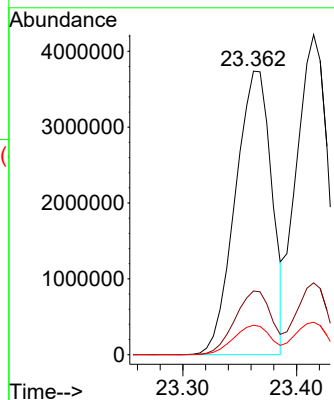

#91
Benzo(k)fluoranthene
Concen: 149.509 ng/ul
RT: 23.415 min Scan# 3405
Delta R.T. 0.018 min
Lab File: BM037873.D
Acq: 07 Dec 2022 15:59

Tgt Ion:252 Resp: 8018770
Ion Ratio Lower Upper
252 100
253 22.4 17.4 26.2
125 10.1 8.1 12.1

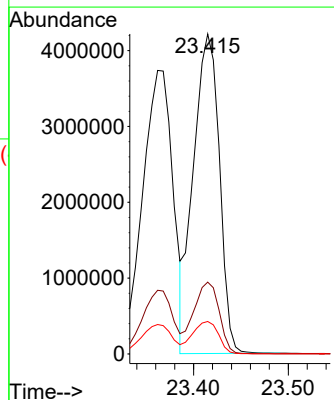



#93

Benzo(a)pyrene

Concen: 156.405 ng/ul

RT: 24.027 min Scan# 3

Delta R.T. 0.029 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:252 Resp: 7540815

Ion Ratio Lower Upper

252 100

253 22.0 17.4 26.0

125 11.2 9.4 14.0



#94

Indeno(1,2,3-cd)pyrene

Concen: 183.927 ng/ul

RT: 26.738 min Scan# 3970

Delta R.T. 0.029 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59




Tgt Ion:276 Resp: 9969585


Ion Ratio Lower Upper

276 100

138 23.9 19.3 28.9

277 25.1 19.8 29.8





#95

Dibenzo(a,h)anthracene

Concen: 165.266 ng/ul

RT: 26.768 min Scan# 3968

Delta R.T. 0.041 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Instrument :

BNA_M

ClientSampleId :

SSTD160010





Tgt Ion:278 Resp: 8153225

Ion Ratio Lower Upper

278 100

139 15.9 12.4 18.6

279 24.4 19.8 29.6

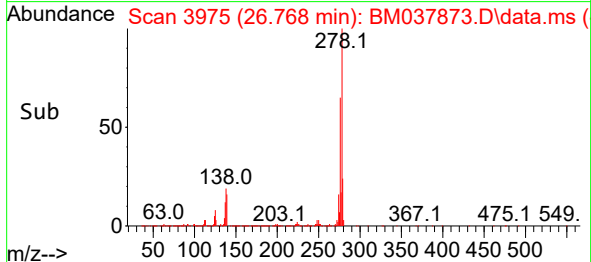

#96

Benzo(g,h,i)perylene

Concen: 180.914 ng/ul

RT: 27.556 min Scan# 4109

Delta R.T. 0.041 min

Lab File: BM037873.D

Acq: 07 Dec 2022 15:59

Tgt Ion:276 Resp: 8557726

Ion Ratio Lower Upper

276 100

138 22.2 17.1 25.7

277 24.1 18.2 27.4

