

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043191.D
 Acq On : 08 Dec 2023 11:48
 Operator : MA/JU
 Sample : PB157621BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.398	33	36	45	rVB	126114	182338	1.33%	0.129%
2	3.816	103	107	127	rBV	1509853	2467921	18.04%	1.747%
3	4.157	162	165	172	rVB2	31285	47137	0.34%	0.033%
4	7.169	669	677	685	rBV	2039114	3265280	23.87%	2.312%
5	7.351	701	708	719	rBV	1716851	2755590	20.15%	1.951%
6	7.539	733	740	749	rBV	2025127	3239468	23.68%	2.293%
7	8.010	812	820	828	rBV	1797332	2850018	20.84%	2.018%
8	8.716	933	940	951	rBV	2584306	4121484	30.13%	2.918%
9	9.180	1010	1019	1030	rBV	2066094	3381771	24.72%	2.394%
10	9.898	1134	1141	1149	rBV	1478454	2470275	18.06%	1.749%
11	10.433	1225	1232	1245	rBV	2611988	4247451	31.05%	3.007%
12	10.816	1290	1297	1305	rVB	2619209	4412097	32.26%	3.123%
13	10.957	1313	1321	1335	rBV	2150603	3629972	26.54%	2.570%
14	12.398	1560	1566	1574	rBV3	49966	94167	0.69%	0.067%
15	13.539	1754	1760	1766	rBV4	28261	55516	0.41%	0.039%
16	13.610	1769	1772	1776	rVV5	10862	15090	0.11%	0.011%
17	14.051	1840	1847	1857	rBV	5385622	7485359	54.72%	5.299%
18	14.327	1887	1894	1903	rBV	6013819	8850641	64.71%	6.266%
19	14.633	1939	1946	1955	rVB	4463065	6569715	48.03%	4.651%
20	14.821	1972	1978	1991	rBV	2418349	3492109	25.53%	2.472%
21	15.051	2013	2017	2021	rBV4	11932	18359	0.13%	0.013%
22	15.621	2107	2114	2127	rBV	7734078	11067947	80.92%	7.835%
23	15.739	2127	2134	2144	rBV	1728019	2406831	17.60%	1.704%
24	15.862	2150	2155	2163	rVB2	36386	61970	0.45%	0.044%
25	16.404	2243	2247	2250	rBV3	13043	18840	0.14%	0.013%
26	17.051	2354	2357	2363	rVB3	12461	22240	0.16%	0.016%
27	17.368	2404	2411	2419	rBV	5744990	8021779	58.65%	5.679%
28	17.468	2421	2428	2444	rVV2	8573644	12106174	88.51%	8.570%
29	17.750	2473	2476	2479	rBV3	12871	15055	0.11%	0.011%
30	18.268	2562	2564	2566	rBV2	14790	15468	0.11%	0.011%
31	19.315	2738	2742	2748	rVV2	95264	134204	0.98%	0.095%
32	19.386	2749	2754	2761	rVB	93908	133470	0.98%	0.094%
33	19.539	2776	2780	2785	rBV2	13152	29038	0.21%	0.021%
34	19.750	2810	2816	2826	rBV	10837130	13678247	100.00%	9.683%
35	21.533	3113	3119	3124	rBV	6688058	8218394	60.08%	5.818%
36	22.150	3220	3224	3231	rBV3	105912	168004	1.23%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043191.D
Acq On : 08 Dec 2023 11:48
Operator : MA/JU
Sample : PB157621BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK621

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Title : SVOA CALIBRATION

37	22.780	3327	3331	3338	rVB	136373	232823	1.70%	0.165%
38	23.485	3448	3451	3458	rVB4	122640	221083	1.62%	0.157%
39	23.779	3492	3501	3515	rBV2	6451700	12750143	93.21%	9.026%
40	23.932	3519	3527	3541	rVB	4247788	8302998	60.70%	5.878%




Sum of corrected areas: 141256466

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043191.D
Acq On : 08 Dec 2023 11:48
Operator : MA/JU
Sample : PB157621BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

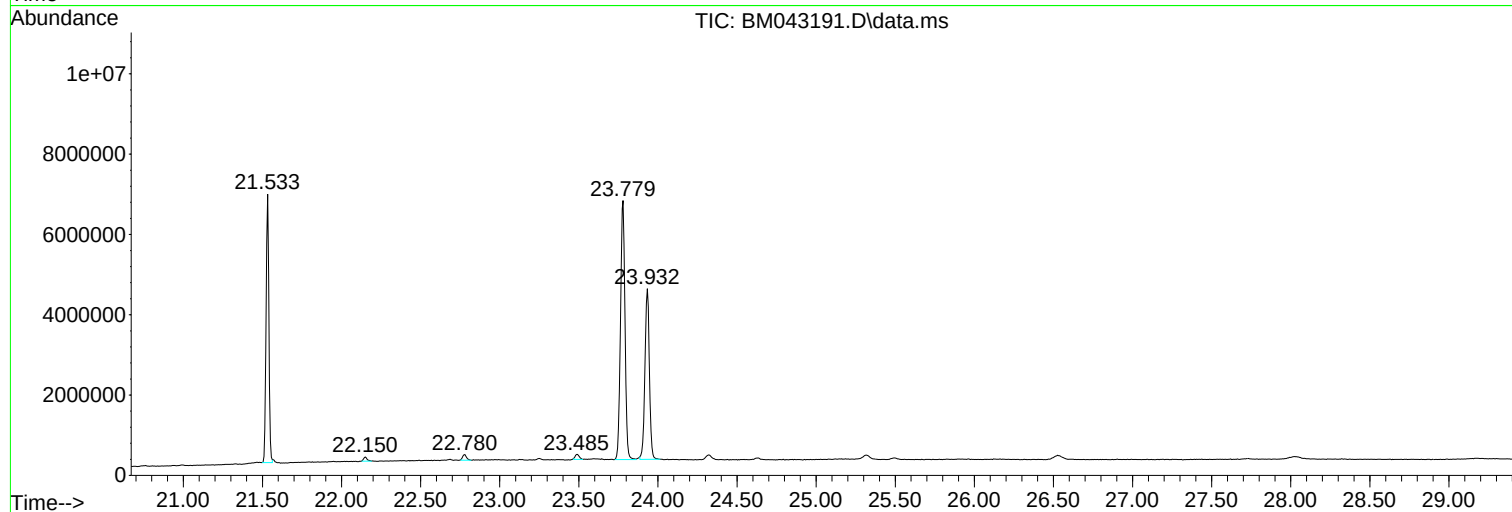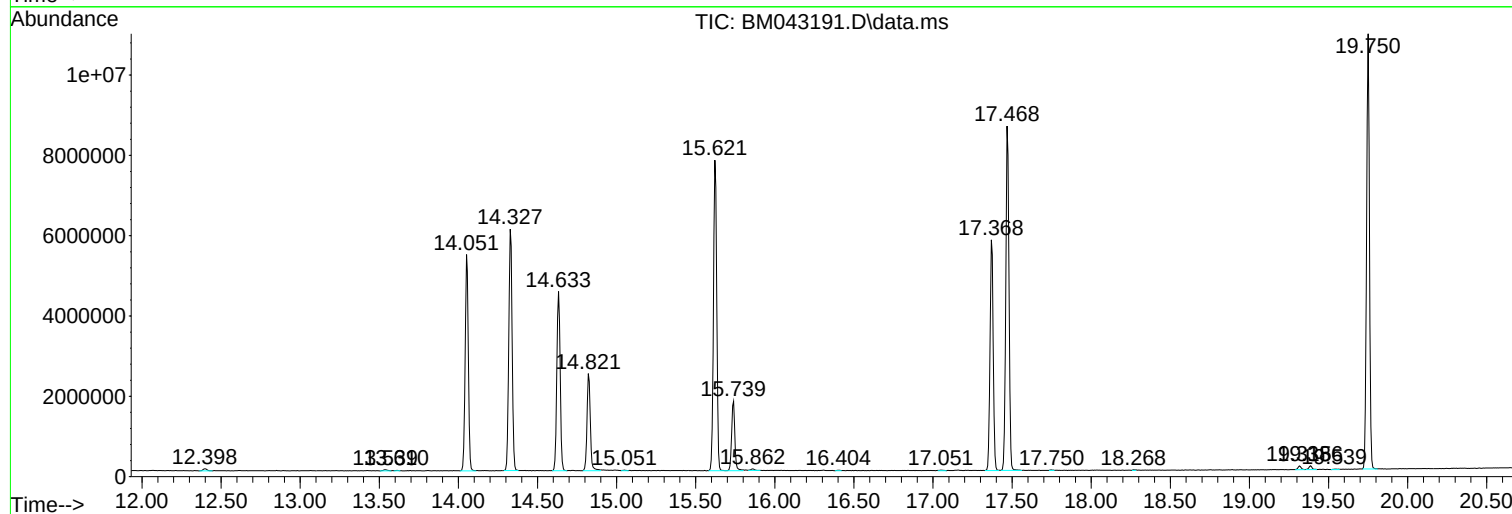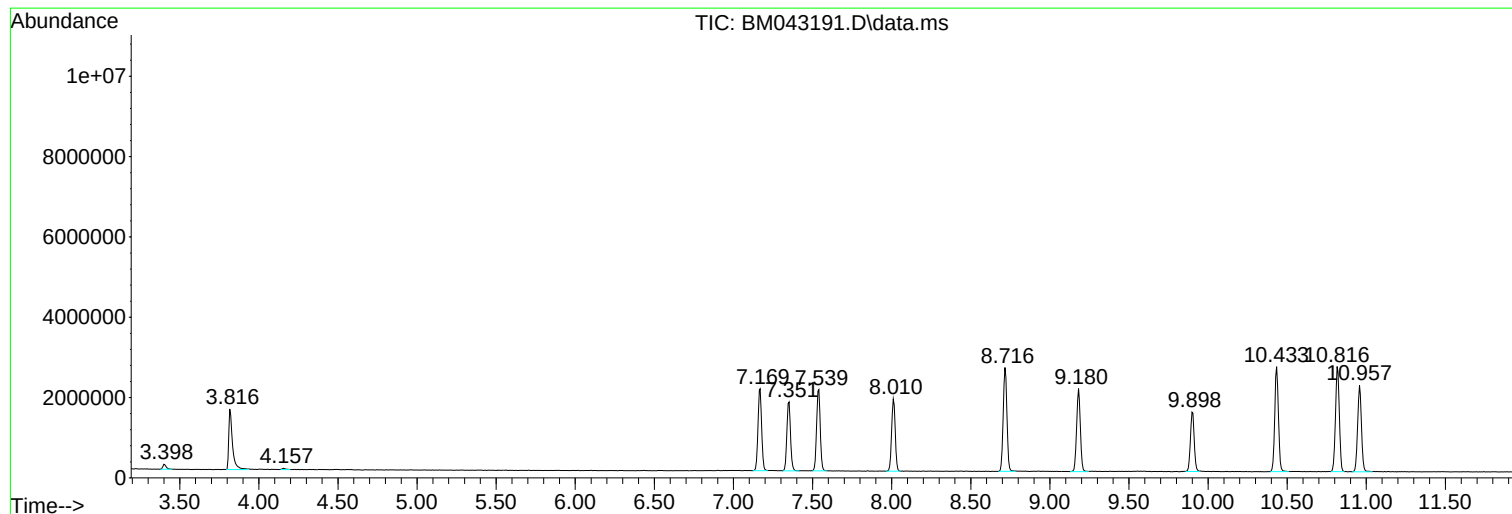

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043191.D
Acq On : 08 Dec 2023 11:48
Operator : MA/JU
Sample : PB157621BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043191.D
Acq On : 08 Dec 2023 11:48
Operator : MA/JU
Sample : PB157621BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------