

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043194.D
 Acq On : 08 Dec 2023 13:43
 Operator : MA/JU
 Sample : 05666-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOY44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	41	rBV2	57322	83936	0.54%	0.065%
2	3.822	105	108	122	rBV	441326	756932	4.89%	0.586%
3	4.058	146	148	154	rVB	32102	43109	0.28%	0.033%
4	4.158	162	165	171	rVB3	26410	34953	0.23%	0.027%
5	6.428	546	551	557	rVB2	45433	78634	0.51%	0.061%
6	7.163	670	676	686	rBV	260935	427690	2.76%	0.331%
7	7.351	701	708	718	rBV	1585310	2588257	16.71%	2.005%
8	7.540	732	740	750	rBV	1308301	2091162	13.50%	1.620%
9	8.010	812	820	828	rBV	1648076	2614052	16.88%	2.025%
10	8.716	932	940	950	rBV	864464	1372400	8.86%	1.063%
11	9.122	1004	1009	1012	rBV3	18129	30903	0.20%	0.024%
12	9.181	1012	1019	1026	rBV	1941304	3163050	20.42%	2.450%
13	9.334	1043	1045	1054	rVB7	9460	19153	0.12%	0.015%
14	9.898	1133	1141	1149	rBV	1302105	2193931	14.17%	1.700%
15	10.434	1223	1232	1241	rBV	2070052	3441921	22.22%	2.666%
16	10.816	1289	1297	1304	rBV	2403745	4028847	26.01%	3.121%
17	10.869	1304	1306	1310	rVV2	15788	19847	0.13%	0.015%
18	10.957	1313	1321	1332	rBV	1461743	2456786	15.86%	1.903%
19	11.628	1433	1435	1443	rVB4	11238	25044	0.16%	0.019%
20	12.233	1531	1538	1543	rBV6	20590	38926	0.25%	0.030%
21	12.398	1560	1566	1573	rVB3	48897	84386	0.54%	0.065%
22	12.475	1573	1579	1583	rBV4	10957	20975	0.14%	0.016%
23	13.175	1695	1698	1702	rBV4	8977	17587	0.11%	0.014%
24	13.469	1743	1748	1753	rBV	25520	38522	0.25%	0.030%
25	13.539	1753	1760	1766	rVV2	93222	153037	0.99%	0.119%
26	14.051	1841	1847	1854	rBV	4970481	6832658	44.12%	5.293%
27	14.157	1864	1865	1871	rVB2	13922	18216	0.12%	0.014%
28	14.327	1882	1894	1901	rBV	5597293	8322759	53.74%	6.447%
29	14.633	1937	1946	1955	rBV	4090858	5997668	38.72%	4.646%
30	14.716	1958	1960	1967	rVB4	12401	15859	0.10%	0.012%
31	14.822	1972	1978	1984	rBV	298338	458474	2.96%	0.355%
32	15.051	2011	2017	2021	rVB4	19086	37394	0.24%	0.029%
33	15.416	2075	2079	2083	rBV3	10525	19787	0.13%	0.015%
34	15.622	2106	2114	2127	rBV	7789379	10881495	70.26%	8.429%
35	15.739	2127	2134	2145	rVV	1838875	2543630	16.42%	1.970%
36	15.857	2149	2154	2163	rVB3	32251	75875	0.49%	0.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043194.D
 Acq On : 08 Dec 2023 13:43
 Operator : MA/JU
 Sample : 05666-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOY44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

37	16.186	2208	2210	2215	rVB2	11426	18204	0.12%	0.014%
38	16.833	2317	2320	2325	rVB6	16324	23513	0.15%	0.018%
39	16.974	2340	2344	2349	rVB7	13356	25871	0.17%	0.020%
40	17.180	2377	2379	2384	rVB5	19422	26195	0.17%	0.020%
41	17.368	2405	2411	2422	rBV	5150652	7347860	47.44%	5.692%
42	17.468	2422	2428	2437	rBV	9300456	13135141	84.81%	10.175%
43	17.745	2469	2475	2477	rBV5	21038	42038	0.27%	0.033%
44	18.051	2525	2527	2531	rVB3	21920	24847	0.16%	0.019%
45	18.139	2540	2542	2545	rBV4	14979	17365	0.11%	0.013%
46	18.268	2559	2564	2569	rBV2	161134	237218	1.53%	0.184%
47	18.568	2613	2615	2619	rBV4	18223	19589	0.13%	0.015%
48	19.315	2738	2742	2747	rBV3	116189	154538	1.00%	0.120%
49	19.386	2750	2754	2758	rVV	109356	147791	0.95%	0.114%
50	19.539	2777	2780	2785	rBV3	70244	88038	0.57%	0.068%
51	19.751	2810	2816	2824	rBV	11920181	15488103	100.00%	11.998%
52	19.815	2824	2827	2832	rVB4	40086	51759	0.33%	0.040%
53	21.109	3043	3047	3051	rBV2	39756	51674	0.33%	0.040%
54	21.256	3068	3072	3077	rBV2	132670	185589	1.20%	0.144%
55	21.533	3113	3119	3129	rBV	6187681	7761505	50.11%	6.012%
56	22.821	3335	3338	3347	rVB	172246	240188	1.55%	0.186%
57	23.780	3493	3501	3515	rBV2	7923932	14987045	96.76%	11.610%
58	23.933	3519	3527	3541	rVB	3990485	7990248	51.59%	6.190%




Sum of corrected areas: 129092174

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043194.D
Acq On : 08 Dec 2023 13:43
Operator : MA/JU
Sample : 05666-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y44

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

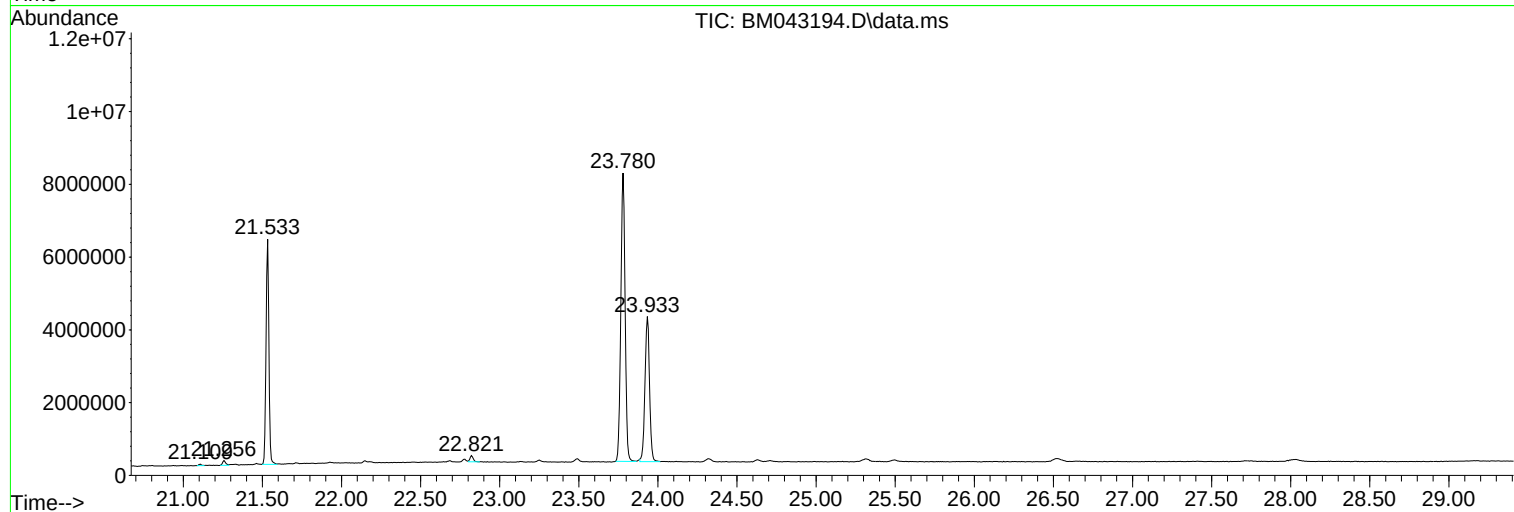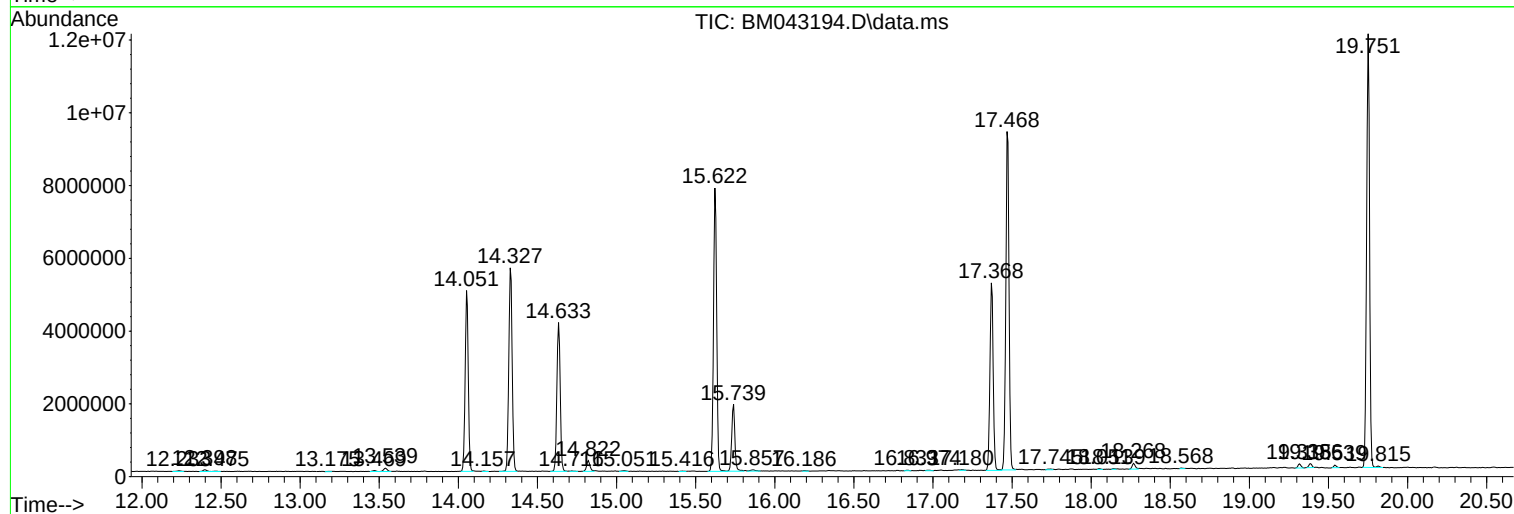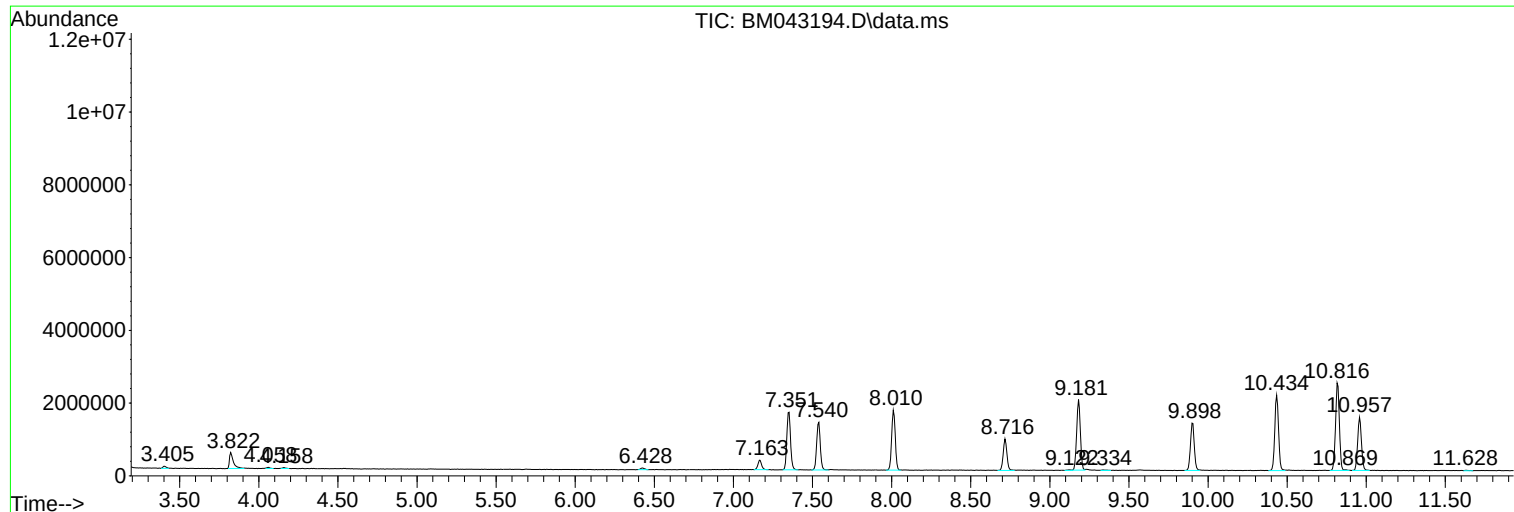

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043194.D
Acq On : 08 Dec 2023 13:43
Operator : MA/JU
Sample : 05666-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y44

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043194.D
Acq On : 08 Dec 2023 13:43
Operator : MA/JU
Sample : 05666-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y44

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc