

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043195.D
 Acq On : 08 Dec 2023 14:19
 Operator : MA/JU
 Sample : 05666-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0Y45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	41	rBV	59248	83385	0.58%	0.065%
2	3.822	105	108	124	rBV	401888	710652	4.92%	0.551%
3	4.058	146	148	153	rVB4	26891	35726	0.25%	0.028%
4	4.157	161	165	170	rVB2	31366	48544	0.34%	0.038%
5	6.422	545	550	559	rVB2	59874	106781	0.74%	0.083%
6	7.163	671	676	684	rVB	311796	510434	3.53%	0.396%
7	7.351	701	708	719	rVB	1639123	2662000	18.43%	2.063%
8	7.540	733	740	748	rBV	1342885	2149130	14.88%	1.666%
9	8.010	812	820	828	rBV	1707288	2704358	18.73%	2.096%
10	8.716	934	940	951	rBV	938829	1482804	10.27%	1.149%
11	9.122	1005	1009	1012	rBV5	20488	32194	0.22%	0.025%
12	9.181	1012	1019	1026	rVV	2029234	3262188	22.59%	2.528%
13	9.345	1043	1047	1051	rBV4	13779	25812	0.18%	0.020%
14	9.575	1081	1086	1095	rVB3	27142	55802	0.39%	0.043%
15	9.898	1134	1141	1154	rBV	1328095	2211621	15.32%	1.714%
16	10.434	1224	1232	1240	rBV	2091239	3443443	23.85%	2.669%
17	10.816	1289	1297	1304	rBV	2454118	4198389	29.07%	3.254%
18	10.863	1304	1305	1311	rVB2	27392	34522	0.24%	0.027%
19	10.957	1314	1321	1329	rBV	1340729	2242653	15.53%	1.738%
20	12.063	1503	1509	1514	rVB2	21019	33259	0.23%	0.026%
21	12.233	1533	1538	1542	rVB3	26232	35668	0.25%	0.028%
22	12.398	1561	1566	1571	rVB2	46155	70573	0.49%	0.055%
23	12.475	1575	1579	1582	rBV5	11798	19378	0.13%	0.015%
24	13.475	1744	1749	1754	rVB3	34195	59183	0.41%	0.046%
25	13.539	1754	1760	1767	rBV4	36466	77661	0.54%	0.060%
26	13.610	1767	1772	1776	rVB3	9694	16074	0.11%	0.012%
27	13.786	1795	1802	1803	rBV4	14936	22741	0.16%	0.018%
28	14.051	1838	1847	1858	rBV	5249379	7294689	50.52%	5.654%
29	14.327	1887	1894	1905	rVB	5642041	8567117	59.33%	6.640%
30	14.539	1926	1930	1933	rVB2	14237	17778	0.12%	0.014%
31	14.633	1939	1946	1953	rBV	4347831	6188264	42.85%	4.796%
32	14.822	1971	1978	1985	rBV2	337091	538069	3.73%	0.417%
33	15.045	2010	2016	2022	rVB4	22331	46659	0.32%	0.036%
34	15.439	2078	2083	2085	rBV3	10429	17590	0.12%	0.014%
35	15.621	2107	2114	2127	rVB	8094353	11201058	77.57%	8.682%
36	15.739	2127	2134	2147	rBV	1736232	2388280	16.54%	1.851%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043195.D
 Acq On : 08 Dec 2023 14:19
 Operator : MA/JU
 Sample : 05666-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0Y45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

37	15.863	2150	2155	2160	rVB2	32901	51355	0.36%	0.040%
38	16.398	2243	2246	2251	rVB5	12077	20899	0.14%	0.016%
39	16.515	2260	2266	2267	rBV	10554	16280	0.11%	0.013%
40	16.768	2306	2309	2315	rBV3	14036	20933	0.14%	0.016%
41	16.833	2315	2320	2323	rBV3	14916	22903	0.16%	0.018%
42	16.915	2329	2334	2337	rVB4	9127	15736	0.11%	0.012%
43	17.057	2354	2358	2361	rVB3	12976	18814	0.13%	0.015%
44	17.151	2367	2374	2377	rBV3	19747	38950	0.27%	0.030%
45	17.180	2377	2379	2385	rVB6	14514	21787	0.15%	0.017%
46	17.374	2405	2412	2417	rBV	5276259	7488367	51.86%	5.804%
47	17.468	2422	2428	2438	rVV	8303011	11921821	82.56%	9.240%
48	17.668	2458	2462	2465	rVB2	13203	19623	0.14%	0.015%
49	17.745	2468	2475	2482	rBV6	22442	62771	0.43%	0.049%
50	18.139	2538	2542	2547	rBV4	15724	27864	0.19%	0.022%
51	18.268	2557	2564	2571	rBV2	145874	233671	1.62%	0.181%
52	18.345	2572	2577	2582	rVB2	19699	30747	0.21%	0.024%
53	18.592	2614	2619	2624	rBV4	18799	33965	0.24%	0.026%
54	18.751	2642	2646	2650	rBV4	27133	39989	0.28%	0.031%
55	18.821	2654	2658	2663	rVB4	8135	14675	0.10%	0.011%
56	19.127	2706	2710	2713	rBV4	86917	127956	0.89%	0.099%
57	19.151	2713	2714	2719	rVB2	47529	59775	0.41%	0.046%
58	19.245	2726	2730	2734	rVB2	12912	17133	0.12%	0.013%
59	19.315	2738	2742	2747	rVB	111805	151655	1.05%	0.118%
60	19.386	2748	2754	2758	rBV2	145543	223278	1.55%	0.173%
61	19.421	2758	2760	2764	rVB5	31364	32304	0.22%	0.025%
62	19.539	2777	2780	2783	rBV4	57849	69498	0.48%	0.054%
63	19.633	2794	2796	2799	rVB3	14905	14772	0.10%	0.011%
64	19.698	2804	2807	2809	rVV3	20992	18312	0.13%	0.014%
65	19.751	2809	2816	2823	rVV	11020792	14440360	100.00%	11.192%
66	19.815	2824	2827	2835	rVB4	42126	65671	0.45%	0.051%
67	20.168	2885	2887	2894	rVB6	27476	32604	0.23%	0.025%
68	20.686	2972	2975	2978	rVB3	21501	26884	0.19%	0.021%
69	21.103	3043	3046	3050	rBV2	54845	67555	0.47%	0.052%
70	21.256	3068	3072	3078	rBV4	132683	182586	1.26%	0.142%
71	21.533	3113	3119	3133	rBV	6485335	7929230	54.91%	6.146%
72	22.821	3334	3338	3347	rVB	239428	349402	2.42%	0.271%
73	23.780	3493	3501	3513	rBV2	7580409	14381927	99.60%	11.147%
74	23.933	3519	3527	3541	rVB	4047727	8132413	56.32%	6.303%

Sum of corrected areas: 129018944

Instrument :

BNA_M

ClientSampleId :




E0Y45

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043195.D
Acq On : 08 Dec 2023 14:19
Operator : MA/JU
Sample : 05666-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

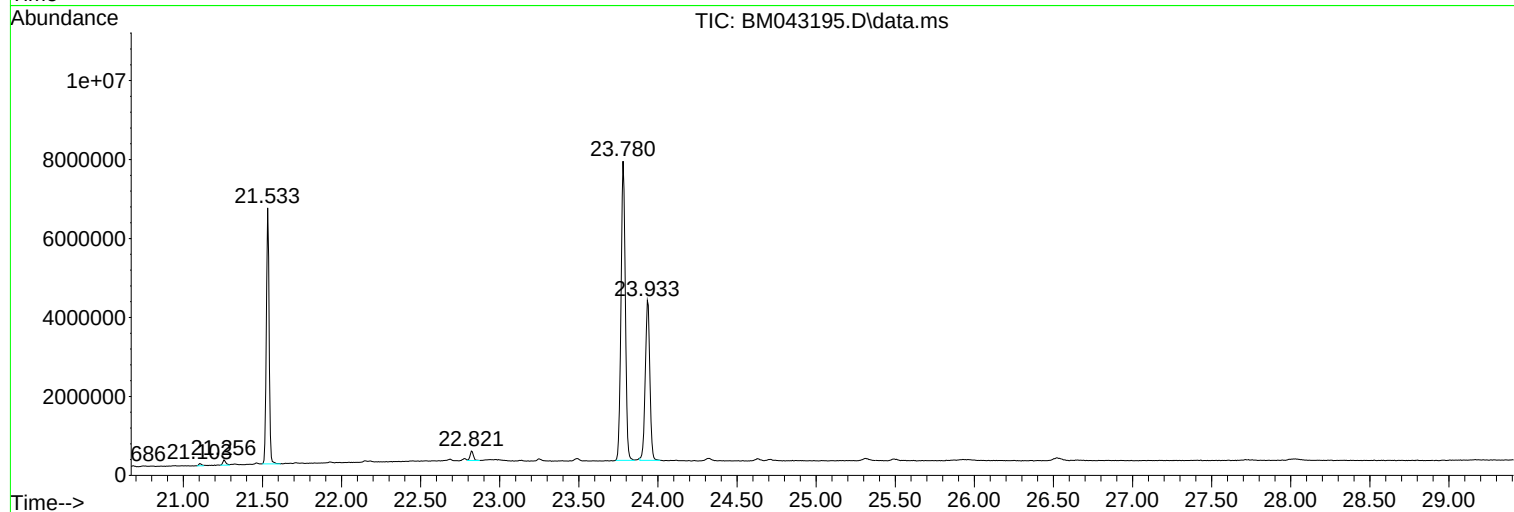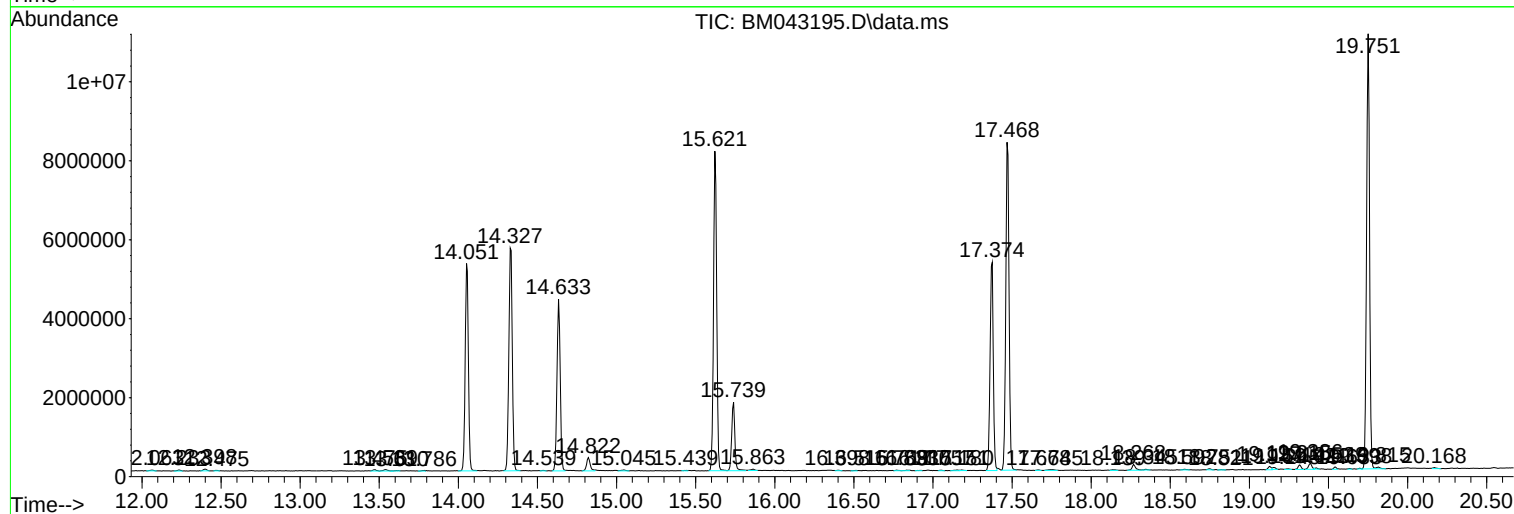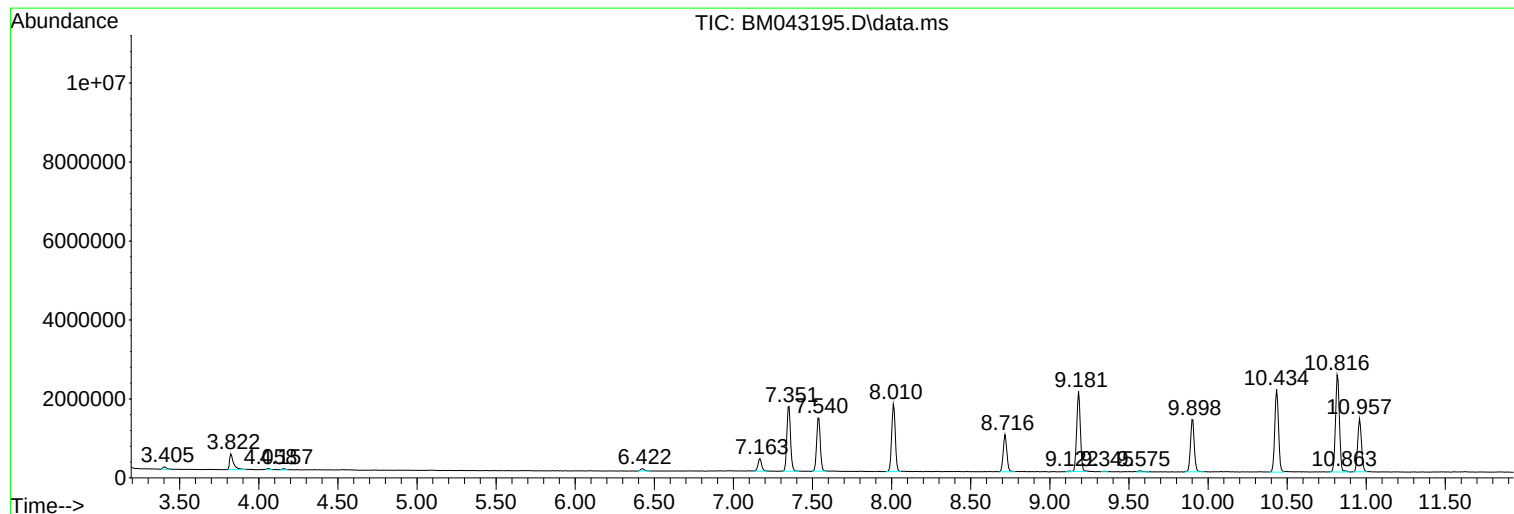

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043195.D
Acq On : 08 Dec 2023 14:19
Operator : MA/JU
Sample : 05666-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043195.D
Acq On : 08 Dec 2023 14:19
Operator : MA/JU
Sample : 05666-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc