

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043196.D
 Acq On : 08 Dec 2023 14:55
 Operator : MA/JU
 Sample : 05666-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0Y32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	33	36	49	rVB	92058	149485	1.06%	0.118%
2	3.822	104	108	128	rBV	498297	883786	6.25%	0.699%
3	4.057	145	148	153	rVB3	32423	52319	0.37%	0.041%
4	4.157	161	165	173	rBV2	44281	72053	0.51%	0.057%
5	7.169	671	677	683	rVB	393268	618028	4.37%	0.489%
6	7.351	701	708	719	rVB	1558277	2501271	17.69%	1.978%
7	7.540	733	740	751	rVV	1406342	2286587	16.17%	1.809%
8	7.622	751	754	758	rVB5	12225	16826	0.12%	0.013%
9	8.010	813	820	830	rVB	1706623	2703350	19.12%	2.138%
10	8.716	931	940	950	rBV	1174760	1873688	13.25%	1.482%
11	9.181	1012	1019	1026	rBV	1859087	3052338	21.59%	2.414%
12	9.569	1079	1085	1090	rVB3	29243	54654	0.39%	0.043%
13	9.898	1134	1141	1150	rBV	1313967	2148761	15.20%	1.700%
14	10.434	1223	1232	1240	rBV	2135789	3511528	24.84%	2.777%
15	10.816	1289	1297	1309	rVV	2432765	4189255	29.63%	3.314%
16	10.957	1314	1321	1330	rBV	2019293	3401855	24.06%	2.691%
17	11.633	1432	1436	1441	rVB4	17155	27239	0.19%	0.022%
18	12.057	1504	1508	1520	rVB3	21086	55291	0.39%	0.044%
19	12.239	1535	1539	1543	rVB5	12236	19276	0.14%	0.015%
20	12.398	1561	1566	1573	rBV3	47094	92749	0.66%	0.073%
21	13.269	1707	1714	1719	rVB4	15426	30935	0.22%	0.024%
22	13.469	1743	1748	1753	rBV3	17293	29124	0.21%	0.023%
23	13.539	1753	1760	1765	rVV3	47167	82457	0.58%	0.065%
24	13.610	1769	1772	1776	rVB3	9420	14862	0.11%	0.012%
25	14.051	1841	1847	1854	rBV	4917311	6852306	48.47%	5.420%
26	14.327	1887	1894	1901	rBV	5443609	8058193	57.00%	6.374%
27	14.633	1939	1946	1954	rBV	4245618	6142491	43.45%	4.858%
28	14.821	1973	1978	1992	rBV	375869	606910	4.29%	0.480%
29	15.051	2012	2017	2020	rBV5	16582	17837	0.13%	0.014%
30	15.621	2106	2114	2127	rBV	7575652	10647818	75.32%	8.422%
31	15.739	2127	2134	2149	rVV	1664333	2322396	16.43%	1.837%
32	15.863	2149	2155	2158	rVV3	32750	43509	0.31%	0.034%
33	16.145	2200	2203	2205	rBV2	20828	27003	0.19%	0.021%
34	16.174	2205	2208	2213	rVB4	52811	73368	0.52%	0.058%
35	16.863	2320	2325	2331	rVB4	16508	31884	0.23%	0.025%
36	17.051	2353	2357	2362	rVB2	14988	18010	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043196.D
 Acq On : 08 Dec 2023 14:55
 Operator : MA/JU
 Sample : 05666-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0Y32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

37	17.157	2371	2375	2379	rBV3	9719	14649	0.10%	0.012%
38	17.221	2381	2386	2390	rBV6	26231	38406	0.27%	0.030%
39	17.374	2405	2412	2421	rBV	5224390	7417436	52.47%	5.867%
40	17.468	2421	2428	2441	rVV	8804648	12390164	87.64%	9.800%
41	17.562	2441	2444	2449	rVB4	27217	43408	0.31%	0.034%
42	17.668	2459	2462	2465	rVB3	13325	17104	0.12%	0.014%
43	17.745	2470	2475	2482	rBV4	14272	25465	0.18%	0.020%
44	18.268	2559	2564	2571	rBV2	90216	129483	0.92%	0.102%
45	19.315	2738	2742	2747	rBV3	91224	136187	0.96%	0.108%
46	19.386	2750	2754	2758	rVV	88319	115010	0.81%	0.091%
47	19.456	2765	2766	2770	rVB2	14817	14480	0.10%	0.011%
48	19.539	2777	2780	2786	rVV4	44430	57323	0.41%	0.045%
49	19.698	2804	2807	2809	rBV3	15821	15265	0.11%	0.012%
50	19.751	2809	2816	2824	rBV	11051523	14137623	100.00%	11.182%
51	19.986	2852	2856	2861	rVB2	44749	63464	0.45%	0.050%
52	20.745	2982	2985	2988	rBV4	17453	27543	0.19%	0.022%
53	21.256	3069	3072	3077	rBV3	59236	76678	0.54%	0.061%
54	21.533	3113	3119	3128	rBV	6285281	7746523	54.79%	6.127%
55	23.780	3492	3501	3513	rBV2	6864949	13348846	94.42%	10.558%
56	23.933	3519	3527	3544	rVB	3899283	7903842	55.91%	6.252%




Sum of corrected areas: 126428341

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043196.D
Acq On : 08 Dec 2023 14:55
Operator : MA/JU
Sample : 05666-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

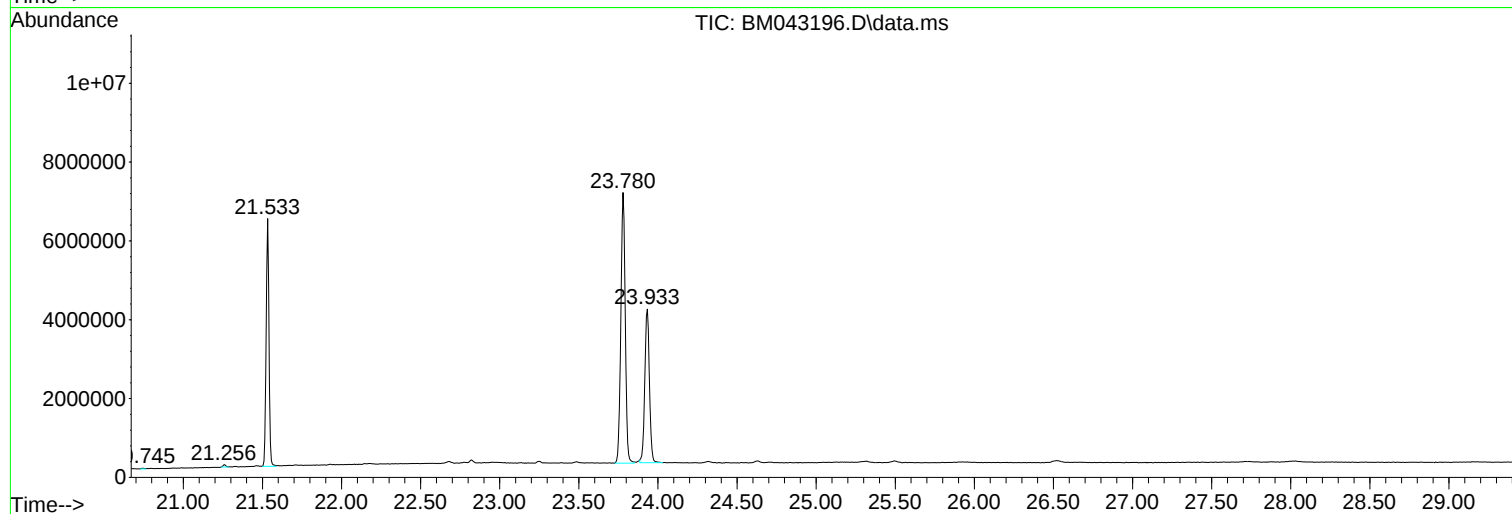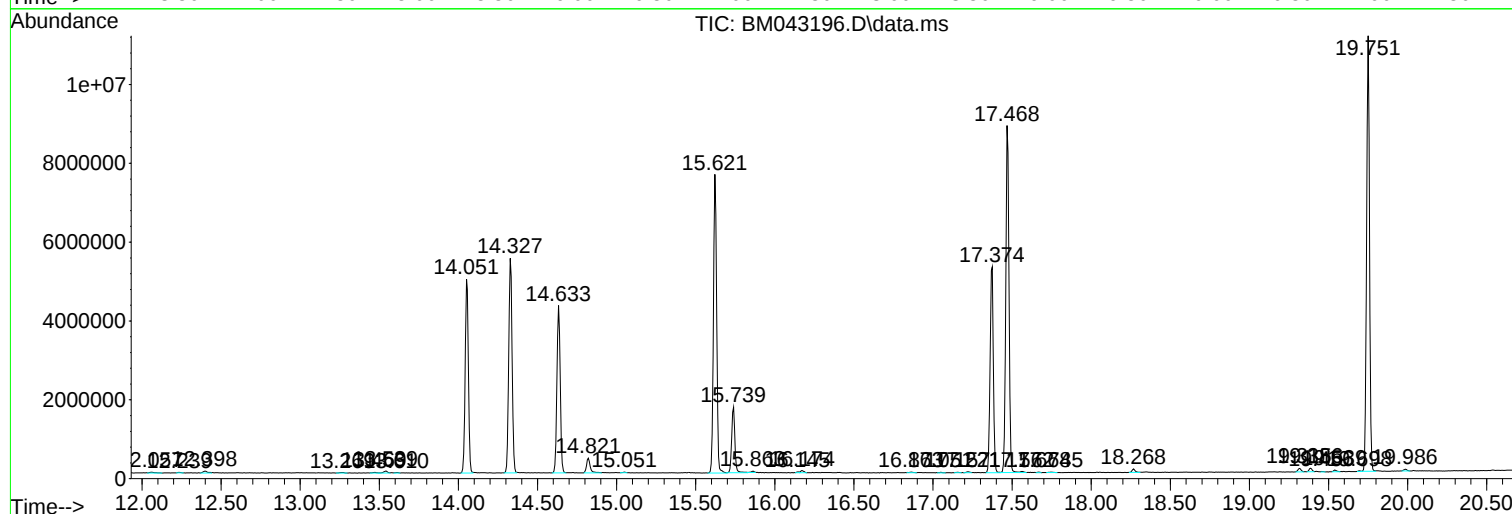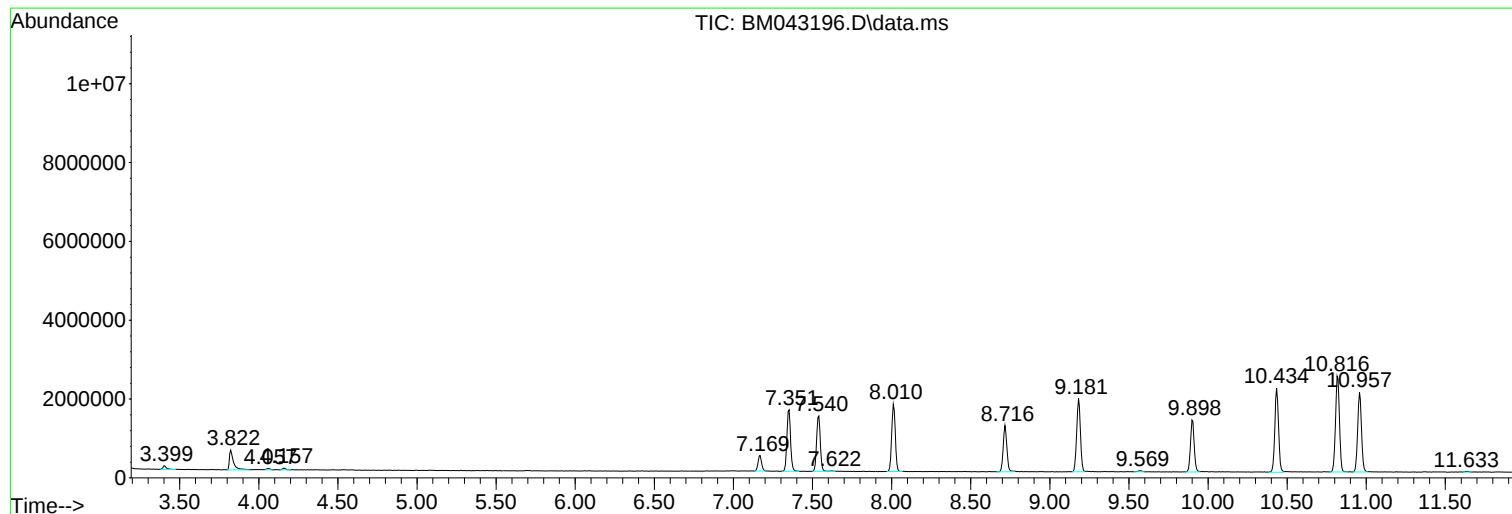

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043196.D
Acq On : 08 Dec 2023 14:55
Operator : MA/JU
Sample : 05666-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043196.D
Acq On : 08 Dec 2023 14:55
Operator : MA/JU
Sample : 05666-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc