

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043197.D
 Acq On : 08 Dec 2023 15:32
 Operator : MA/JU
 Sample : 05666-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOY33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.404	33	37	43	rVB	86975	131577	0.83%	0.095%
2	3.822	105	108	123	rBV	468123	790203	5.01%	0.568%
3	4.063	145	149	152	rVB2	35253	54139	0.34%	0.039%
4	4.157	161	165	171	rVB	164955	235937	1.49%	0.170%
5	4.487	217	221	223	rBV2	12714	16880	0.11%	0.012%
6	7.169	670	677	688	rVB	487246	801216	5.08%	0.576%
7	7.351	701	708	718	rVB	1822863	2924355	18.53%	2.101%
8	7.539	731	740	750	rBV	1679542	2708610	17.16%	1.946%
9	8.010	812	820	827	rBV	1641850	2650673	16.79%	1.905%
10	8.716	933	940	949	rBV	1416827	2242638	14.21%	1.611%
11	9.181	1011	1019	1027	rBV	2228163	3621609	22.95%	2.602%
12	9.351	1044	1048	1051	rVB4	12577	17159	0.11%	0.012%
13	9.569	1079	1085	1092	rVB3	19851	36737	0.23%	0.026%
14	9.898	1131	1141	1149	rBV	1512139	2556224	16.20%	1.837%
15	10.433	1224	1232	1240	rBV	2560038	4141986	26.24%	2.976%
16	10.816	1289	1297	1304	rBV	2405567	4107422	26.02%	2.951%
17	10.957	1313	1321	1332	rBV	2474562	4178697	26.48%	3.003%
18	11.427	1397	1401	1406	rBV	8742	18625	0.12%	0.013%
19	12.057	1507	1508	1515	rVB3	13768	16968	0.11%	0.012%
20	12.233	1535	1538	1542	rBV2	21703	29180	0.18%	0.021%
21	12.398	1560	1566	1572	rBV2	52220	83909	0.53%	0.060%
22	13.127	1686	1690	1695	rVB4	13005	19323	0.12%	0.014%
23	13.469	1744	1748	1753	rVB3	26887	38364	0.24%	0.028%
24	13.539	1755	1760	1766	rBV3	33205	54835	0.35%	0.039%
25	14.051	1839	1847	1857	rBV	5662851	7799761	49.42%	5.605%
26	14.327	1886	1894	1907	rVB	6222554	9381599	59.44%	6.741%
27	14.539	1926	1930	1934	rVB3	10226	18123	0.11%	0.013%
28	14.633	1939	1946	1955	rBV	4289520	6024096	38.17%	4.329%
29	14.821	1971	1978	1988	rBV	452548	709966	4.50%	0.510%
30	15.051	2013	2017	2021	rVB3	24706	41917	0.27%	0.030%
31	15.621	2106	2114	2121	rBV	8346144	11929877	75.59%	8.572%
32	15.668	2121	2122	2127	rVV3	18490	21314	0.14%	0.015%
33	15.739	2127	2134	2149	rVV	1927322	2660576	16.86%	1.912%
34	15.862	2149	2155	2162	rVB3	36735	70533	0.45%	0.051%
35	16.780	2306	2311	2314	rBV4	9315	15829	0.10%	0.011%
36	17.057	2354	2358	2360	rVB3	14156	18892	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043197.D
 Acq On : 08 Dec 2023 15:32
 Operator : MA/JU
 Sample : 05666-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0Y33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

37	17.180	2370	2379	2384	rBV2	73284	122368	0.78%	0.088%
38	17.368	2404	2411	2422	rBV	5022256	7301872	46.26%	5.247%
39	17.468	2422	2428	2439	rBV	9788037	13834741	87.65%	9.941%
40	17.668	2457	2462	2467	rBV4	11092	21399	0.14%	0.015%
41	17.745	2470	2475	2480	rBV5	15897	30479	0.19%	0.022%
42	18.268	2554	2564	2570	rBV2	163027	256826	1.63%	0.185%
43	18.339	2574	2576	2582	rVB2	14664	23873	0.15%	0.017%
44	19.315	2737	2742	2748	rVB	99852	147108	0.93%	0.106%
45	19.386	2749	2754	2758	rBV	106595	141457	0.90%	0.102%
46	19.539	2777	2780	2786	rBV3	88045	112184	0.71%	0.081%
47	19.698	2804	2807	2809	rBV4	23763	20840	0.13%	0.015%
48	19.750	2809	2816	2824	rVV	12329148	15783311	100.00%	11.341%
49	19.986	2852	2856	2862	rVB	67073	95509	0.61%	0.069%
50	21.103	3043	3046	3048	rBV3	28375	31421	0.20%	0.023%
51	21.256	3069	3072	3079	rBV4	101907	157682	1.00%	0.113%
52	21.533	3113	3119	3128	rBV	6090368	7624309	48.31%	5.479%
53	22.821	3335	3338	3345	rVB	120738	176172	1.12%	0.127%
54	23.780	3492	3501	3514	rBV2	7723784	15288942	96.87%	10.986%
55	23.933	3519	3527	3539	rVB	3877022	7825617	49.58%	5.623%




Sum of corrected areas: 139165859

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043197.D
Acq On : 08 Dec 2023 15:32
Operator : MA/JU
Sample : 05666-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

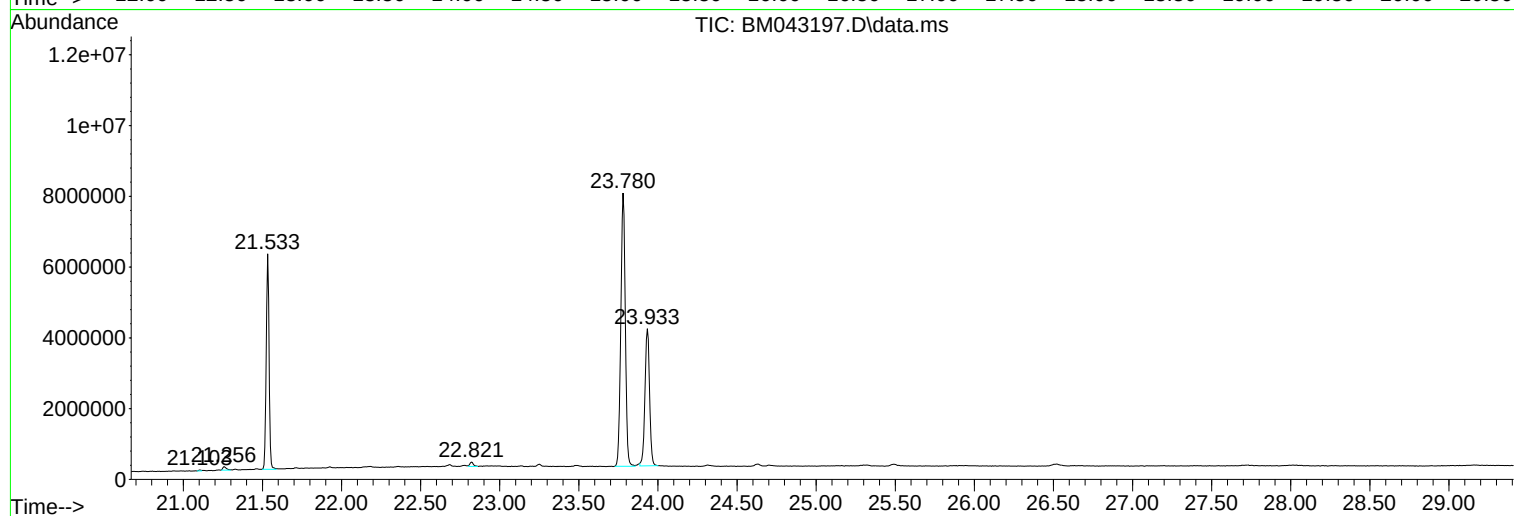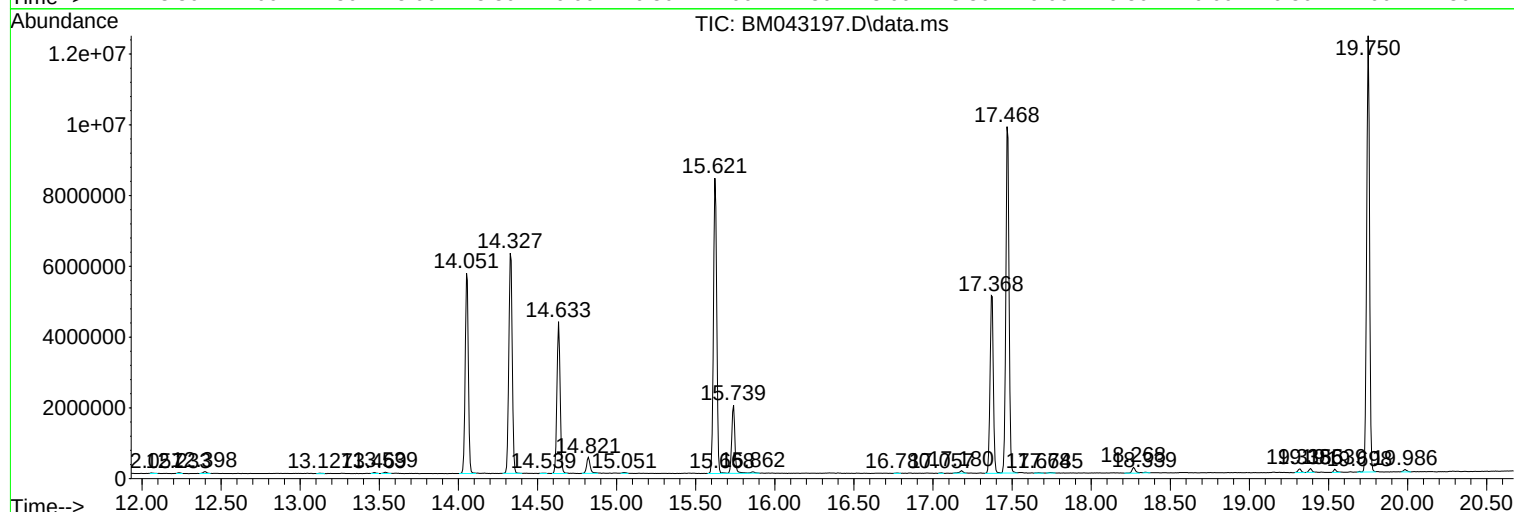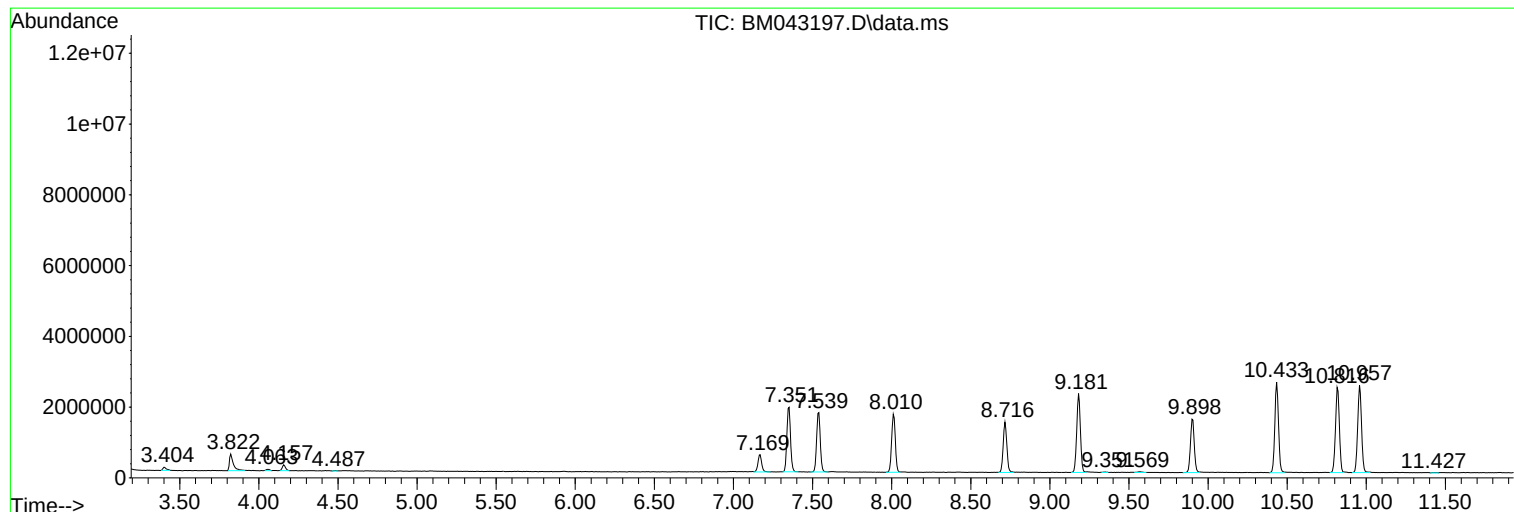

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043197.D
Acq On : 08 Dec 2023 15:32
Operator : MA/JU
Sample : 05666-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043197.D
Acq On : 08 Dec 2023 15:32
Operator : MA/JU
Sample : 05666-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc