

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043199.D
 Acq On : 08 Dec 2023 16:44
 Operator : MA/JU
 Sample : 05666-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOY43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	33	36	45	rVB2	76215	125599	0.84%	0.099%
2	3.822	104	108	122	rBV	323640	562847	3.77%	0.446%
3	4.063	144	149	153	rVB2	30823	52536	0.35%	0.042%
4	4.157	162	165	171	rVB3	32680	43038	0.29%	0.034%
5	7.169	670	677	686	rVB	348883	591815	3.96%	0.469%
6	7.351	700	708	716	rBV	1523320	2488236	16.66%	1.971%
7	7.539	733	740	749	rBV	1346925	2188117	14.65%	1.733%
8	8.010	812	820	828	rBV	1621671	2593649	17.37%	2.054%
9	8.716	932	940	948	rBV	1105275	1729053	11.58%	1.369%
10	9.181	1011	1019	1028	rBV	1860171	3043939	20.38%	2.411%
11	9.898	1132	1141	1153	rBV	1243008	2117541	14.18%	1.677%
12	10.433	1224	1232	1240	rBV	2111958	3405873	22.80%	2.698%
13	10.816	1290	1297	1309	rBV	2370736	4003425	26.80%	3.171%
14	10.957	1312	1321	1334	rBV	1992553	3353237	22.45%	2.656%
15	11.463	1406	1407	1414	rVB3	10438	19314	0.13%	0.015%
16	12.398	1560	1566	1573	rVB2	46774	79953	0.54%	0.063%
17	12.810	1633	1636	1642	rBV3	7219	15334	0.10%	0.012%
18	13.474	1745	1749	1754	rBV5	16042	21830	0.15%	0.017%
19	13.539	1754	1760	1764	rBV2	37639	59666	0.40%	0.047%
20	14.051	1841	1847	1862	rBV	4962742	6845019	45.83%	5.422%
21	14.168	1862	1867	1869	rBV5	12594	18553	0.12%	0.015%
22	14.327	1887	1894	1902	rBV	5465555	7886250	52.80%	6.246%
23	14.633	1939	1946	1954	rBV	4032698	5822378	38.98%	4.612%
24	14.821	1971	1978	1991	rBV2	349188	564015	3.78%	0.447%
25	15.045	2010	2016	2020	rVB6	20280	37362	0.25%	0.030%
26	15.621	2103	2114	2121	rBV	7603954	10642335	71.25%	8.429%
27	15.739	2127	2134	2143	rBV	1745133	2472242	16.55%	1.958%
28	15.857	2150	2154	2161	rVB2	31572	57621	0.39%	0.046%
29	16.404	2244	2247	2251	rVB4	11983	17747	0.12%	0.014%
30	16.839	2316	2321	2326	rBV5	17843	25915	0.17%	0.021%
31	16.968	2336	2343	2347	rBV4	40973	68592	0.46%	0.054%
32	17.045	2352	2356	2363	rVB3	13251	21370	0.14%	0.017%
33	17.162	2369	2376	2377	rBV3	11779	20225	0.14%	0.016%
34	17.368	2405	2411	2418	rBV	4942503	7017012	46.98%	5.558%
35	17.468	2421	2428	2440	rBV	9479524	12969306	86.83%	10.272%
36	17.745	2468	2475	2479	rBV5	16333	34206	0.23%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
 Data File : BM043199.D
 Acq On : 08 Dec 2023 16:44
 Operator : MA/JU
 Sample : 05666-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0Y43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

37	18.268	2559	2564	2571	rBV3	154826	225093	1.51%	0.178%
38	18.345	2575	2577	2581	rVB3	14957	16178	0.11%	0.013%
39	18.545	2607	2611	2617	rBV4	24480	32598	0.22%	0.026%
40	19.150	2711	2714	2719	rVB3	15622	22517	0.15%	0.018%
41	19.315	2738	2742	2748	rBV3	100954	142012	0.95%	0.112%
42	19.386	2749	2754	2758	rBV	101938	141001	0.94%	0.112%
43	19.456	2764	2766	2770	rVB2	14713	17271	0.12%	0.014%
44	19.539	2776	2780	2784	rBV3	75035	100835	0.68%	0.080%
45	19.639	2793	2797	2798	rBV2	13418	15619	0.10%	0.012%
46	19.697	2804	2807	2809	rBV2	17435	19697	0.13%	0.016%
47	19.750	2809	2816	2825	rVV	11315149	14936020	100.00%	11.830%
48	19.986	2851	2856	2862	rVB	90142	118831	0.80%	0.094%
49	21.256	3068	3072	3076	rBV2	75509	100778	0.67%	0.080%
50	21.533	3113	3119	3129	rBV	5922506	7385991	49.45%	5.850%
51	23.780	3493	3501	3515	rBV	7548660	14374120	96.24%	11.385%
52	23.932	3519	3527	3539	rVB	3802241	7590668	50.82%	6.012%




Sum of corrected areas: 126254379

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043199.D
Acq On : 08 Dec 2023 16:44
Operator : MA/JU
Sample : 05666-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

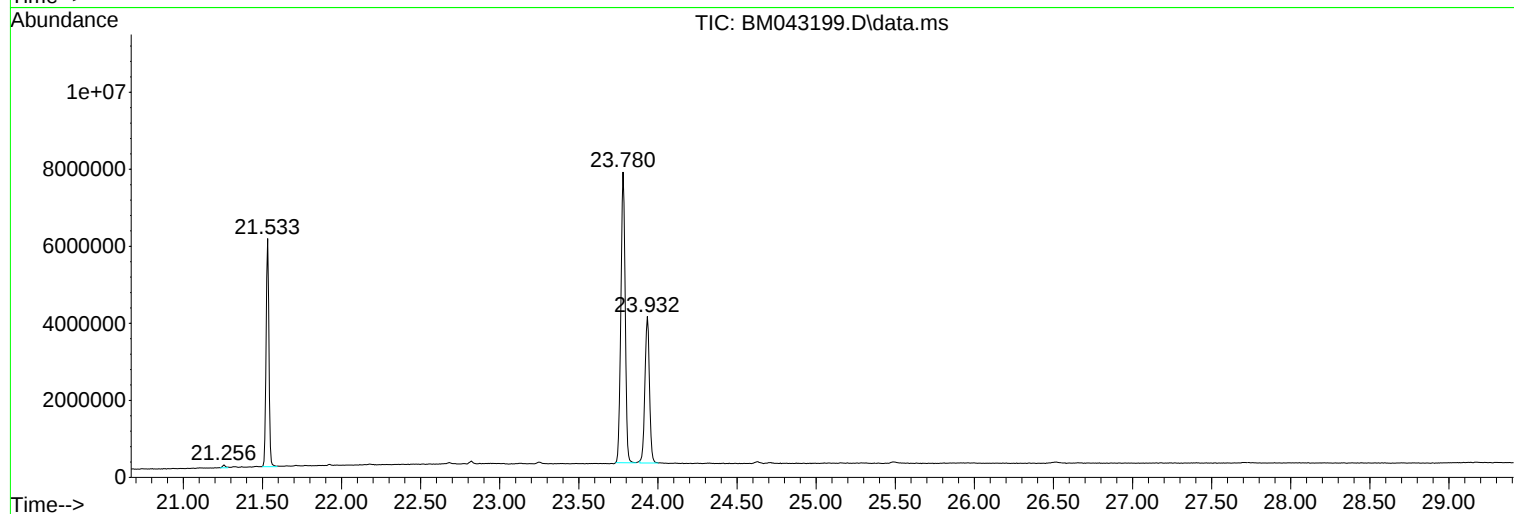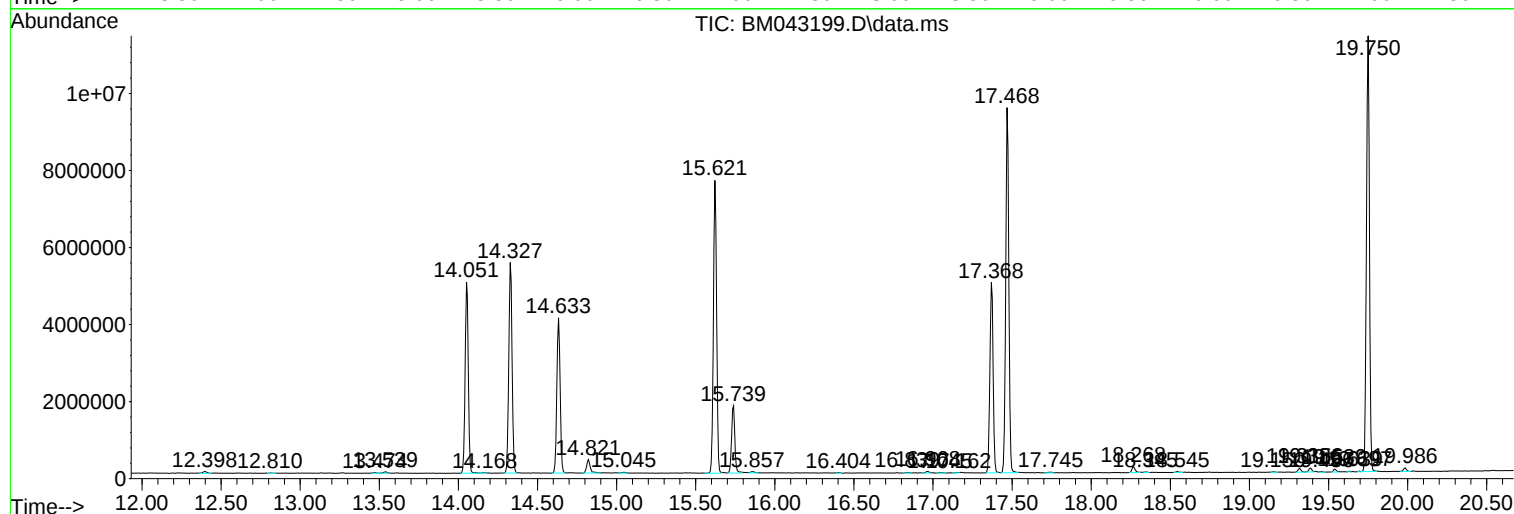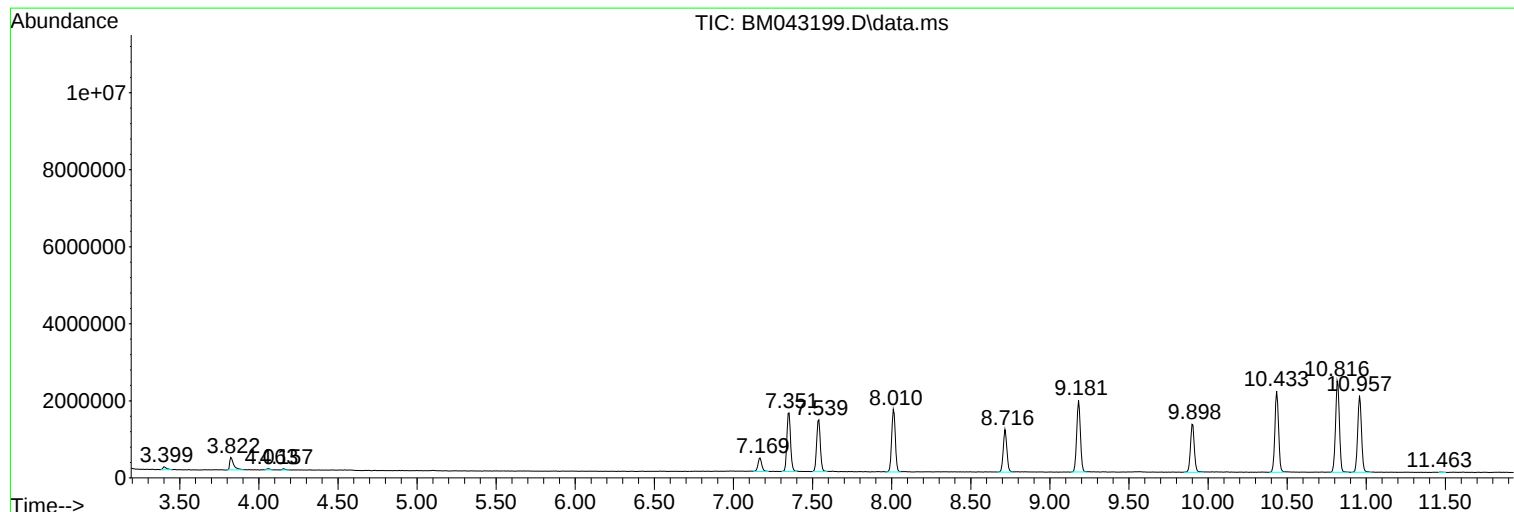

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043199.D
Acq On : 08 Dec 2023 16:44
Operator : MA/JU
Sample : 05666-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120823\
Data File : BM043199.D
Acq On : 08 Dec 2023 16:44
Operator : MA/JU
Sample : 05666-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0Y43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc