

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120915\  
 Data File : BM003445.D  
 Acq On : 10 Dec 2015 10:41  
 Operator : UM/IZ  
 Sample : G4690-07  
 Misc :  
 ALS Vial : 32 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :

Quant Time: Dec 10 11:26:56 2015  
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 09 18:52:47 2015  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|-------|------|----------|--------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 7.72  | 152  | 76490    | 20.00  | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.51 | 136  | 352221   | 20.00  | ng    | 0.00     |
| 38) Acenaphthene-d10        | 14.37 | 164  | 218930   | 20.00  | ng    | 0.00     |
| 63) Phenanthrene-d10        | 17.12 | 188  | 516886   | 20.00  | ng    | 0.00     |
| 75) Chrysene-d12            | 21.32 | 240  | 498680   | 20.00  | ng    | 0.00     |
| 86) Perylene-d12            | 23.57 | 264  | 404178   | 20.00  | ng    | 0.00     |
| System Monitoring Compounds |       |      |          |        |       |          |
| 5) 2-Fluorophenol           | 5.30  | 112  | 275531   | 64.04  | ng    | 0.00     |
| 7) Phenol-d6                | 6.89  | 99   | 240365   | 40.23  | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 8.88  | 82   | 495058   | 87.15  | ng    | 0.00     |
| 41) 2,4,6-Tribromophenol    | 15.87 | 330  | 327009   | 149.56 | ng    | 0.00     |
| 44) 2-Fluorobiphenyl        | 12.99 | 172  | 1316754  | 81.94  | ng    | 0.00     |
| 78) Terphenyl-d14           | 19.76 | 244  | 1818249  | 85.99  | ng    | 0.00     |


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120915\  
Data File : BM003445.D  
Acq On : 10 Dec 2015 10:41  
Operator : UM/IZ  
Sample : G4690-07  
Misc :  
ALS Vial : 32 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :

Quant Time: Dec 10 11:26:56 2015  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 09 18:52:47 2015  
Response via : Initial Calibration

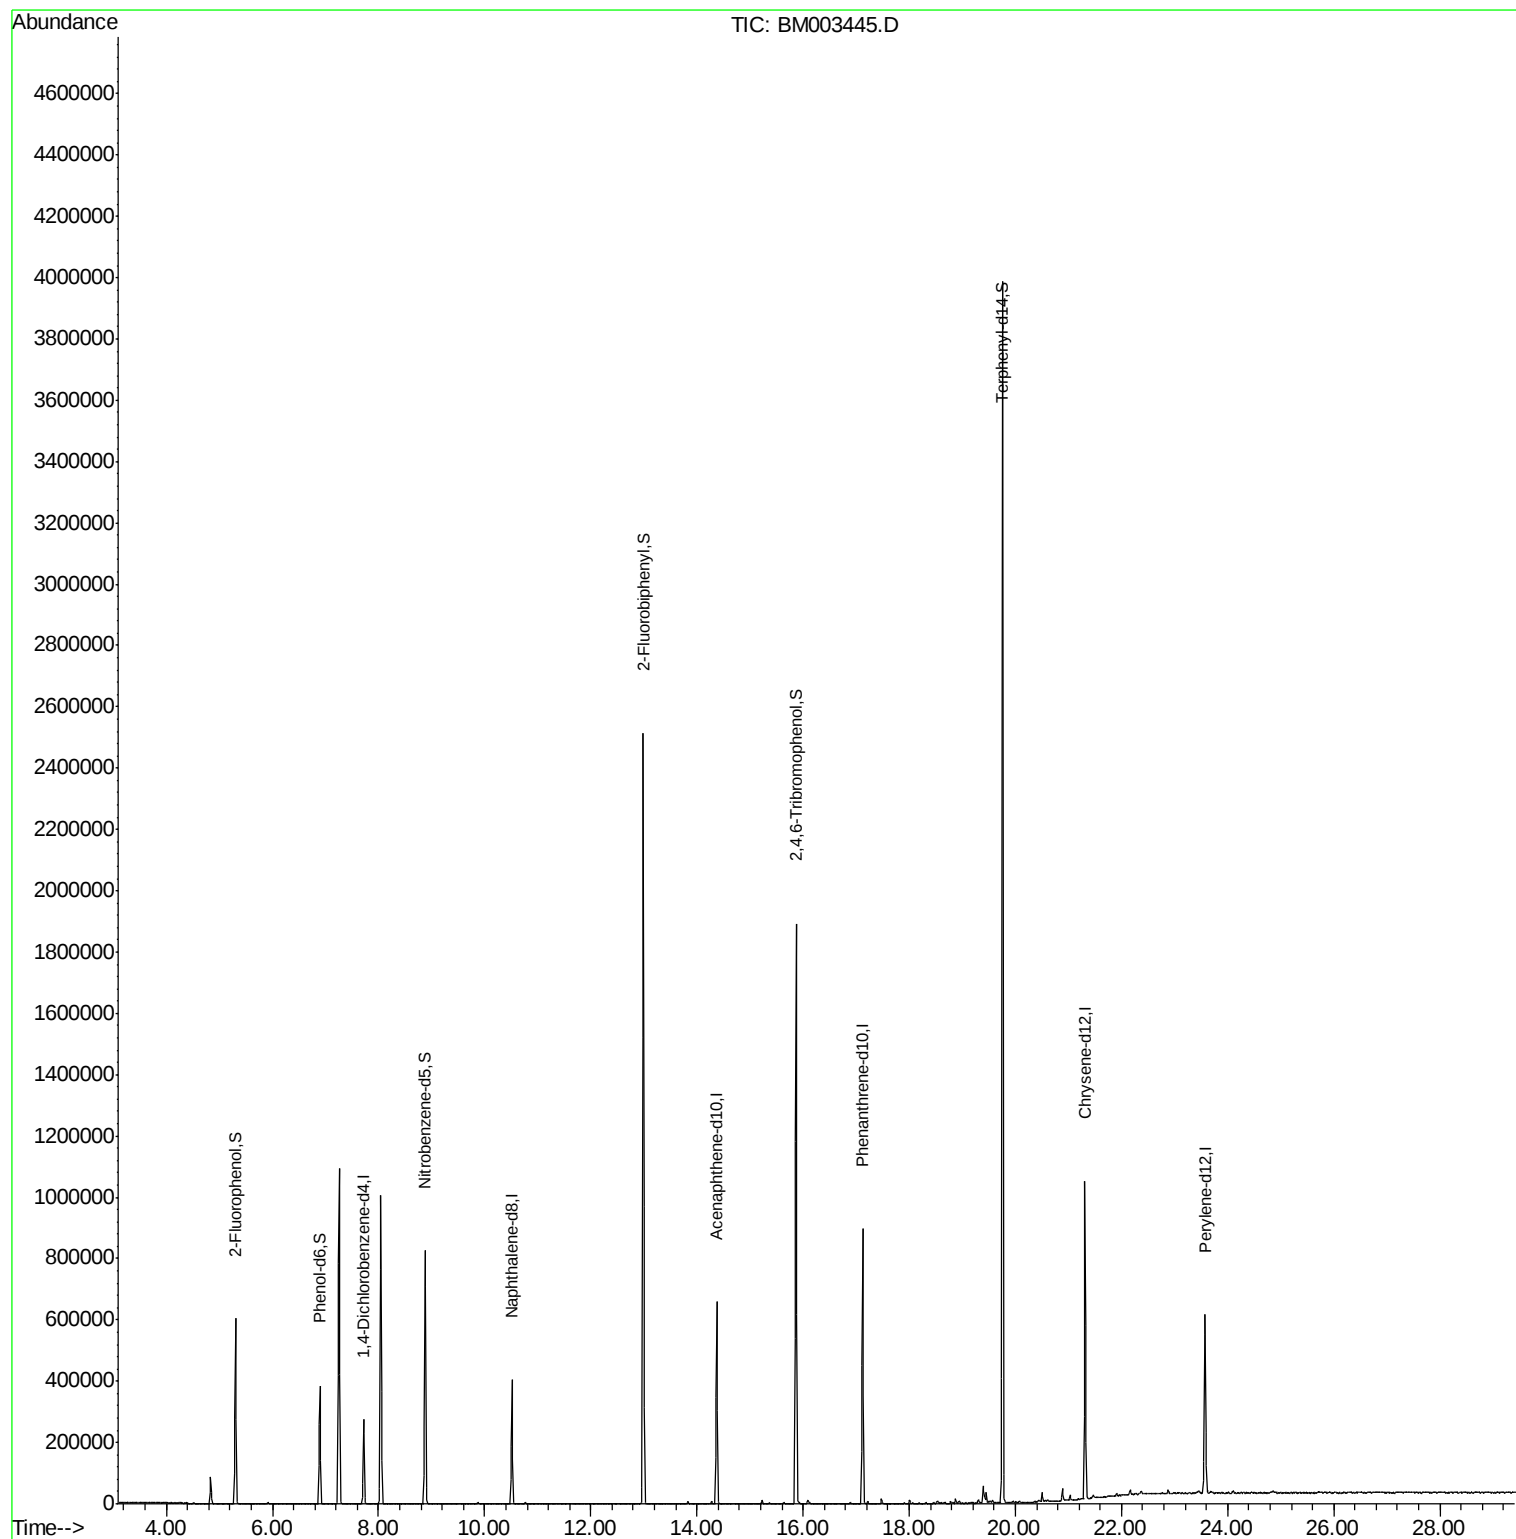

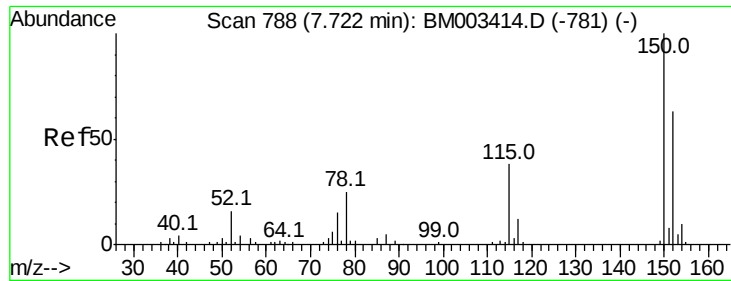


#1




1,4-Dichlorobenzene-d4  
Concen: 20.00 ng  
RT: 7.72 min Scan# 788  
Delta R.T. -0.00 min  
Lab File: BM003445.D  
Acq: 10 Dec 2015 10:41

Instrument :  
BNA\_M  
ClientSampleId :

Tot Ion:152 Resp: 76490  
Ion Ratio Lower Upper  
152 100  
150 160.7 119.5 179.3  
115 59.2 43.0 64.4

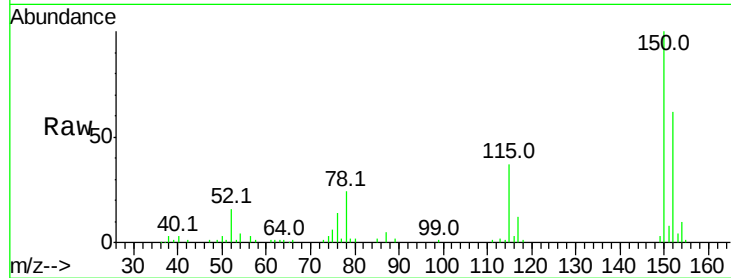


Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

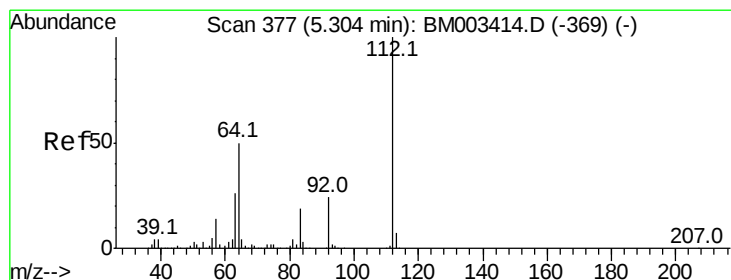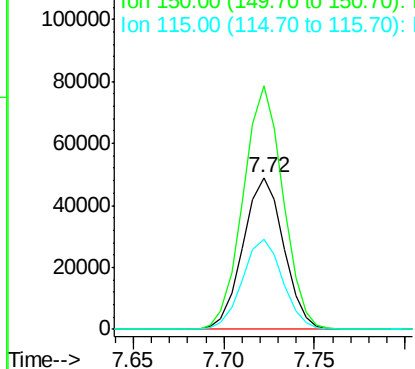



#5


2-Fluorophenol  
Concen: 64.04 ng  
RT: 5.30 min Scan# 377  
Delta R.T. 0.00 min  
Lab File: BM003445.D  
Acq: 10 Dec 2015 10:41

Tgt Ion:112 Resp: 275531  
Ion Ratio Lower Upper  
112 100  
64 49.5 38.6 57.8  
63 25.7 19.3 28.9

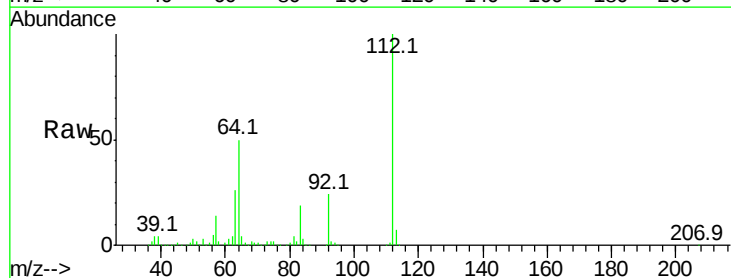

Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BM0  
Ion 63.00 (62.70 to 63.70): BM0

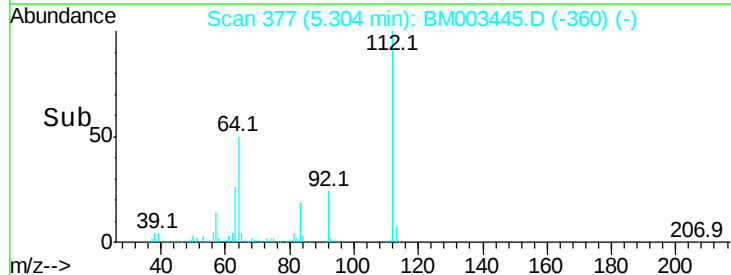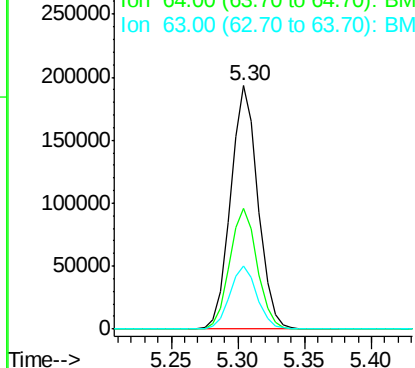



#7

Phenol-d6

Concen: 40.23 ng

RT: 6.89 min Scan# 647

Delta R.T. -0.00 min

Lab File: BM003445.D

Acq: 10 Dec 2015 10:41

Instrument :

BNA\_M

ClientSampleId :





Tot Ion: 99 Resp: 240365

Ion Ratio Lower Upper

99 100

42 13.1 11.0 16.4

71 32.0 23.4 35.2

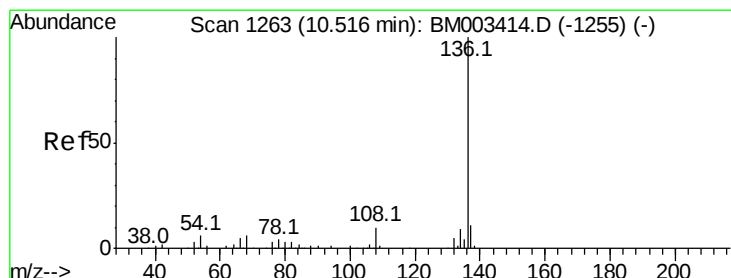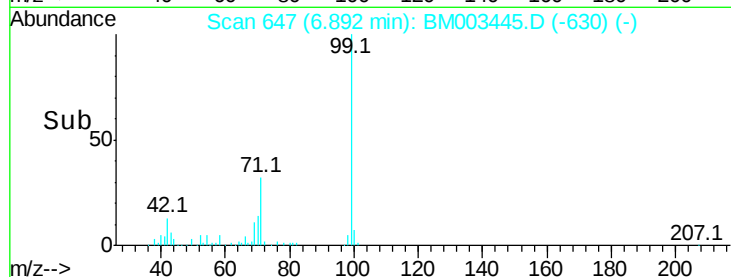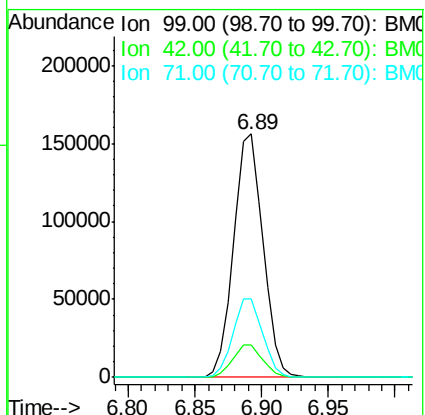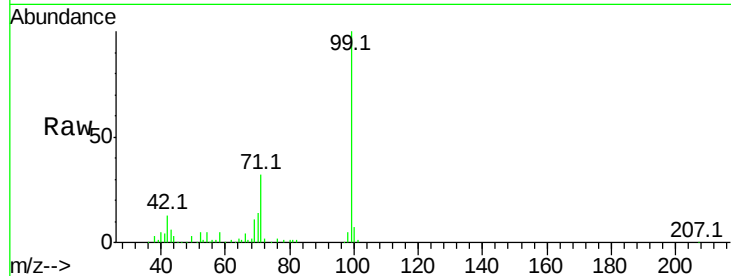

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.51 min Scan# 1262

Delta R.T. -0.01 min

Lab File: BM003445.D

Acq: 10 Dec 2015 10:41

Tgt Ion: 136 Resp: 352221




Ion Ratio Lower Upper


136 100

137 10.8 8.7 13.1

54 5.8 4.6 6.8

68 5.5 3.7 5.5



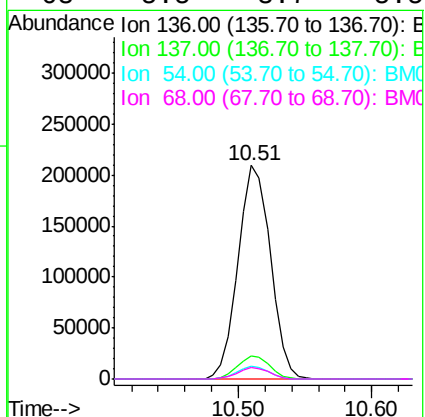
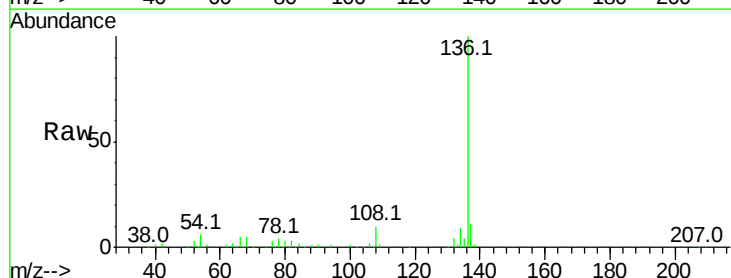




#23  
 Nitrobenzene-d5  
 Concen: 87.15 ng  
 RT: 8.88 min Scan# 985  
 Delta R.T. -0.00 min  
 Lab File: BM003445.D  
 Acq: 10 Dec 2015 10:41




Instrument :  
 BNA\_M  
 ClientSampled :


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 82      | 100   |       |       |
| 128     | 47.2  | 32.8  | 49.2  |
| 54      | 39.8  | 40.6  | 60.8  |

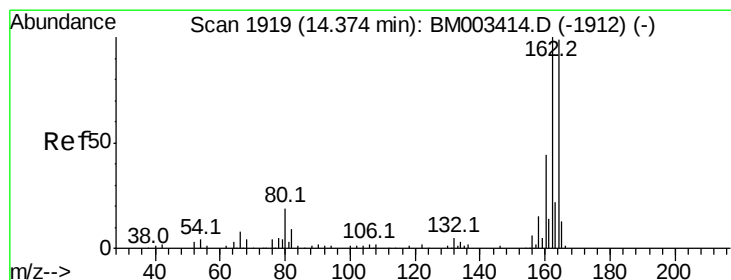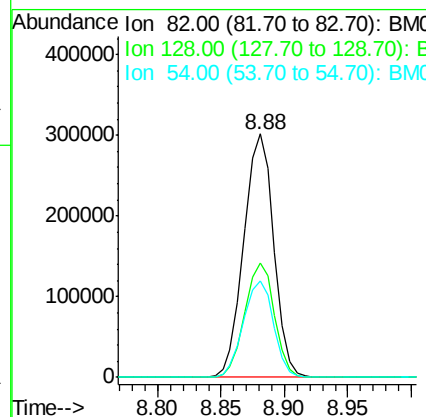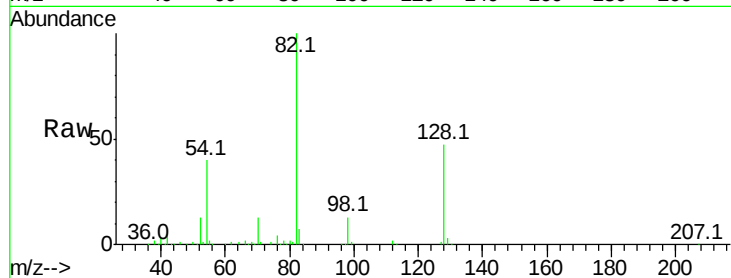

#38  
 Acenaphthene-d10  
 Concen: 20.00 ng  
 RT: 14.37 min Scan# 1919  
 Delta R.T. -0.00 min  
 Lab File: BM003445.D  
 Acq: 10 Dec 2015 10:41

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 164     | 100   |       |       |
| 162     | 101.3 | 82.4  | 123.6 |
| 160     | 45.4  | 35.8  | 53.6  |



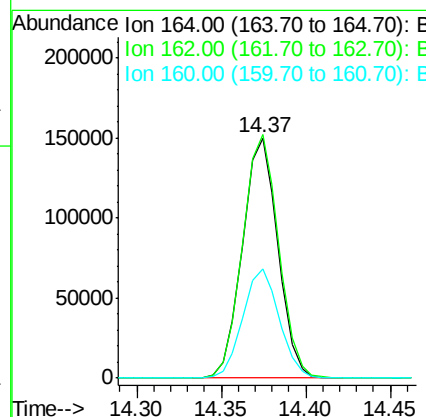
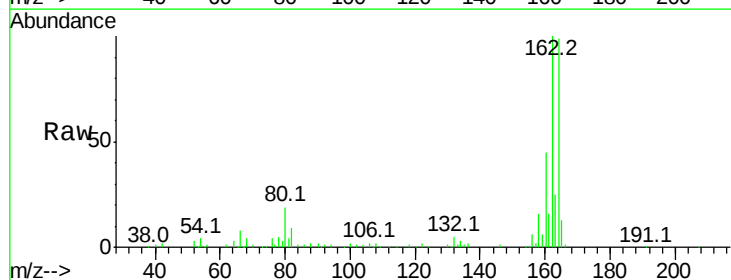




#41  
 2,4,6-Tribromophenol  
 Concen: 149.56 ng  
 RT: 15.87 min Scan# 2173  
 Delta R.T. -0.00 min  
 Lab File: BM003445.D  
 Acq: 10 Dec 2015 10:41




Instrument :  
 BNA\_M  
 ClientSampleId :


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 330     | 100   |       |       |
| 332     | 96.7  | 0.0   | 0.0#  |
| 141     | 43.2  | 0.0   | 0.0#  |

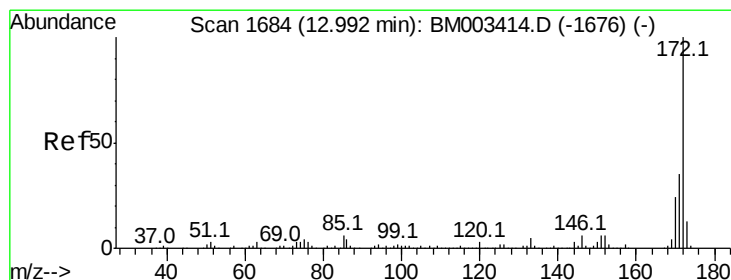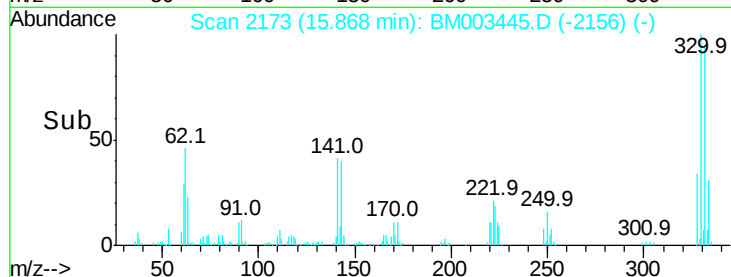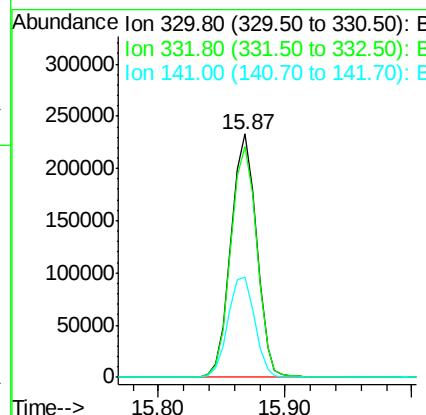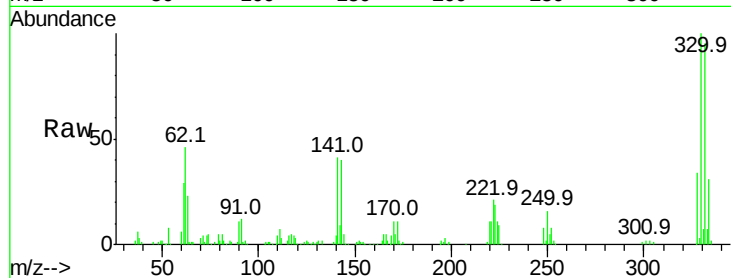

#44  
 2-Fluorobiphenyl  
 Concen: 81.94 ng  
 RT: 12.99 min Scan# 1684  
 Delta R.T. -0.00 min  
 Lab File: BM003445.D  
 Acq: 10 Dec 2015 10:41

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 172     | 100   |       |       |
| 171     | 35.1  | 28.5  | 42.7  |
| 170     | 23.5  | 18.8  | 28.2  |

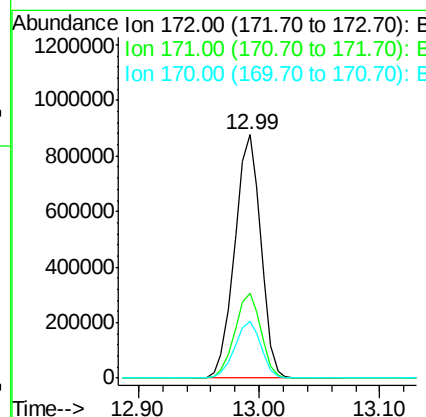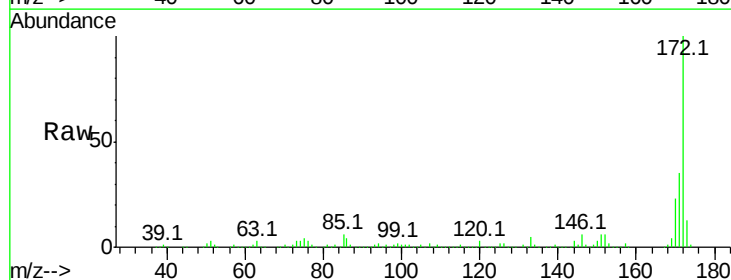







#63  
Phenanthrene-d10  
Concen: 20.00 ng  
RT: 17.12 min Scan# 2386  
Delta R.T. -0.00 min  
Lab File: BM003445.D  
Acq: 10 Dec 2015 10:41

Instrument :  
BNA\_M  
ClientSampled :

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 188     | 100   |       |       |
| 94      | 8.9   | 8.7   | 13.1  |
| 80      | 9.6   | 9.3   | 13.9  |

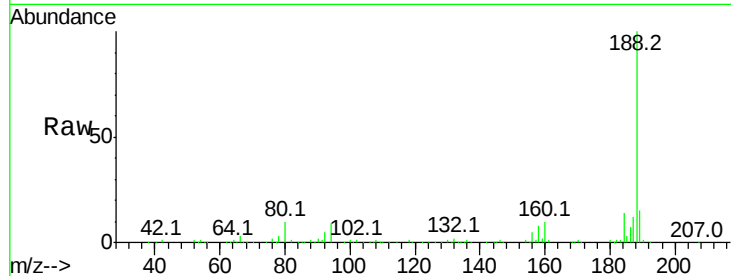


Abundance Ion 188.00 (187.70 to 188.70): E  
Ion 94.00 (93.70 to 94.70): BM  
Ion 80.00 (79.70 to 80.70): BM

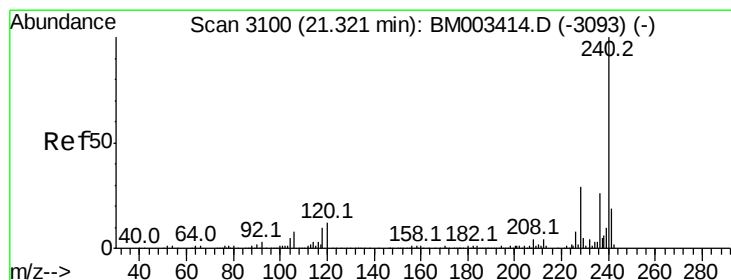
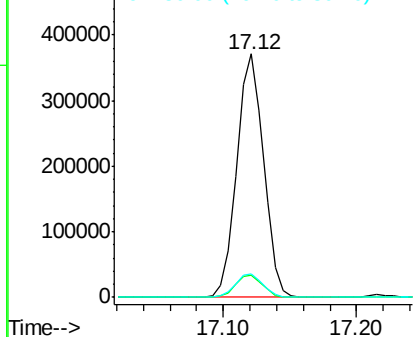



#75  
Chrysene-d12  
Concen: 20.00 ng  
RT: 21.32 min Scan# 3099  
Delta R.T. -0.01 min  
Lab File: BM003445.D  
Acq: 10 Dec 2015 10:41

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 240     | 100   |       |       |
| 120     | 12.1  | 8.2   | 12.2  |
| 236     | 26.3  | 20.0  | 30.0  |

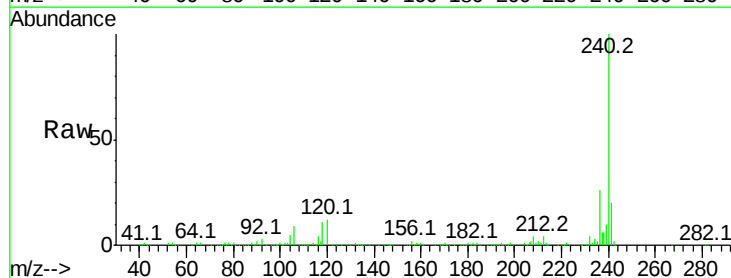

Abundance Ion 240.00 (239.70 to 240.70): E  
Ion 120.00 (119.70 to 120.70): E  
Ion 236.00 (235.70 to 236.70): E

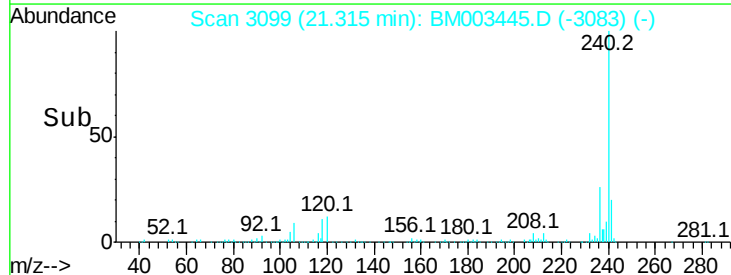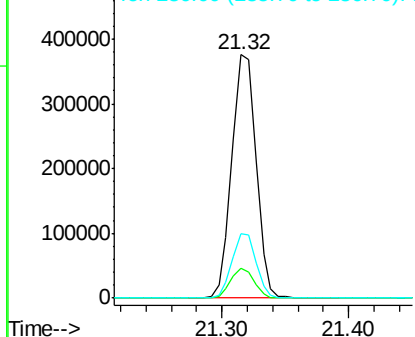

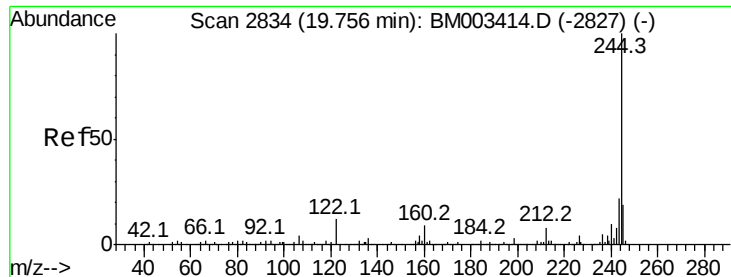

#78

Terphenyl-d14

Concen: 85.99 ng

RT: 19.76 min Scan# 2834

Delta R.T. -0.00 min

Lab File: BM003445.D

Acq: 10 Dec 2015 10:41

Instrument :

BNA\_M

ClientSampleId :


Tot Ion:244 Resp: 1818249

Ion Ratio Lower Upper

244 100

212 8.2 4.9 7.3#




122 11.6 6.2 9.4#

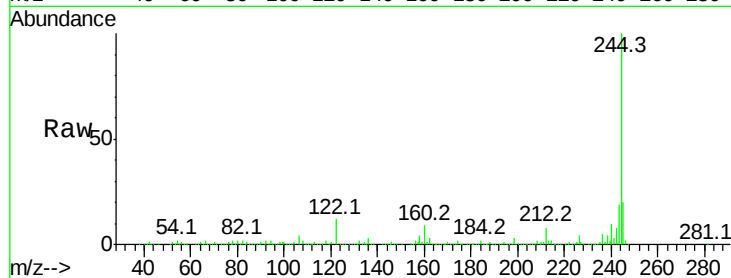

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

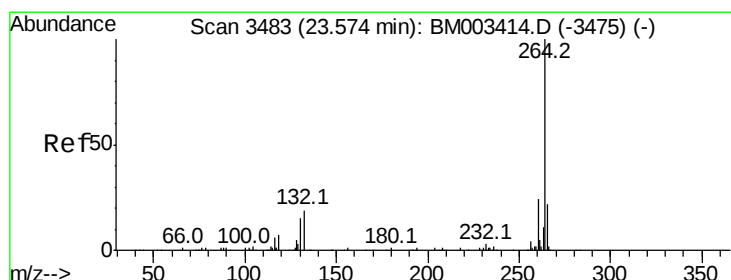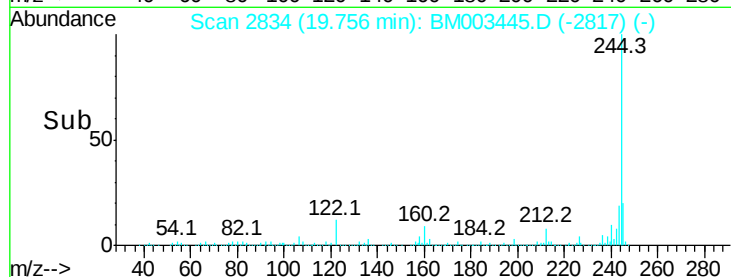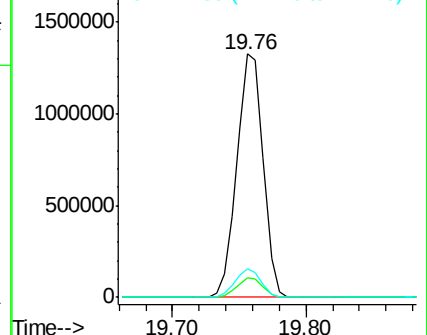

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.57 min Scan# 3483

Delta R.T. -0.00 min

Lab File: BM003445.D

Acq: 10 Dec 2015 10:41


Tgt Ion:264 Resp: 404178

Ion Ratio Lower Upper

264 100

260 23.6 18.6 27.8

265 21.0 17.3 25.9

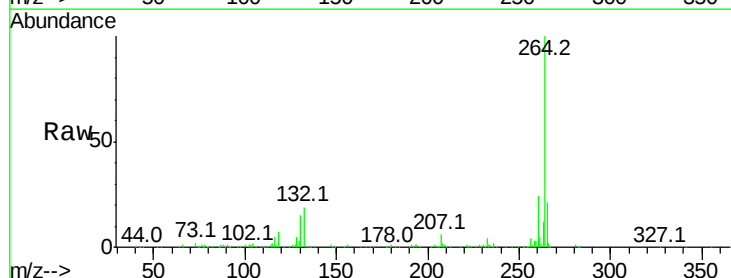

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

