

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120915\
 Data File : BM003439.D
 Acq On : 10 Dec 2015 07:06
 Operator : UM/IZ
 Sample : G4690-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 10 11:25:49 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 18:52:47 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	70054	20.00	ng	0.00
21) Naphthalene-d8	10.51	136	289757	20.00	ng	0.00
38) Acenaphthene-d10	14.37	164	186879	20.00	ng	0.00
63) Phenanthrene-d10	17.12	188	307271	20.00	ng	0.00
75) Chrysene-d12	21.32	240	330673	20.00	ng	0.00
86) Perylene-d12	23.57	264	327835	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	227019	57.62	ng	0.00
7) Phenol-d6	6.89	99	175967	32.16	ng	0.00
23) Nitrobenzene-d5	8.88	82	413687	88.52	ng	0.00
41) 2,4,6-Tribromophenol	15.87	330	200812	107.60	ng	0.00
44) 2-Fluorobiphenyl	12.99	172	926125	67.52	ng	0.00
78) Terphenyl-d14	19.76	244	822012	58.62	ng	0.00
Target Compounds						
49) Dimethylphthalate	13.83	163	50771	3.30	ng	Qvalue # 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120915\
Data File : BM003439.D
Acq On : 10 Dec 2015 07:06
Operator : UM/IZ
Sample : G4690-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 10 11:25:49 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

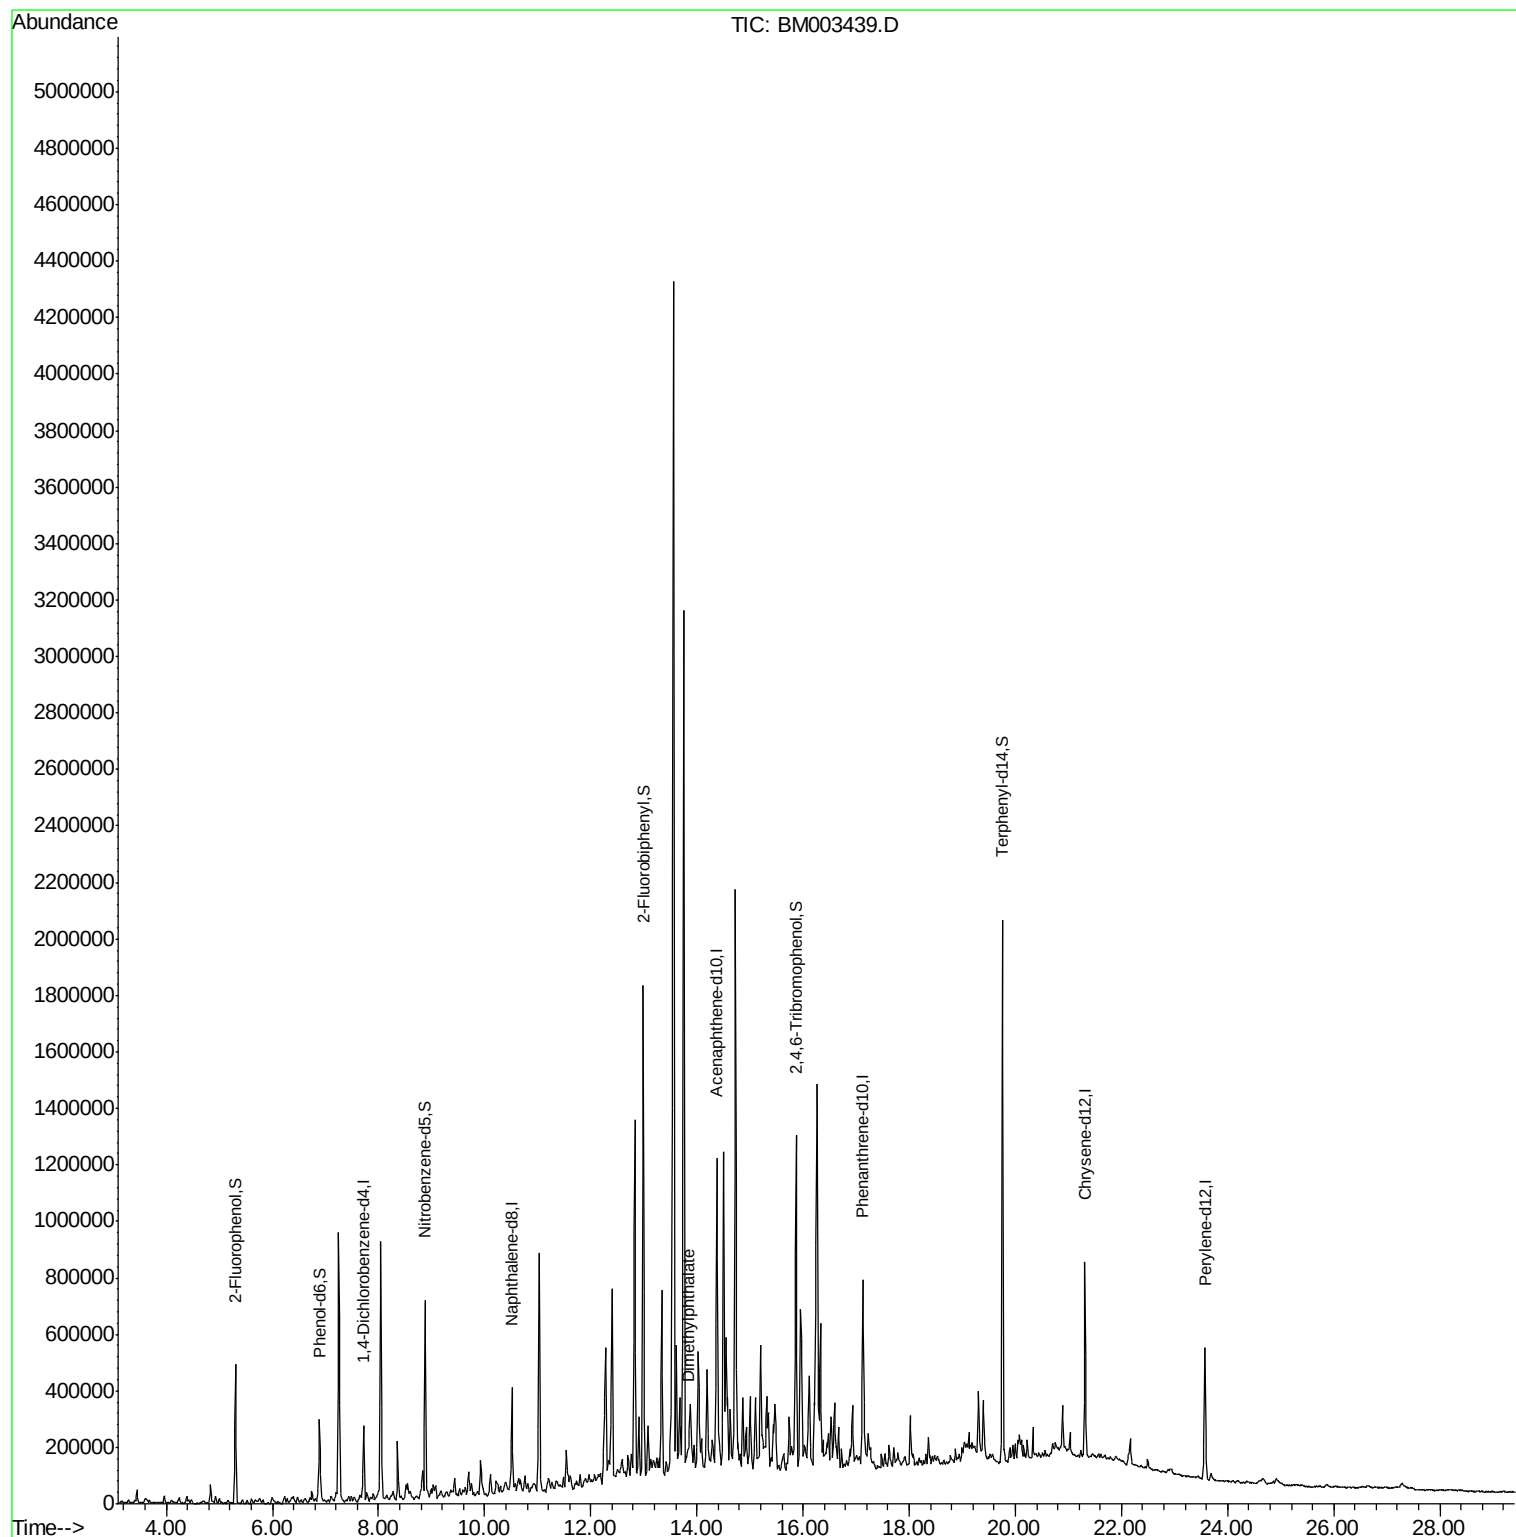

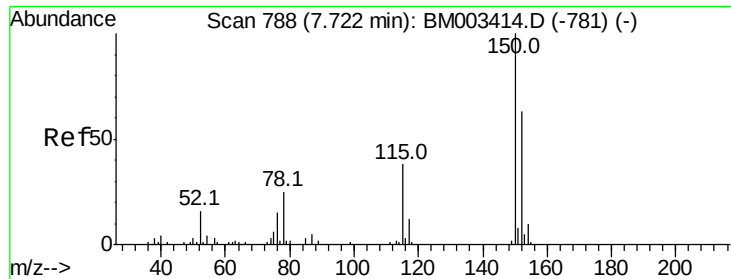


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.72 min Scan# 788
Delta R.T. -0.00 min
Lab File: BM003439.D
Acq: 10 Dec 2015 07:06

Instrument :
BNA_M
ClientSampleId :

Tot Ion:152 Resp: 70054
Ion Ratio Lower Upper
152 100
150 155.2 119.5 179.3
115 59.4 43.0 64.4

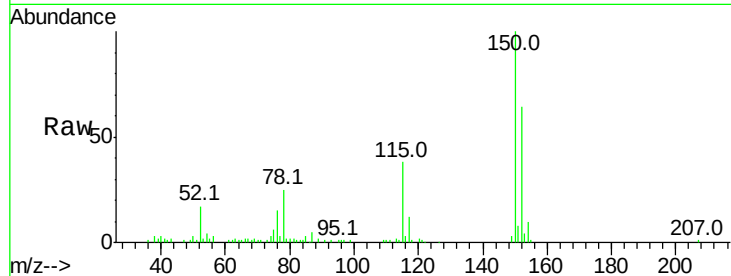


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

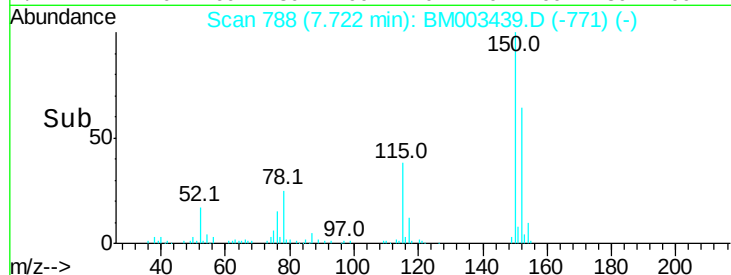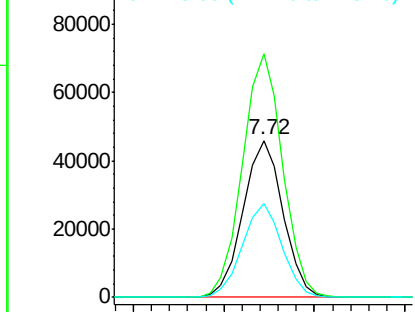



#5


2-Fluorophenol
Concen: 57.62 ng
RT: 5.30 min Scan# 377
Delta R.T. 0.00 min
Lab File: BM003439.D
Acq: 10 Dec 2015 07:06

Tgt Ion:112 Resp: 227019
Ion Ratio Lower Upper
112 100
64 49.4 38.6 57.8
63 25.8 19.3 28.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

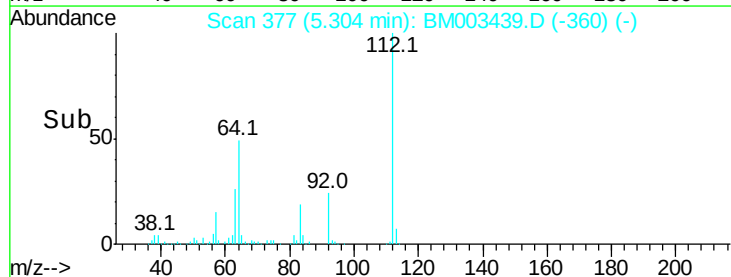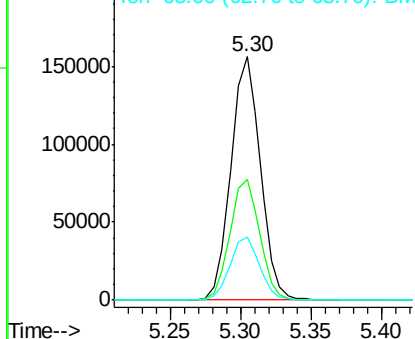

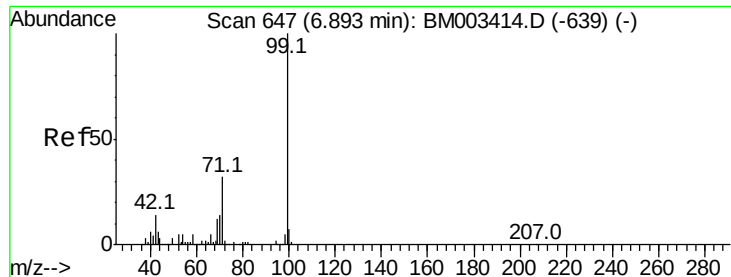

#7

Phenol-d6

Concen: 32.16 ng

RT: 6.89 min Scan# 646

Delta R.T. -0.01 min

Lab File: BM003439.D

Acq: 10 Dec 2015 07:06


Instrument :

BNA_M

ClientSampled :

Tot Ion: 99 Resp: 175967

Ion	Ratio	Lower	Upper
99	100		
42	13.9	11.0	16.4
71	33.2	23.4	35.2






Abundance

Ion 99.00 (98.70 to 99.70): BM003414.D (-639) (-)

Ion 42.00 (41.70 to 42.70): BM003414.D (-639) (-)

Ion 71.00 (70.70 to 71.70): BM003414.D (-639) (-)

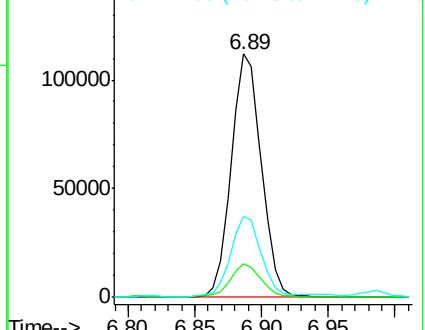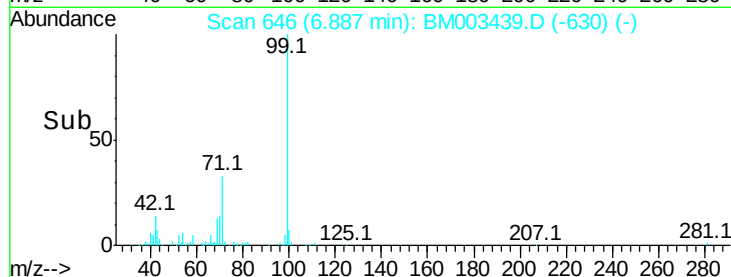

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.51 min Scan# 1262


Delta R.T. -0.01 min

Lab File: BM003439.D

Acq: 10 Dec 2015 07:06

Tgt Ion: 136 Resp: 289757

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.7	13.1
54	6.4	4.6	6.8
68	6.2	3.7	5.5





Abundance


Ion 136.00 (135.70 to 136.70): BM003414.D (-1255) (-)

Ion 137.00 (136.70 to 137.70): BM003414.D (-1255) (-)

Ion 54.00 (53.70 to 54.70): BM003414.D (-1255) (-)

Ion 68.00 (67.70 to 68.70): BM003414.D (-1255) (-)

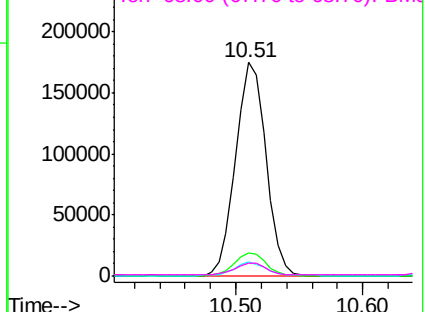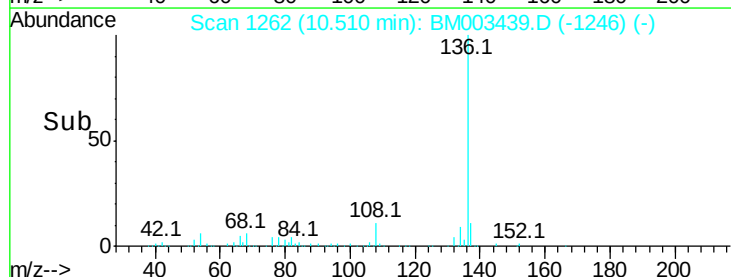

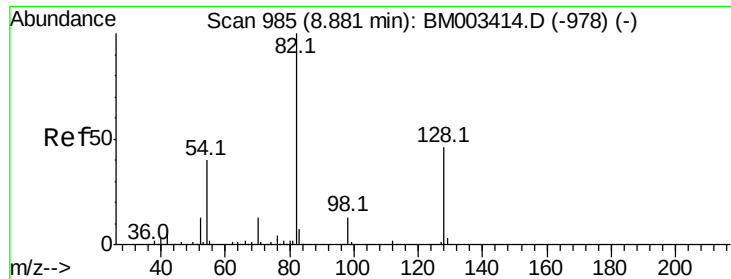

#23

Nitrobenzene-d5

Concen: 88.52 ng

RT: 8.88 min Scan# 985

Delta R.T. -0.00 min

Lab File: BM003439.D

Acq: 10 Dec 2015 07:06

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 82 Resp: 413687

Ion Ratio Lower Upper

82 100

128 47.6 32.8 49.2

54 39.7 40.6 60.8#


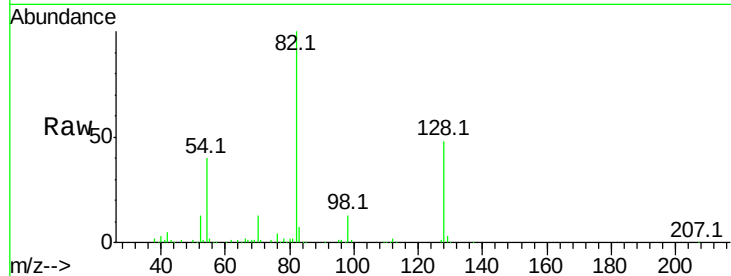


Abundance Ion 82.00 (81.70 to 82.70): BM003439.D (-968) (-)

Ion 128.00 (127.70 to 128.70): BM003439.D (-968) (-)

Ion 54.00 (53.70 to 54.70): BM003439.D (-968) (-)

Time-->

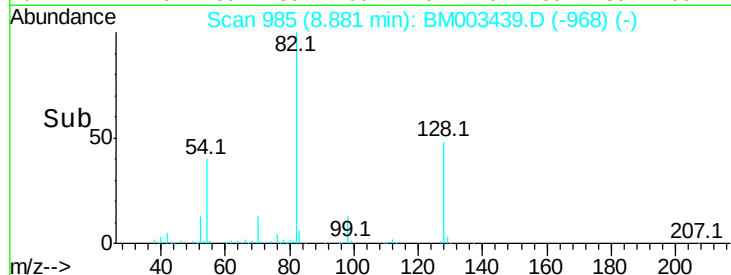

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.37 min Scan# 1919

Delta R.T. -0.00 min

Lab File: BM003439.D

Acq: 10 Dec 2015 07:06


Tgt Ion:164 Resp: 186879

Ion Ratio Lower Upper

164 100

162 81.5 82.4 123.6#

160 89.6 35.8 53.6#





Abundance Ion 164.00 (163.70 to 164.70): BM003439.D (-1902) (-)

Ion 162.00 (161.70 to 162.70): BM003439.D (-1902) (-)

Ion 160.00 (159.70 to 160.70): BM003439.D (-1902) (-)

Time-->

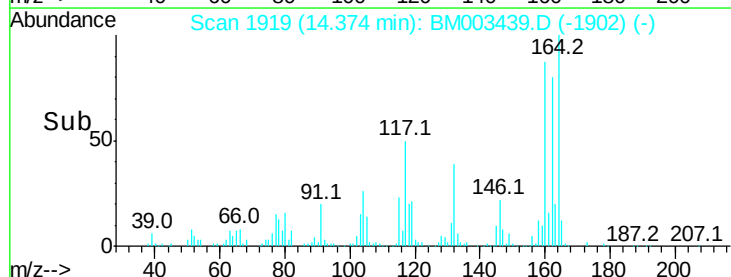


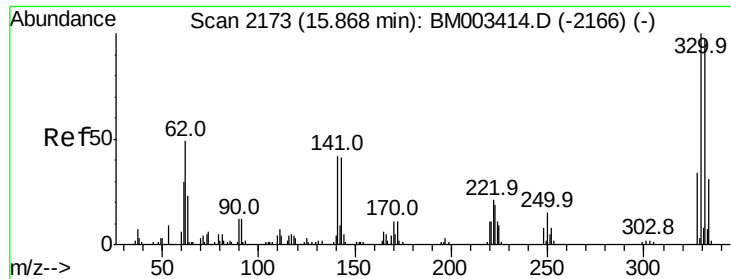




#41
 2,4,6-Tribromophenol
 Concen: 107.60 ng
 RT: 15.87 min Scan# 2173
 Delta R.T. -0.00 min
 Lab File: BM003439.D
 Acq: 10 Dec 2015 07:06

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	0.0	0.0#
141	43.1	0.0	0.0#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

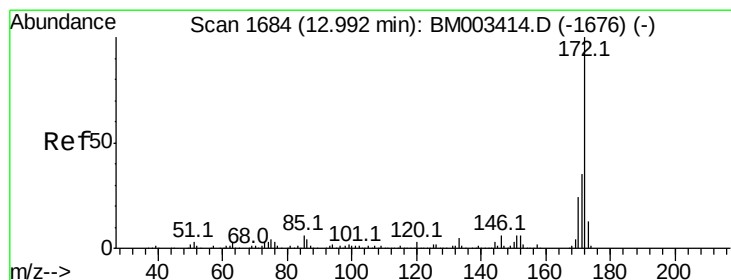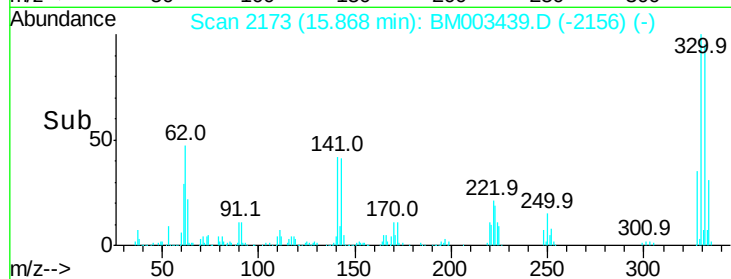
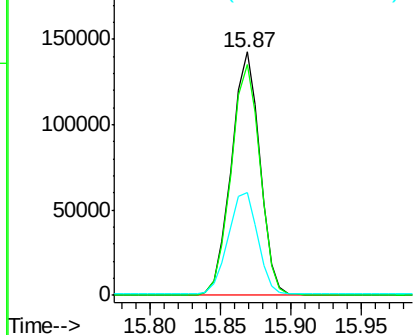



#44
 2-Fluorobiphenyl
 Concen: 67.52 ng
 RT: 12.99 min Scan# 1684
 Delta R.T. -0.00 min
 Lab File: BM003439.D
 Acq: 10 Dec 2015 07:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.7	28.5	42.7
170	23.3	18.8	28.2

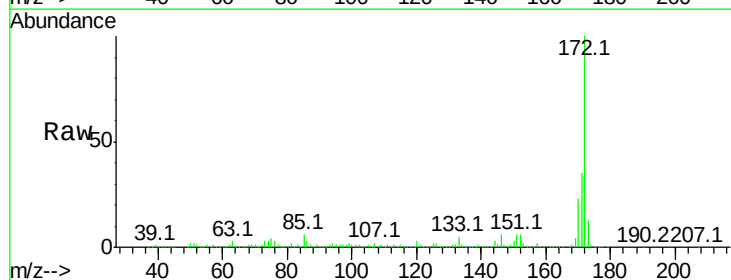

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

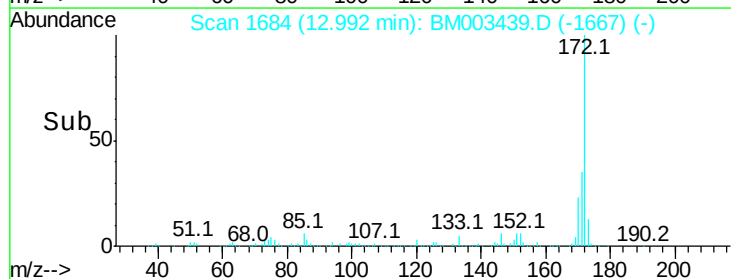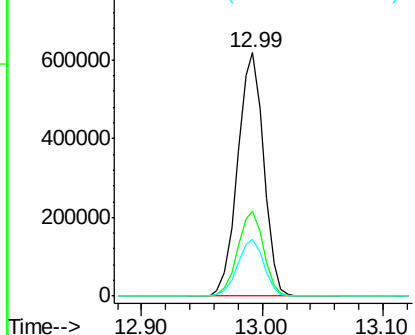

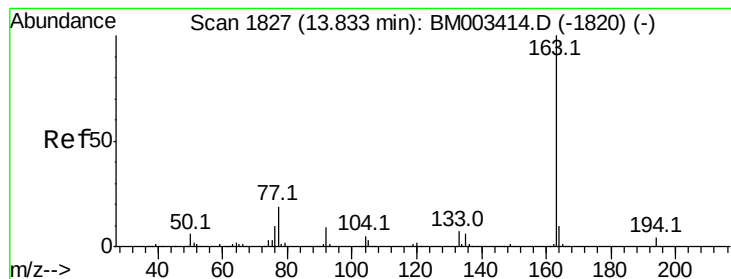

#49

Dimethylphthalate

Concen: 3.30 ng

RT: 13.83 min Scan# 1826

Delta R.T. -0.01 min

Lab File: BM003439.D

Acq: 10 Dec 2015 07:06

Instrument :

BNA_M

ClientSampled :


Tot Ion:163 Resp: 50771

Ion Ratio Lower Upper

163 100

194 4.2 2.7 4.1#




164 11.3 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

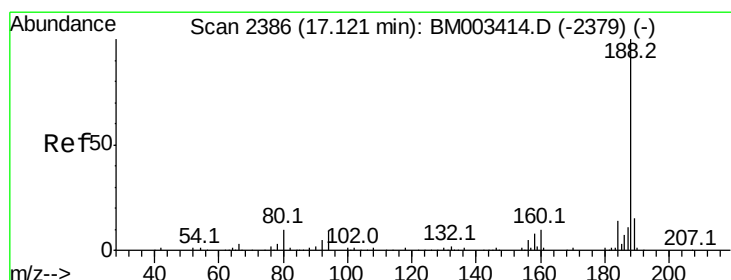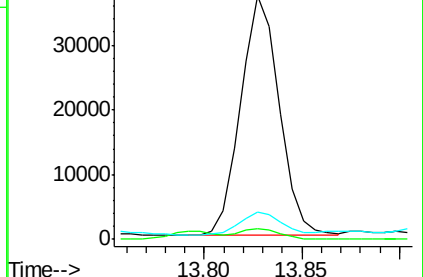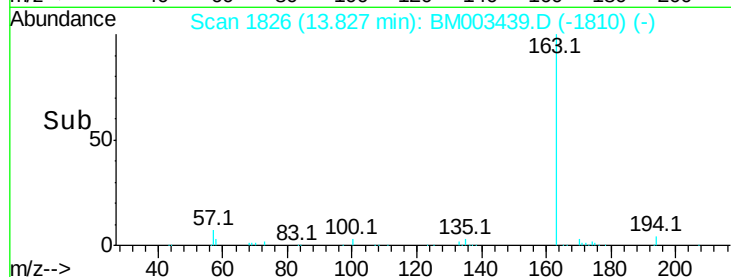

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.12 min Scan# 2386

Delta R.T. -0.00 min

Lab File: BM003439.D

Acq: 10 Dec 2015 07:06


Tgt Ion:188 Resp: 307271

Ion Ratio Lower Upper

188 100

94 9.1 8.7 13.1



80 9.7 9.3 13.9




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

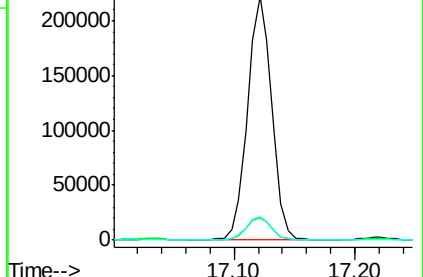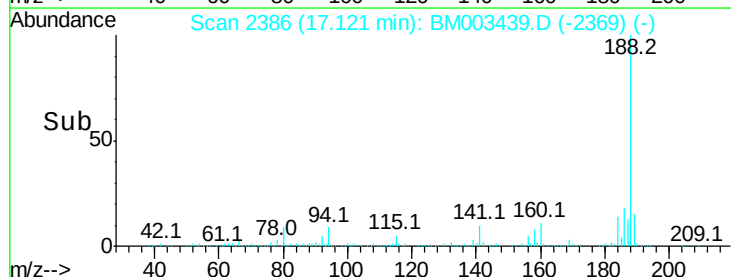

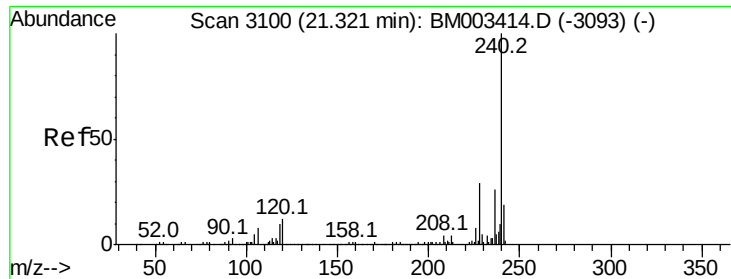

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.32 min Scan# 3099

Delta R.T. -0.01 min

Lab File: BM003439.D

Acq: 10 Dec 2015 07:06

Instrument :

BNA_M

ClientSampleId :


Tot Ion:240 Resp: 330673

Ion Ratio Lower Upper

240 100

120 12.6 8.2 12.2#




236 25.9 20.0 30.0

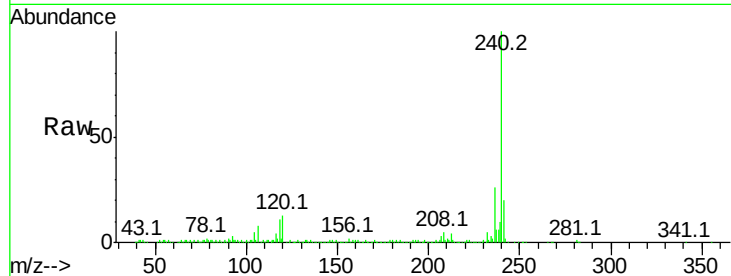

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

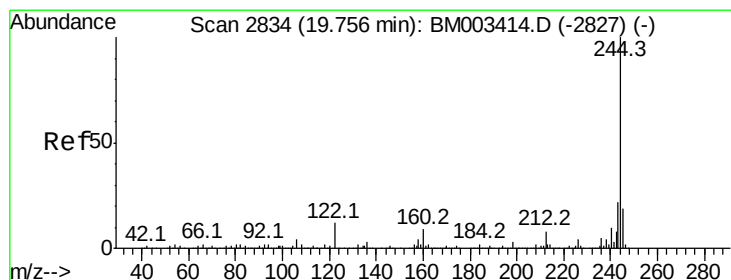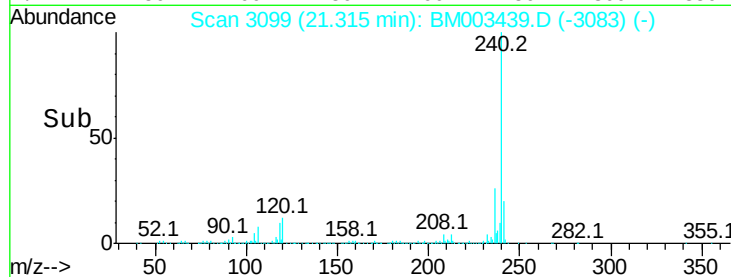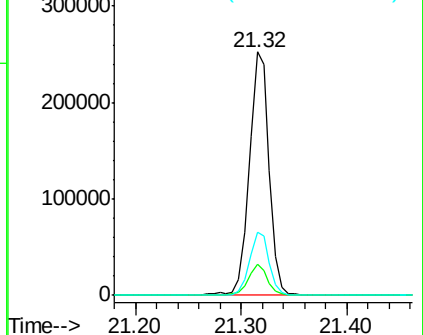

#78

Terphenyl-d14

Concen: 58.62 ng

RT: 19.76 min Scan# 2834

Delta R.T. -0.00 min

Lab File: BM003439.D

Acq: 10 Dec 2015 07:06


Tgt Ion:244 Resp: 822012

Ion Ratio Lower Upper

244 100

212 8.0 4.9 7.3#



122 11.4 6.2 9.4#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

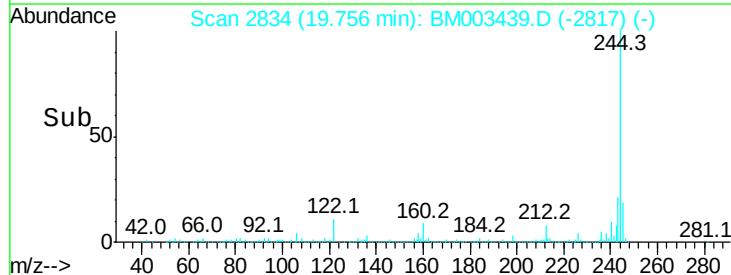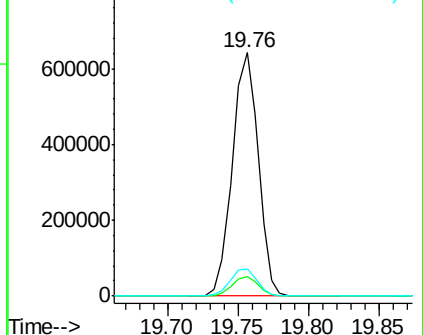


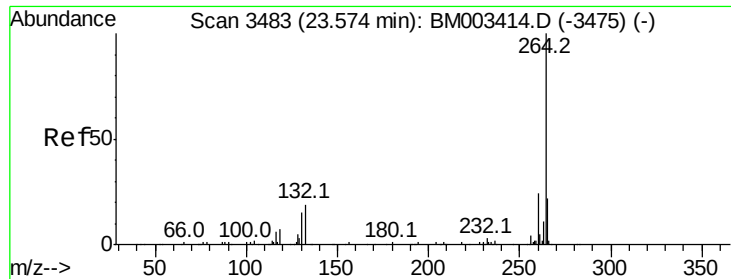

#86
Pervlene-d12
Concen: 20.00 ng
RT: 23.57 min Scan# 3483
Delta R.T. -0.00 min
Lab File: BM003439.D
Acq: 10 Dec 2015 07:06

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.7	18.6	27.8
265	21.6	17.3	25.9



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

