
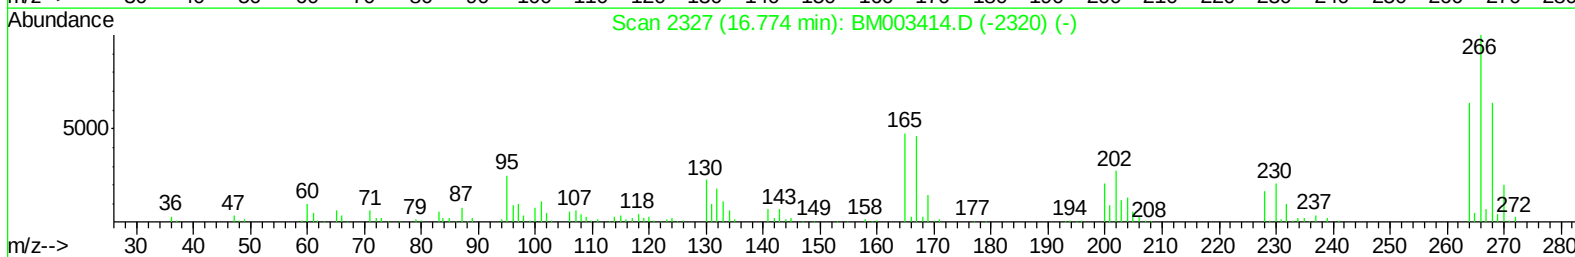
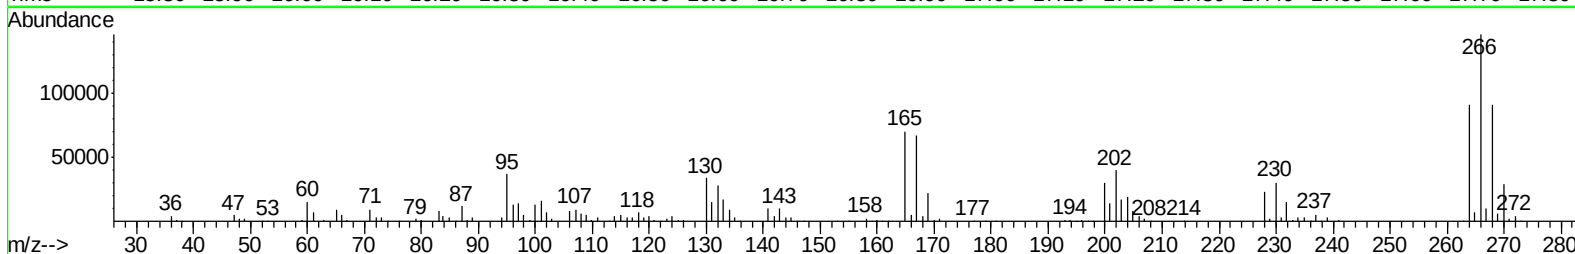


Data Path : Z:\HPCHEM1\BNA M\DATA\BM120915\
Data File : BM003410.D
Acq On : 09 Dec 2015 09:42
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 19:10:14 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

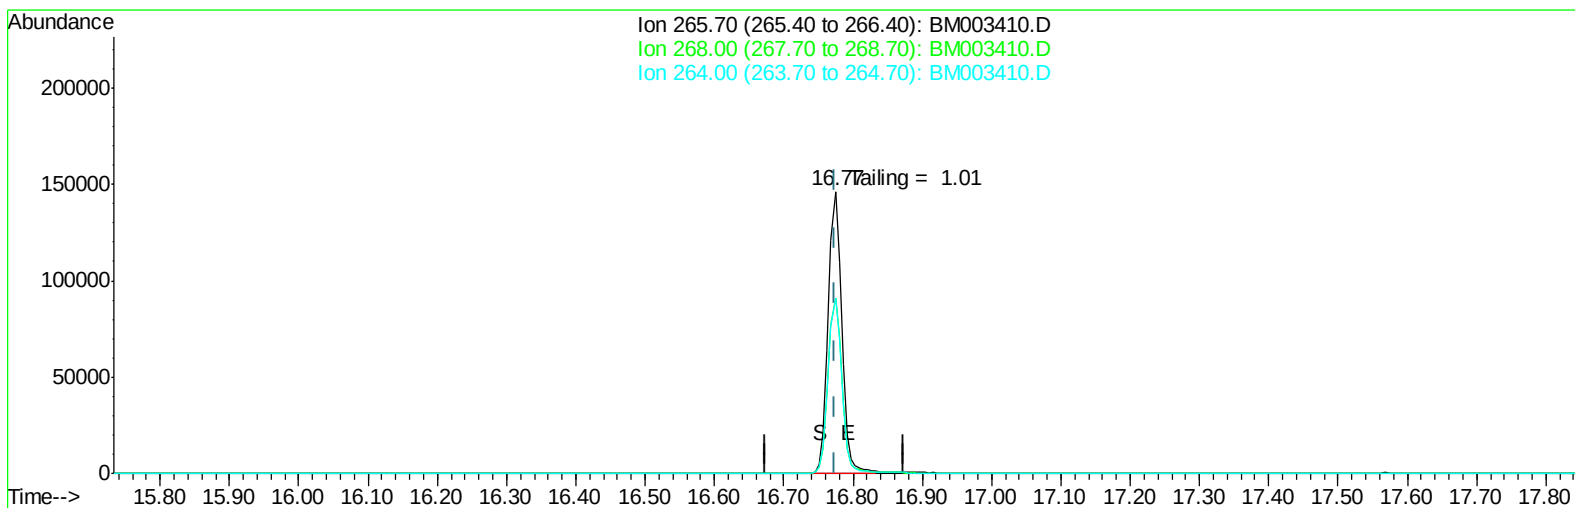

TIC: BM003410.D

(69) Pentachlorophenol (C)




16.774min (+0.000) 0.00ng

response 199690

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.45
264.00	61.20	62.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM120915\
Data File : BM003410.D
Acq On : 09 Dec 2015 09:42
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 19:10:14 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

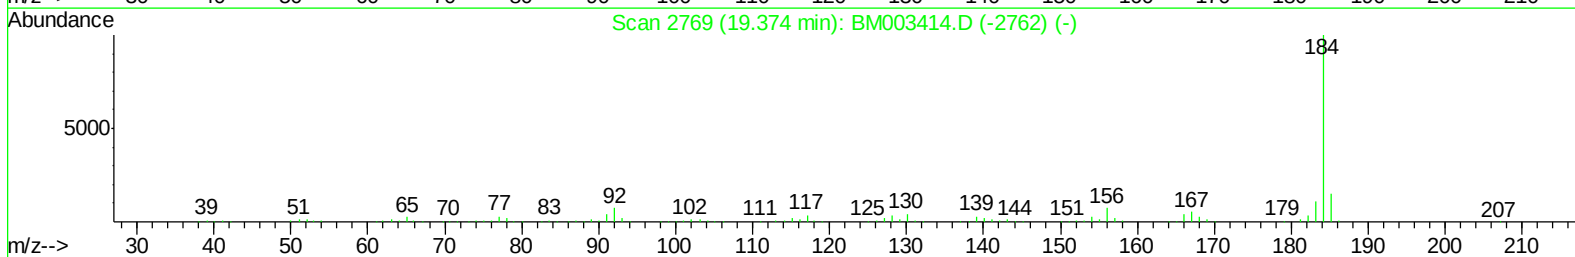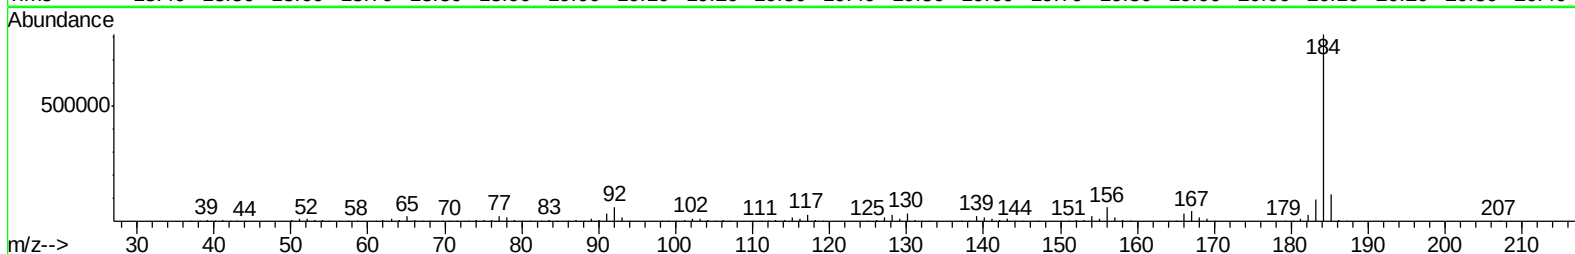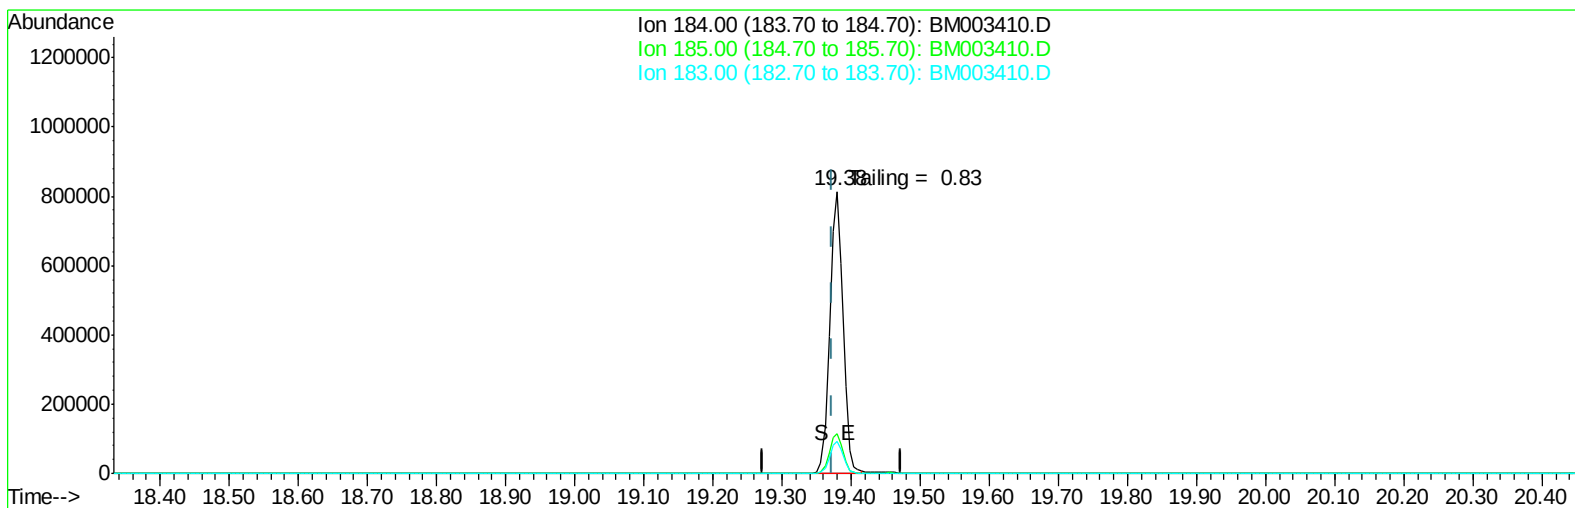

TIC: BM003410.D

(76) Benzidine

19.380min (+0.006) 11497.49ng

response 1081430

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.18
183.00	11.10	11.42
0.00	0.00	0.00