
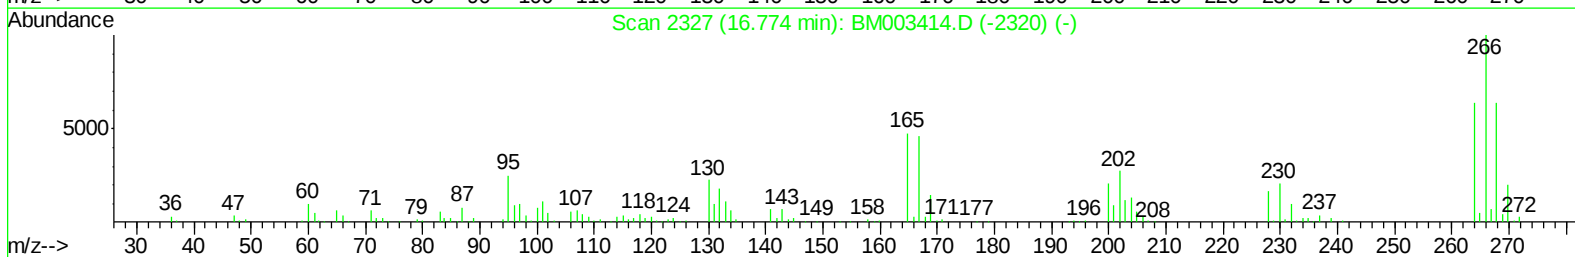
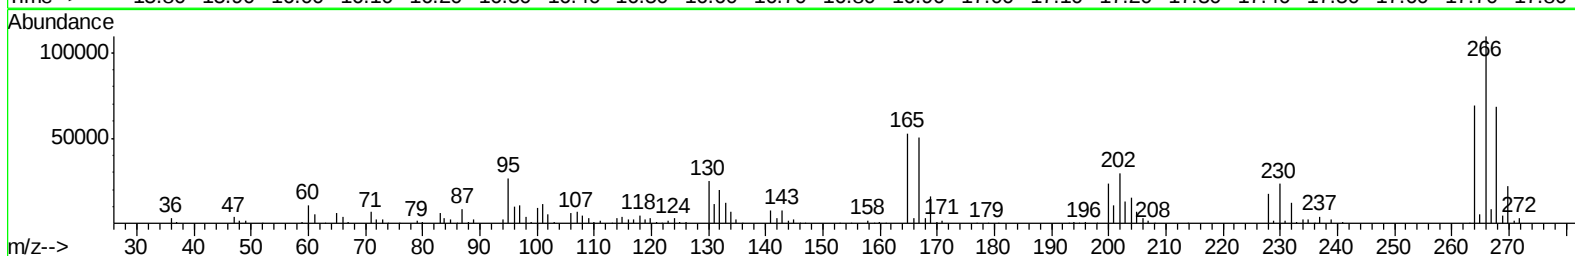


Data Path : Z:\HPCHEM1\BNA M\Data\BM120915\
Data File : BM003419.D
Acq On : 09 Dec 2015 19:05
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 07:17:30 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

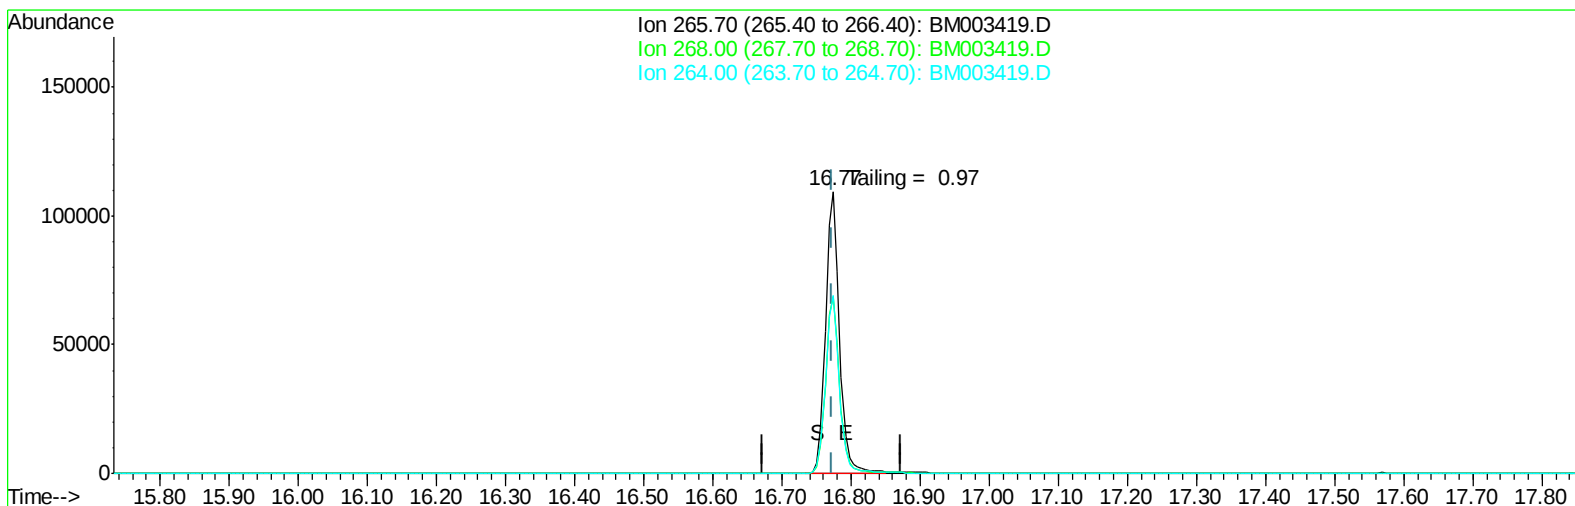

TIC: BM003419.D

(69) Pentachlorophenol (C)




16.774min (+0.000) 0.00ng

response 153017

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.62
264.00	61.20	63.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM120915\
Data File : BM003419.D
Acq On : 09 Dec 2015 19:05
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 07:17:30 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

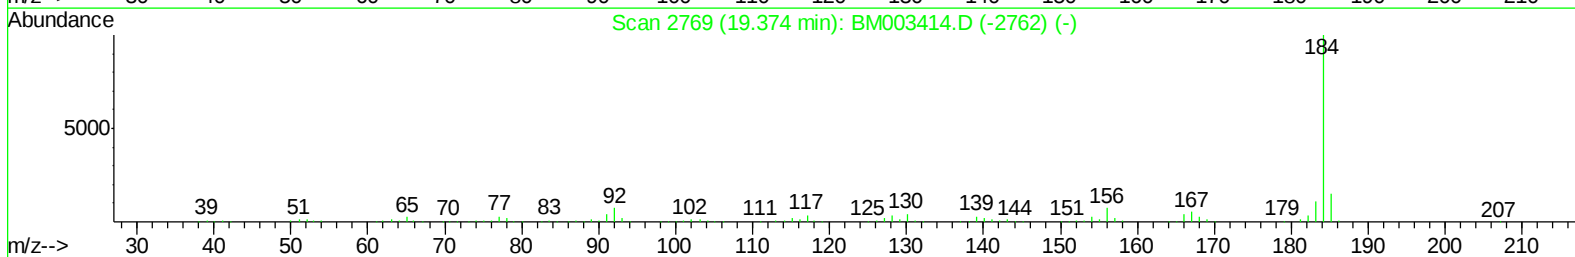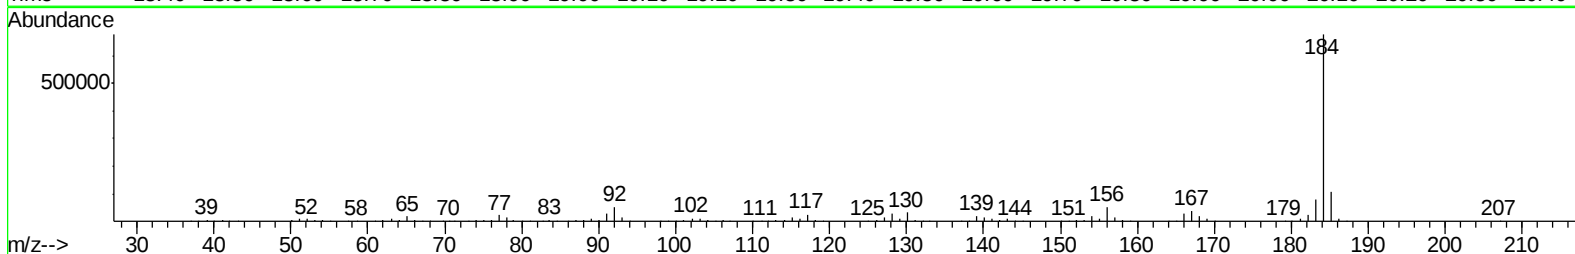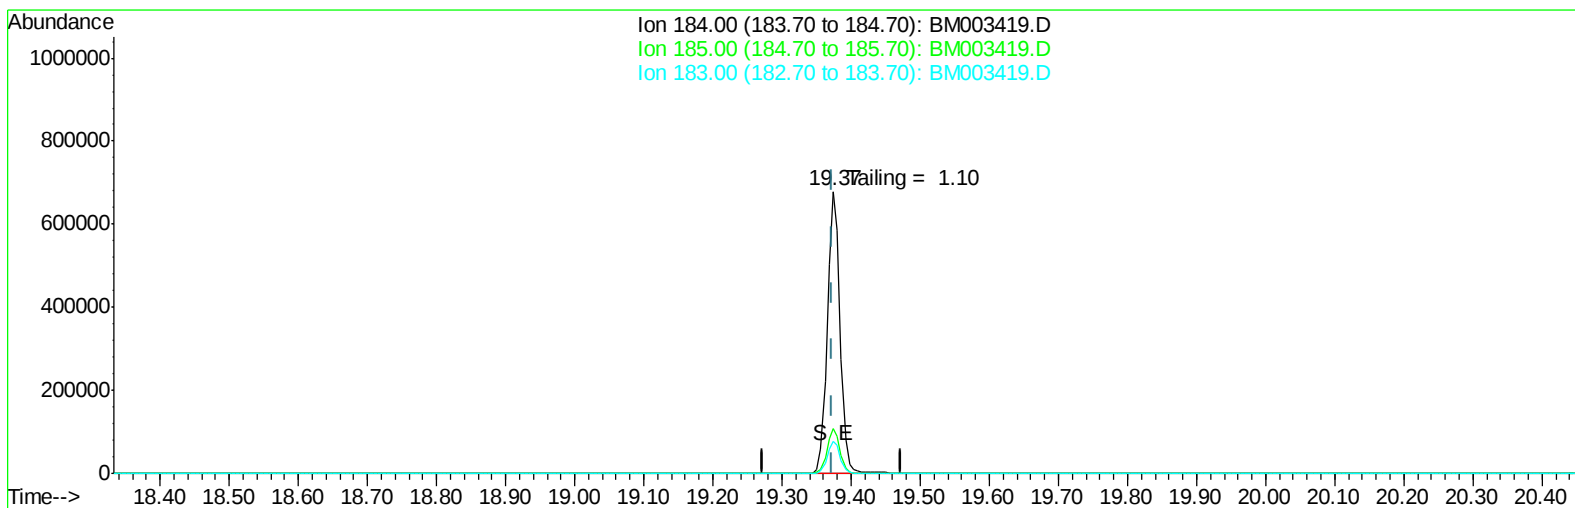

TIC: BM003419.D

(76) Benzidine

19.374min (-0.000) 0.00ng

response 872309

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	15.75
183.00	11.10	11.54
0.00	0.00	0.00