

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120915\
 Data File : BM003444.D
 Acq On : 10 Dec 2015 10:05
 Operator : UM/IZ
 Sample : G4690-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MW-24

Quant Time: Dec 10 11:26:44 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 18:52:47 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	74350	20.00	ng	0.00
21) Naphthalene-d8	10.51	136	339754	20.00	ng	0.00
38) Acenaphthene-d10	14.37	164	208063	20.00	ng	0.00
63) Phenanthrene-d10	17.12	188	475533	20.00	ng	0.00
75) Chrysene-d12	21.32	240	429743	20.00	ng	0.00
86) Perylene-d12	23.57	264	352636	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	313036	74.85	ng	0.00
7) Phenol-d6	6.89	99	274438	47.26	ng	0.00
23) Nitrobenzene-d5	8.88	82	555668	101.41	ng	0.00
41) 2,4,6-Tribromophenol	15.87	330	344173	165.63	ng	0.00
44) 2-Fluorobiphenyl	12.99	172	1428362	93.53	ng	0.00
78) Terphenyl-d14	19.76	244	1735438	95.24	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM120915\
Data File : BM003444.D
Acq On : 10 Dec 2015 10:05
Operator : UM/IZ
Sample : G4690-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-24

Quant Time: Dec 10 11:26:44 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

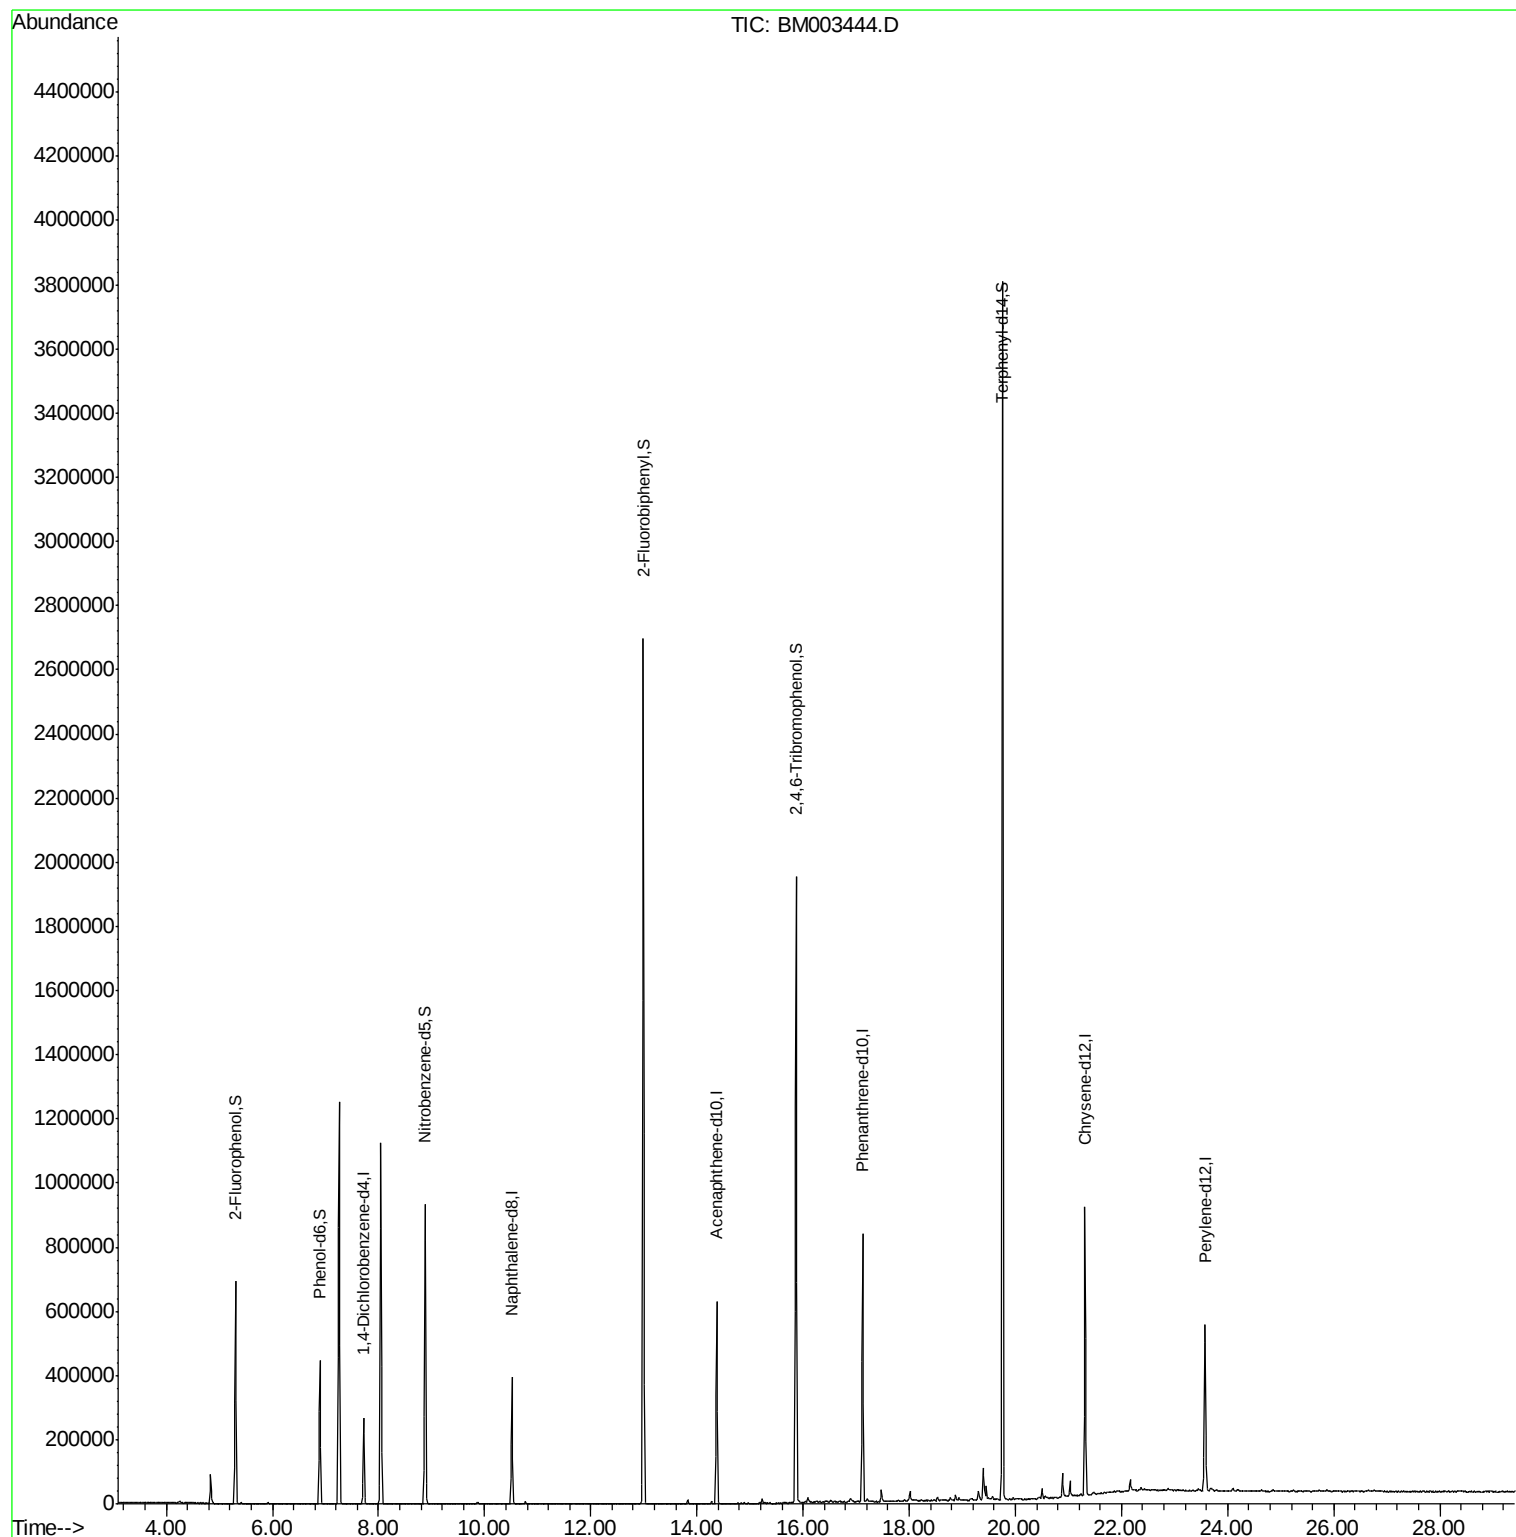

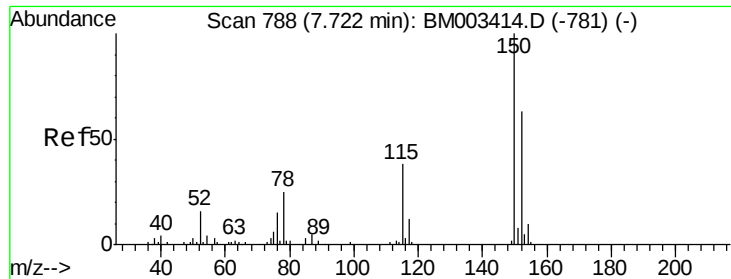


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.72 min Scan# 788
Delta R.T. -0.00 min
Lab File: BM003444.D
Acq: 10 Dec 2015 10:05

Instrument :
BNA_M
ClientSampled :
MW-24

Tgt Ion:152 Resp: 74350
Ion Ratio Lower Upper
152 100
150 156.5 119.5 179.3
115 59.4 43.0 64.4

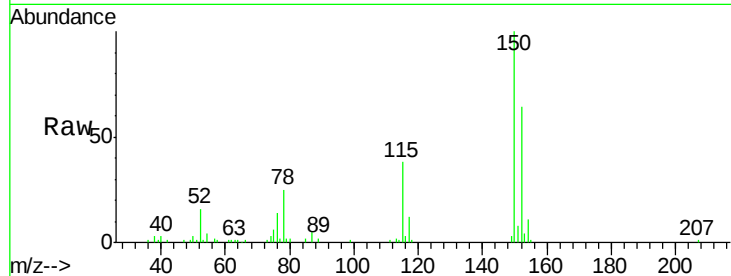


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

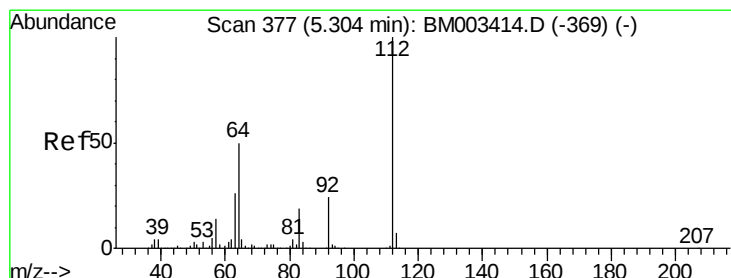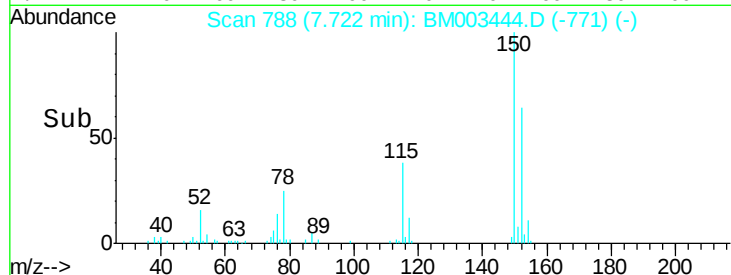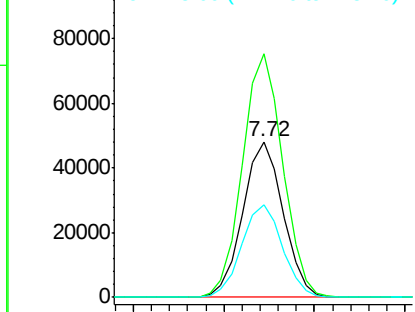



#5


2-Fluorophenol
Concen: 74.85 ng
RT: 5.30 min Scan# 377
Delta R.T. 0.00 min
Lab File: BM003444.D
Acq: 10 Dec 2015 10:05

Tgt Ion:112 Resp: 313036
Ion Ratio Lower Upper
112 100
64 48.9 38.6 57.8
63 26.4 19.3 28.9

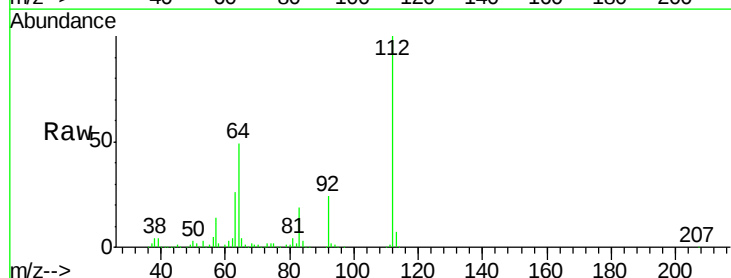

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

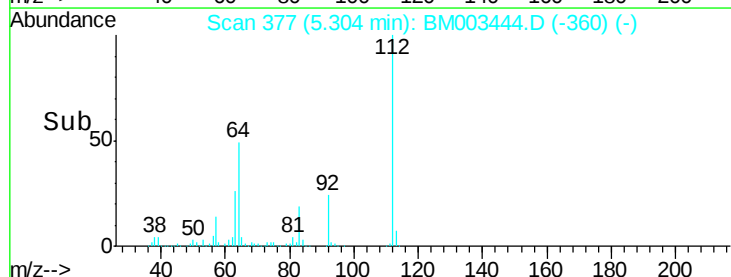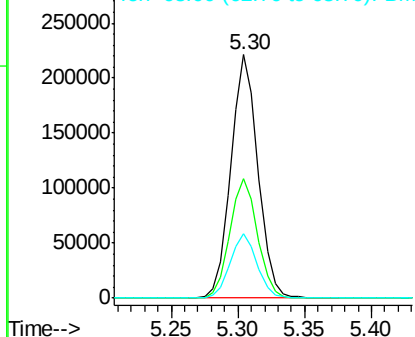

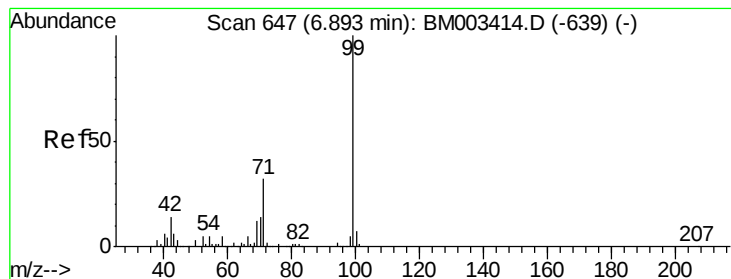

#7

Phenol-d6

Concen: 47.26 ng

RT: 6.89 min Scan# 647

Delta R.T. -0.00 min

Lab File: BM003444.D

Acq: 10 Dec 2015 10:05

Instrument :

BNA_M

ClientSampleId :

MW-24


Tgt Ion: 99 Resp: 274438

Ion Ratio Lower Upper

99 100

42 13.5 11.0 16.4




71 32.8 23.4 35.2

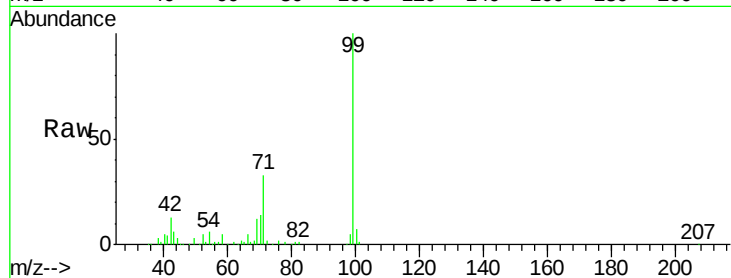

Abundance Ion 99.00 (98.70 to 99.70): BM003444.D (-639) (-)

Ion 42.00 (41.70 to 42.70): BM003444.D (-639) (-)

Ion 71.00 (70.70 to 71.70): BM003444.D (-639) (-)

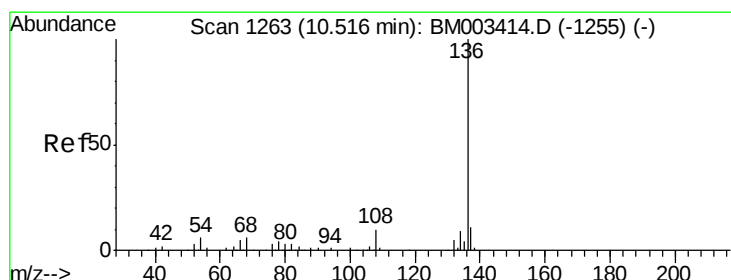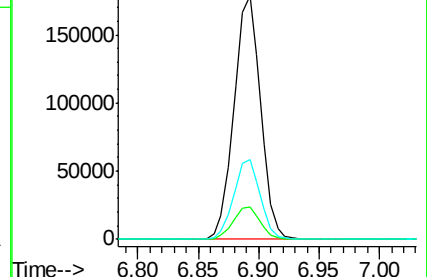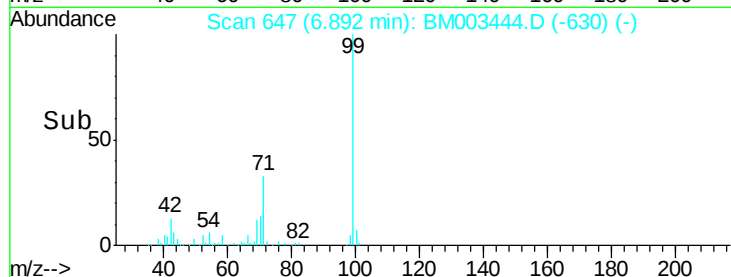

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.51 min Scan# 1262

Delta R.T. -0.01 min

Lab File: BM003444.D

Acq: 10 Dec 2015 10:05

Tgt Ion: 136 Resp: 339754


Ion Ratio Lower Upper

136 100

137 11.0 8.7 13.1

54 5.8 4.6 6.8

68 5.2 3.7 5.5


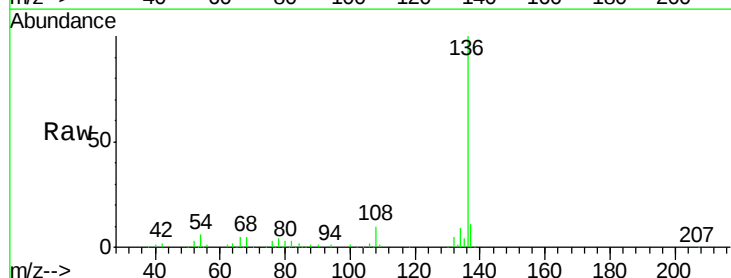



Abundance Ion 136.00 (135.70 to 136.70): BM003444.D (-1255) (-)

Ion 137.00 (136.70 to 137.70): BM003444.D (-1255) (-)

Ion 54.00 (53.70 to 54.70): BM003444.D (-1255) (-)

Ion 68.00 (67.70 to 68.70): BM003444.D (-1255) (-)

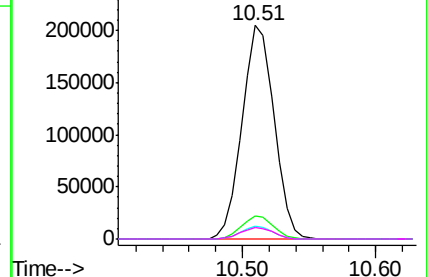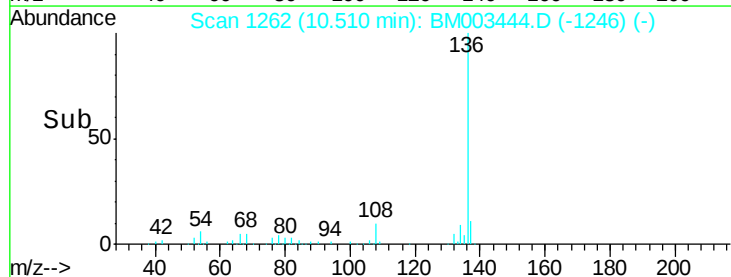

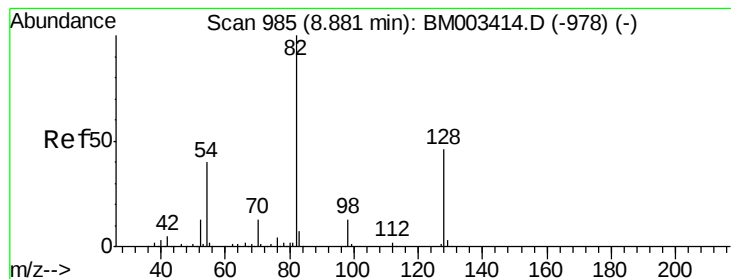

#23

Nitrobenzene-d5

Concen: 101.41 ng

RT: 8.88 min Scan# 985

Delta R.T. -0.00 min

Lab File: BM003444.D

Acq: 10 Dec 2015 10:05

Instrument :

BNA_M

ClientSampled :

MW-24


Tgt Ion: 82 Resp: 555668

Ion Ratio Lower Upper

82 100

128 47.1 32.8 49.2




54 39.8 40.6 60.8#

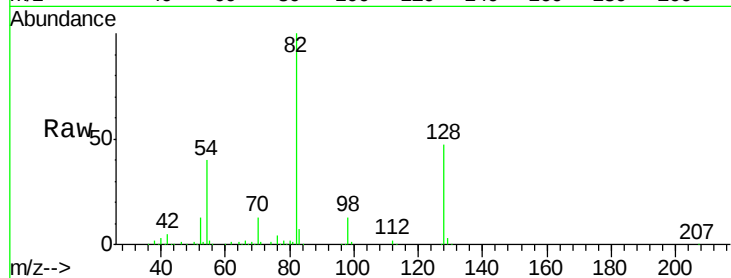

Abundance Ion 82.00 (81.70 to 82.70): BM003444.D (-968) (-)

Ion 128.00 (127.70 to 128.70): BM003444.D (-968) (-)

Ion 54.00 (53.70 to 54.70): BM003444.D (-968) (-)

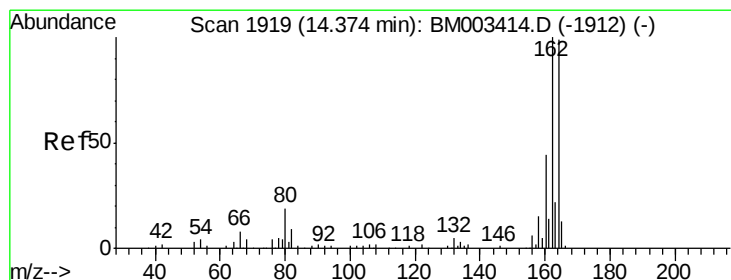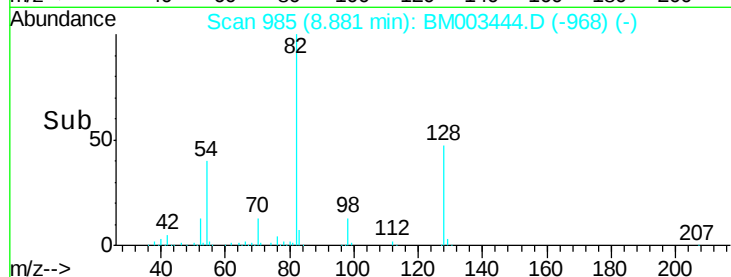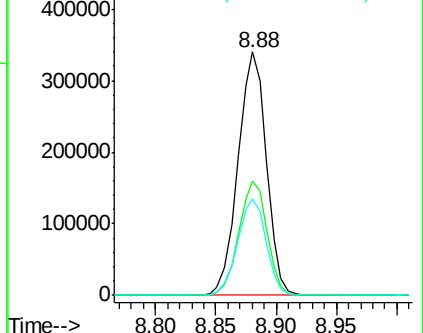

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.37 min Scan# 1919

Delta R.T. -0.00 min

Lab File: BM003444.D

Acq: 10 Dec 2015 10:05


Tgt Ion:164 Resp: 208063

Ion Ratio Lower Upper

164 100

162 100.3 82.4 123.6



160 45.5 35.8 53.6

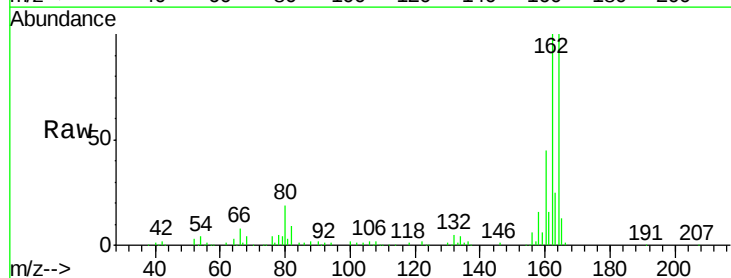

Abundance Ion 164.00 (163.70 to 164.70): BM003444.D (-1902) (-)

Ion 162.00 (161.70 to 162.70): BM003444.D (-1902) (-)

Ion 160.00 (159.70 to 160.70): BM003444.D (-1902) (-)



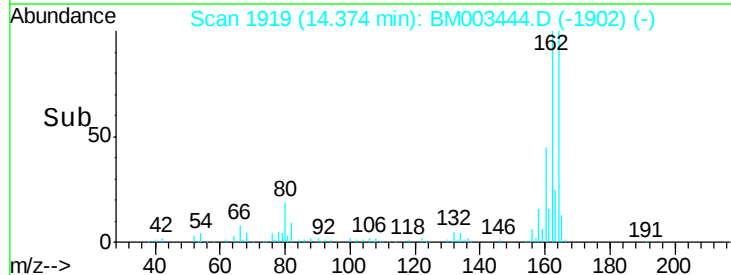
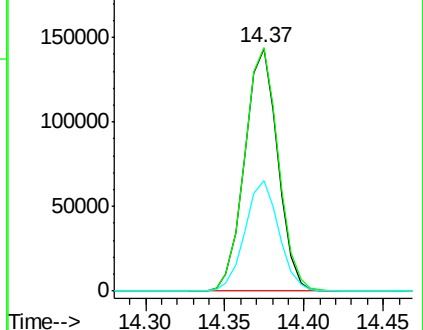




#41
 2,4,6-Tribromophenol
 Concen: 165.63 ng
 RT: 15.87 min Scan# 2173
 Delta R.T. -0.00 min
 Lab File: BM003444.D
 Acq: 10 Dec 2015 10:05




Instrument :
 BNA_M
 ClientSampleId :
 MW-24


Tgt Ion:330 Resp: 344173
 Ion Ratio Lower Upper
 330 100
 332 96.3 0.0 0.0#
 141 43.5 0.0 0.0#

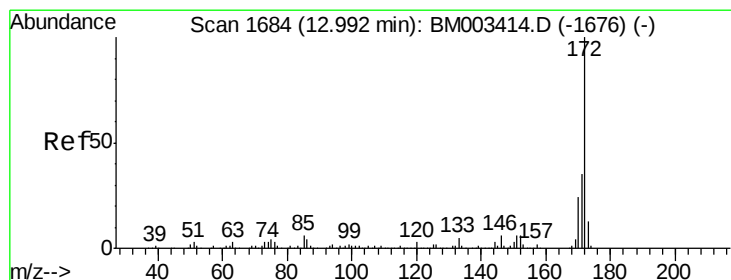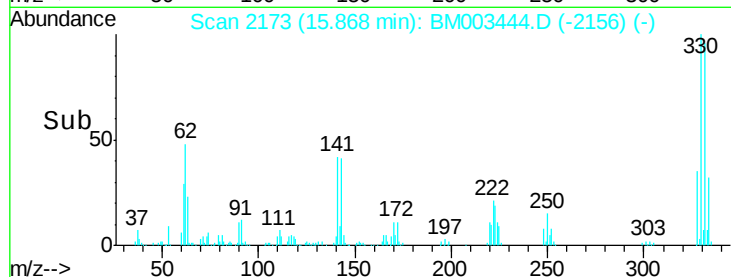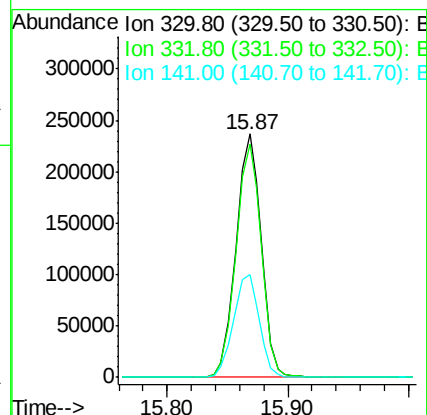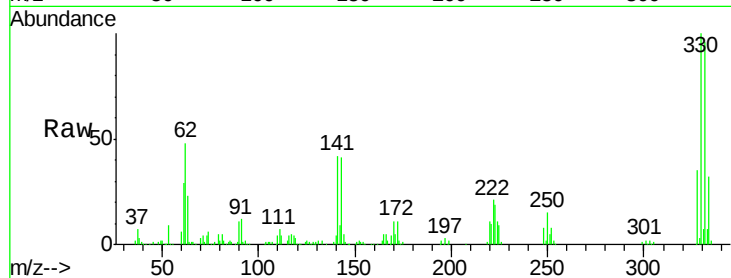

#44
 2-Fluorobiphenyl
 Concen: 93.53 ng
 RT: 12.99 min Scan# 1684
 Delta R.T. -0.00 min
 Lab File: BM003444.D
 Acq: 10 Dec 2015 10:05

Tgt Ion:172 Resp: 1428362
 Ion Ratio Lower Upper
 172 100
 171 34.9 28.5 42.7
 170 23.3 18.8 28.2

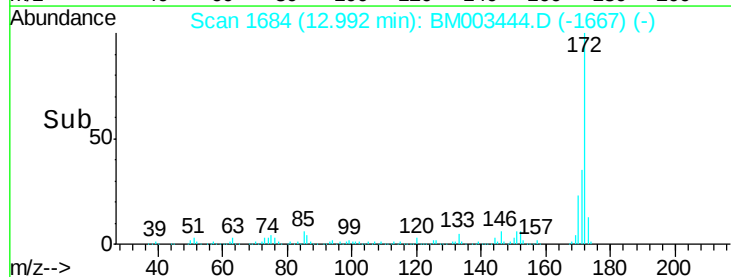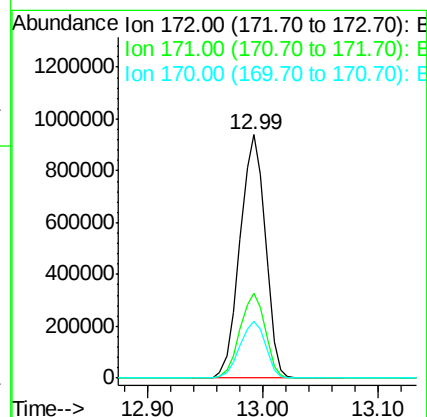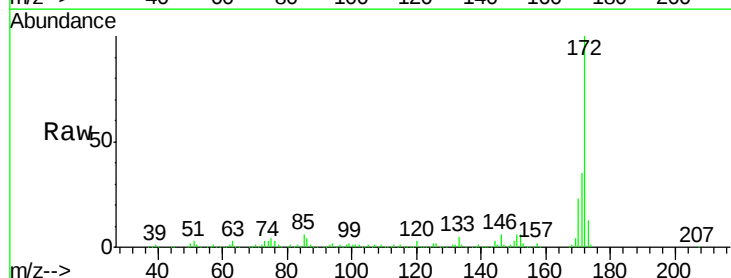


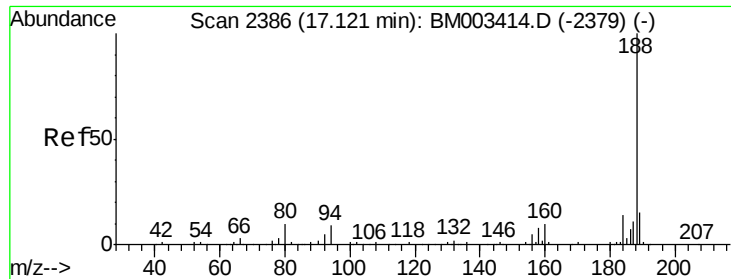




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.12 min Scan# 2386
Delta R.T. -0.00 min
Lab File: BM003444.D
Acq: 10 Dec 2015 10:05

Instrument :
BNA_M
ClientSampleId :
MW-24

Tgt Ion:188 Resp: 475533
Ion Ratio Lower Upper
188 100
94 8.8 8.7 13.1
80 9.6 9.3 13.9

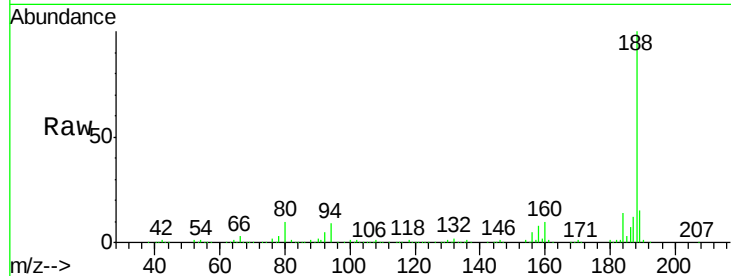


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

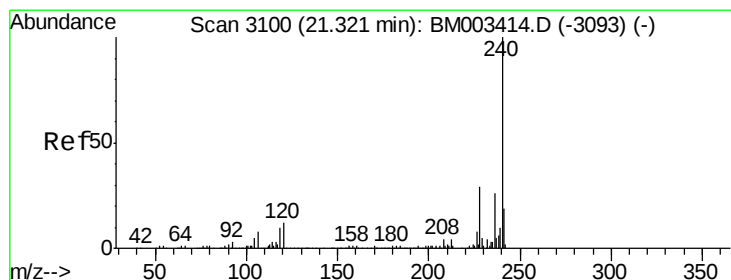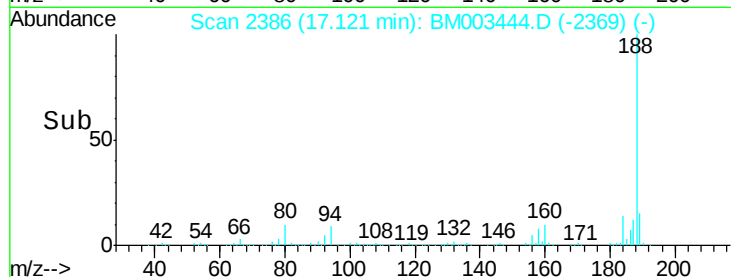
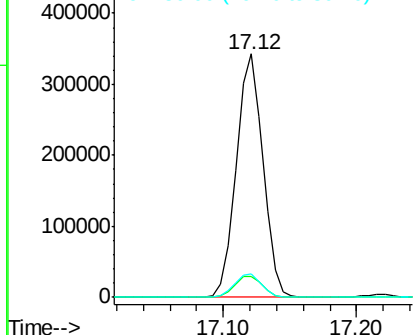



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.32 min Scan# 3099
Delta R.T. -0.01 min
Lab File: BM003444.D
Acq: 10 Dec 2015 10:05

Tgt Ion:240 Resp: 429743
Ion Ratio Lower Upper
240 100
120 12.1 8.2 12.2
236 26.5 20.0 30.0

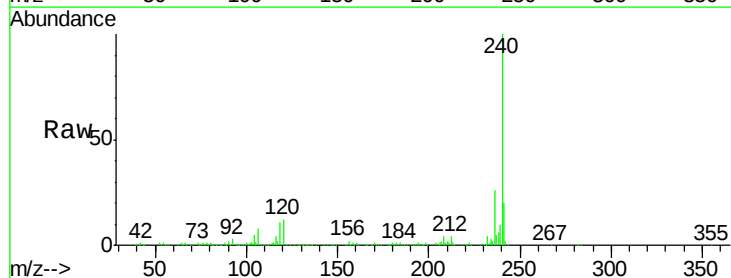

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

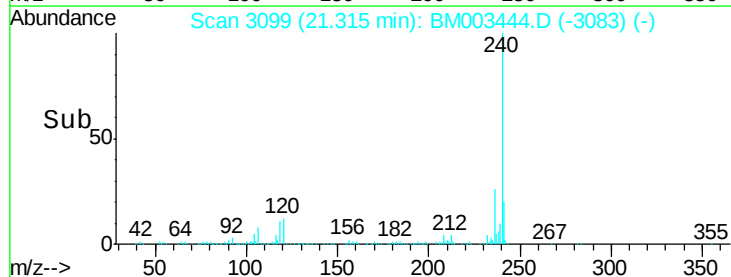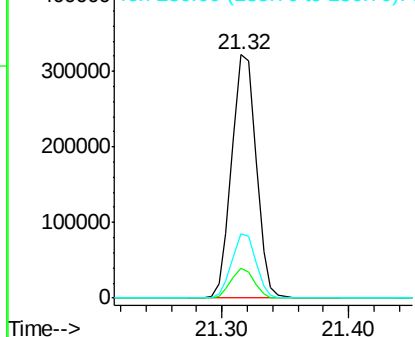

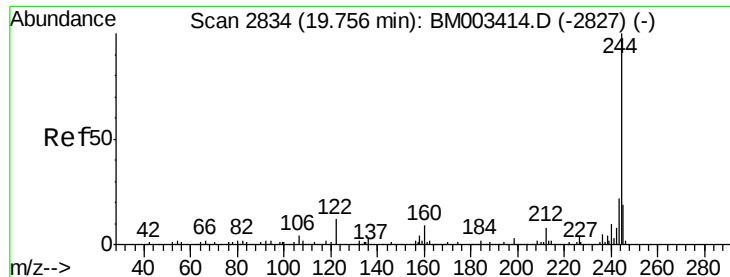

#78

Terphenyl-d14

Concen: 95.24 ng

RT: 19.76 min Scan# 2834

Delta R.T. -0.00 min

Lab File: BM003444.D

Acq: 10 Dec 2015 10:05

Instrument :

BNA_M

ClientSampleId :

MW-24


Tgt Ion:244 Resp: 1735438

Ion Ratio Lower Upper

244 100

212 8.1 4.9 7.3#




122 11.5 6.2 9.4#

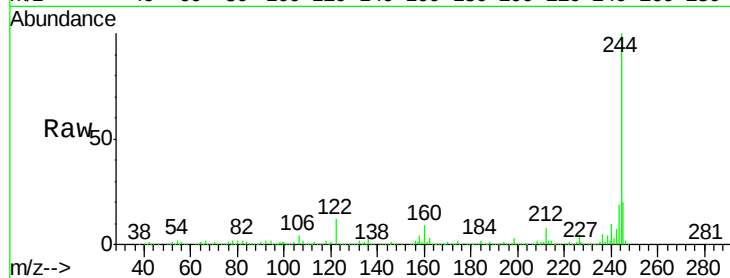

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

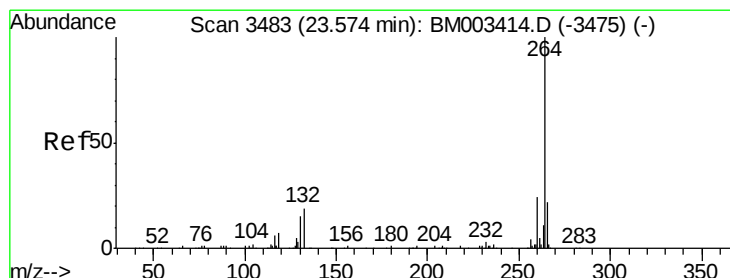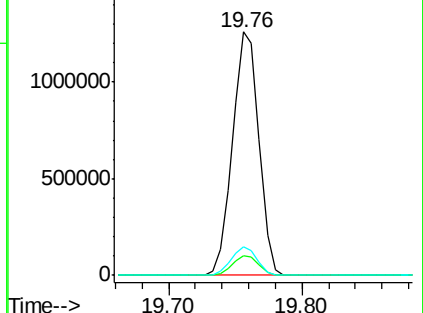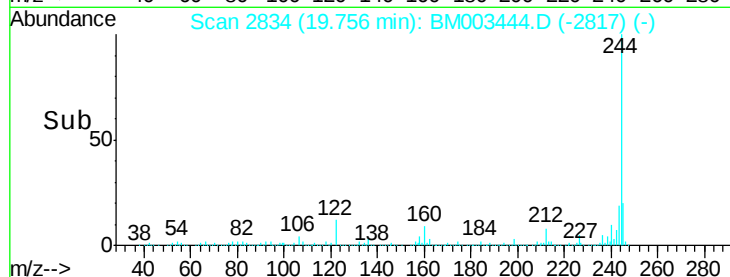

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.57 min Scan# 3483

Delta R.T. -0.00 min

Lab File: BM003444.D

Acq: 10 Dec 2015 10:05


Tgt Ion:264 Resp: 352636

Ion Ratio Lower Upper

264 100

260 23.8 18.6 27.8

265 21.5 17.3 25.9

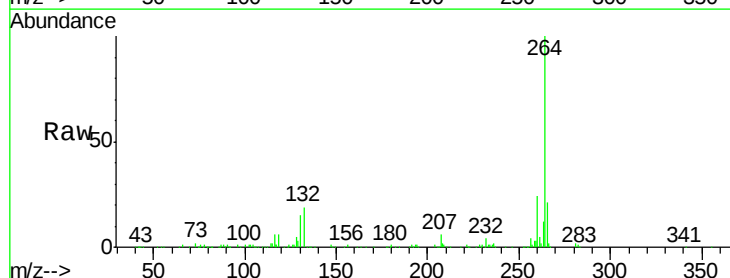

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

