


Data Path : Z:\HPCHEM1\BNA\_M\Data\BM120915\  
Data File : BM003410.D  
Acq On : 09 Dec 2015 09:42  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-BM120915.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Dec 09 18:52:47 2015

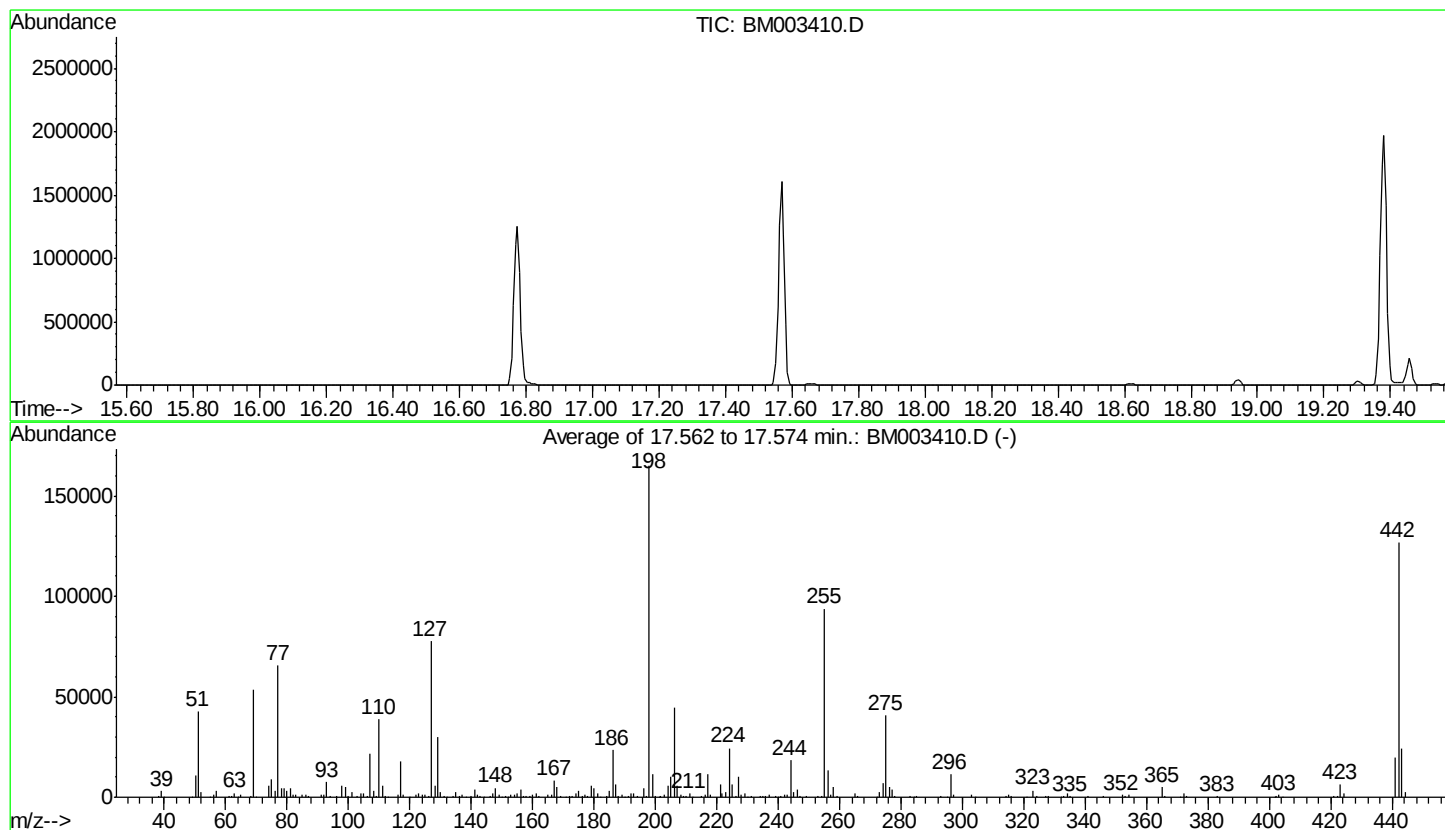

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 25.8      | 42560   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 898     | PASS             |
| 69          | 198          | 0.00         | 100          | 32.5      | 53656   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 234     | PASS             |
| 127         | 198          | 10           | 80           | 46.9      | 77493   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 864     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 165120  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 11302   | PASS             |
| 275         | 198          | 10           | 60           | 24.7      | 40794   | PASS             |
| 365         | 198          | 1            | 100          | 3.0       | 4948    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.5      | 19568   | PASS             |
| 442         | 198          | 50           | 100          | 76.7      | 126640  | PASS             |
| 443         | 442          | 15           | 24           | 19.4      | 24520   | PASS             |