


Data Path : Z:\HPCHEM1\BNA_M\Data\BM120915\
 Data File : BM003437.D
 Acq On : 10 Dec 2015 05:54
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 09 18:52:47 2015

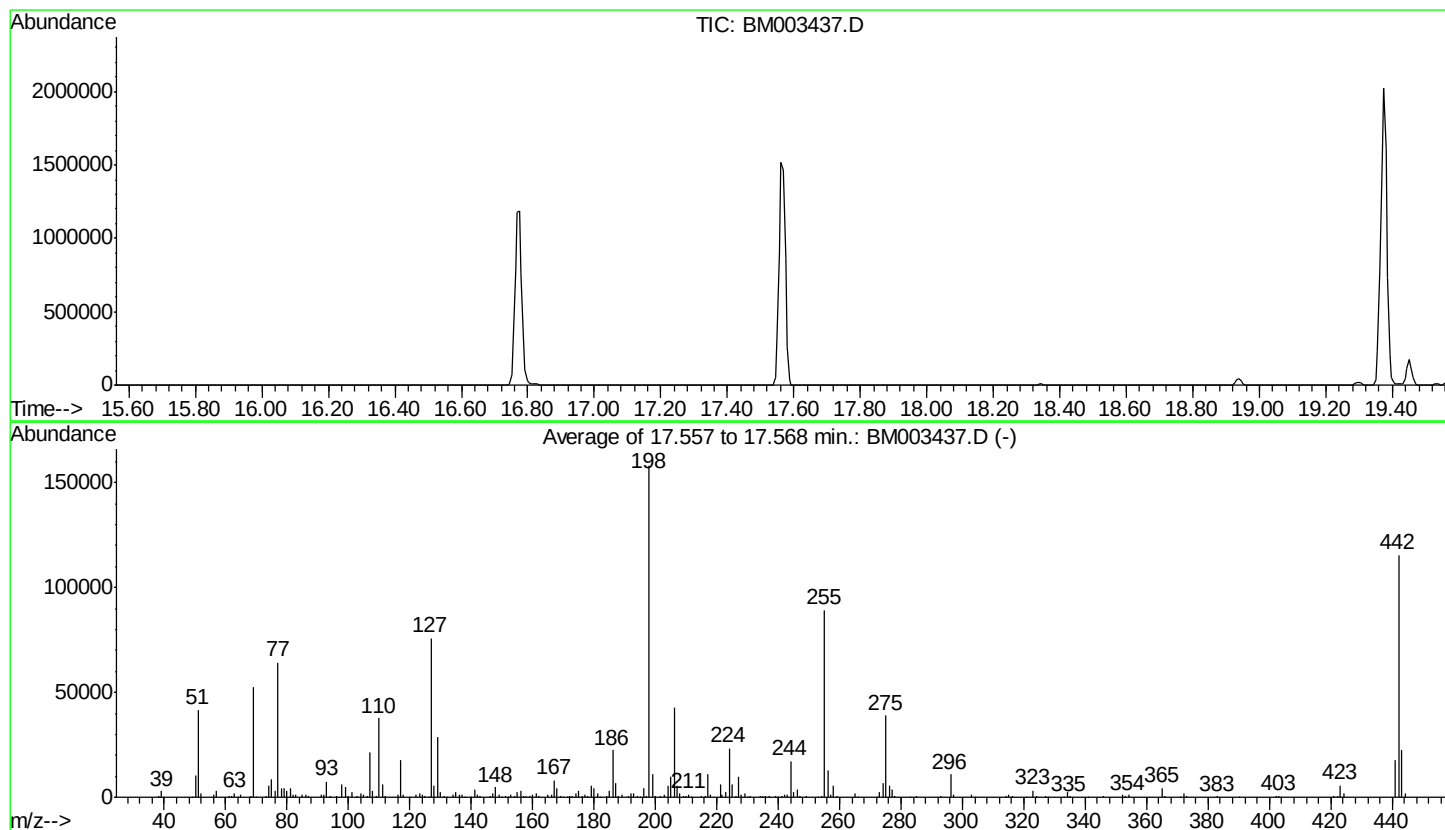

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	41778	PASS
68	69	0.00	2	1.7	890	PASS
69	198	0.00	100	33.3	52690	PASS
70	69	0.00	2	0.2	120	PASS
127	198	10	80	47.9	75840	PASS
197	198	0.00	2	0.6	917	PASS
198	198	100	100	100.0	158168	PASS
199	198	5	9	6.8	10798	PASS
275	198	10	60	24.6	38954	PASS
365	198	1	100	2.9	4515	PASS
441	442	0.01	24	15.4	17750	PASS
442	198	50	100	73.1	115560	PASS
443	442	15	24	19.7	22753	PASS