


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121015\
 Data File : BM003457.D
 Acq On : 10 Dec 2015 17:57
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 09 18:52:47 2015

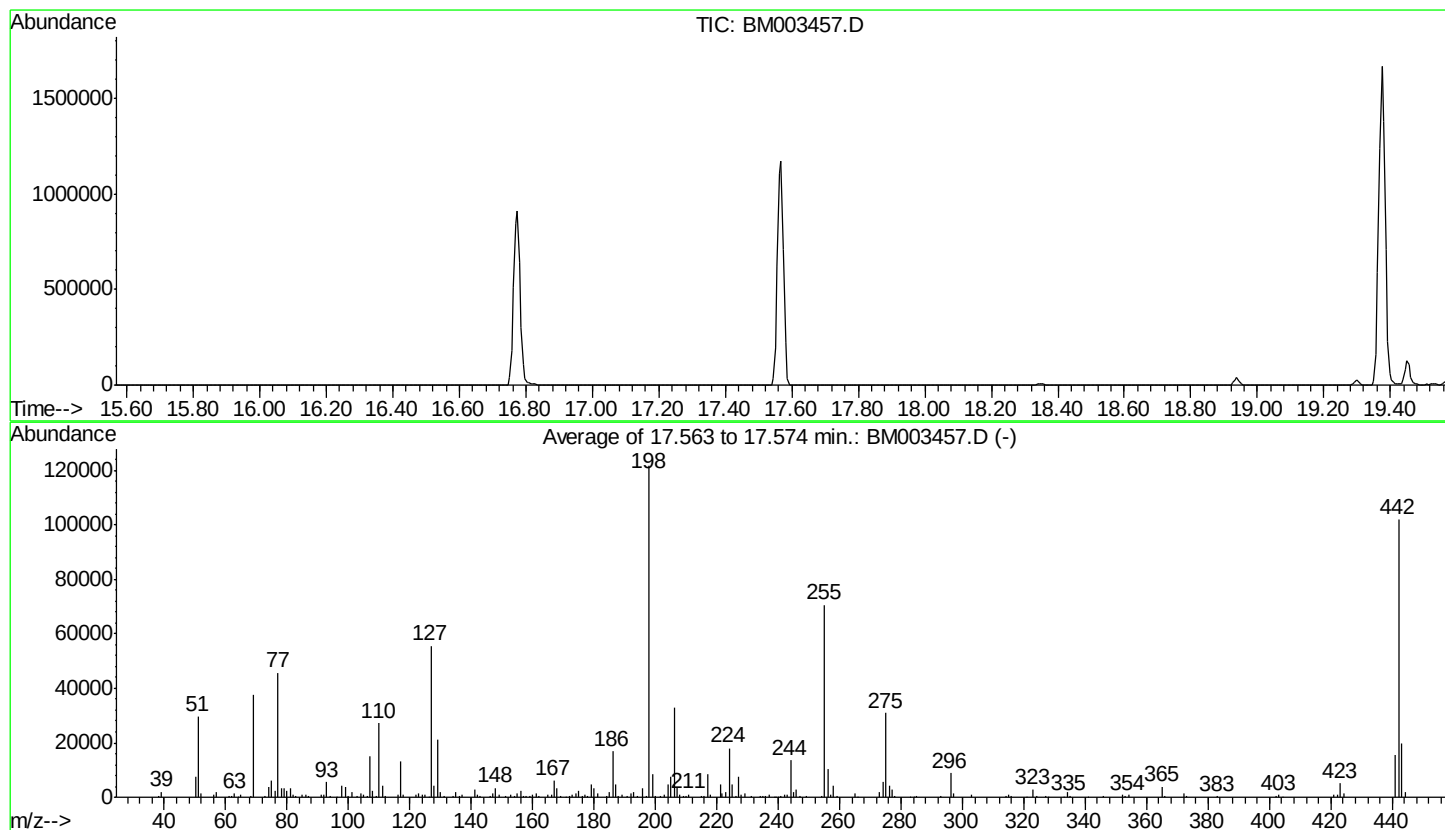

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.3	29626	PASS
68	69	0.00	2	1.6	594	PASS
69	198	0.00	100	30.8	37520	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	55517	PASS
197	198	0.00	2	0.5	637	PASS
198	198	100	100	100.0	121834	PASS
199	198	5	9	6.8	8321	PASS
275	198	10	60	25.4	30986	PASS
365	198	1	100	3.1	3778	PASS
441	442	0.01	24	15.1	15434	PASS
442	198	50	100	83.6	101898	PASS
443	442	15	24	19.4	19816	PASS