


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121015\
Data File : BM003470.D
Acq On : 11 Dec 2015 01:47
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 09 18:52:47 2015

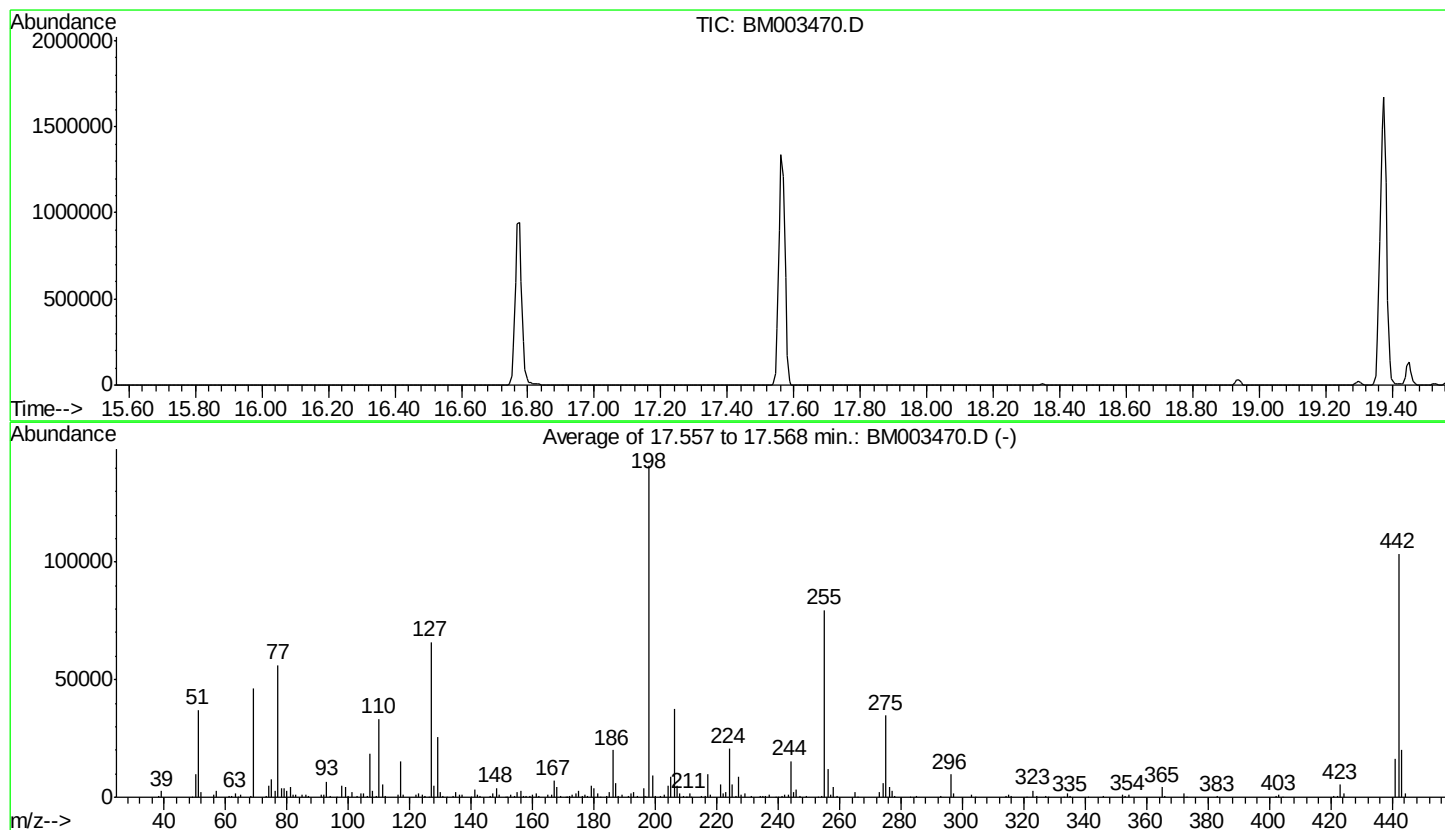

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	37192	PASS
68	69	0.00	2	1.7	780	PASS
69	198	0.00	100	32.9	46448	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	66026	PASS
197	198	0.00	2	0.3	422	PASS
198	198	100	100	100.0	141045	PASS
199	198	5	9	6.8	9535	PASS
275	198	10	60	24.5	34616	PASS
365	198	1	100	2.9	4156	PASS
441	442	0.01	24	15.5	16095	PASS
442	198	50	100	73.5	103613	PASS
443	442	15	24	19.7	20391	PASS