


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121016\
Data File : BM008224.D
Acq On : 10 Dec 2016 09:36
Operator : UM/SJ
Sample : DFTPP64
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP64

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
Title : SVOA CALIBRATION
Last Update : Wed Nov 30 00:32:18 2016

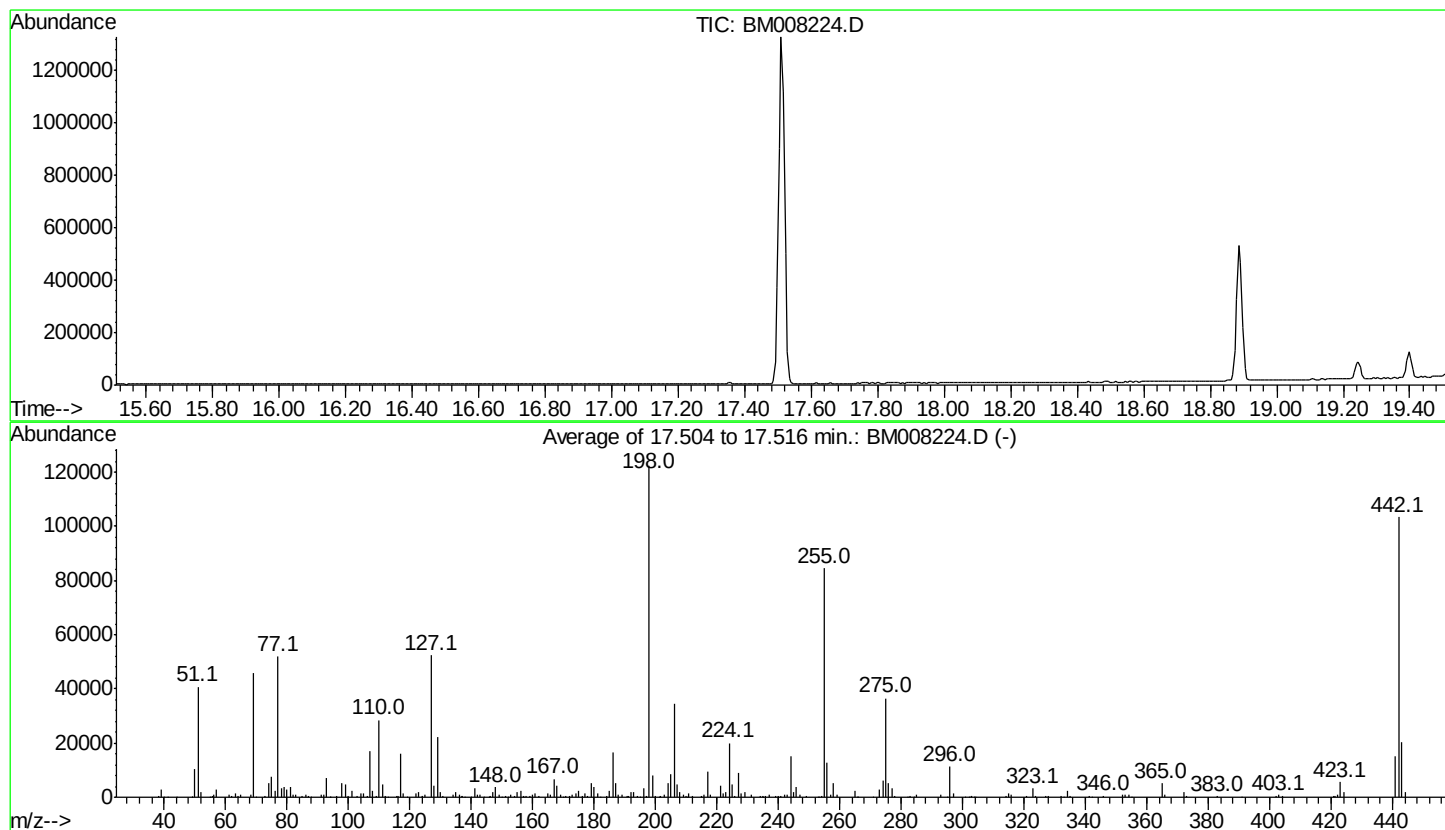

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	40842	PASS
68	69	0.00	2	1.6	745	PASS
69	198	0.00	100	37.5	45872	PASS
70	69	0.00	2	0.3	117	PASS
127	198	10	80	42.8	52378	PASS
197	198	0.00	2	0.4	487	PASS
198	198	100	100	100.0	122429	PASS
199	198	5	9	6.5	7972	PASS
275	198	10	60	29.8	36482	PASS
365	198	1	100	4.2	5135	PASS
441	443	0.01	100	73.6	15000	PASS
442	198	50	100	84.4	103328	PASS
443	442	15	24	19.7	20371	PASS

Scan 2531 (17.474 min): BM008224.D
DFTPP64

m/z	Abundance
40.00	2499.0
44.00	443.0
73.00	545.0
207.00	1593.0
281.00	634.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

m/z	Abundance
38.10	394.0
39.00	2674.0
40.00	2848.0
44.00	775.0
49.00	566.0
50.10	9877.0
51.10	40448.0
52.10	2212.0
55.90	1103.0
57.00	2604.0
61.00	655.0
62.10	441.0
63.00	1481.0
64.10	367.0
65.10	712.0
68.00	666.0
69.00	43184.0
73.00	828.0
74.00	4898.0
75.00	7094.0
76.10	2042.0
77.10	47720.0
78.10	3597.0
79.00	3670.0
80.00	3197.0
81.00	4233.0
82.00	1228.0
83.00	698.0
84.90	404.0
86.00	1217.0
87.00	495.0
91.10	960.0
92.10	1098.0
93.00	6942.0
96.00	457.0
98.00	4934.0
99.00	4710.0
101.10	2292.0
102.90	630.0
104.00	1371.0
105.00	1196.0
106.20	435.0
107.00	15636.0
108.00	2005.0
110.00	25528.0
111.00	4311.0
111.90	425.0
115.90	837.0
117.00	14431.0
118.10	1295.0
122.10	1013.0
123.10	1709.0
123.90	824.0
125.00	582.0
127.00	46144.0
128.00	3453.0
129.00	20416.0
130.00	1970.0
131.00	410.0
134.00	638.0
135.10	1473.0
136.10	715.0
136.90	934.0
140.10	325.0
141.00	2878.0
142.00	755.0
142.90	706.0
146.10	467.0
147.00	1655.0
148.00	3021.0
149.10	918.0
151.00	369.0
152.90	854.0
154.00	666.0
155.10	1233.0
156.00	2075.0
157.00	357.0
158.00	733.0
159.00	338.0
160.00	789.0
160.90	1142.0
165.00	1302.0
165.90	827.0
167.00	5631.0
168.00	4002.0
169.10	920.0
171.00	339.0
171.90	579.0
173.00	682.0
174.00	1219.0
175.00	2145.0
176.10	666.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

176.90	996.0
178.00	567.0
179.00	4842.0
180.00	3458.0
181.00	1054.0
184.00	331.0
185.10	2413.0
186.00	13488.0
187.00	4355.0
188.10	489.0
189.10	858.0
191.20	549.0
192.00	1446.0
193.00	1618.0
193.90	361.0
196.00	3176.0
196.80	586.0
198.00	97184.0
199.00	6606.0
200.00	611.0
201.40	450.0
203.00	1232.0
204.00	4353.0
205.10	6371.0
206.10	27688.0
207.10	5400.0
208.00	1430.0
209.00	638.0
210.00	511.0
211.00	1160.0
214.80	308.0
215.10	309.0
216.00	726.0
217.00	7813.0
218.00	917.0
221.00	2999.0
221.80	1001.0
223.00	1704.0
224.10	15985.0
225.00	3933.0
226.00	497.0
227.00	6618.0
228.00	1028.0
229.00	1481.0
231.10	651.0
234.00	495.0
234.90	763.0
235.90	355.0
237.10	885.0
240.00	313.0
241.00	532.0
242.00	919.0
243.00	896.0
244.10	11599.0
245.10	1642.0
246.00	2177.0
247.00	676.0
249.10	455.0
254.20	596.0
255.00	64120.0
256.00	9209.0
257.00	1095.0
258.00	4017.0
259.00	668.0
265.10	1774.0
265.80	429.0
273.00	1893.0
274.00	5192.0
275.00	26800.0
276.00	4000.0
277.00	2452.0
277.90	561.0
281.00	703.0
285.20	446.0
292.90	740.0
296.00	7486.0
297.00	1124.0
302.90	776.0
314.10	504.0
315.00	1161.0
316.00	757.0
323.10	2434.0
324.00	403.0
328.10	341.0
334.00	1431.0
335.00	381.0
341.00	377.0
346.00	538.0
352.10	437.0
353.00	441.0
354.10	729.0
365.00	3085.0
365.90	559.0
372.10	1126.0
373.10	300.0
403.10	570.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

420.90	444.0
421.90	493.0
423.00	3134.0
424.00	1139.0
441.00	9065.0
442.10	65384.0
443.10	13249.0
444.00	1104.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

m/z	Abundance
38.10	614.0
39.10	3290.0
40.00	2523.0
41.10	459.0
44.00	505.0
49.20	545.0
50.10	12486.0
51.10	48808.0
52.10	2403.0
55.10	460.0
56.10	1362.0
57.00	3128.0
61.00	1059.0
62.00	553.0
63.00	2145.0
64.10	432.0
65.00	931.0
68.10	952.0
69.00	54928.0
70.10	351.0
73.00	1330.0
74.10	6215.0
75.10	8351.0
76.10	2906.0
77.10	62368.0
78.10	3861.0
79.00	4336.0
80.00	3093.0
81.00	4598.0
82.00	1306.0
83.00	839.0
85.00	813.0
86.00	1300.0
87.10	534.0
87.90	329.0
91.00	1188.0
92.00	1136.0
93.00	7875.0
93.90	651.0
96.00	469.0
98.00	6833.0
99.00	5521.0
100.00	594.0
101.00	2814.0
103.00	741.0
104.00	1784.0
104.90	1540.0
106.10	469.0
107.00	19416.0
108.00	2879.0
109.20	670.0
110.00	33600.0
111.00	5698.0
112.10	415.0
112.90	300.0
116.00	1059.0
117.00	18624.0
118.00	1335.0
122.00	1647.0
123.00	2429.0
124.10	1005.0
124.90	891.0
127.10	62424.0
128.00	5157.0
129.00	25128.0
129.90	1920.0
130.90	331.0
134.00	771.0
135.00	1994.0
136.00	884.0
137.00	1125.0
137.80	336.0
140.00	357.0
141.00	3848.0
142.10	1110.0
143.00	864.0
144.10	338.0
146.00	562.0
146.90	2205.0
148.00	4203.0
149.00	1292.0
149.90	447.0
151.00	575.0
152.00	355.0
153.00	1455.0
154.00	763.0
155.00	2366.0
156.00	2771.0
156.90	435.0
158.00	749.0
159.00	596.0
159.90	1259.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

161.00	1785.0
162.20	620.0
165.00	1503.0
166.00	1101.0
167.00	8392.0
168.00	4533.0
169.00	792.0
170.00	326.0
171.00	459.0
172.00	691.0
173.00	1018.0
173.90	1705.0
175.10	3277.0
175.90	727.0
177.00	1437.0
177.90	712.0
179.00	6157.0
180.00	4349.0
181.00	1438.0
182.10	417.0
184.00	597.0
185.10	2690.0
186.00	19512.0
187.10	5845.0
188.00	1007.0
189.00	1327.0
190.90	1254.0
192.00	2184.0
193.00	2061.0
194.00	308.0
196.00	3833.0
196.90	877.0
198.00	146560.0
199.00	9880.0
200.00	827.0
201.60	588.0
203.10	1218.0
204.00	5608.0
205.10	10037.0
206.10	41712.0
207.10	7389.0
208.00	2037.0
209.00	1118.0
210.10	537.0
211.00	1707.0
211.90	413.0
214.90	480.0
216.00	1037.0
217.00	11096.0
217.90	1276.0
221.00	5520.0
221.90	1721.0
223.00	2226.0
224.00	23880.0
225.10	6123.0
226.00	920.0
227.00	10896.0
228.10	1678.0
229.00	1940.0
231.10	1070.0
234.00	549.0
234.90	771.0
236.00	395.0
237.00	1522.0
239.00	438.0
239.80	518.0
241.00	651.0
242.00	1061.0
243.00	1281.0
244.10	18512.0
245.00	2401.0
246.00	4314.0
247.00	624.0
248.90	577.0
252.90	539.0
254.00	659.0
255.00	100552.0
256.00	16528.0
257.10	1007.0
258.00	6828.0
259.00	1370.0
265.00	2825.0
266.00	316.0
273.00	3877.0
274.00	7430.0
275.00	44352.0
276.00	5912.0
277.00	4322.0
278.00	689.0
281.10	582.0
281.90	328.0
283.00	319.0
284.10	309.0
285.00	1033.0
293.00	703.0
295.00	301.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

296.00	13975.0
297.00	1846.0
300.90	343.0
302.00	368.0
302.90	1295.0
303.90	649.0
314.00	439.0
315.00	1394.0
316.00	920.0
321.00	540.0
323.10	3442.0
323.90	762.0
326.90	951.0
327.90	575.0
332.00	340.0
332.90	449.0
334.00	2801.0
334.90	539.0
341.10	561.0
346.00	652.0
352.00	1275.0
353.00	897.0
354.10	1606.0
355.00	342.0
365.00	6430.0
366.00	876.0
372.00	1870.0
373.10	457.0
383.00	453.0
390.90	340.0
402.00	989.0
403.10	1167.0
404.00	563.0
420.90	788.0
422.00	851.0
423.10	7193.0
424.00	2186.0
441.00	17240.0
442.10	119024.0
443.10	22800.0
444.00	1971.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

m/z	Abundance
38.00	414.0
39.10	2051.0
40.00	2539.0
44.10	429.0
50.10	9175.0
51.10	33272.0
52.10	1430.0
56.00	919.0
57.00	2414.0
61.00	464.0
62.00	555.0
63.10	1368.0
65.10	887.0
68.00	619.0
69.00	39504.0
73.00	1060.0
74.00	4321.0
75.00	6723.0
76.10	2173.0
77.10	45552.0
78.00	3034.0
79.00	3465.0
80.00	2358.0
81.00	3161.0
82.00	805.0
83.00	899.0
85.10	522.0
86.00	1052.0
86.90	532.0
91.00	999.0
92.00	1246.0
93.00	6105.0
94.10	658.0
96.10	524.0
98.00	4455.0
99.00	3837.0
100.00	327.0
101.00	1995.0
103.00	582.0
104.00	1339.0
105.00	1140.0
106.00	494.0
107.00	15420.0
108.00	1808.0
109.10	504.0
110.00	26392.0
111.00	3967.0
112.00	429.0
116.20	836.0
117.00	14865.0
118.10	1053.0
118.90	364.0
122.00	1214.0
123.00	1634.0
124.00	718.0
124.90	823.0
127.00	48568.0
128.00	3913.0
129.00	20960.0
130.00	1531.0
131.00	483.0
134.00	767.0
135.00	1860.0
136.10	910.0
137.20	1457.0
141.10	2843.0
142.00	989.0
143.00	867.0
145.80	393.0
146.10	376.0
147.00	1467.0
148.00	3968.0
149.10	798.0
150.00	307.0
151.00	367.0
153.00	1152.0
153.90	684.0
155.00	1790.0
156.00	2315.0
157.20	391.0
157.90	539.0
158.90	402.0
160.00	1283.0
160.90	1250.0
162.20	406.0
165.00	1034.0
166.00	1093.0
167.00	6457.0
168.00	3838.0
169.00	690.0
170.10	325.0
170.90	369.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

171.90	896.0
172.90	756.0
174.10	1329.0
175.10	2086.0
176.10	345.0
177.00	1429.0
177.90	433.0
179.00	4168.0
180.00	2930.0
181.00	1257.0
184.00	585.0
185.00	1931.0
186.00	16968.0
187.00	4878.0
188.00	818.0
189.00	962.0
191.10	937.0
192.00	2090.0
192.90	1707.0
194.10	478.0
194.90	353.0
196.00	3251.0
197.10	654.0
198.00	123544.0
199.00	7431.0
200.00	701.0
201.70	482.0
203.00	1017.0
204.00	5227.0
205.00	8579.0
206.10	34256.0
207.00	6874.0
208.10	1574.0
209.10	856.0
210.30	635.0
211.00	1487.0
211.80	379.0
215.00	418.0
216.00	665.0
217.00	9803.0
218.00	1405.0
221.10	4171.0
221.90	1354.0
223.00	1773.0
224.10	20152.0
225.00	4810.0
226.00	738.0
227.00	8987.0
228.00	1483.0
229.00	2190.0
231.00	746.0
234.00	471.0
235.10	703.0
235.90	654.0
237.00	845.0
239.10	328.0
240.10	467.0
241.00	616.0
242.00	1224.0
243.10	1060.0
244.00	15165.0
245.00	1991.0
246.00	4328.0
247.00	948.0
248.90	862.0
253.10	369.0
254.00	437.0
255.00	88912.0
256.00	13063.0
257.00	855.0
258.00	5358.0
259.00	868.0
265.00	2141.0
265.90	300.0
271.00	373.0
273.10	2366.0
274.00	6445.0
275.00	38296.0
276.00	6103.0
277.00	3605.0
278.00	647.0
281.10	569.0
283.00	552.0
284.90	826.0
292.90	1103.0
296.00	11986.0
297.00	1424.0
303.10	1576.0
304.10	532.0
313.90	642.0
315.00	1249.0
316.00	851.0
321.00	456.0
323.00	3858.0
324.00	654.0
327.00	860.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64

328.00	400.0
332.10	423.0
334.00	2717.0
335.10	541.0
341.00	398.0
341.90	347.0
346.00	926.0
352.00	1272.0
353.00	951.0
354.10	1243.0
365.00	5892.0
365.90	834.0
372.00	2364.0
373.00	489.0
383.00	469.0
402.00	945.0
403.00	1015.0
404.00	583.0
421.10	1132.0
422.00	932.0
423.10	6467.0
424.10	1692.0
441.00	18696.0
442.10	125576.0
443.10	25064.0
444.10	2245.0

Instrument :
BNA_M
ClientSampleId :
DFTPP64