
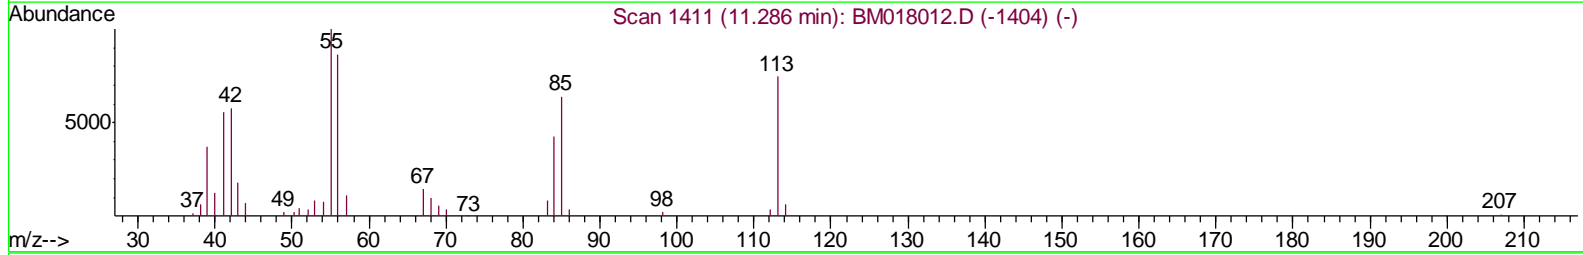
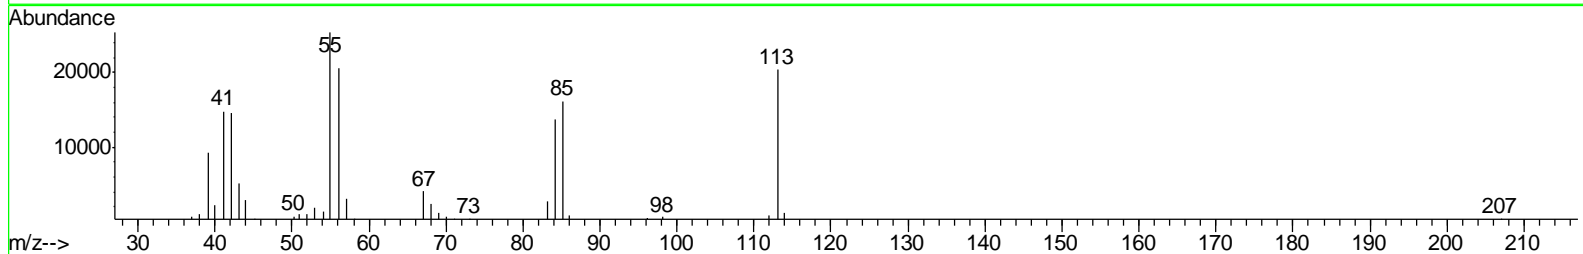


Data File : BM018025.D  
Acq On : 10 Dec 2018 13:37  
Operator : JU/SJ  
Sample : SSTDCCC020  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 11 06:16:08 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM11918MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Dec 10 03:53:59 2018  
Response via : Initial Calibration

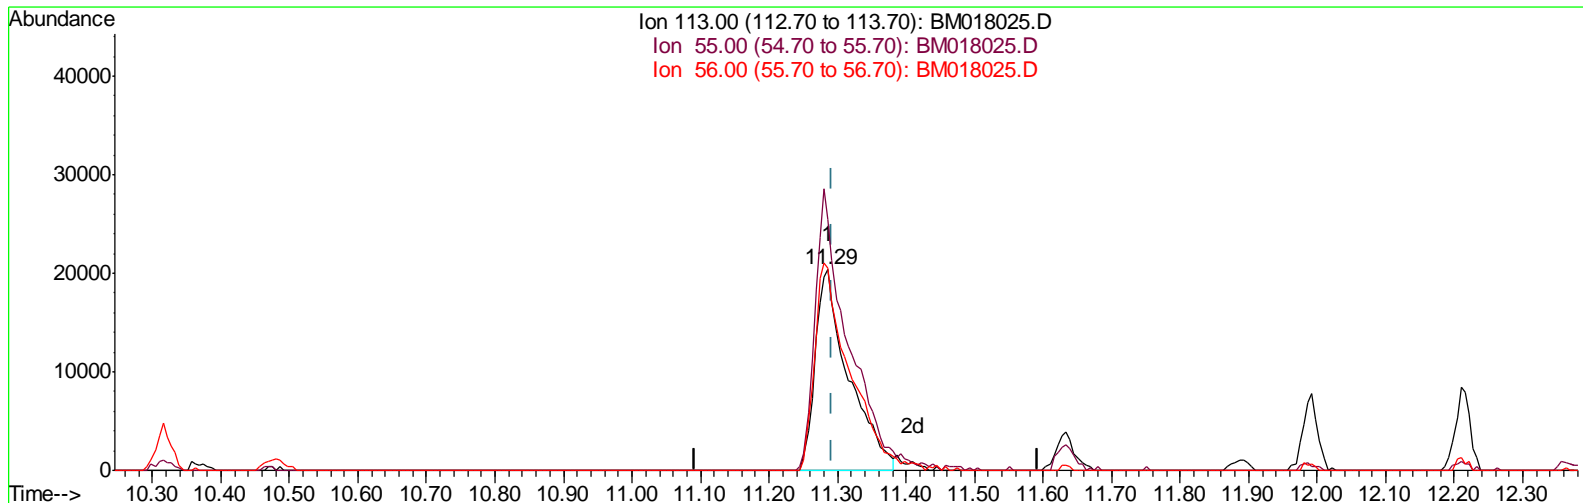

TIC: BM018025.D

(32) Caprolactam

11.286min (-0.006) 19.74ng/ul

response 68766

Ion	Exp%	Act%
113.00	100	100
55.00	138.30	124.75
56.00	110.30	100.86
0.00	0.00	0.00