
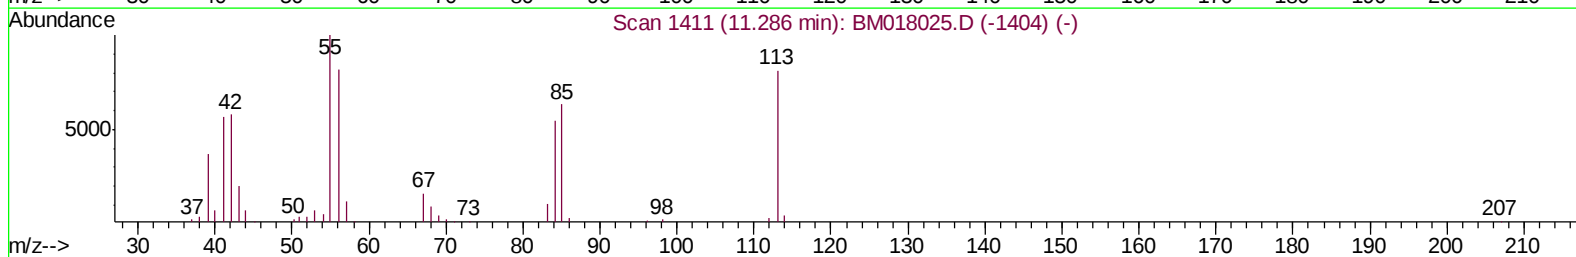
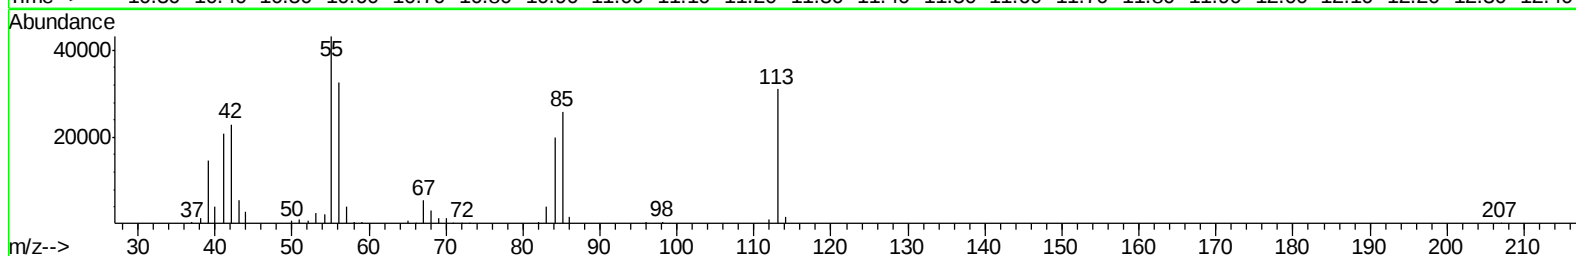


Data File : BM018026.D
Acq On : 10 Dec 2018 15:39
Operator : JU/SJ
Sample : J6155-22
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 11 06:19:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 11 06:16:54 2018
Response via : Initial Calibration

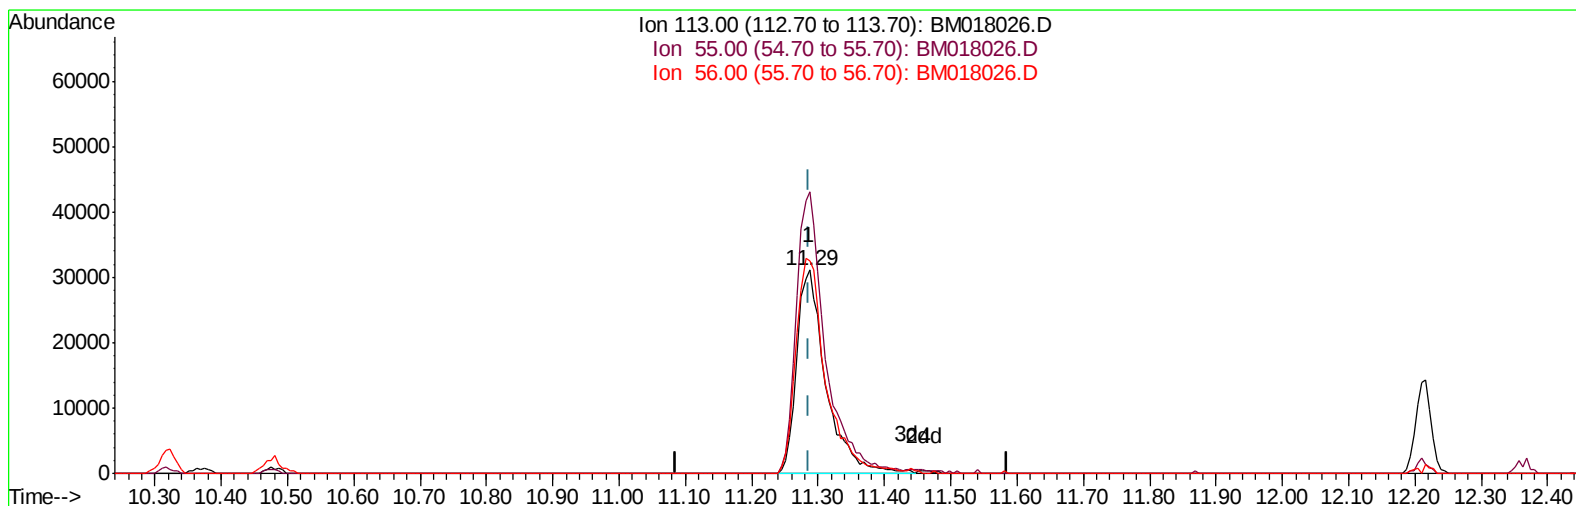

TIC: BM018026.D

(32) Caprolactam

11.287min (+0.000) 29.84ng/ul m

response 93236

Ion	Exp%	Act%
113.00	100	100
55.00	138.30	138.68
56.00	110.30	104.58
0.00	0.00	0.00