
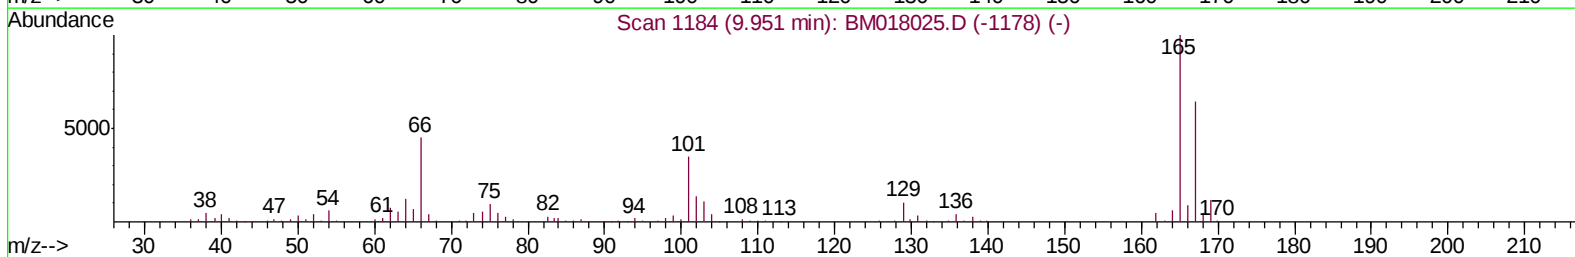
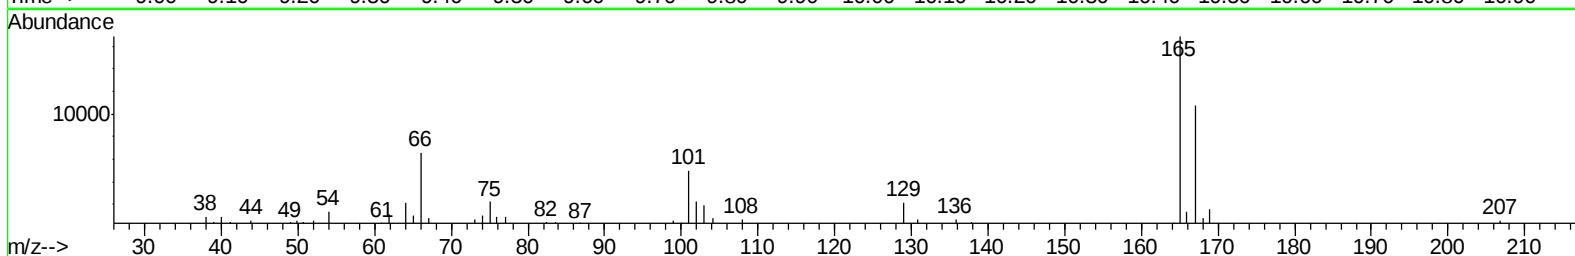


Data File : BM018030.D
Acq On : 10 Dec 2018 18:05
Operator : JU/SJ
Sample : J6155-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Dec 11 06:20:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 11 06:16:54 2018
Response via : Initial Calibration

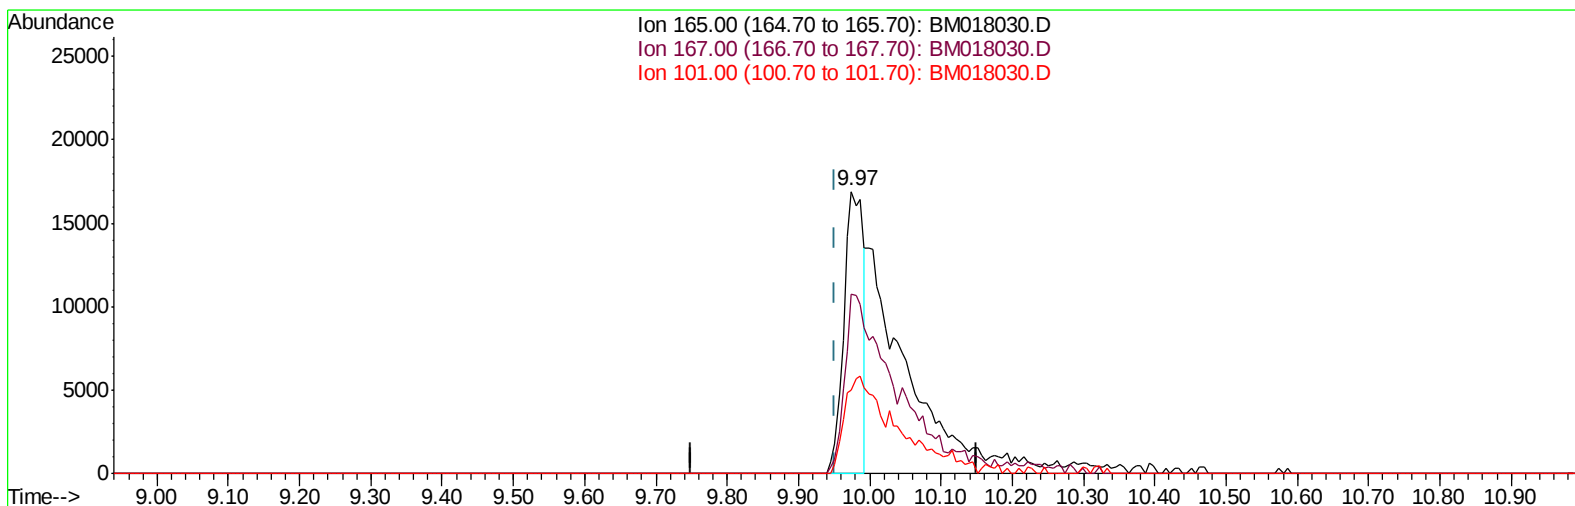

TIC: BM018030.D

(26) 2,4-Dichlorophenol-d3 (S)

9.975min (+0.024) 2.98ng/ul

response 32585

Ion	Exp%	Act%
165.00	100	100
167.00	65.50	63.83
101.00	34.80	29.61
0.00	0.00	0.00