
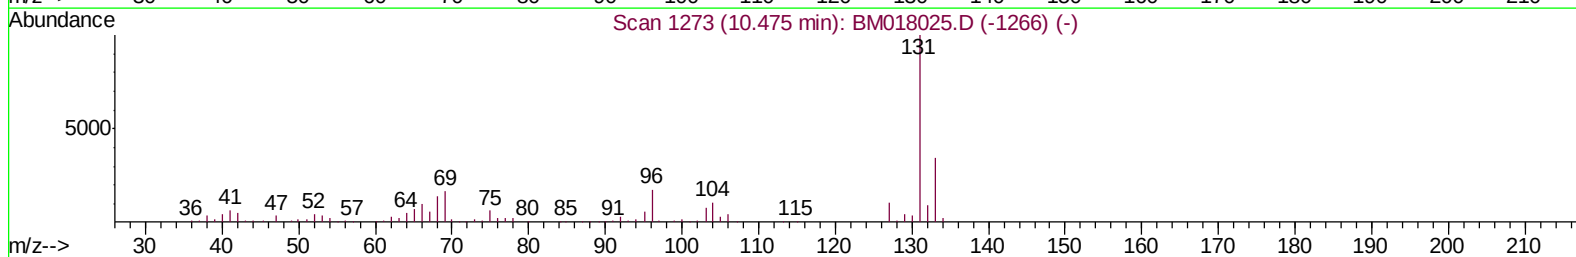
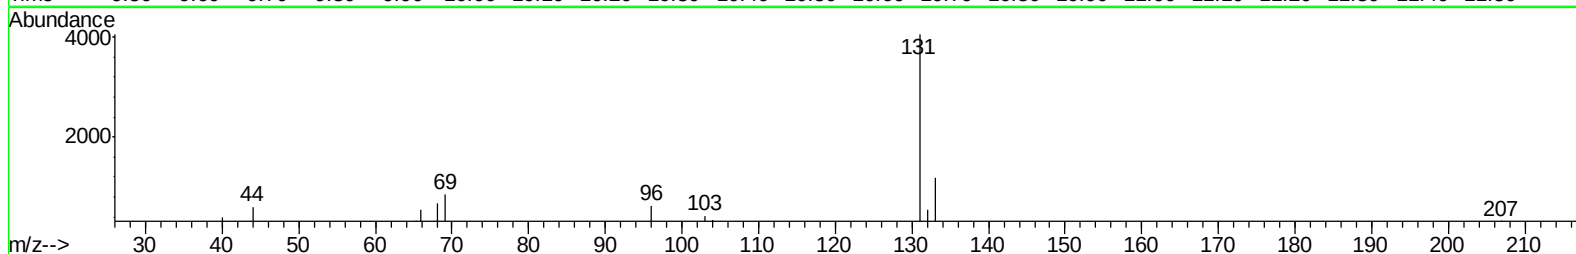


Data File : BM018035.D
Acq On : 10 Dec 2018 21:06
Operator : JU/SJ
Sample : J6155-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 11 06:20:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 11 06:16:54 2018
Response via : Initial Calibration

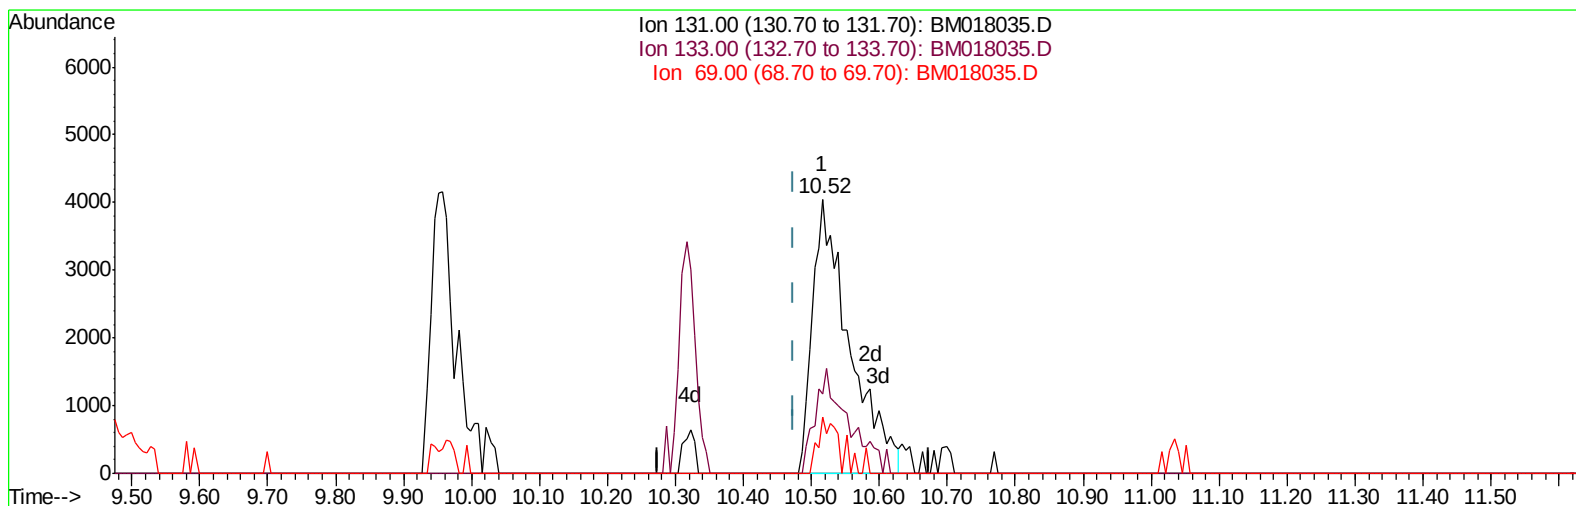

TIC: BM018035.D

(29) 4-Chloroaniline-d4 (S)

10.516min (+0.042) 1.46ng/ul m

response 15254

Ion	Exp%	Act%
131.00	100	100
133.00	32.40	28.99
69.00	18.90	20.74
0.00	0.00	0.00