
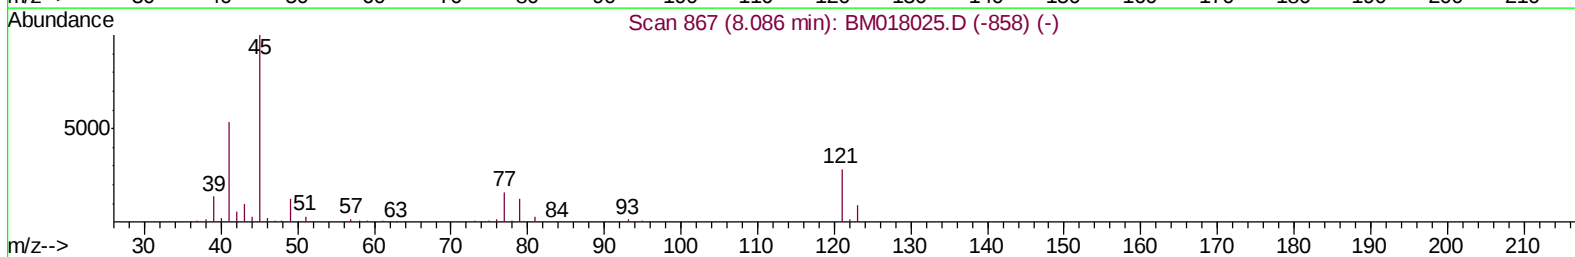
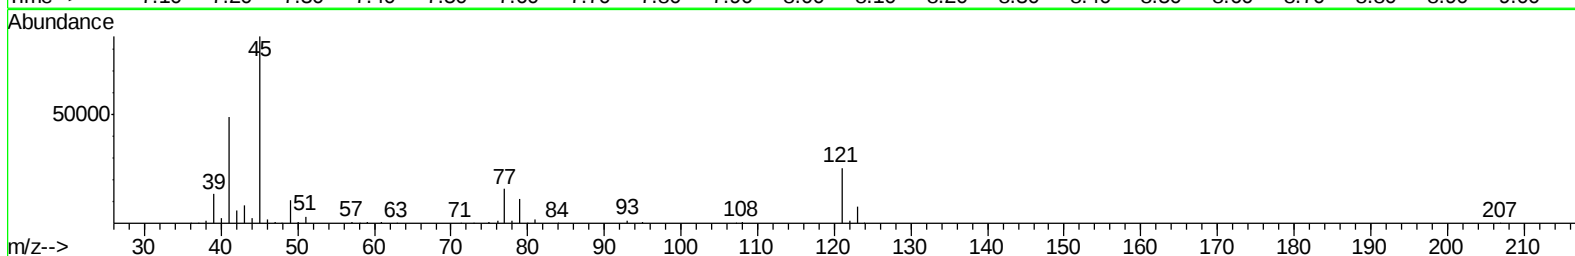


Data File : BM018036.D
Acq On : 10 Dec 2018 21:43
Operator : JU/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 11 06:20:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 11 06:16:54 2018
Response via : Initial Calibration

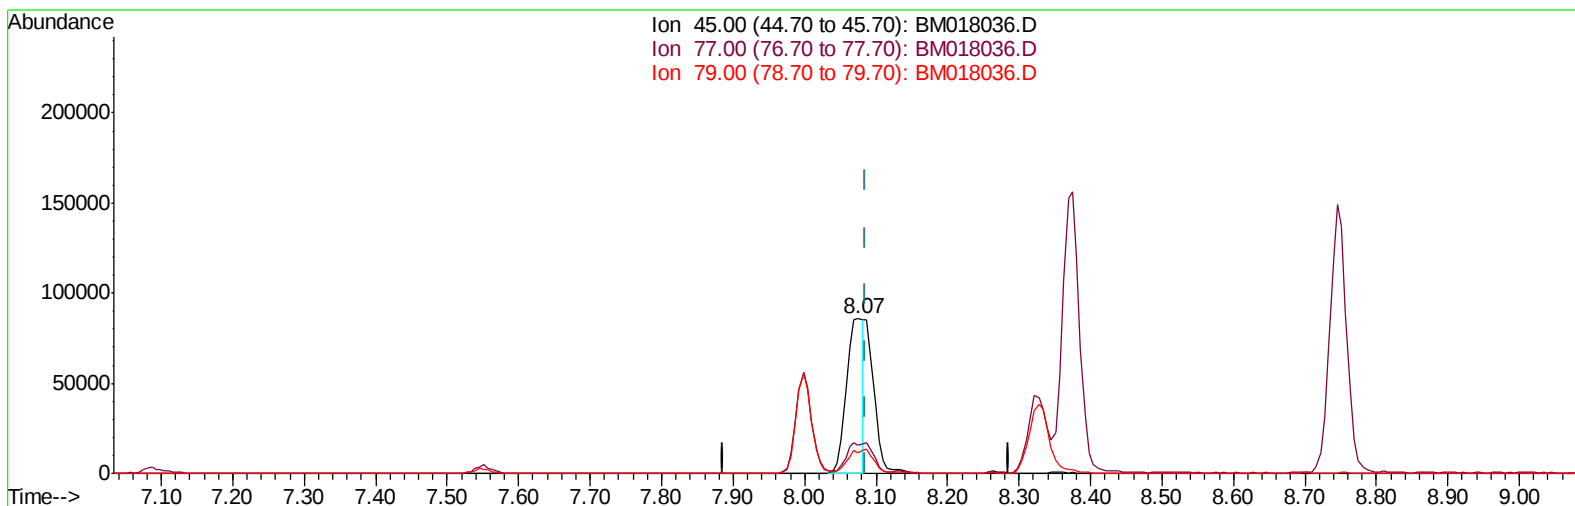

TIC: BM018036.D

(12) 2,2'-oxybis(1-Chloropropane)

8.075min (-0.012) 10.67ng/ul

response 140197

Ion	Exp%	Act%
45.00	100	100
77.00	19.10	18.54
79.00	14.20	13.58
0.00	0.00	0.00