
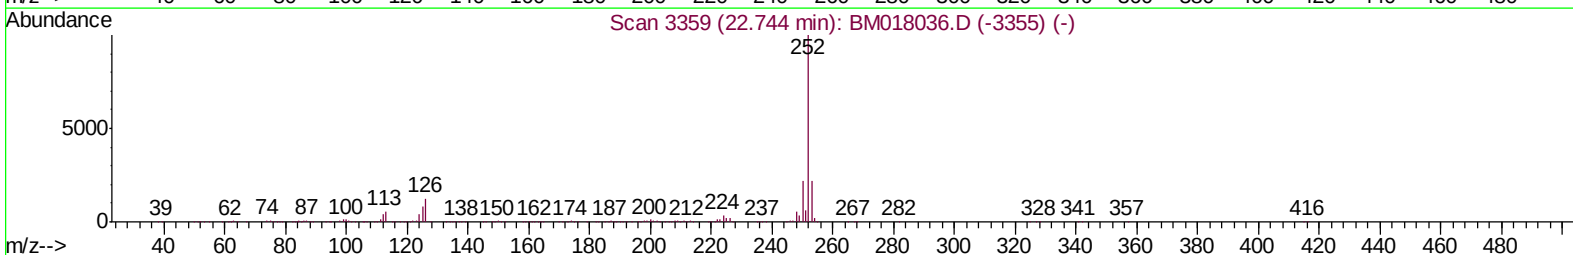
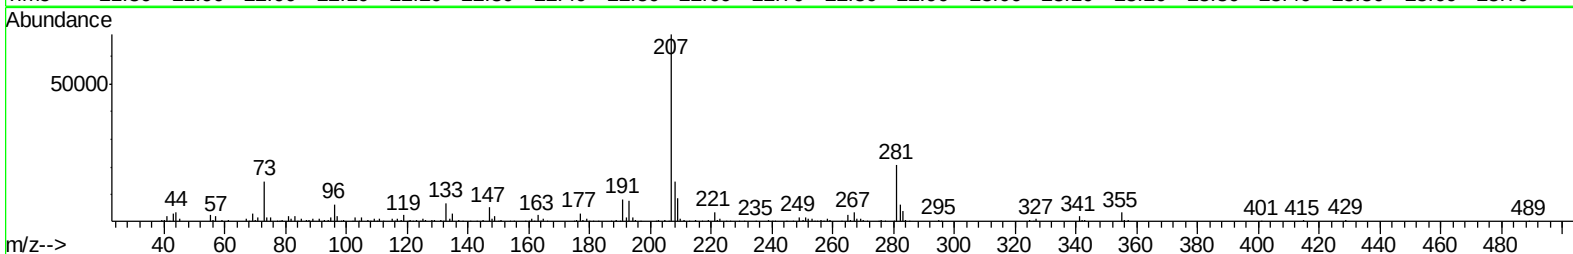


Data File : BM018037.D
Acq On : 10 Dec 2018 22:55
Operator : JU/SJ
Sample : J6077-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 11 06:46:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 11 06:43:59 2018
Response via : Initial Calibration

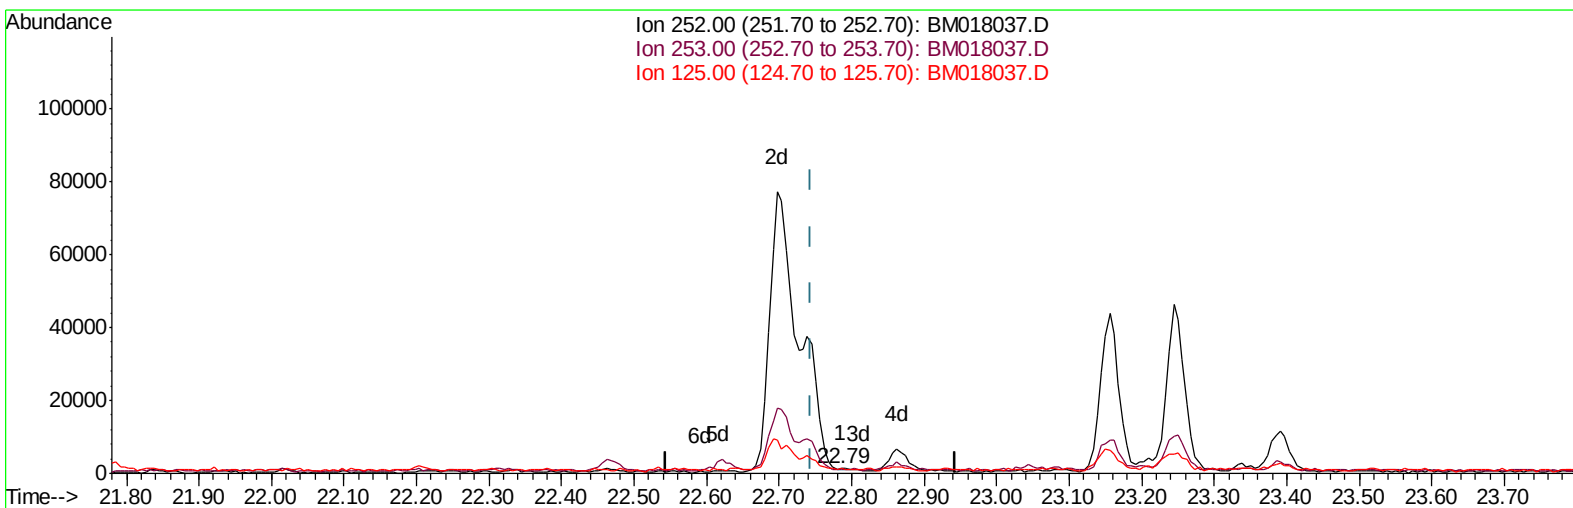

TIC: BM018037.D

(88) Benzo(k)fluoranthene
22.786min (+0.041) 0.00ng/ul
response 257

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	78.38#
125.00	8.90	93.13#
0.00	0.00	0.00