
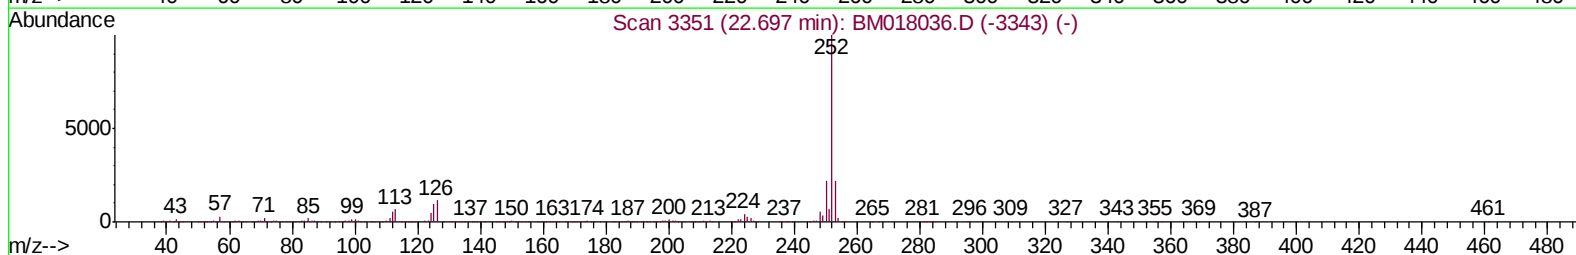
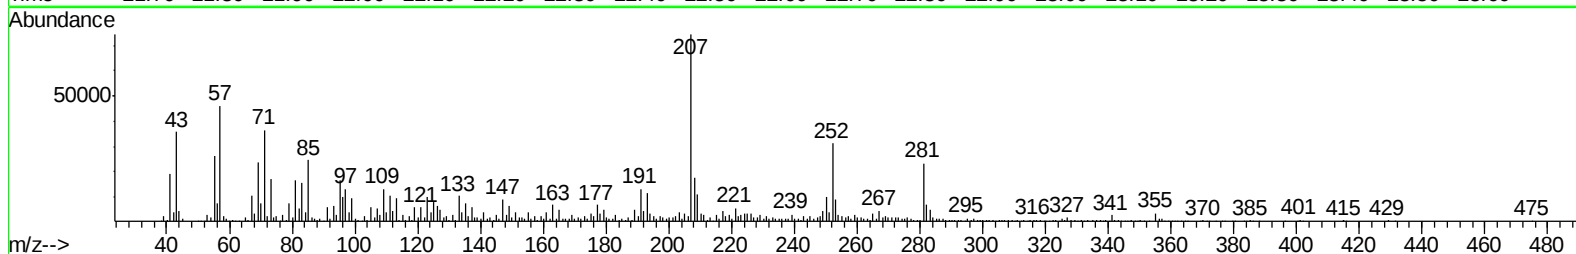


Data File : BM018040.D
Acq On : 11 Dec 2018 00:44
Operator : JU/SJ
Sample : J6077-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 11 06:47:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 11 06:43:59 2018
Response via : Initial Calibration

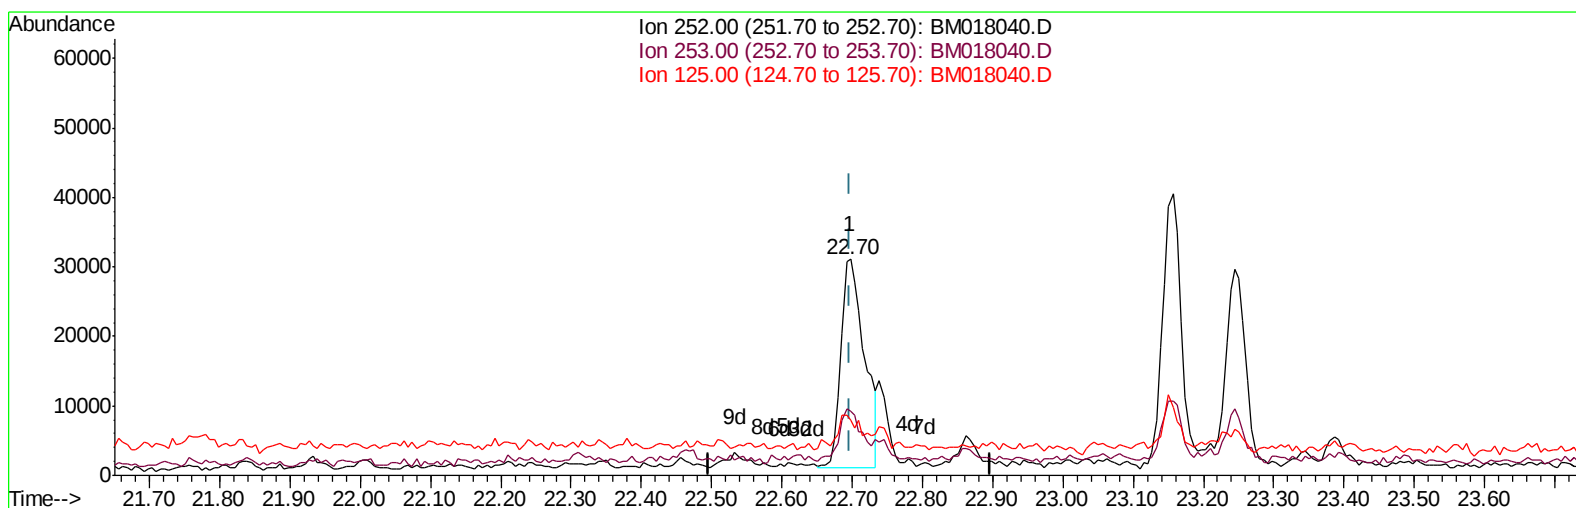

TIC: BM018040.D

(87) Benzo(b)fluoranthene

22.698min (+0.000) 1.35ng/ul m

response 70025

Ion	Exp%	Act%
252.00	100	100
253.00	21.20	29.37#
125.00	9.10	25.28#
0.00	0.00	0.00