

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121018\
 Data File : BM018035.D
 Acq On : 10 Dec 2018 21:06
 Operator : JU/SJ
 Sample : J6155-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4182

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	35	rVB	31754	42894	0.88%	0.095%
2	3.752	125	130	136	rVB	16224	23362	0.48%	0.052%
3	3.946	158	163	169	rBV5	14860	23796	0.49%	0.053%
4	4.740	291	298	309	rVB2	39931	66388	1.36%	0.148%
5	5.981	503	509	515	rVB2	14200	20753	0.43%	0.046%
6	6.746	633	639	651	rBV	130673	265433	5.45%	0.590%
7	6.905	658	666	678	rBV	544629	858312	17.63%	1.909%
8	7.087	691	697	713	rBV	596608	997273	20.48%	2.218%
9	7.552	768	776	789	rBV	567748	952790	19.57%	2.119%
10	8.263	891	897	909	rBV	426893	767494	15.76%	1.707%
11	8.340	909	910	916	rVB3	4155	5067	0.10%	0.011%
12	8.705	965	972	983	rBV	641501	1095660	22.50%	2.437%
13	9.087	1033	1037	1043	rBV5	2412	5004	0.10%	0.011%
14	9.416	1086	1093	1105	rBV	552936	971412	19.95%	2.161%
15	9.951	1177	1184	1217	rBV	550703	1395251	28.66%	3.104%
16	10.316	1238	1246	1260	rVB	875169	1445914	29.70%	3.216%
17	10.504	1275	1278	1279	rBV2	8668	8460	0.17%	0.019%
18	10.522	1279	1281	1293	rVB5	9836	21235	0.44%	0.047%
19	11.028	1364	1367	1377	rVB3	3841	7374	0.15%	0.016%
20	11.951	1518	1524	1530	rBV3	8471	18601	0.38%	0.041%
21	12.540	1619	1624	1632	rBV4	10420	18793	0.39%	0.042%
22	12.798	1664	1668	1674	rBV4	15328	22747	0.47%	0.051%
23	13.622	1800	1808	1822	rBV	1712006	2556082	52.50%	5.686%
24	13.887	1844	1853	1868	rBV	2012387	3012671	61.87%	6.701%
25	14.198	1900	1906	1917	rBV2	1299983	2056084	42.23%	4.574%
26	14.287	1917	1921	1930	rVV5	20157	42630	0.88%	0.095%
27	14.469	1945	1952	1958	rBV3	40601	108945	2.24%	0.242%
28	14.969	2033	2037	2043	rVV	7806	10679	0.22%	0.024%
29	15.045	2047	2050	2054	rVB2	15989	19236	0.40%	0.043%
30	15.204	2070	2077	2089	rBV	2540467	3793449	77.91%	8.438%
31	15.345	2095	2101	2113	rBV	811425	1264313	25.97%	2.812%
32	15.445	2114	2118	2126	rVB	30345	52716	1.08%	0.117%
33	16.745	2335	2339	2344	rBV3	6001	9631	0.20%	0.021%
34	16.957	2369	2375	2386	rBV2	1826835	2498562	51.31%	5.558%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121018\
Data File : BM018035.D
Acq On : 10 Dec 2018 21:06
Operator : JU/SJ
Sample : J6155-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4182

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Title : SVOA CALIBRATION

35	17.057	2386	2392	2406	rVV	2805909	4126583	84.75%	9.179%
36	17.869	2525	2530	2541	rBV3	44862	89832	1.84%	0.200%
37	18.998	2719	2722	2728	rBV	29341	45567	0.94%	0.101%
38	19.163	2745	2750	2756	rBV4	53807	86085	1.77%	0.191%
39	19.257	2761	2766	2768	rVV2	24919	35148	0.72%	0.078%
40	19.304	2771	2774	2775	rVV3	6392	5954	0.12%	0.013%
41	19.363	2778	2784	2803	rVV	3401843	4855331	99.72%	10.800%
42	19.533	2810	2813	2816	rBV5	4690	7339	0.15%	0.016%
43	20.357	2951	2953	2954	rBV2	8662	5907	0.12%	0.013%
44	21.168	3086	3091	3106	rBV	2124961	3098395	63.63%	6.892%
45	22.204	3265	3267	3275	rVB2	73538	98089	2.01%	0.218%
46	22.692	3347	3350	3356	rVB2	106553	149911	3.08%	0.333%
47	23.209	3431	3438	3449	rBV	2566571	4869104	100.00%	10.831%
48	23.345	3454	3461	3475	rVB	1450061	2814005	57.79%	6.260%
49	23.845	3543	3546	3553	rVB4	126035	209057	4.29%	0.465%


Sum of corrected areas: 44955318

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121018\
Data File : BM018035.D
Acq On : 10 Dec 2018 21:06
Operator : JU/SJ
Sample : J6155-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4182

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

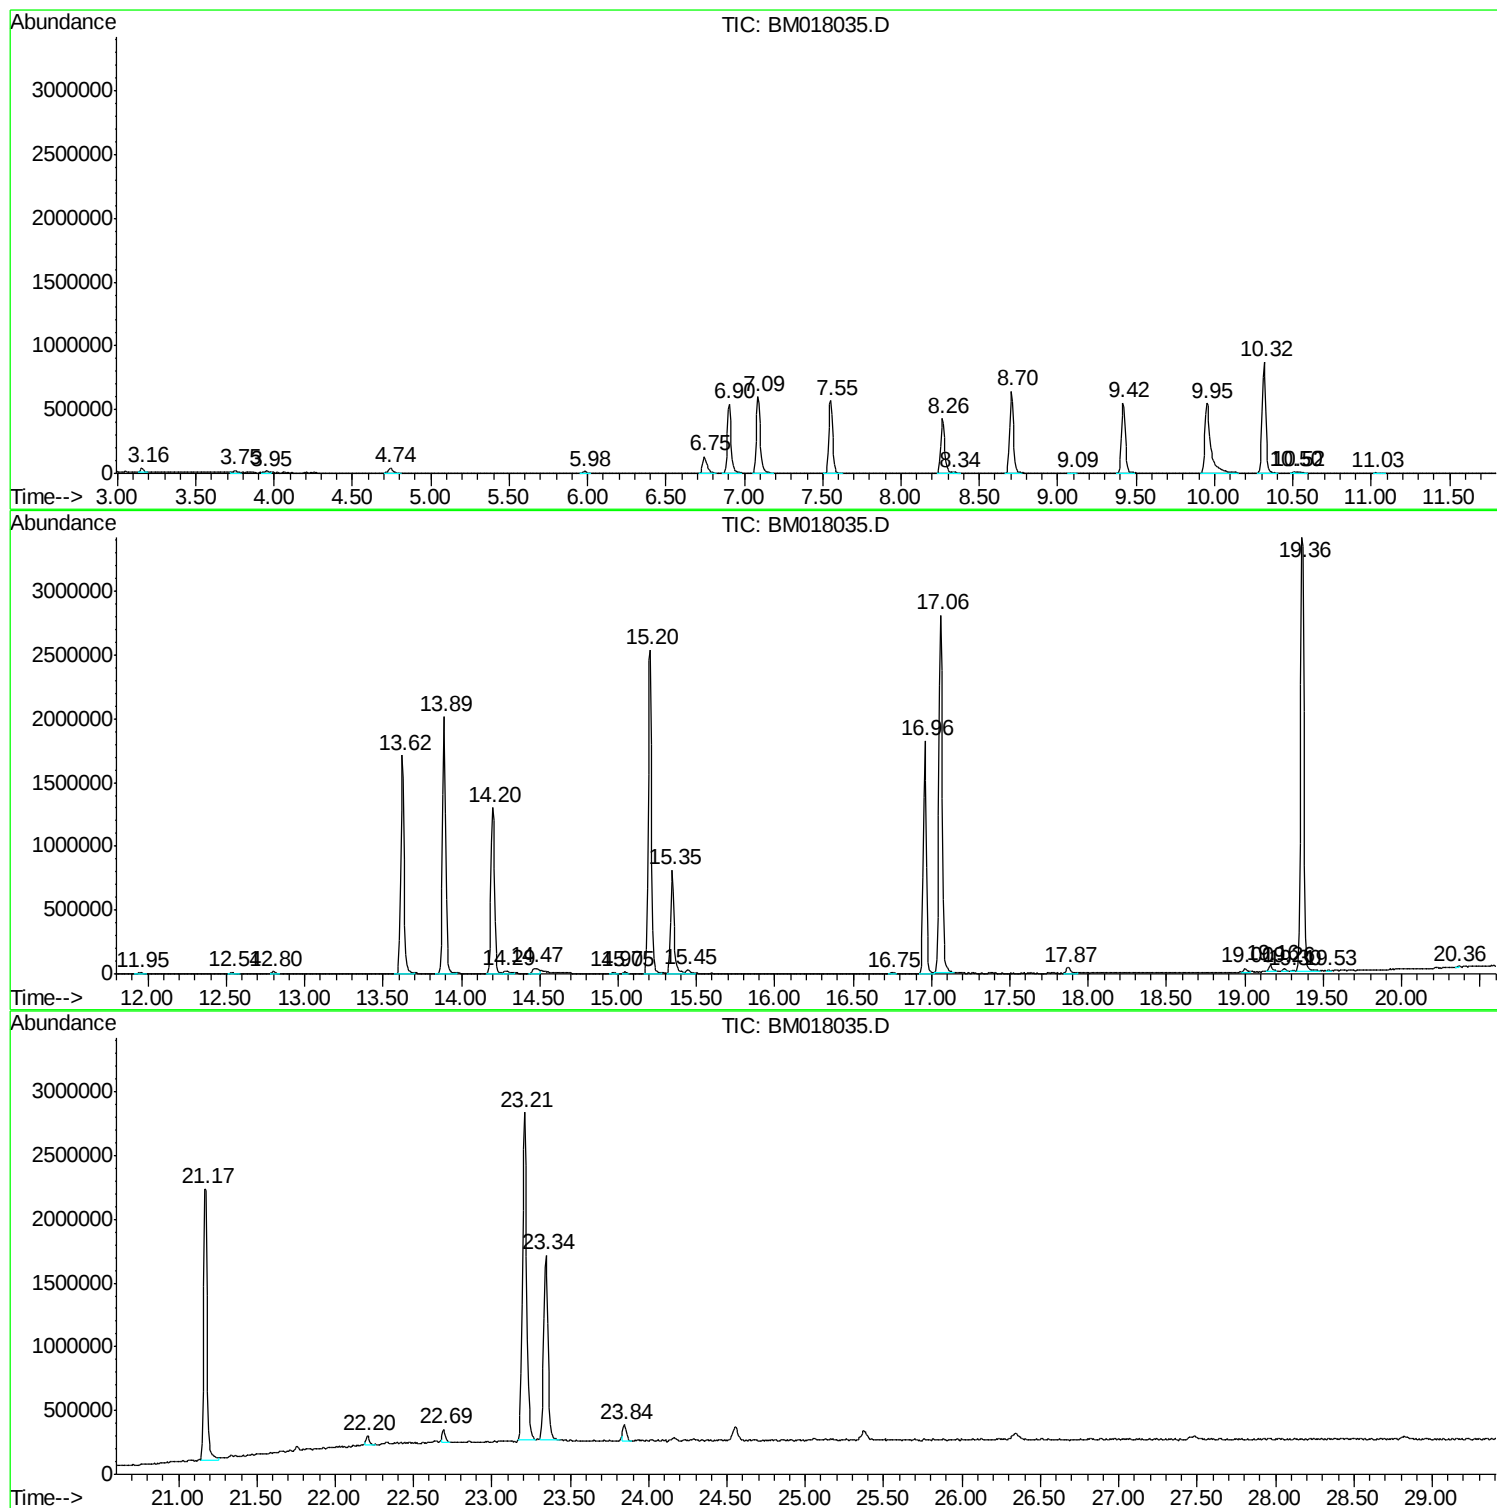

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121018\
Data File : BM018035.D
Acq On : 10 Dec 2018 21:06
Operator : JU/SJ
Sample : J6155-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4182

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121018\
Data File : BM018035.D
Acq On : 10 Dec 2018 21:06
Operator : JU/SJ
Sample : J6155-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4182

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc