

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037928.D
 Acq On : 10 Dec 2022 10:19
 Operator : CG/JU
 Sample : PB149532BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK532

Quant Time: Dec 11 21:25:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.081	152	190031	20.000	ng/ul	0.00
20) Naphthalene-d8	10.898	136	714505	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.710	164	355808	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.451	188	676042	20.000	ng/ul	0.00
79) Chrysene-d12	21.615	240	666573	20.000	ng/ul	0.00
88) Perylene-d12	24.097	264	718423	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	18892	4.514	ng/uL	0.00
4) Pyridine-d5	3.857	84	267819	21.571	ng/ul	0.00
7) Phenol-d5	7.234	99	379968	24.606	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.404	67	234580	24.947	ng/ul	0.00
11) 2-Chlorophenol-d4	7.604	132	333877	26.357	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	285930	23.721	ng/ul	0.00
21) Nitrobenzene-d5	9.251	128	154004	27.223	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	159555	26.913	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.516	165	270576	24.029	ng/ul	0.00
31) 4-Chloroaniline-d4	11.039	131	369209	23.753	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	684233	26.974	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	827004	26.675	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	85412	19.757	ng/ul	0.00
60) Fluorene-d10	15.698	176	598279	26.473	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	58491	16.183	ng/ul	0.00
73) Anthracene-d10	17.545	188	950871	30.137	ng/ul	0.00
81) Pyrene-d10	19.833	212	1089888	27.219	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.939	264	1103435	30.750	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.509	149	29857	1.122	ng/ul	96
96) Benzo(g,h,i)perylene	27.509	276	41792	1.038	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037928.D
Acq On : 10 Dec 2022 10:19
Operator : CG/JU
Sample : PB149532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK532

Quant Time: Dec 11 21:25:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration




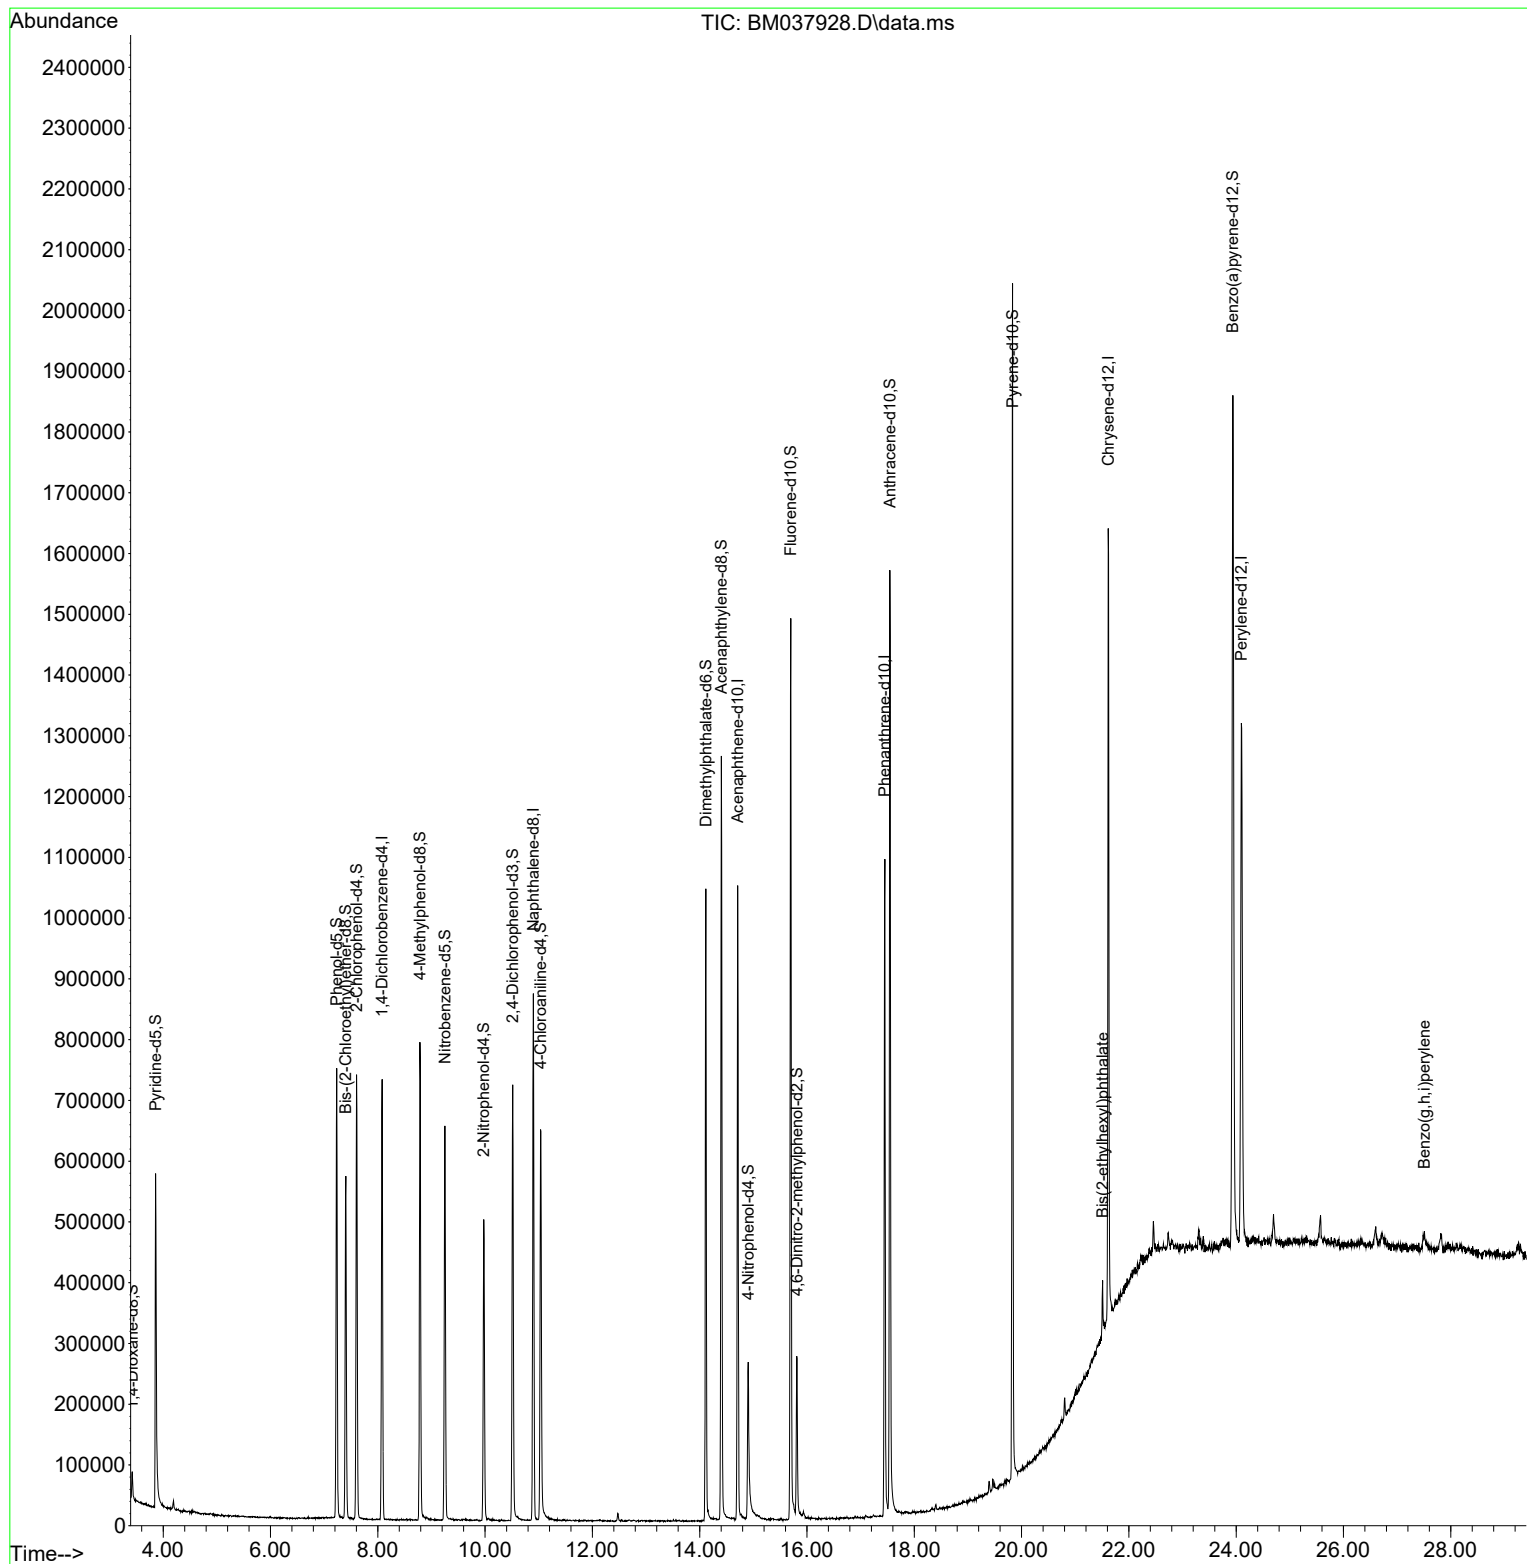


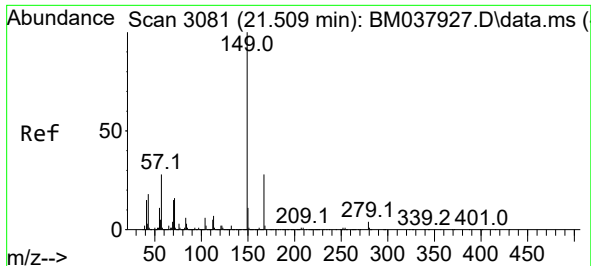

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.122 ng/ul
 RT: 21.509 min Scan# 3081
 Delta R.T. -0.000 min
 Lab File: BM037928.D
 Acq: 10 Dec 2022 10:19

Instrument :
 BNA_M
 ClientSampleId :
 SBLK532

Tgt Ion:	149	Resp:	29857
Ion Ratio	Lower	Upper	
149	100		
167	24.5	21.5	32.3
279	4.3	3.2	4.8

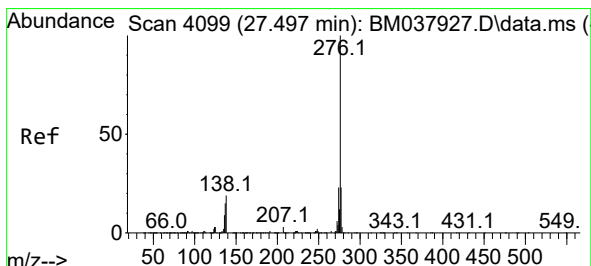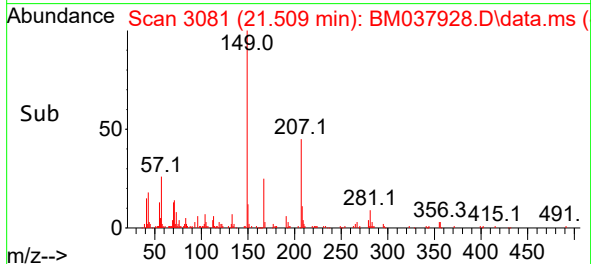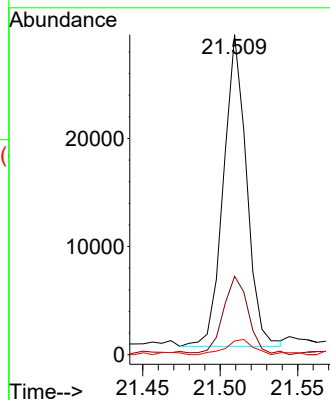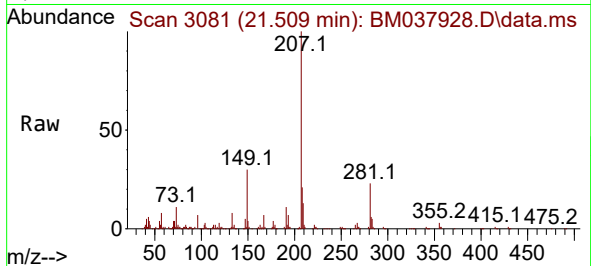

#96
 Benzo(g,h,i)perylene
 Concen: 1.038 ng/ul
 RT: 27.509 min Scan# 4101
 Delta R.T. 0.006 min
 Lab File: BM037928.D
 Acq: 10 Dec 2022 10:19

Tgt Ion:	276	Resp:	41792
Ion Ratio	Lower	Upper	
276	100		
138	22.7	17.1	25.7
277	24.1	18.2	27.4

