

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037943.D
 Acq On : 10 Dec 2022 20:55
 Operator : CG/JU
 Sample : PB149543BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK543

Quant Time: Dec 11 21:29:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	222854	20.000	ng/ul	0.00
20) Naphthalene-d8	10.898	136	860285	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.710	164	449284	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	795159	20.000	ng/ul	0.00
79) Chrysene-d12	21.615	240	714524	20.000	ng/ul	0.00
88) Perylene-d12	24.097	264	751524	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	22767	4.639	ng/uL	0.00
4) Pyridine-d5	3.858	84	330709	22.714	ng/ul	0.00
7) Phenol-d5	7.234	99	425531	23.498	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.398	67	260161	23.593	ng/ul	0.00
11) 2-Chlorophenol-d4	7.604	132	358143	24.108	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	319543	22.605	ng/ul	0.00
21) Nitrobenzene-d5	9.251	128	175110	25.708	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	177623	24.884	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.516	165	310631	22.911	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	423877	22.649	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	795537	24.837	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	963883	24.622	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	89413	16.379	ng/ul	0.00
60) Fluorene-d10	15.692	176	685816	24.032	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	55706	13.103	ng/ul	0.00
73) Anthracene-d10	17.545	188	997556	26.880	ng/ul	0.00
81) Pyrene-d10	19.827	212	1079181	25.143	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.933	264	1057518	28.173	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.509	149	29340	1.029	ng/ul	97
96) Benzo(g,h,i)perylene	27.497	276	42320	1.005	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037943.D
Acq On : 10 Dec 2022 20:55
Operator : CG/JU
Sample : PB149543BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK543

Quant Time: Dec 11 21:29:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration




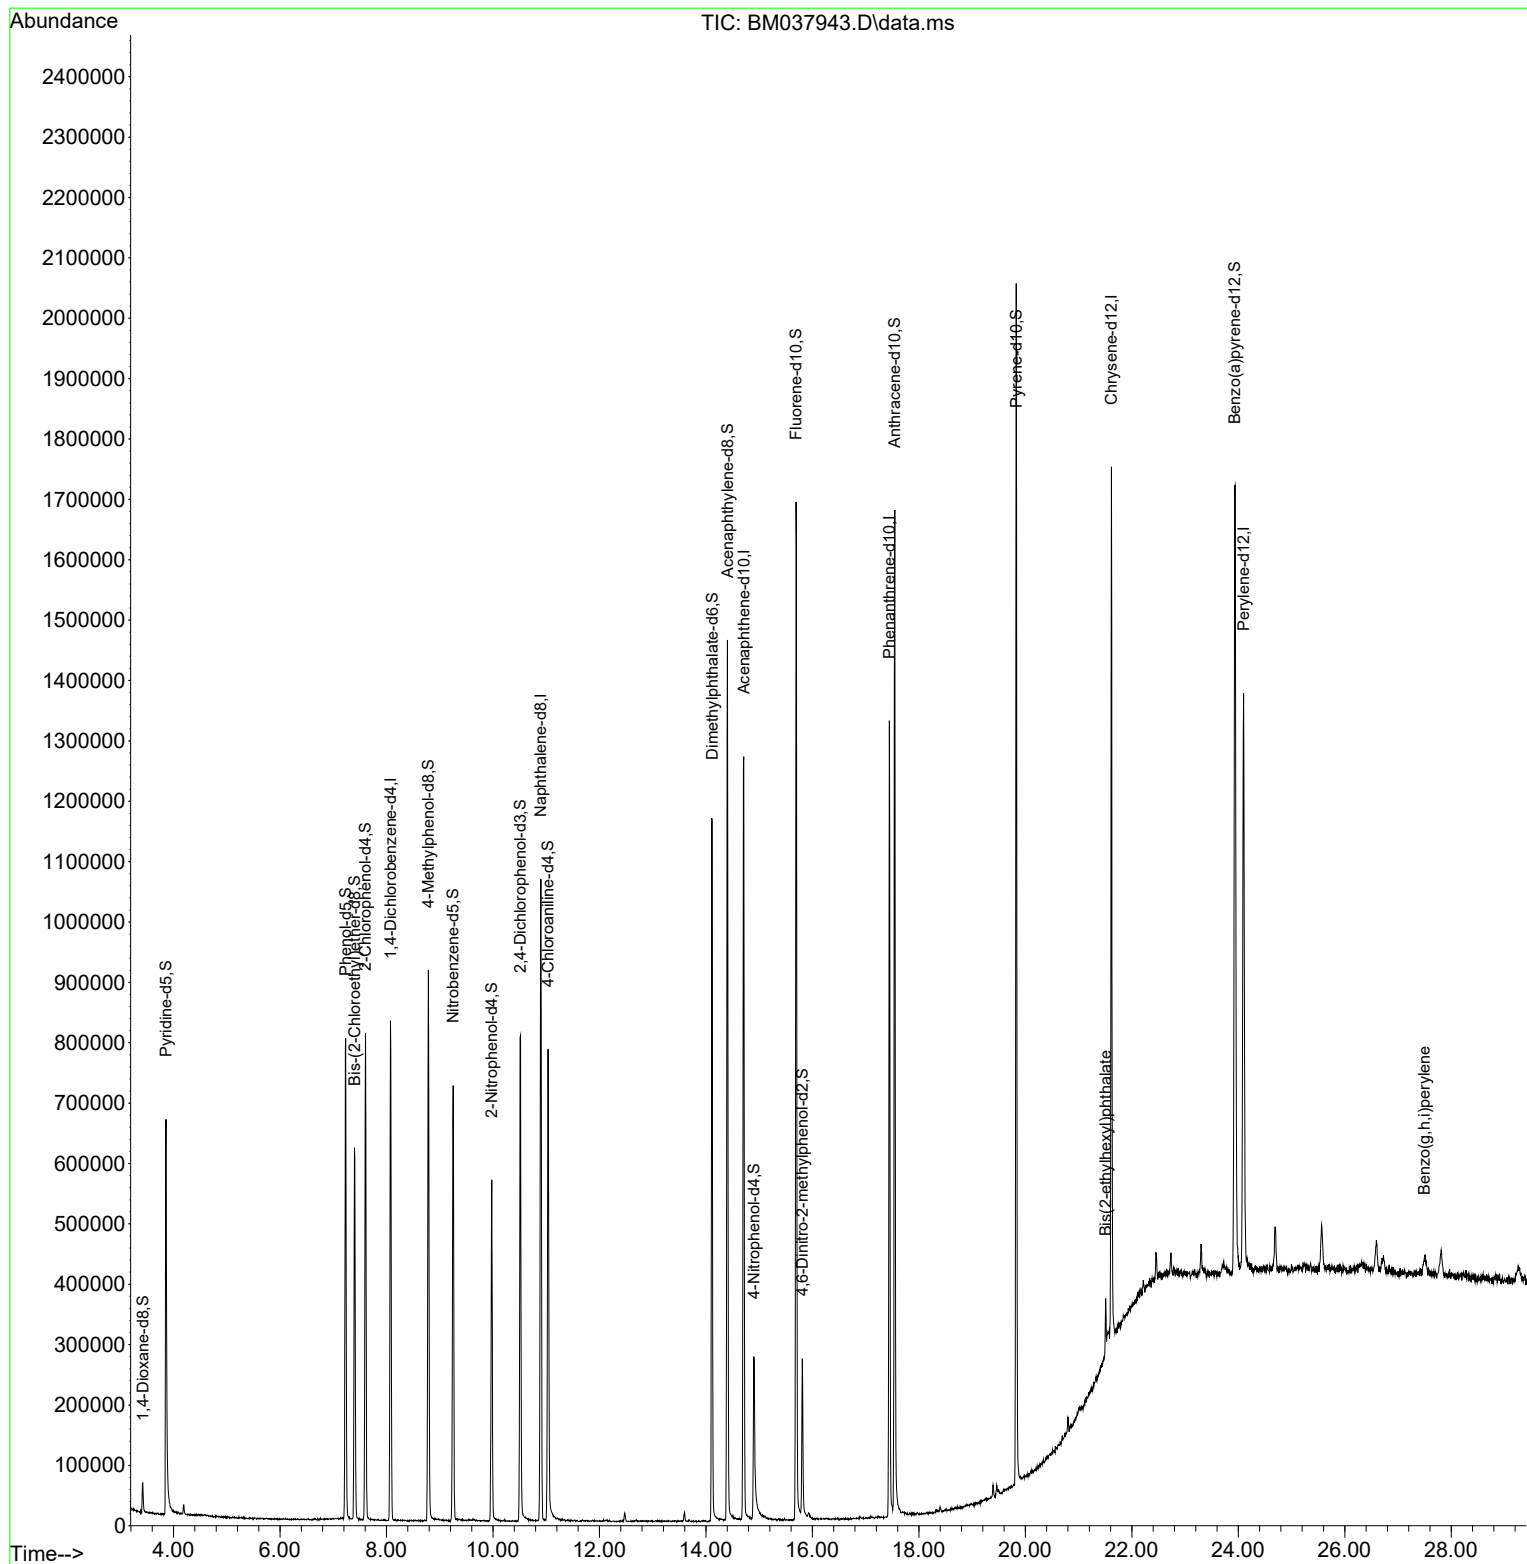


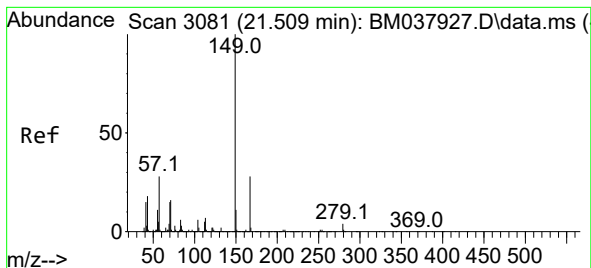

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.029 ng/ul
RT: 21.509 min Scan# 3115
Delta R.T. 0.000 min
Lab File: BM037943.D
Acq: 10 Dec 2022 20:55

Instrument :
BNA_M
ClientSampleId :
SBLK543

Tgt Ion:	149	Resp:	29340
Ion Ratio	Lower	Upper	
149	100		
167	28.3	21.5	32.3
279	3.7	3.2	4.8

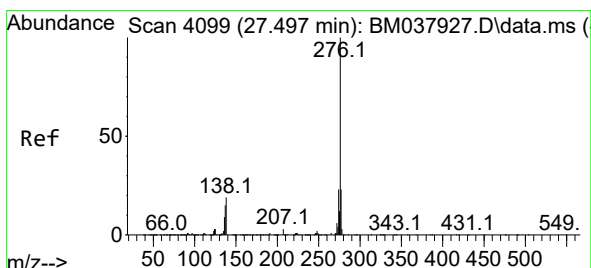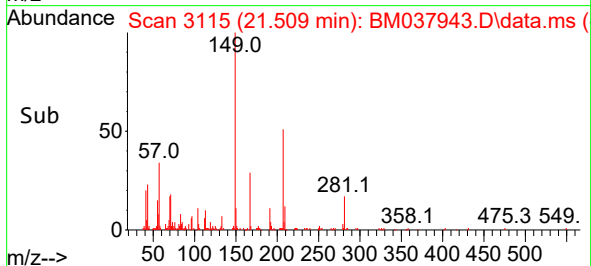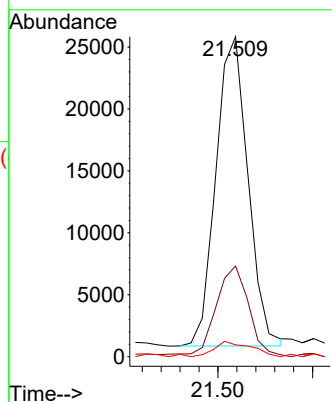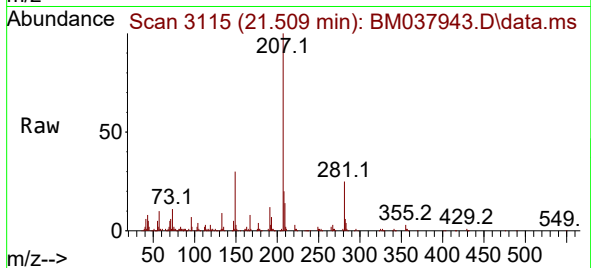

#96
Benzo(g,h,i)perylene
Concen: 1.005 ng/ul
RT: 27.497 min Scan# 4133
Delta R.T. -0.006 min
Lab File: BM037943.D
Acq: 10 Dec 2022 20:55

Tgt Ion:	276	Resp:	42320
Ion Ratio	Lower	Upper	
276	100		
138	18.2	17.1	25.7
277	29.0	18.2	27.4#

