

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037953.D
 Acq On : 11 Dec 2022 02:58
 Operator : CG/JU
 Sample : N5927-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ88

Quant Time: Dec 11 21:31:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	166010	20.000	ng/ul	0.00
20) Naphthalene-d8	10.898	136	608209	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.704	164	320718	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	642317	20.000	ng/ul	0.00
79) Chrysene-d12	21.615	240	685588	20.000	ng/ul	0.00
88) Perylene-d12	24.091	264	753538	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.416	96	18089	4.947	ng/uL	0.00
4) Pyridine-d5	3.857	84	115499	10.649	ng/ul	0.00
7) Phenol-d5	7.228	99	91406	6.776	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.398	67	281397	34.257	ng/ul	0.00
11) 2-Chlorophenol-d4	7.604	132	297302	26.865	ng/ul	0.00
15) 4-Methylphenol-d8	8.781	113	163574	15.534	ng/ul	-0.01
21) Nitrobenzene-d5	9.251	128	184532	38.320	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	181647	35.995	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	293948	30.667	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.033	131	381522	28.835	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166	917697	40.135	ng/ul	-0.01
49) Acenaphthylene-d8	14.404	160	1080443	38.663	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	20663	5.303	ng/ul	0.00
60) Fluorene-d10	15.692	176	796986	39.123	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	97411	28.366	ng/ul	0.00
73) Anthracene-d10	17.545	188	1338175	44.639	ng/ul	0.00
81) Pyrene-d10	19.827	212	1673643	40.639	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.933	264	1716553	45.607	ng/ul	-0.01
Target Compounds						
78) Di-n-butylphthalate	18.398	149	48266	1.315	ng/ul#	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037953.D
Acq On : 11 Dec 2022 02:58
Operator : CG/JU
Sample : N5927-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ88

Quant Time: Dec 11 21:31:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

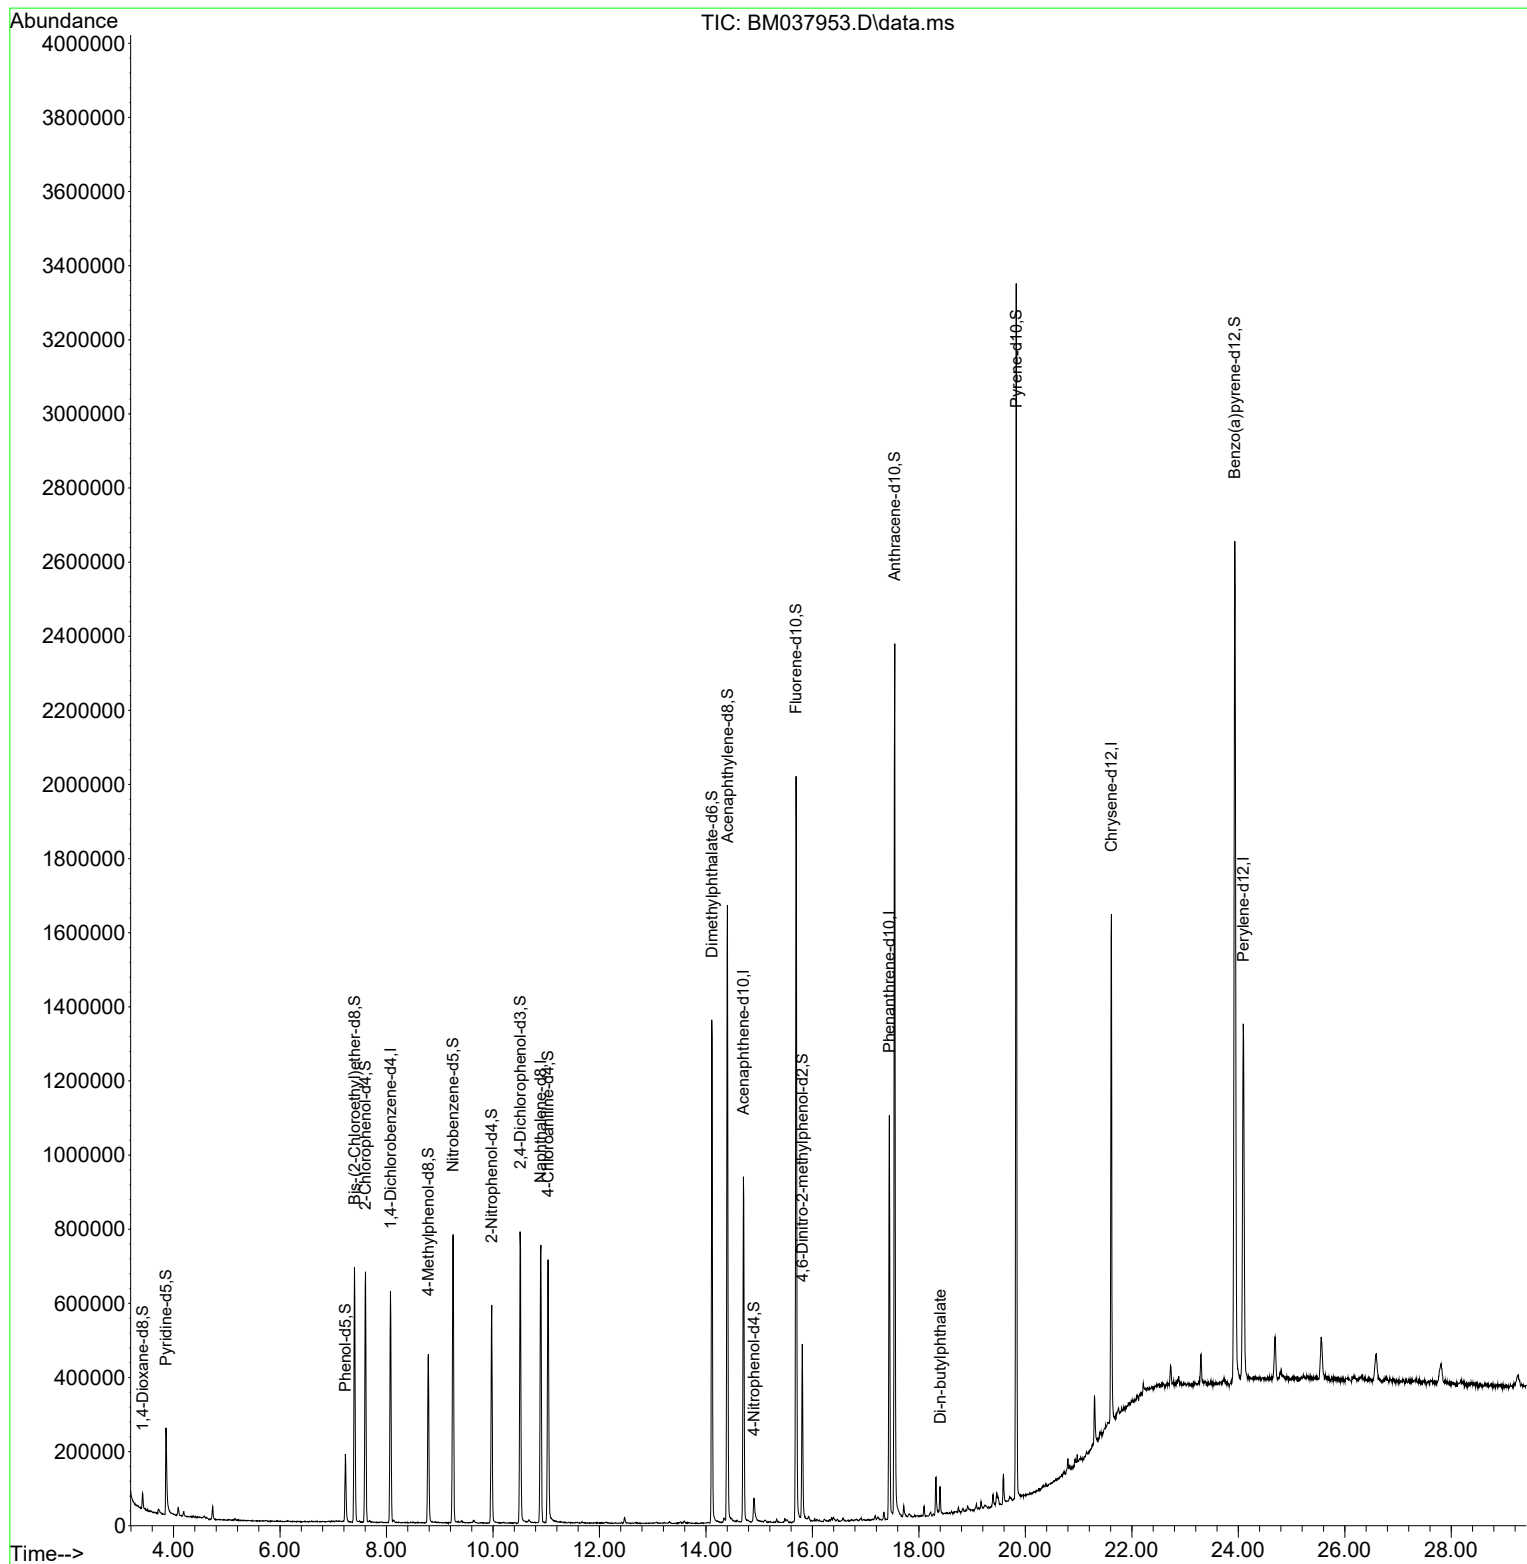

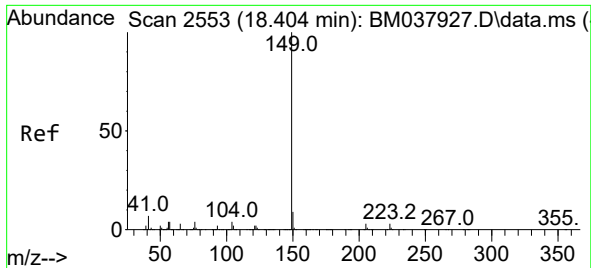

#78
 Di-n-butylphthalate
 Concen: 1.315 ng/ul
 RT: 18.398 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM037953.D
 Acq: 11 Dec 2022 02:58

Instrument :
 BNA_M
 ClientSampleId :
 EXZ88

Tgt Ion:149 Resp: 48266
 Ion Ratio Lower Upper
 149 100
 150 9.6 7.3 10.9
 104 6.1 3.4 5.2#

