




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037928.D
Acq On : 10 Dec 2022 10:19
Operator : CG/JU
Sample : PB149532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK532

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/12/2022
Supervised By :mohammad ahmed 12/12/2022

Quant Time: Dec 11 21:25:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

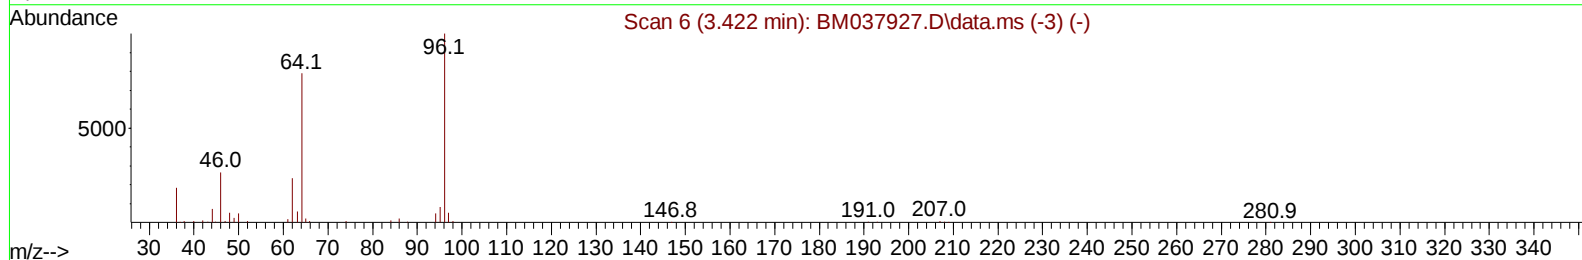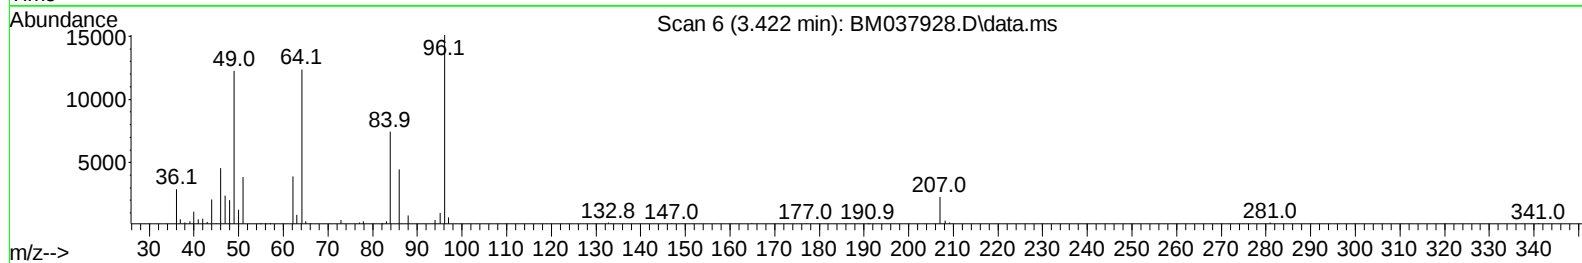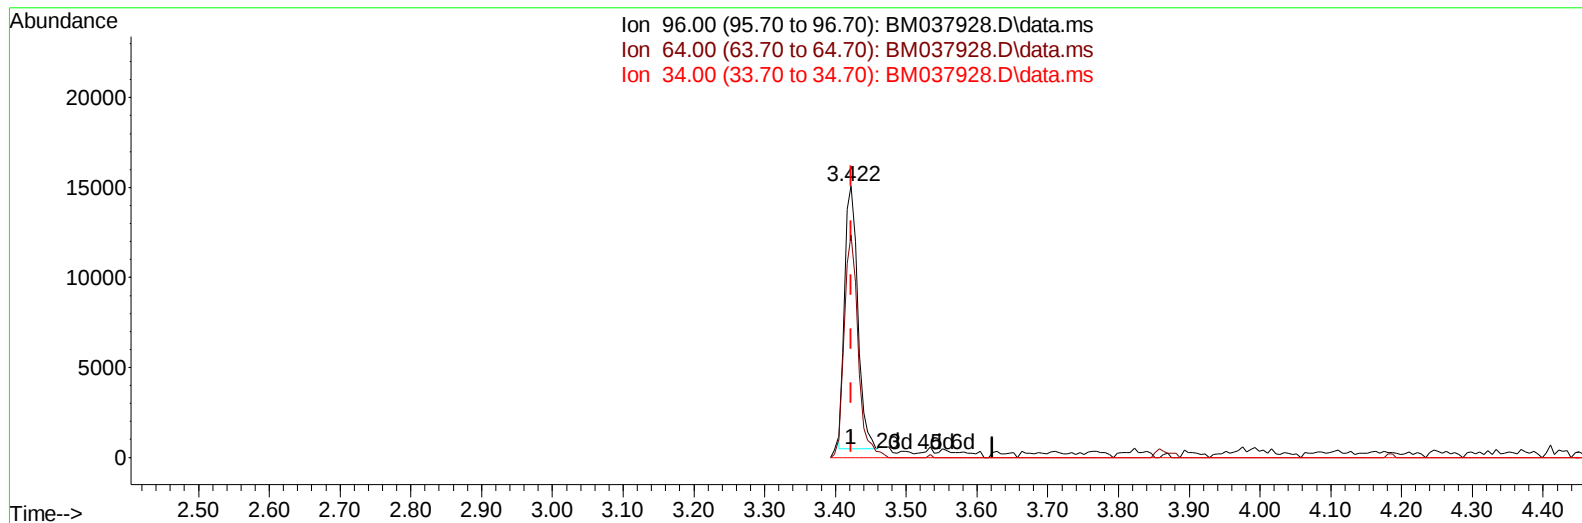

TIC: BM037928.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.422min (-0.000) 4.51 ng/uL****response 18892**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	81.99
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037928.D
 Acq On : 10 Dec 2022 10:19
 Operator : CG/JU
 Sample : PB149532BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK532

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/12/2022
 Supervised By :mohammad ahmed 12/12/2022

Quant Time: Dec 11 21:25:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

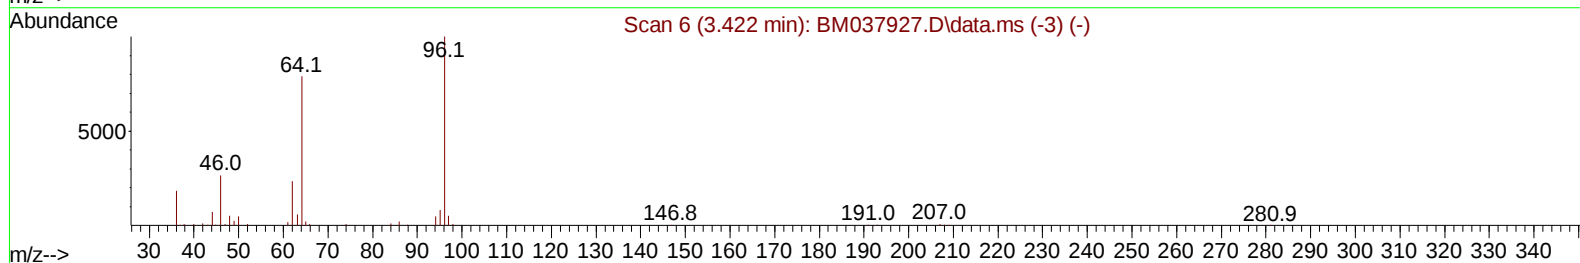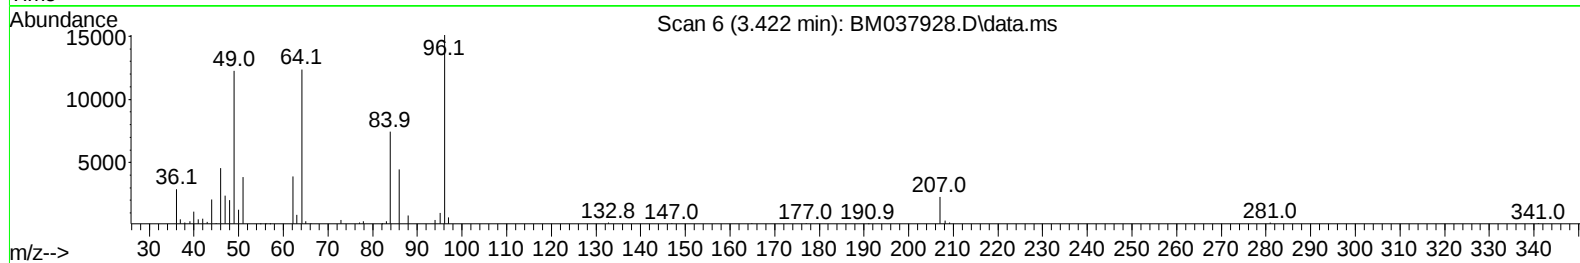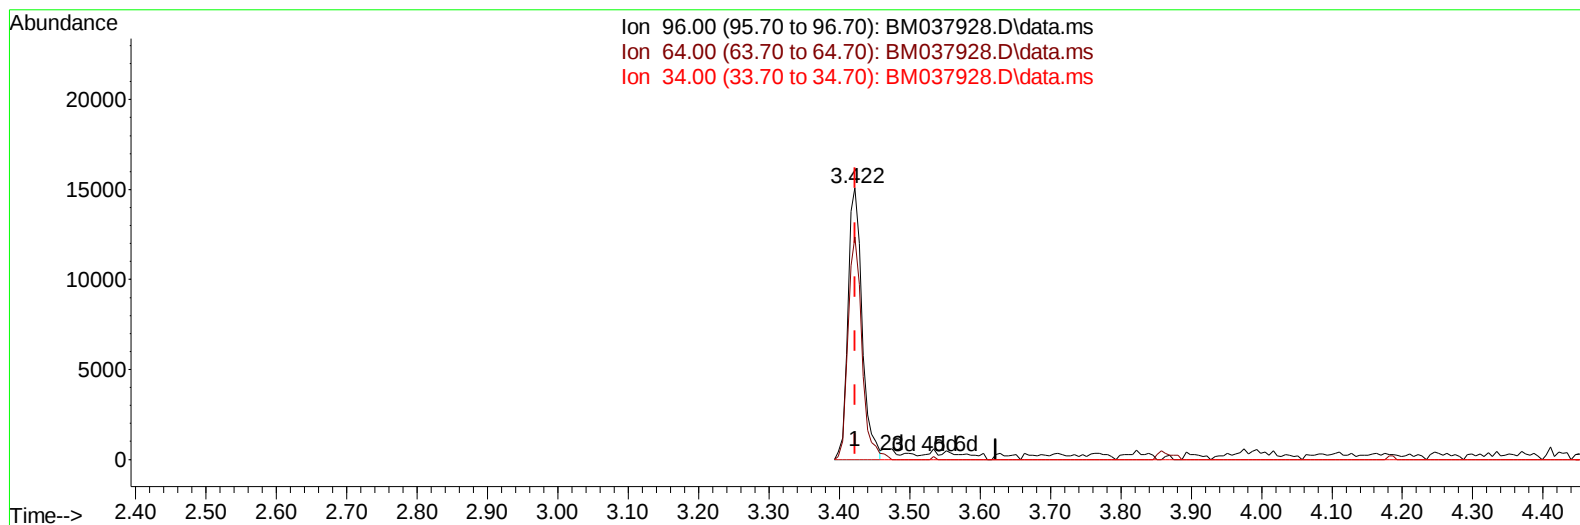

TIC: BM037928.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.422min (-0.000) 5.02 ng/uL m

response 20996

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	81.99
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037928.D
 Acq On : 10 Dec 2022 10:19
 Operator : CG/JU
 Sample : PB149532BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK532

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/12/2022
 Supervised By :mohammad ahmed 12/12/2022

Quant Time: Dec 11 21:25:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.081	152	190031	20.000	ng/ul	0.00
20) Naphthalene-d8	10.898	136	714505	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.710	164	355808	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.451	188	676042	20.000	ng/ul	0.00
79) Chrysene-d12	21.615	240	666573	20.000	ng/ul	0.00
88) Perylene-d12	24.097	264	718423	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	20996m	5.017	ng/uL	0.00
4) Pyridine-d5	3.857	84	267819	21.571	ng/ul	0.00
7) Phenol-d5	7.234	99	379968	24.606	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.404	67	234580	24.947	ng/ul	0.00
11) 2-Chlorophenol-d4	7.604	132	333877	26.357	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	285930	23.721	ng/ul	0.00
21) Nitrobenzene-d5	9.251	128	154004	27.223	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	159555	26.913	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.516	165	270576	24.029	ng/ul	0.00
31) 4-Chloroaniline-d4	11.039	131	369209	23.753	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	684233	26.974	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	827004	26.675	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	85412	19.757	ng/ul	0.00
60) Fluorene-d10	15.698	176	598279	26.473	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	58491	16.183	ng/ul	0.00
73) Anthracene-d10	17.545	188	950871	30.137	ng/ul	0.00
81) Pyrene-d10	19.833	212	1089888	27.219	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.939	264	1103435	30.750	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037928.D
Acq On : 10 Dec 2022 10:19
Operator : CG/JU
Sample : PB149532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK532

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/12/2022
Supervised By :mohammad ahmed 12/12/2022

Quant Time: Dec 11 21:25:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

