

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037946.D
 Acq On : 10 Dec 2022 22:44
 Operator : CG/JU
 Sample : N5927-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ81

Quant Time: Dec 11 21:30:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	178229	20.000	ng/u1	0.00
20) Naphthalene-d8	10.898	136	677073	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.704	164	369556	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	695873	20.000	ng/u1	0.00
79) Chrysene-d12	21.615	240	710142	20.000	ng/u1	0.00
88) Perylene-d12	24.097	264	789834	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	18515	4.717	ng/uL	0.00
4) Pyridine-d5	3.863	84	96161	8.258	ng/u1	0.00
7) Phenol-d5	7.228	99	85897	5.931	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.398	67	273784	31.045	ng/u1	0.00
11) 2-Chlorophenol-d4	7.604	132	290676	24.466	ng/u1	0.00
15) 4-Methylphenol-d8	8.787	113	158997	14.064	ng/u1	0.00
21) Nitrobenzene-d5	9.251	128	186472	34.785	ng/u1	0.00
24) 2-Nitrophenol-d4	9.975	143	186531	33.203	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	300133	28.127	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.034	131	275020	18.672	ng/u1	0.00
46) Dimethylphthalate-d6	14.116	166	948148	35.987	ng/u1	0.00
49) Acenaphthylene-d8	14.404	160	1073296	33.331	ng/u1	0.00
54) 4-Nitrophenol-d4	14.904	143	18053	4.021	ng/u1	0.00
60) Fluorene-d10	15.692	176	799510	34.061	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	90877	24.426	ng/u1	0.00
73) Anthracene-d10	17.545	188	1240620	38.200	ng/u1	0.00
81) Pyrene-d10	19.827	212	1486500	34.847	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.933	264	1540591	39.051	ng/u1	-0.01
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.458	88	14105	3.425	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037946.D
Acq On : 10 Dec 2022 22:44
Operator : CG/JU
Sample : N5927-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ81

Quant Time: Dec 11 21:30:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

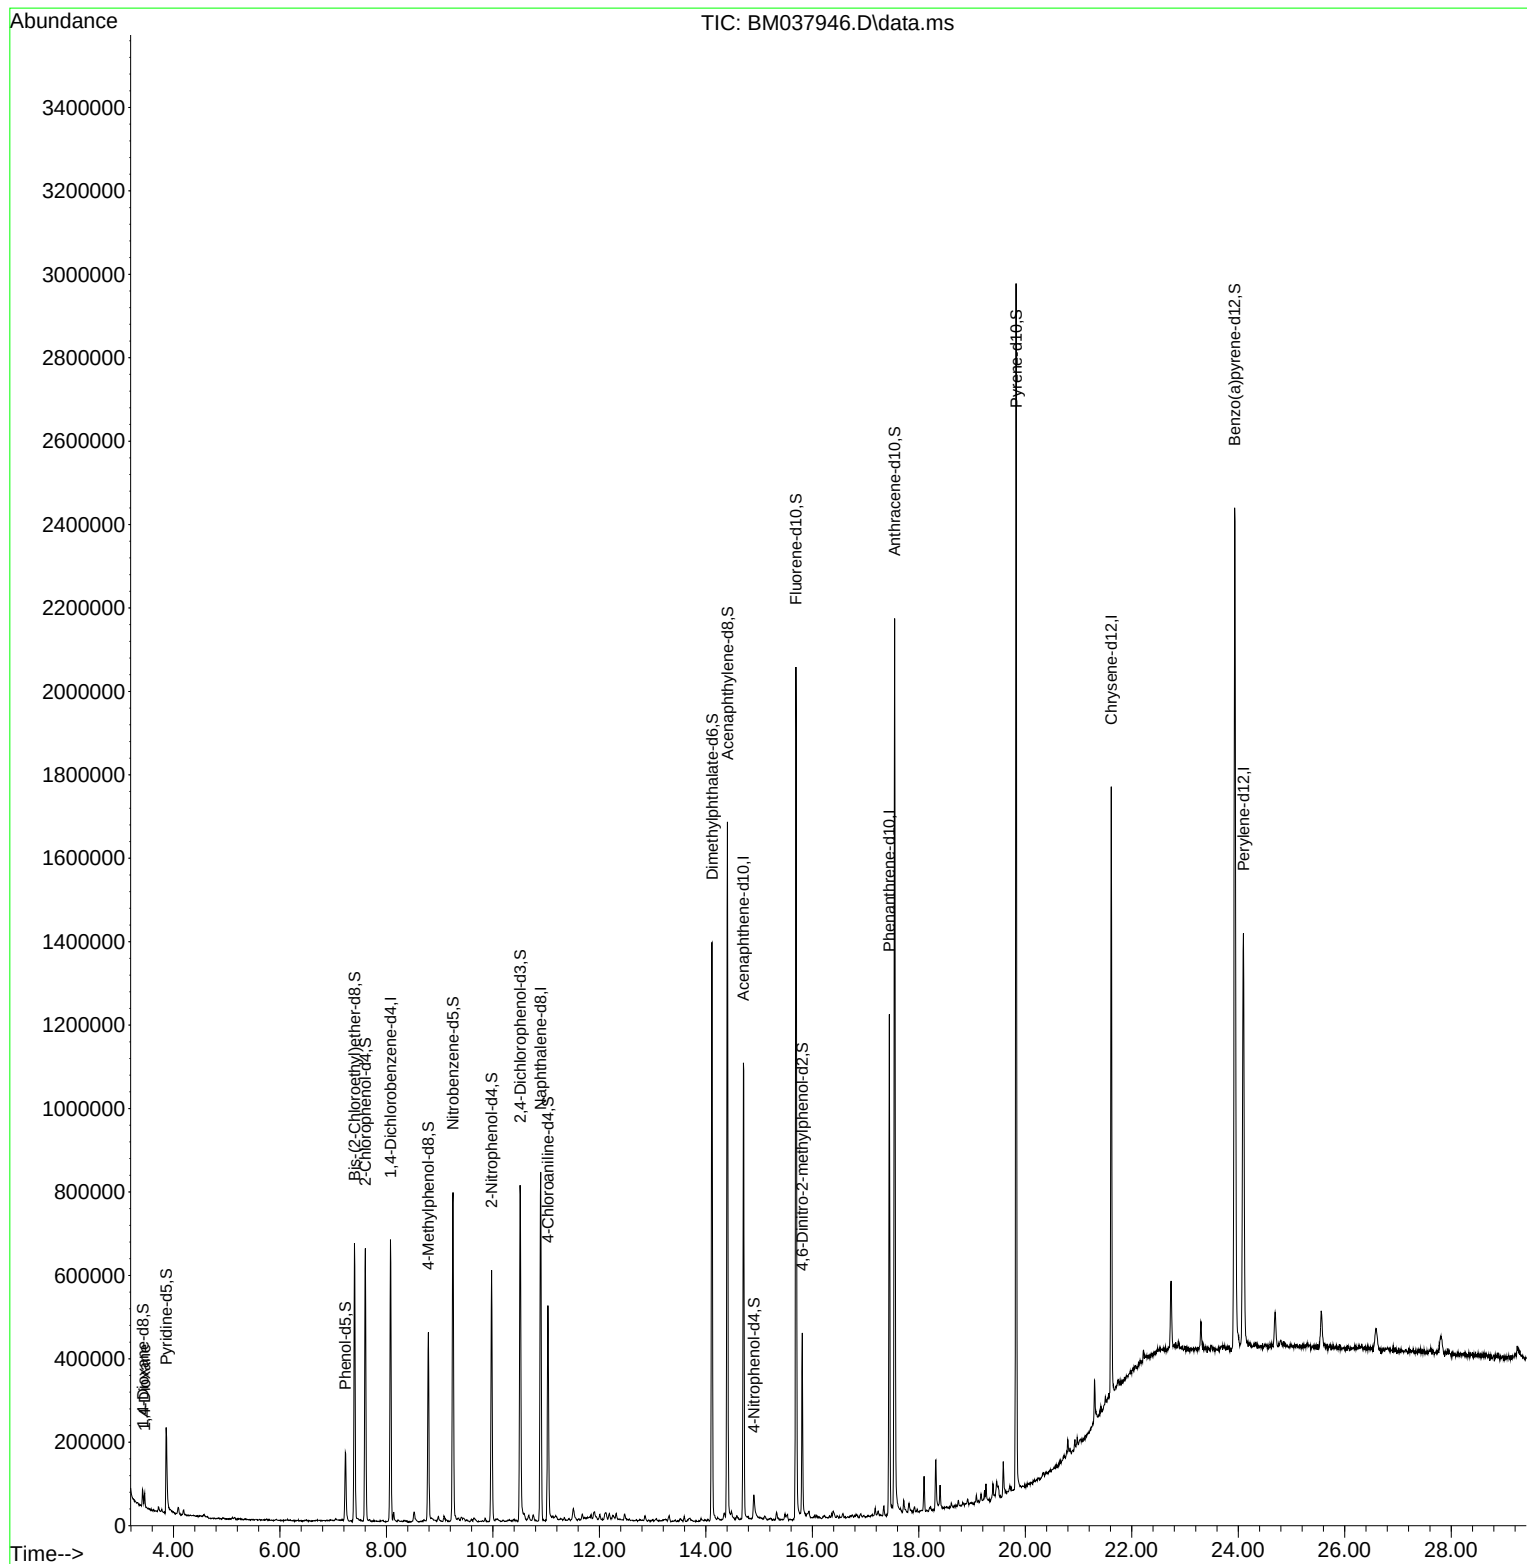

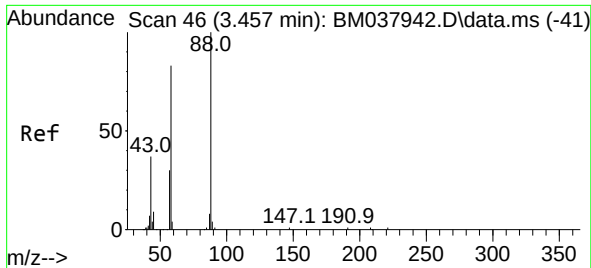

#2
 1,4-Dioxane
 Concen: 3.425 ng/uL
 RT: 3.458 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BM037946.D
 Acq: 10 Dec 2022 22:44

Instrument :
 BNA_M
 ClientSampleId :
 EXZ81

Tgt Ion: 88	Resp:	14105
Ion	Ratio	Lower Upper
88	100	
43	40.6	32.8 49.2
58	77.5	64.6 97.0

