

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037928.D
 Acq On : 10 Dec 2022 10:19
 Operator : CG/JU
 Sample : PB149532BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK532

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	3	6	15	rVB	48465	71191	2.55%	0.215%
2	3.857	77	80	101	rBV	549722	875968	31.34%	2.641%
3	4.193	133	137	144	rVB2	15551	22185	0.79%	0.067%
4	4.375	166	168	170	rBV3	4021	2893	0.10%	0.009%
5	6.375	505	508	511	rBV5	2088	3070	0.11%	0.009%
6	6.851	587	589	592	rBV3	2339	3219	0.12%	0.010%
7	7.234	647	654	663	rBV	738855	1108426	39.66%	3.341%
8	7.404	674	683	691	rBV	563111	867553	31.04%	2.615%
9	7.493	696	698	702	rBV5	3039	3664	0.13%	0.011%
10	7.604	710	717	726	rBV	730034	1133843	40.56%	3.418%
11	8.081	791	798	807	rBV	724568	1107448	39.62%	3.338%
12	8.540	873	876	877	rVB3	3212	3055	0.11%	0.009%
13	8.787	910	918	932	rBV	786815	1265797	45.29%	3.816%
14	8.916	938	940	944	rVB4	3257	3890	0.14%	0.012%
15	9.251	990	997	1009	rBV	648338	1036799	37.09%	3.125%
16	9.504	1037	1040	1045	rVB7	2062	3723	0.13%	0.011%
17	9.592	1053	1055	1061	rBV5	2209	4631	0.17%	0.014%
18	9.975	1113	1120	1129	rBV	495405	808320	28.92%	2.437%
19	10.063	1132	1135	1141	rVB7	3462	5833	0.21%	0.018%
20	10.310	1172	1177	1180	rBV5	2769	4078	0.15%	0.012%
21	10.516	1205	1212	1223	rBV	717602	1195616	42.77%	3.604%
22	10.898	1268	1277	1286	rBV	867092	1435342	51.35%	4.327%
23	11.033	1293	1300	1322	rBV	641905	1173903	42.00%	3.539%
24	11.486	1374	1377	1380	rVB5	3059	3116	0.11%	0.009%
25	11.528	1380	1384	1387	rBV5	2533	3114	0.11%	0.009%
26	12.475	1541	1545	1554	rVB2	13472	22353	0.80%	0.067%
27	12.545	1554	1557	1562	rBV6	2802	4387	0.16%	0.013%
28	14.116	1818	1824	1830	rBV	1039811	1396485	49.96%	4.210%
29	14.404	1866	1873	1889	rBV	1256097	1857855	66.47%	5.600%
30	14.710	1918	1925	1933	rBV	1043740	1523408	54.50%	4.592%
31	14.904	1951	1958	1976	rBV	257404	561682	20.09%	1.693%
32	15.516	2059	2062	2065	rVB3	3587	3911	0.14%	0.012%
33	15.568	2068	2071	2074	rBV5	2669	4196	0.15%	0.013%
34	15.698	2086	2093	2107	rBV	1482664	2156904	77.17%	6.502%
35	15.810	2107	2112	2122	rVB	259481	394395	14.11%	1.189%
36	15.933	2130	2133	2139	rVB8	11356	18829	0.67%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037928.D
 Acq On : 10 Dec 2022 10:19
 Operator : CG/JU
 Sample : PB149532BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK532

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	16.080	2156	2158	2160	rBV3	3651	2839	0.10%	0.009%
38	16.274	2189	2191	2194	rBV3	2514	3115	0.11%	0.009%
39	16.392	2208	2211	2216	rBV6	2209	4621	0.17%	0.014%
40	16.898	2294	2297	2300	rBV4	3738	4624	0.17%	0.014%
41	17.092	2327	2330	2335	rBV7	5049	9801	0.35%	0.030%
42	17.239	2350	2355	2360	rBV5	3824	7749	0.28%	0.023%
43	17.451	2384	2391	2401	rBV	1081517	1581426	56.58%	4.767%
44	17.545	2401	2407	2425	rVB	1549872	2289534	81.91%	6.902%
45	17.827	2451	2455	2457	rBV5	3662	4559	0.16%	0.014%
46	18.233	2522	2524	2528	rBV5	3223	4346	0.16%	0.013%
47	18.404	2550	2553	2557	rVB	8185	9939	0.36%	0.030%
48	19.398	2718	2722	2727	rBV4	18463	27017	0.97%	0.081%
49	19.462	2731	2733	2737	rVV2	15526	18555	0.66%	0.056%
50	19.833	2790	2796	2812	rBV	1966910	2732369	97.75%	8.236%
51	21.509	3079	3081	3084	rVB	74874	63758	2.28%	0.192%
52	21.615	3095	3099	3110	rVB	1287917	1758738	62.92%	5.302%
53	23.939	3488	3494	3505	rVB	1377254	2795150	100.00%	8.426%
54	24.097	3515	3521	3530	rVB2	838403	1765015	63.15%	5.320%


Sum of corrected areas: 33174237

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037928.D
Acq On : 10 Dec 2022 10:19
Operator : CG/JU
Sample : PB149532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK532

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

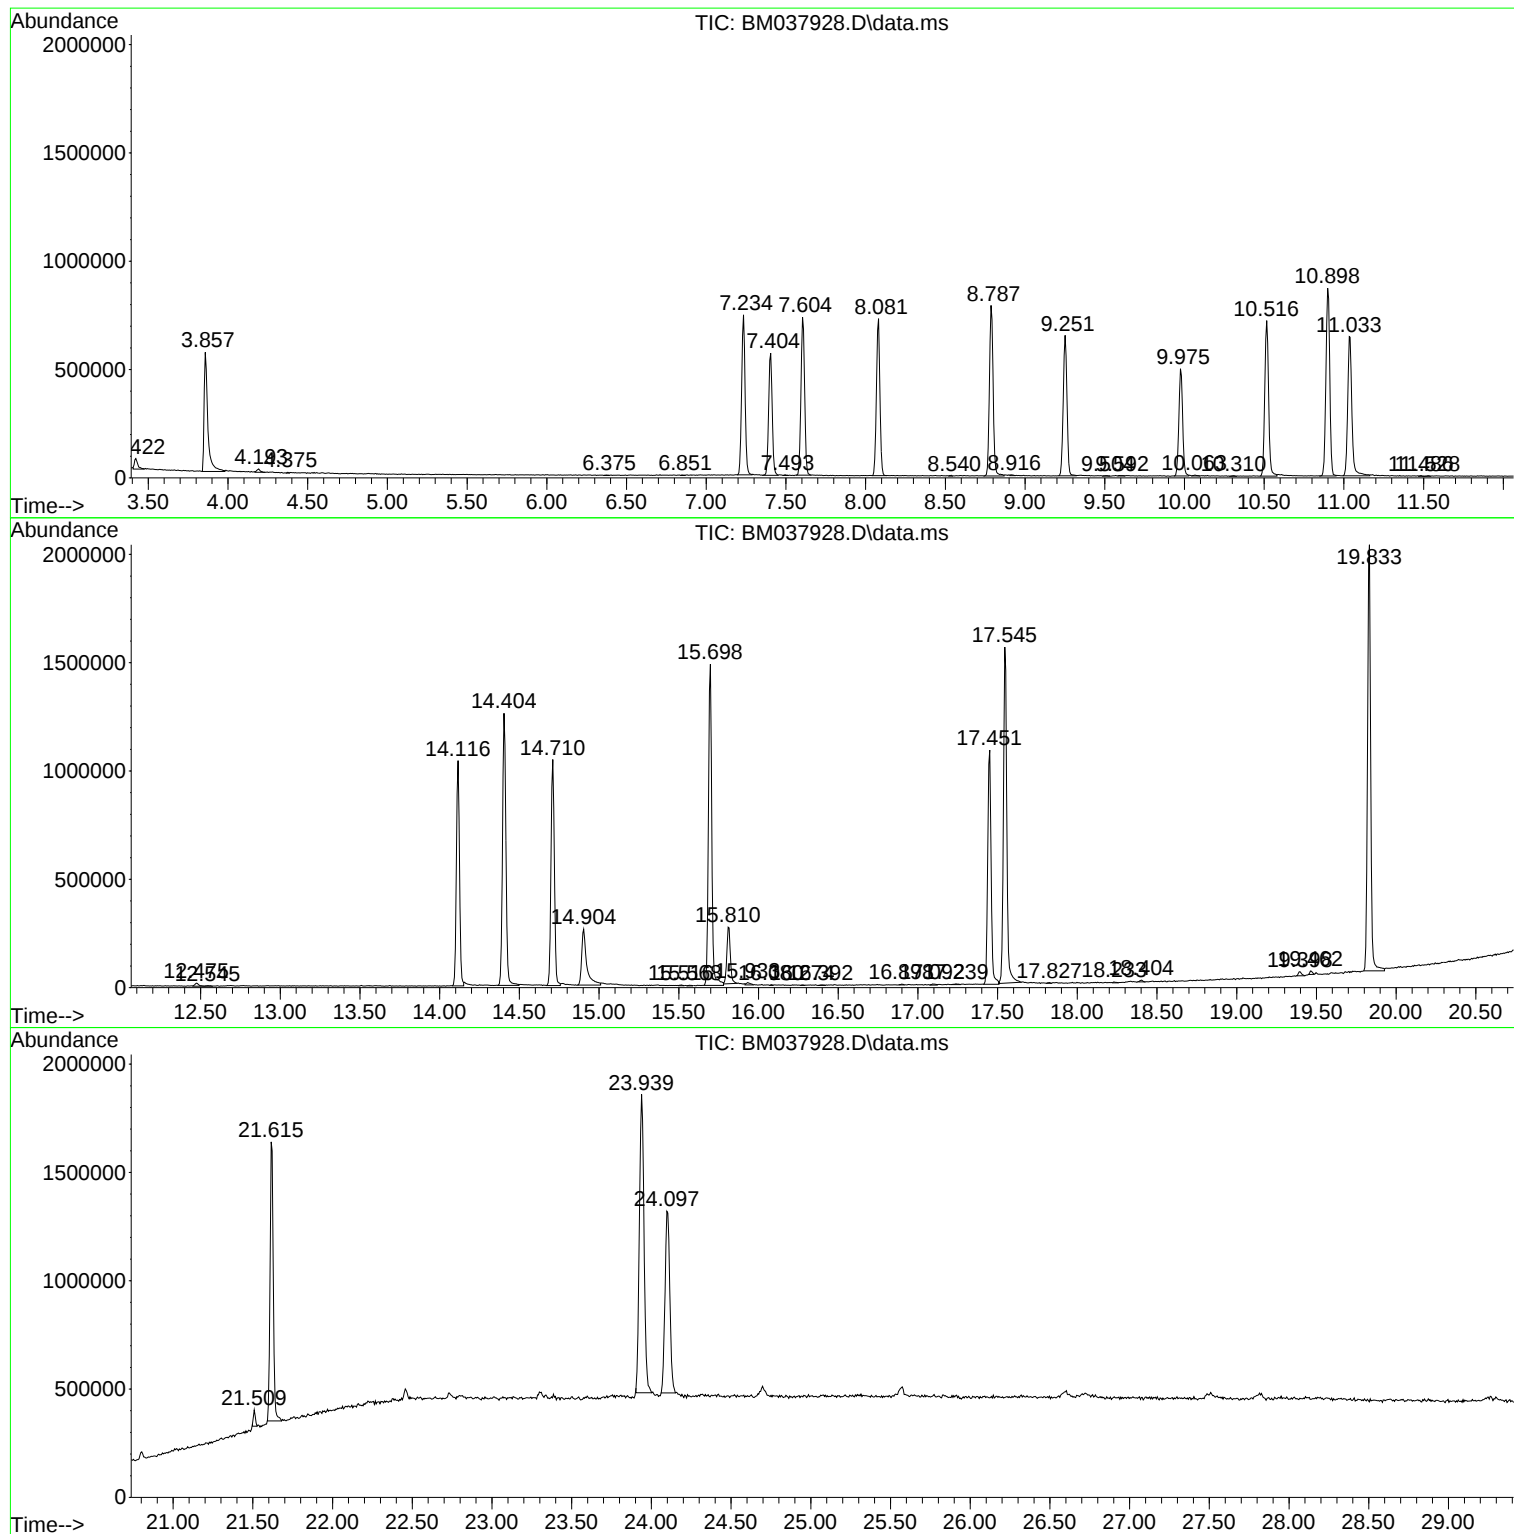

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037928.D
Acq On : 10 Dec 2022 10:19
Operator : CG/JU
Sample : PB149532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK532

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037928.D
Acq On : 10 Dec 2022 10:19
Operator : CG/JU
Sample : PB149532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK532

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc