

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037943.D
 Acq On : 10 Dec 2022 20:55
 Operator : CG/JU
 Sample : PB149543BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK543

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	36	40	48	rBV	48625	69136	2.46%	0.187%
2	3.858	110	114	128	rBV	653399	1026907	36.58%	2.776%
3	4.087	151	153	158	rVB6	3704	4851	0.17%	0.013%
4	4.187	167	170	176	rVB	15858	22093	0.79%	0.060%
5	5.999	475	478	481	rBV4	2092	2931	0.10%	0.008%
6	7.234	681	688	699	rBV	796243	1258834	44.84%	3.403%
7	7.398	710	716	730	rVB	616341	967244	34.45%	2.615%
8	7.604	743	751	767	rVB	806678	1238618	44.12%	3.348%
9	8.075	823	831	841	rBV	828157	1291801	46.02%	3.492%
10	8.787	945	952	965	rBV	912277	1434434	51.10%	3.878%
11	9.251	1022	1031	1041	rBV	722253	1184423	42.19%	3.202%
12	9.416	1056	1059	1062	rVB5	2774	3403	0.12%	0.009%
13	9.975	1145	1154	1165	rBV	565531	917914	32.70%	2.481%
14	10.516	1238	1246	1260	rBV	805293	1385845	49.36%	3.746%
15	10.898	1302	1311	1319	rBV	1062572	1729482	61.61%	4.675%
16	11.034	1327	1334	1351	rBV	780582	1354539	48.25%	3.662%
17	11.469	1405	1408	1411	rBV5	2477	2969	0.11%	0.008%
18	11.681	1441	1444	1446	rBV4	2847	3567	0.13%	0.010%
19	12.269	1536	1544	1547	rVB6	1706	4021	0.14%	0.011%
20	12.475	1573	1579	1586	rBV2	14752	25888	0.92%	0.070%
21	12.686	1612	1615	1620	rVB5	3149	5084	0.18%	0.014%
22	12.928	1652	1656	1658	rBV4	2204	3203	0.11%	0.009%
23	13.428	1739	1741	1744	rVB4	2263	2898	0.10%	0.008%
24	13.598	1765	1770	1775	rVB2	15236	22017	0.78%	0.060%
25	13.680	1781	1784	1788	rBV6	2793	3140	0.11%	0.008%
26	14.110	1851	1857	1870	rBV	1164701	1648480	58.72%	4.456%
27	14.404	1900	1907	1921	rBV	1457595	2144652	76.39%	5.798%
28	14.710	1951	1959	1968	rBV	1263616	1917746	68.31%	5.184%
29	14.898	1985	1991	2011	rBV	268007	598747	21.33%	1.619%
30	15.110	2024	2027	2030	rVB5	4383	5550	0.20%	0.015%
31	15.369	2069	2071	2074	rVB4	3387	3759	0.13%	0.010%
32	15.474	2086	2089	2092	rBV5	2840	2996	0.11%	0.008%
33	15.692	2120	2126	2140	rVV	1686853	2463833	87.76%	6.661%
34	15.810	2140	2146	2161	rVV	266374	433765	15.45%	1.173%
35	15.927	2164	2166	2171	rVV5	10053	16722	0.60%	0.045%
36	15.963	2171	2172	2176	rVB4	4188	3294	0.12%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037943.D
 Acq On : 10 Dec 2022 20:55
 Operator : CG/JU
 Sample : PB149543BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK543

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	16.257	2216	2222	2224	rBV6	1865	3071	0.11%	0.008%
38	16.468	2257	2258	2261	rVB3	3241	3002	0.11%	0.008%
39	16.521	2264	2267	2269	rBV4	2341	3299	0.12%	0.009%
40	16.586	2274	2278	2280	rVV5	2660	3475	0.12%	0.009%
41	16.663	2287	2291	2294	rVB6	2406	2920	0.10%	0.008%
42	17.057	2355	2358	2362	rBV6	2182	3100	0.11%	0.008%
43	17.445	2418	2424	2435	rBV	1317669	1839308	65.52%	4.972%
44	17.545	2435	2441	2463	rVB	1662883	2437832	86.84%	6.590%
45	17.827	2486	2489	2492	rBV5	3632	4426	0.16%	0.012%
46	17.968	2509	2513	2517	rBV5	3930	6656	0.24%	0.018%
47	18.168	2545	2547	2549	rVB3	3318	3064	0.11%	0.008%
48	18.321	2572	2573	2579	rBV6	4419	6298	0.22%	0.017%
49	18.398	2583	2586	2592	rVB3	8548	12678	0.45%	0.034%
50	19.392	2752	2755	2761	rVB5	20658	27126	0.97%	0.073%
51	19.462	2763	2767	2770	rBV2	18660	27833	0.99%	0.075%
52	19.827	2823	2829	2841	rBV	1991202	2684407	95.62%	7.257%
53	21.509	3112	3115	3118	rBV2	87089	104356	3.72%	0.282%
54	21.615	3128	3133	3144	rVB	1434079	1891744	67.39%	5.114%
55	23.939	3521	3528	3542	rVB2	1299542	2807344	100.00%	7.589%
56	24.097	3548	3555	3564	rBV2	942350	1914038	68.18%	5.174%


Sum of corrected areas: 36990763

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037943.D
Acq On : 10 Dec 2022 20:55
Operator : CG/JU
Sample : PB149543BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

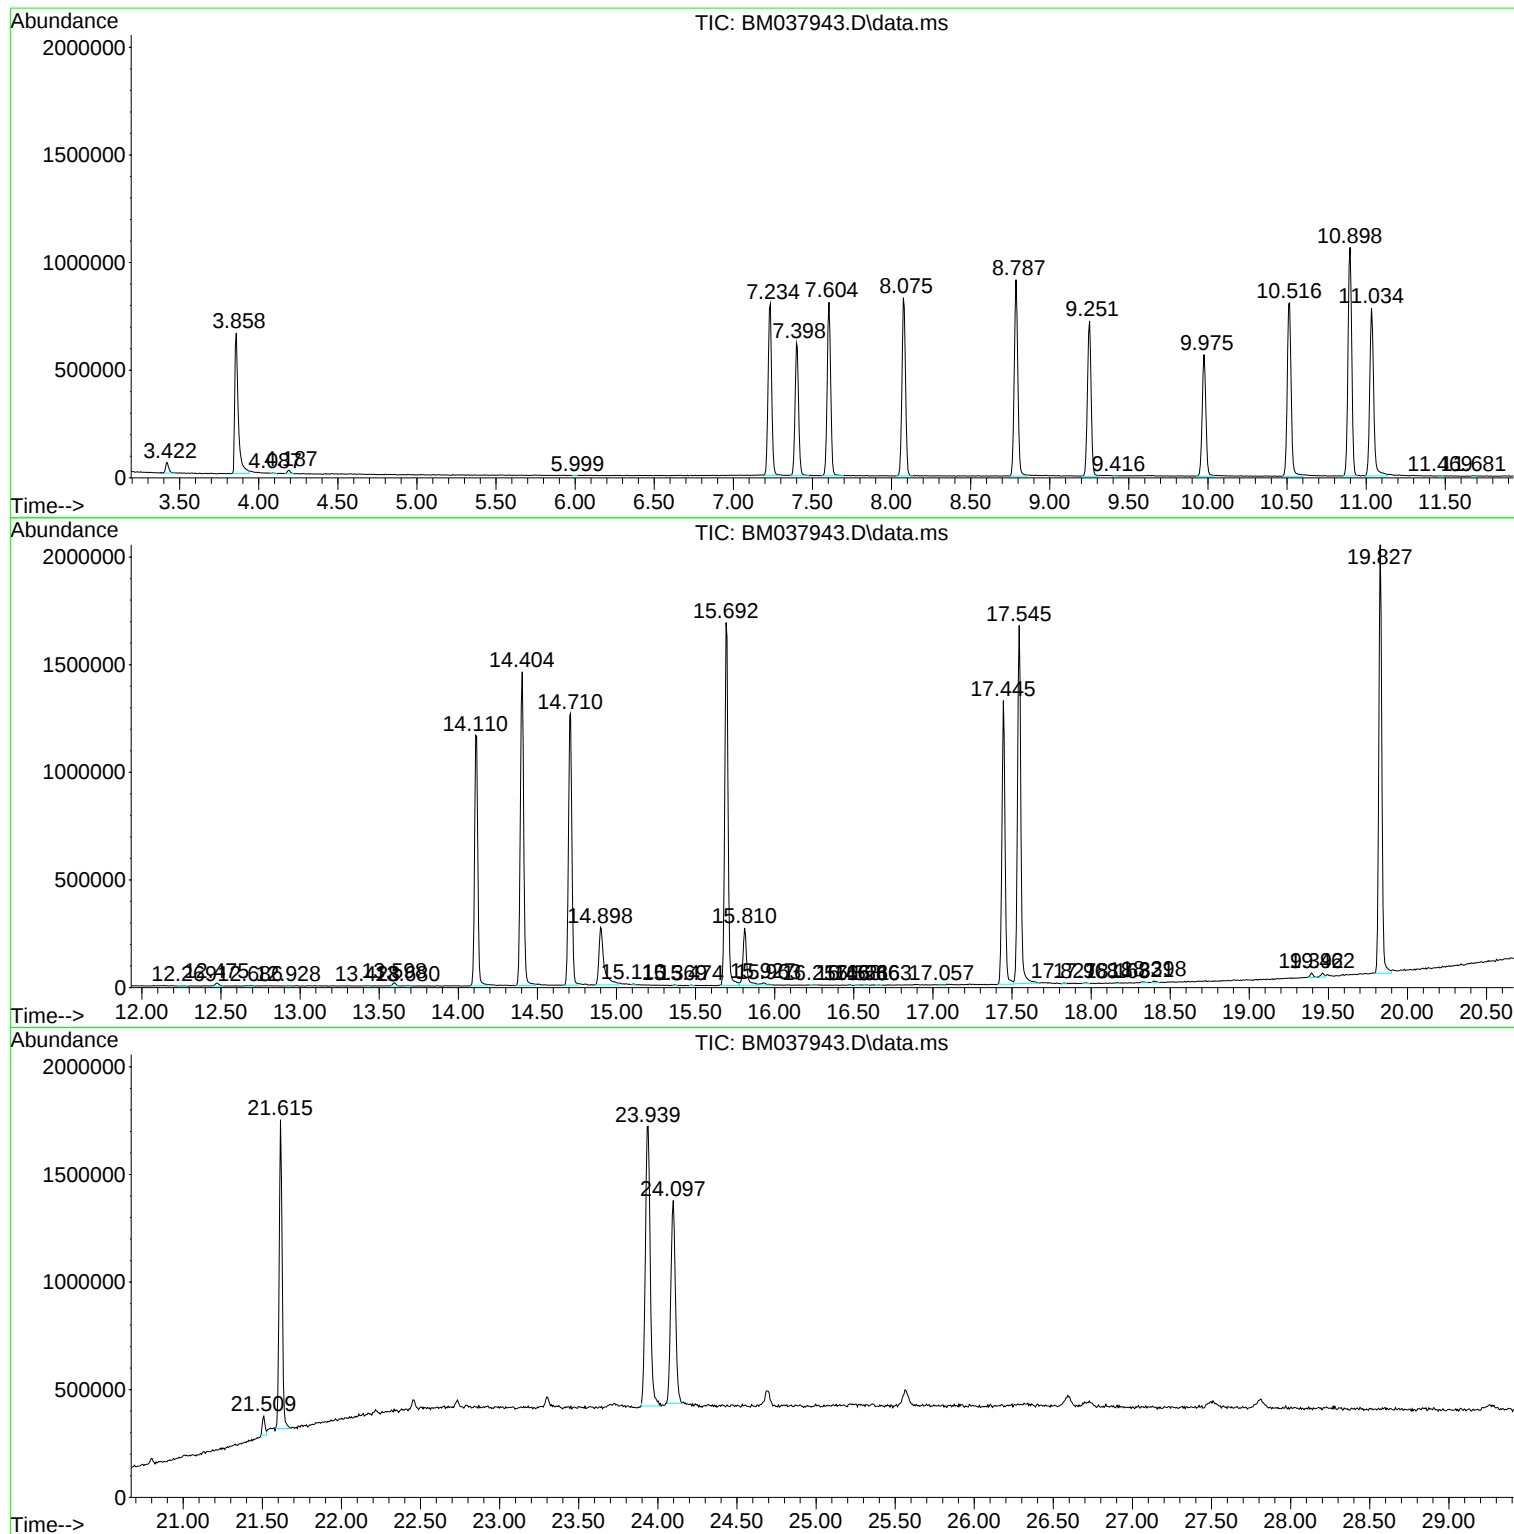

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037943.D
Acq On : 10 Dec 2022 20:55
Operator : CG/JU
Sample : PB149543BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037943.D
Acq On : 10 Dec 2022 20:55
Operator : CG/JU
Sample : PB149543BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc