

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037944.D
 Acq On : 10 Dec 2022 21:32
 Operator : CG/JU
 Sample : PB149493BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK493

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	36	40	46	rVB	54163	69930	1.92%	0.188%
2	3.858	110	114	132	rBV	625936	961636	26.42%	2.586%
3	4.187	167	170	174	rVB	11132	13538	0.37%	0.036%
4	7.175	674	678	681	rBV6	2756	3816	0.10%	0.010%
5	7.228	681	687	697	rVV	759087	1198374	32.92%	3.222%
6	7.398	710	716	727	rVB	607101	933260	25.64%	2.509%
7	7.604	744	751	759	rBV	816081	1220872	33.54%	3.283%
8	8.075	825	831	840	rVB	683616	1070406	29.41%	2.878%
9	8.787	945	952	960	rBV	870952	1347862	37.03%	3.624%
10	9.251	1024	1031	1040	rBV	700334	1118275	30.72%	3.007%
11	9.345	1046	1047	1053	rVB6	2456	4351	0.12%	0.012%
12	9.975	1147	1154	1163	rBV	554251	885396	24.32%	2.381%
13	10.510	1238	1245	1260	rBV	784873	1323280	36.35%	3.558%
14	10.898	1304	1311	1318	rVB	848312	1363184	37.45%	3.665%
15	11.034	1326	1334	1351	rBV	709626	1227207	33.71%	3.300%
16	11.681	1440	1444	1445	rBV3	3296	4816	0.13%	0.013%
17	12.475	1574	1579	1585	rVB2	14124	21257	0.58%	0.057%
18	12.863	1640	1645	1646	rBV3	2398	3643	0.10%	0.010%
19	13.592	1766	1769	1773	rVB3	4583	5682	0.16%	0.015%
20	14.116	1851	1858	1872	rBV	1113362	1578815	43.37%	4.245%
21	14.404	1900	1907	1919	rBV	1454023	2085897	57.30%	5.609%
22	14.710	1952	1959	1970	rBV	1024894	1525605	41.91%	4.102%
23	14.898	1985	1991	2005	rBV	339600	684435	18.80%	1.840%
24	15.692	2120	2126	2138	rBV	1657205	2444625	67.16%	6.573%
25	15.810	2141	2146	2159	rVV	349262	535888	14.72%	1.441%
26	15.933	2163	2167	2171	rVV5	12920	21239	0.58%	0.057%
27	16.398	2241	2246	2248	rBV5	2462	4952	0.14%	0.013%
28	17.268	2392	2394	2399	rVB6	2684	4506	0.12%	0.012%
29	17.351	2403	2408	2412	rVV7	2017	4079	0.11%	0.011%
30	17.445	2418	2424	2435	rBV	1170651	1685089	46.29%	4.531%
31	17.545	2435	2441	2457	rVV2	1867192	2643513	72.62%	7.108%
32	17.915	2501	2504	2507	rBV5	3003	4837	0.13%	0.013%
33	18.327	2570	2574	2577	rVV5	4913	8289	0.23%	0.022%
34	19.392	2751	2755	2759	rBV3	22003	31974	0.88%	0.086%
35	19.468	2763	2768	2770	rBV3	19686	29550	0.81%	0.079%
36	19.827	2824	2829	2838	rBV	2449607	3261773	89.60%	8.770%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037944.D
Acq On : 10 Dec 2022 21:32
Operator : CG/JU
Sample : PB149493BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK493

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Title : SVOA CALIBRATION

37	21.615	3128	3133	3143	rBV	1504886	2037724	55.98%	5.479%
38	23.939	3521	3528	3546	rVB2	1696434	3640212	100.00%	9.788%
39	24.097	3549	3555	3572	rVB2	1035148	2180494	59.90%	5.863%




Sum of corrected areas: 37190281

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037944.D
Acq On : 10 Dec 2022 21:32
Operator : CG/JU
Sample : PB149493BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

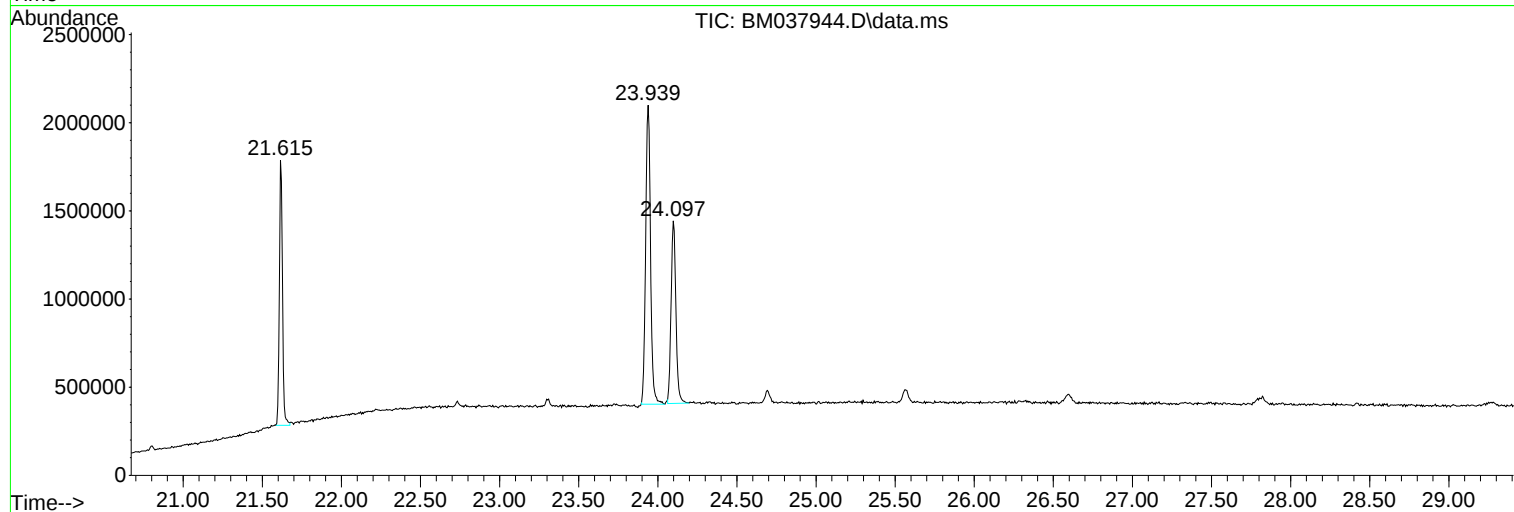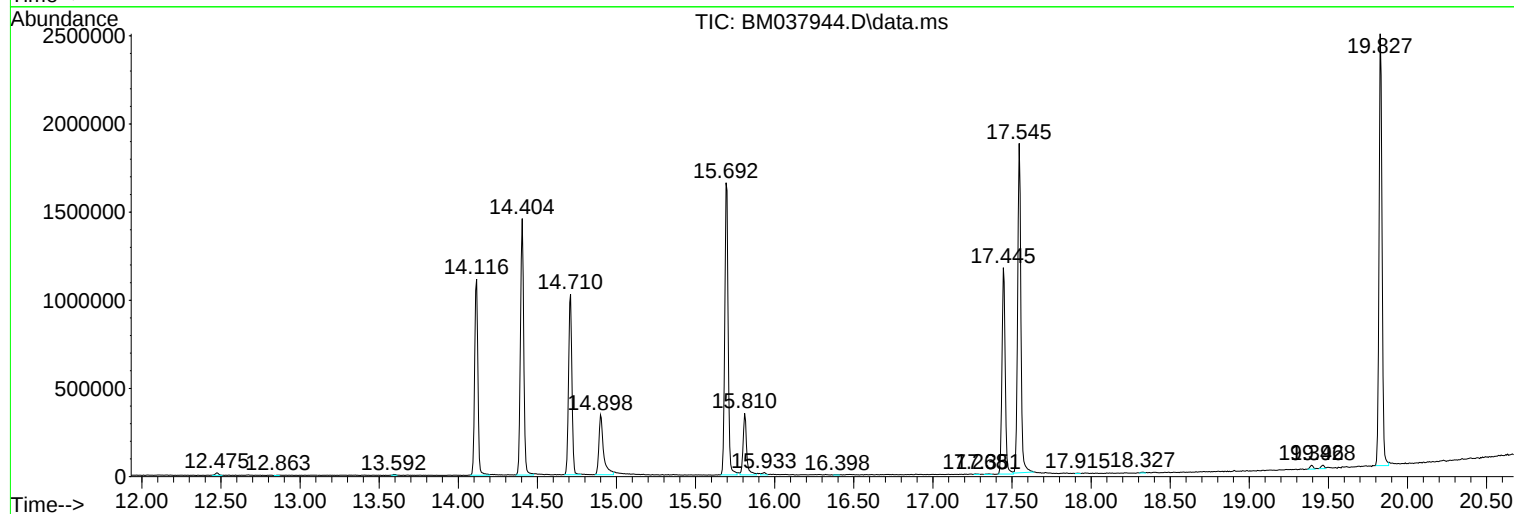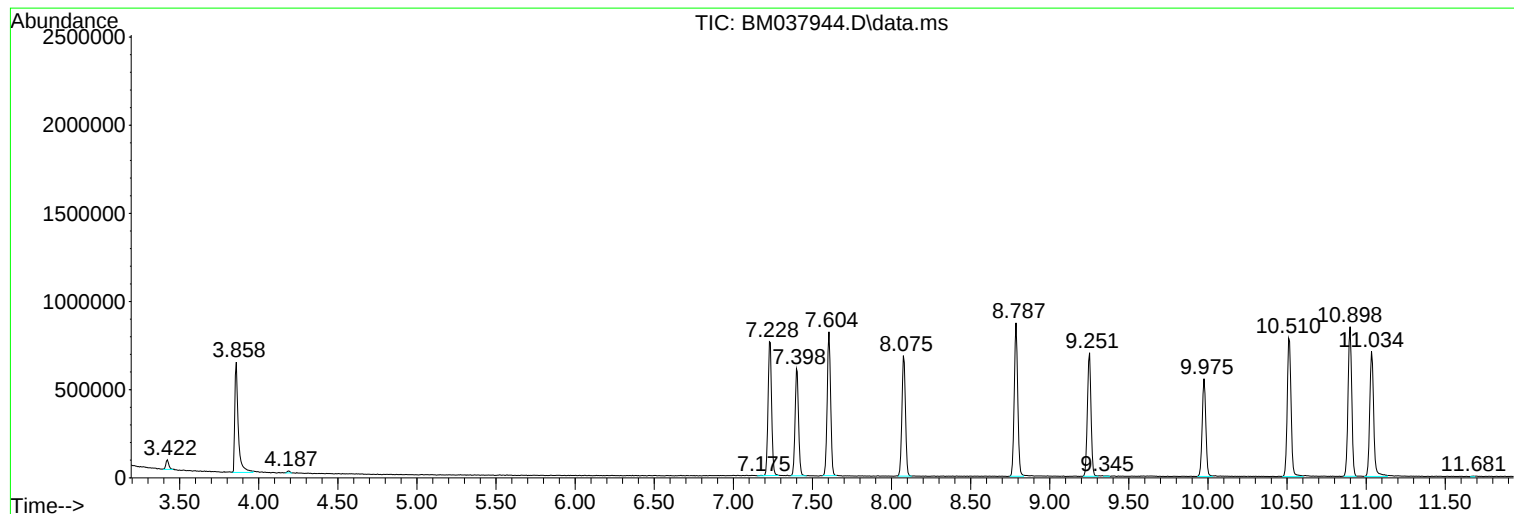

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037944.D
Acq On : 10 Dec 2022 21:32
Operator : CG/JU
Sample : PB149493BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037944.D
Acq On : 10 Dec 2022 21:32
Operator : CG/JU
Sample : PB149493BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc