

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037945.D
 Acq On : 10 Dec 2022 22:08
 Operator : CG/JU
 Sample : PB149486BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK486

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	36	40	45	rVB	50060	62895	2.14%	0.177%
2	3.857	110	114	132	rBV	644146	978191	33.31%	2.752%
3	4.193	167	171	175	rVB3	12676	17100	0.58%	0.048%
4	5.746	432	435	438	rBV5	2501	3638	0.12%	0.010%
5	7.234	681	688	697	rBV	761816	1199552	40.84%	3.375%
6	7.398	710	716	724	rBV	585635	906108	30.85%	2.549%
7	7.457	724	726	731	rVB5	3180	4707	0.16%	0.013%
8	7.604	744	751	760	rBV	799907	1221103	41.58%	3.436%
9	8.075	825	831	841	rBV	737296	1142819	38.91%	3.215%
10	8.786	945	952	963	rBV	884433	1368594	46.60%	3.851%
11	9.251	1023	1031	1039	rBV	683146	1126611	38.36%	3.170%
12	9.975	1146	1154	1163	rBV	533268	878930	29.93%	2.473%
13	10.516	1238	1246	1257	rBV	778325	1324583	45.10%	3.727%
14	10.898	1303	1311	1319	rBV	963436	1528546	52.05%	4.301%
15	11.033	1327	1334	1355	rBV	712549	1259845	42.90%	3.545%
16	12.474	1574	1579	1586	rVB2	13893	21883	0.75%	0.062%
17	13.586	1765	1768	1775	rBV8	5957	9738	0.33%	0.027%
18	14.110	1850	1857	1870	rBV	1094549	1548203	52.72%	4.356%
19	14.404	1900	1907	1918	rBV	1399944	2034262	69.27%	5.723%
20	14.704	1951	1958	1968	rBV	1116181	1689957	57.54%	4.755%
21	14.898	1985	1991	2010	rBV	287907	604216	20.57%	1.700%
22	15.104	2023	2026	2030	rBV6	2634	4706	0.16%	0.013%
23	15.315	2060	2062	2067	rVB4	1855	3251	0.11%	0.009%
24	15.363	2067	2070	2072	rBV4	3010	3181	0.11%	0.009%
25	15.645	2115	2118	2120	rBV3	2634	3471	0.12%	0.010%
26	15.692	2120	2126	2140	rVV	1644600	2334875	79.50%	6.569%
27	15.810	2140	2146	2155	rVB	268584	399626	13.61%	1.124%
28	15.933	2163	2167	2171	rVB4	7650	12049	0.41%	0.034%
29	17.145	2372	2373	2378	rVB4	3038	3248	0.11%	0.009%
30	17.239	2386	2389	2392	rBV4	2678	3847	0.13%	0.011%
31	17.445	2417	2424	2435	rBV	1184311	1703615	58.01%	4.793%
32	17.545	2435	2441	2462	rVB2	1601056	2370929	80.73%	6.671%
33	18.127	2538	2540	2544	rVV4	3169	4298	0.15%	0.012%
34	18.156	2544	2545	2549	rVB4	3655	2988	0.10%	0.008%
35	18.315	2570	2572	2577	rBV6	4098	7378	0.25%	0.021%
36	18.539	2606	2610	2611	rBV4	3090	4550	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037945.D
 Acq On : 10 Dec 2022 22:08
 Operator : CG/JU
 Sample : PB149486BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK486

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	18.686	2633	2635	2638	rBV4	3392	4513	0.15%	0.013%
38	18.774	2648	2650	2651	rBV2	3839	3166	0.11%	0.009%
39	18.903	2668	2672	2673	rBV4	4437	4328	0.15%	0.012%
40	19.398	2752	2756	2759	rVB5	16714	23857	0.81%	0.067%
41	19.462	2764	2767	2771	rBV	17743	25446	0.87%	0.072%
42	19.827	2823	2829	2844	rBV	2128894	2809509	95.66%	7.905%
43	21.615	3128	3133	3141	rBV	1453407	1934022	65.85%	5.441%
44	23.938	3521	3528	3539	rVB2	1411480	2936840	100.00%	8.263%
45	24.097	3548	3555	3567	rVB2	952675	2007819	68.37%	5.649%




Sum of corrected areas: 35542993

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037945.D
Acq On : 10 Dec 2022 22:08
Operator : CG/JU
Sample : PB149486BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

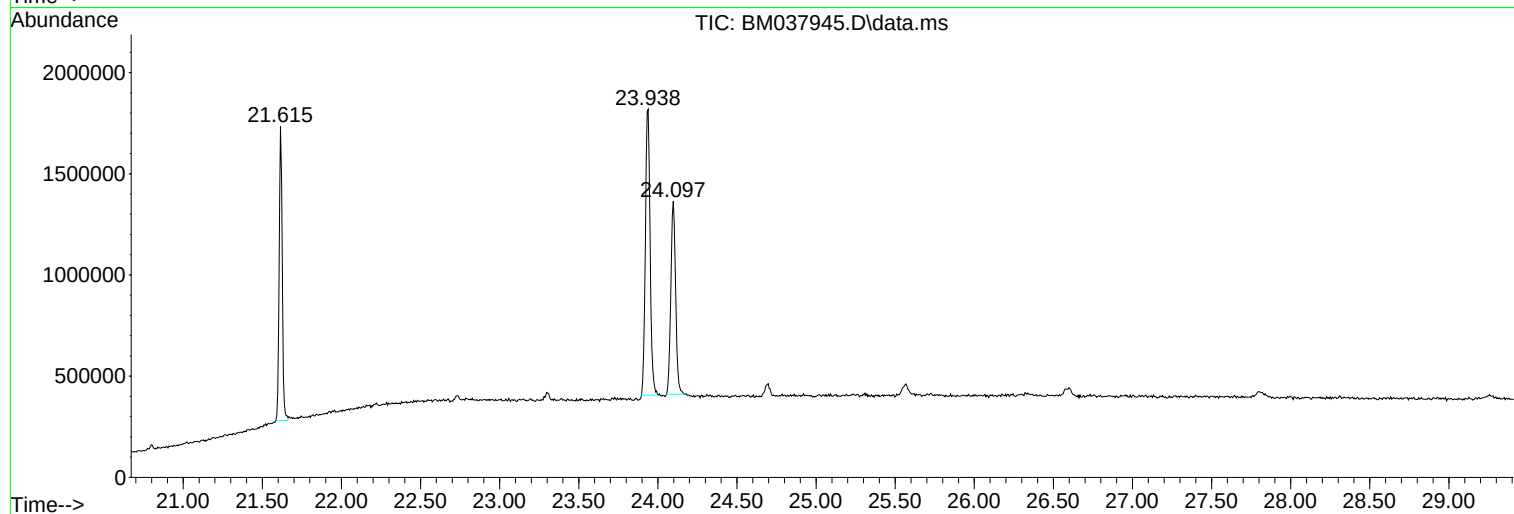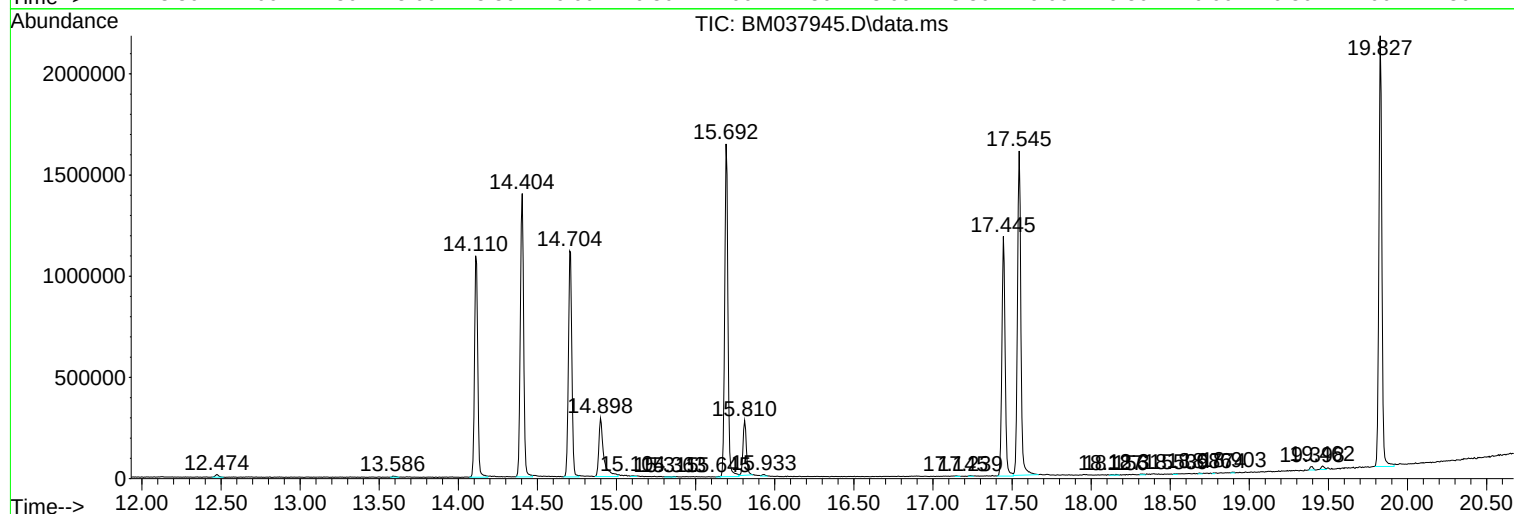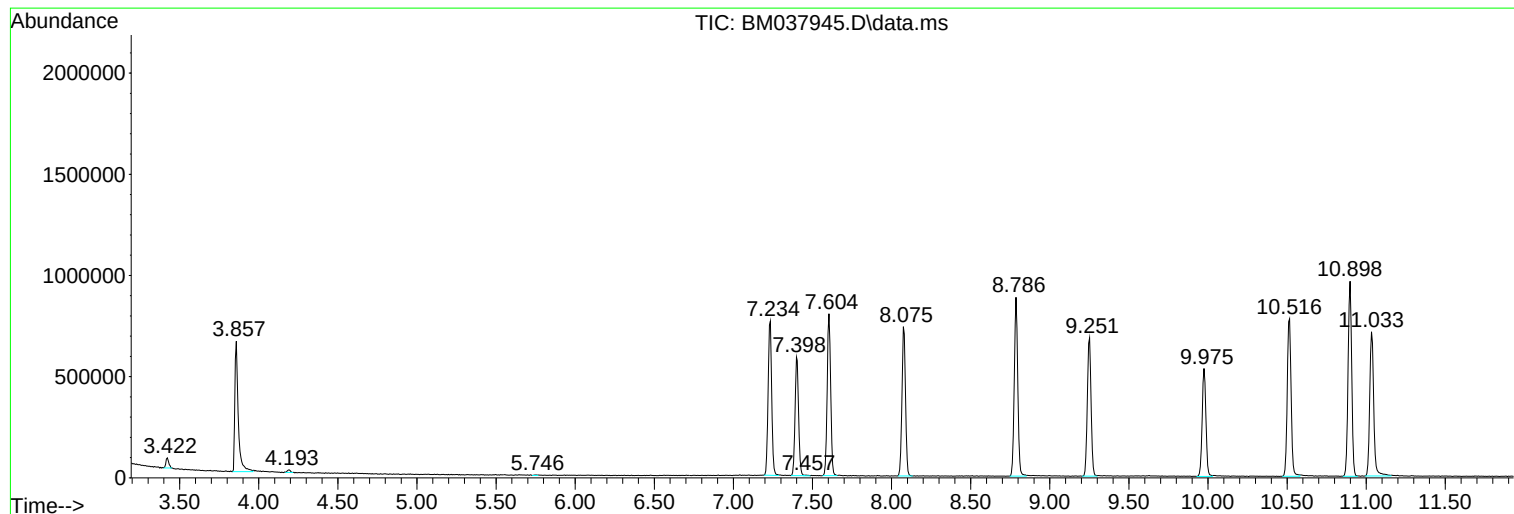

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037945.D
Acq On : 10 Dec 2022 22:08
Operator : CG/JU
Sample : PB149486BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037945.D
Acq On : 10 Dec 2022 22:08
Operator : CG/JU
Sample : PB149486BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
