

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037947.D
 Acq On : 10 Dec 2022 23:20
 Operator : CG/JU
 Sample : N5927-12
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	36	39	50	rVB	41599	65171	1.60%	0.172%
2	3.863	111	115	129	rBV	188823	316730	7.80%	0.836%
3	4.087	150	153	160	rVB2	20346	30861	0.76%	0.081%
4	4.187	167	170	175	rVB2	15930	22444	0.55%	0.059%
5	7.228	681	687	697	rVB	177158	281836	6.94%	0.744%
6	7.398	710	716	726	rVB	692990	1039485	25.58%	2.742%
7	7.604	742	751	759	rBV	671630	1042048	25.65%	2.749%
8	7.681	762	764	769	rVB5	5391	6011	0.15%	0.016%
9	8.075	824	831	839	rBV	678844	1044575	25.71%	2.756%
10	8.134	839	841	846	rVB6	4128	5191	0.13%	0.014%
11	8.787	945	952	962	rBV	464805	745772	18.35%	1.967%
12	9.251	1022	1031	1040	rBV	816977	1330346	32.74%	3.510%
13	9.345	1043	1047	1049	rVV5	5016	6853	0.17%	0.018%
14	9.404	1053	1057	1063	rVB3	16645	24031	0.59%	0.063%
15	9.645	1094	1098	1102	rVV6	4117	5870	0.14%	0.015%
16	9.975	1144	1154	1166	rBV	607107	973346	23.96%	2.568%
17	10.516	1237	1246	1254	rBV	810873	1373320	33.80%	3.623%
18	10.898	1303	1311	1319	rBV	877640	1419198	34.93%	3.744%
19	11.033	1327	1334	1351	rBV	764701	1341285	33.01%	3.539%
20	11.675	1438	1443	1449	rBV9	6874	15165	0.37%	0.040%
21	12.469	1574	1578	1587	rVB	17616	27768	0.68%	0.073%
22	12.692	1609	1616	1619	rVB6	3260	5912	0.15%	0.016%
23	13.486	1747	1751	1754	rBV3	4346	5546	0.14%	0.015%
24	13.592	1763	1769	1774	rBV4	7938	12200	0.30%	0.032%
25	13.669	1780	1782	1788	rVB7	2652	4531	0.11%	0.012%
26	14.116	1851	1858	1868	rBV	1474041	2027808	49.91%	5.350%
27	14.339	1893	1896	1899	rVB5	3697	4507	0.11%	0.012%
28	14.404	1899	1907	1922	rBV	1796328	2594270	63.85%	6.844%
29	14.645	1945	1948	1951	rBV4	6060	6684	0.16%	0.018%
30	14.704	1953	1958	1969	rVV2	1103235	1620911	39.89%	4.276%
31	14.798	1971	1974	1976	rVB4	3747	4102	0.10%	0.011%
32	14.904	1986	1992	2004	rBV2	53349	118102	2.91%	0.312%
33	15.116	2024	2028	2034	rVB8	9141	15779	0.39%	0.042%
34	15.621	2110	2114	2117	rBV2	7563	7675	0.19%	0.020%
35	15.698	2120	2127	2141	rVV	2109835	3112947	76.61%	8.213%
36	15.810	2141	2146	2160	rVV	414739	595206	14.65%	1.570%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037947.D
 Acq On : 10 Dec 2022 23:20
 Operator : CG/JU
 Sample : N5927-12
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	15.933	2163	2167	2174	rVB5	18697	29170	0.72%	0.077%
38	16.245	2215	2220	2222	rBV4	3649	5701	0.14%	0.015%
39	16.339	2230	2236	2237	rBV	17328	20032	0.49%	0.053%
40	16.363	2238	2240	2243	rVV	18480	18944	0.47%	0.050%
41	16.392	2243	2245	2248	rVV4	5072	5972	0.15%	0.016%
42	16.474	2257	2259	2263	rVB4	3931	4841	0.12%	0.013%
43	16.551	2269	2272	2274	rBV4	4387	5300	0.13%	0.014%
44	16.663	2287	2291	2296	rVB	29735	37653	0.93%	0.099%
45	16.821	2312	2318	2325	rBV3	18606	29284	0.72%	0.077%
46	16.892	2325	2330	2334	rBV8	6995	11964	0.29%	0.032%
47	17.057	2354	2358	2364	rVB8	3297	5996	0.15%	0.016%
48	17.345	2402	2407	2410	rVB6	5514	8221	0.20%	0.022%
49	17.445	2418	2424	2430	rBV	1165627	1588192	39.09%	4.190%
50	17.545	2435	2441	2451	rVV2	2214596	3130424	77.04%	8.259%
51	17.715	2467	2470	2477	rVB9	7357	14587	0.36%	0.038%
52	17.968	2510	2513	2517	rBV6	4070	5659	0.14%	0.015%
53	18.098	2533	2535	2539	rVB5	6150	7408	0.18%	0.020%
54	18.215	2552	2555	2561	rVB3	9634	17023	0.42%	0.045%
55	18.321	2568	2573	2578	rBV3	46929	67188	1.65%	0.177%
56	18.486	2599	2601	2604	rBV4	5426	5630	0.14%	0.015%
57	18.609	2620	2622	2628	rVB5	8273	9123	0.22%	0.024%
58	18.827	2654	2659	2665	rBV	28741	50618	1.25%	0.134%
59	19.080	2698	2702	2706	rBV2	44039	56671	1.39%	0.150%
60	19.392	2751	2755	2760	rBV4	27453	37263	0.92%	0.098%
61	19.462	2763	2767	2770	rBV2	29714	42143	1.04%	0.111%
62	19.586	2785	2788	2795	rBV3	58426	88786	2.19%	0.234%
63	19.827	2823	2829	2840	rBV	2858910	3708958	91.28%	9.785%
64	20.798	2991	2994	2998	rVB3	59027	59116	1.45%	0.156%
65	20.927	3014	3016	3020	rVB3	47040	50274	1.24%	0.133%
66	21.615	3128	3133	3144	rBV	1308384	1691525	41.63%	4.463%
67	23.933	3520	3527	3539	rBV2	1953969	4063208	100.00%	10.719%
68	24.097	3548	3555	3562	rBV	872761	1774585	43.67%	4.682%




Sum of corrected areas: 37904945

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037947.D
Acq On : 10 Dec 2022 23:20
Operator : CG/JU
Sample : N5927-12
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

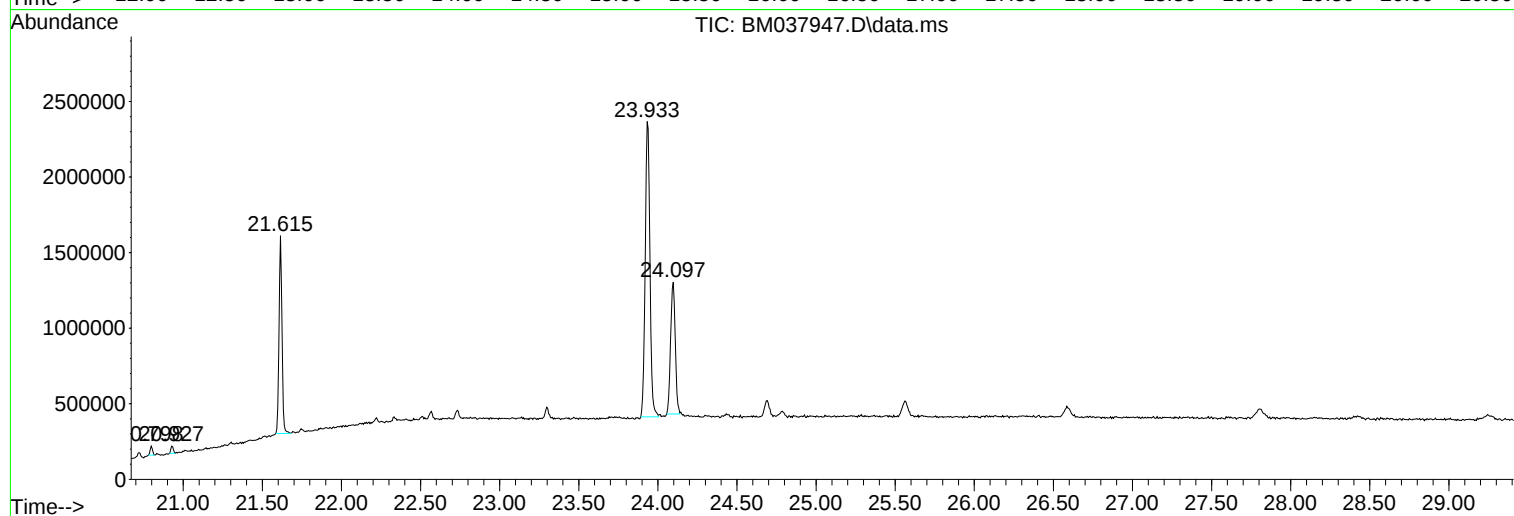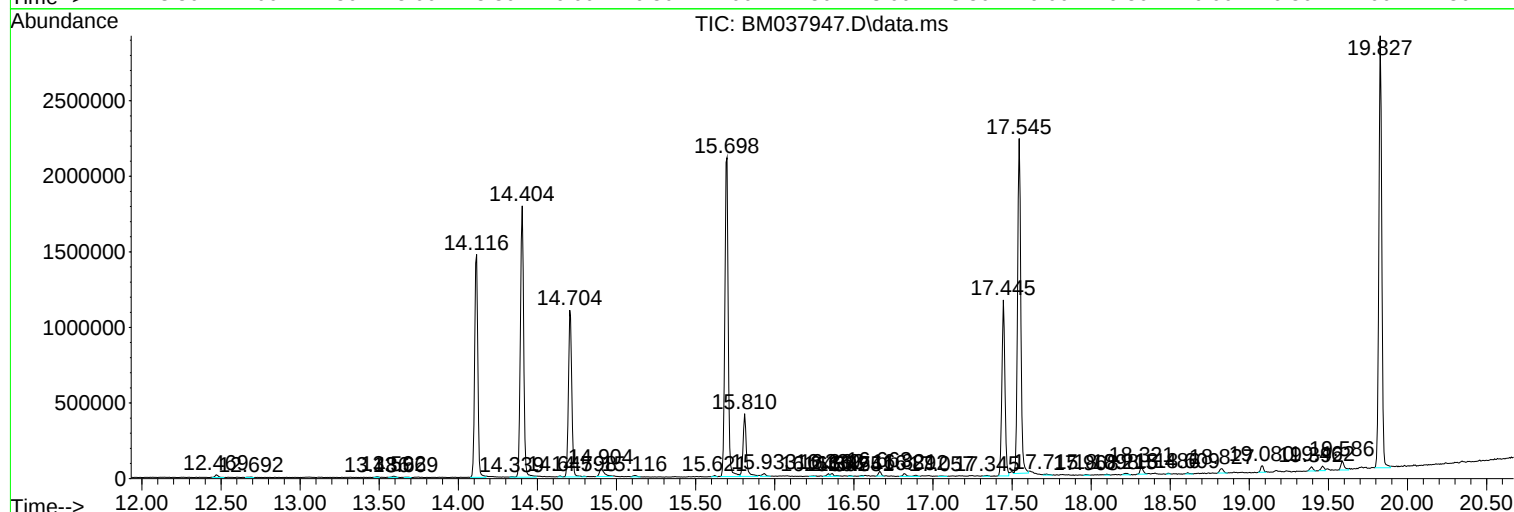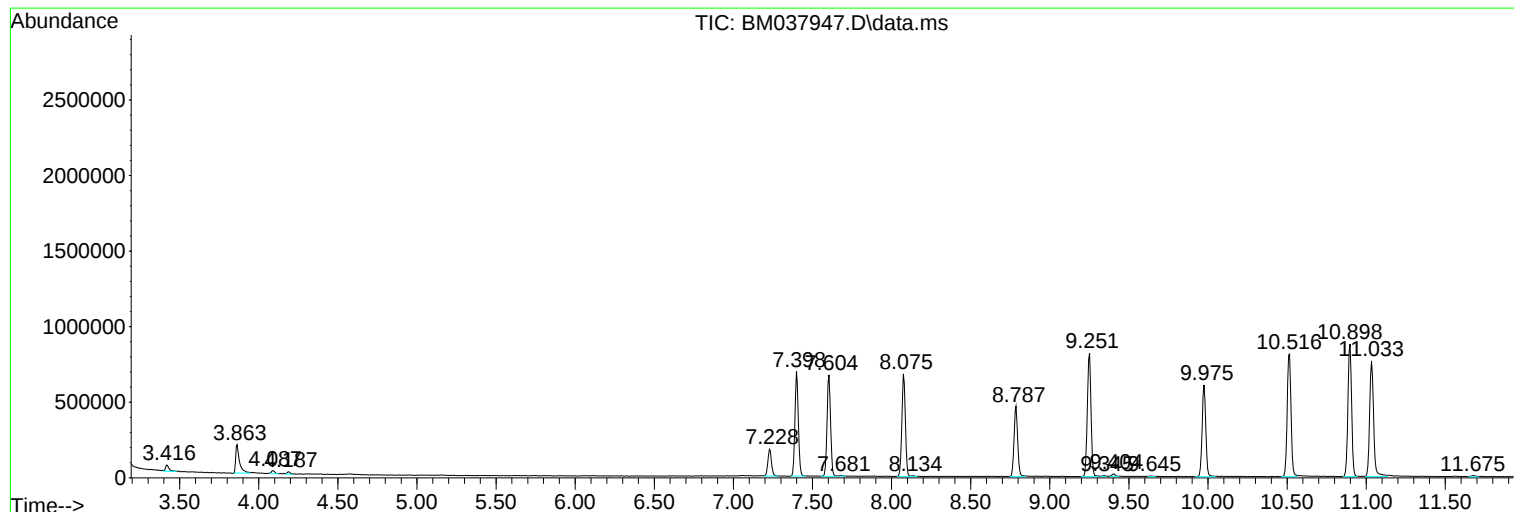

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037947.D
Acq On : 10 Dec 2022 23:20
Operator : CG/JU
Sample : N5927-12
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037947.D
Acq On : 10 Dec 2022 23:20
Operator : CG/JU
Sample : N5927-12
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc