

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037948.D
 Acq On : 10 Dec 2022 23:57
 Operator : CG/JU
 Sample : N5927-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	36	40	43	rBV	36531	47461	1.26%	0.131%
2	3.451	43	45	50	rVB3	9848	13238	0.35%	0.037%
3	3.863	111	115	130	rBV	159994	281822	7.50%	0.778%
4	4.087	150	153	162	rVB3	19347	31963	0.85%	0.088%
5	4.187	166	170	175	rBV2	13701	19536	0.52%	0.054%
6	4.569	233	235	240	rVV5	4521	6486	0.17%	0.018%
7	4.728	258	262	266	rBV3	7578	12358	0.33%	0.034%
8	7.228	681	687	696	rVB	180232	282492	7.52%	0.780%
9	7.398	710	716	724	rBV	685148	1040391	27.68%	2.873%
10	7.604	744	751	761	rBV	687382	1064353	28.32%	2.939%
11	7.681	761	764	769	rVB6	5253	7185	0.19%	0.020%
12	8.075	824	831	839	rBV	614970	946844	25.19%	2.614%
13	8.128	839	840	846	rVB6	3721	5040	0.13%	0.014%
14	8.786	945	952	963	rBV	481605	756275	20.12%	2.088%
15	9.251	1022	1031	1041	rBV	848350	1352034	35.97%	3.733%
16	9.975	1146	1154	1162	rBV	640464	998095	26.56%	2.756%
17	10.516	1237	1246	1255	rBV	844345	1418078	37.73%	3.916%
18	10.798	1292	1294	1299	rBV4	2569	4037	0.11%	0.011%
19	10.898	1303	1311	1318	rVV	794447	1295370	34.46%	3.577%
20	11.033	1326	1334	1349	rBV	740132	1276571	33.96%	3.525%
21	11.686	1443	1445	1451	rVB5	3495	4447	0.12%	0.012%
22	11.780	1459	1461	1469	rVB8	2239	5360	0.14%	0.015%
23	12.127	1515	1520	1522	rBV5	2530	3862	0.10%	0.011%
24	12.474	1574	1579	1585	rVB3	15440	24111	0.64%	0.067%
25	13.598	1765	1770	1778	rVB2	11260	18273	0.49%	0.050%
26	13.674	1780	1783	1788	rVB6	3411	4552	0.12%	0.013%
27	14.116	1850	1858	1872	rBV	1515726	2047743	54.48%	5.654%
28	14.404	1900	1907	1919	rBV	1826983	2584860	68.77%	7.137%
29	14.704	1952	1958	1970	rBV	1002782	1489981	39.64%	4.114%
30	14.904	1987	1992	2005	rBV2	51468	111349	2.96%	0.307%
31	15.110	2022	2027	2032	rBV8	4082	6987	0.19%	0.019%
32	15.368	2068	2071	2076	rVB6	3069	5516	0.15%	0.015%
33	15.486	2087	2091	2093	rBV3	4842	5952	0.16%	0.016%
34	15.692	2115	2126	2140	rBV	2119703	3103092	82.56%	8.568%
35	15.810	2140	2146	2154	rVV	373852	533575	14.20%	1.473%
36	15.927	2163	2166	2171	rVB4	12689	18034	0.48%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037948.D
 Acq On : 10 Dec 2022 23:57
 Operator : CG/JU
 Sample : N5927-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	16.968	2338	2343	2345	rBV6	2160	4125	0.11%	0.011%
38	17.127	2365	2370	2372	rBV4	2873	4265	0.11%	0.012%
39	17.239	2386	2389	2392	rBV4	3457	4406	0.12%	0.012%
40	17.345	2404	2407	2411	rBV6	5854	6677	0.18%	0.018%
41	17.445	2418	2424	2435	rBV	1039424	1462417	38.91%	4.038%
42	17.545	2435	2441	2464	rVV	2292982	3225432	85.82%	8.906%
43	17.715	2467	2470	2477	rVB8	10261	20196	0.54%	0.056%
44	18.092	2532	2534	2542	rVB8	8477	14263	0.38%	0.039%
45	18.321	2567	2573	2579	rBV3	43370	73015	1.94%	0.202%
46	18.398	2584	2586	2588	rVB	8923	7169	0.19%	0.020%
47	19.392	2752	2755	2758	rBV2	28614	31797	0.85%	0.088%
48	19.462	2763	2767	2771	rBV2	29318	47595	1.27%	0.131%
49	19.586	2785	2788	2795	rBV4	41832	61555	1.64%	0.170%
50	19.827	2823	2829	2841	rBV	2686383	3556794	94.63%	9.821%
51	21.615	3128	3133	3141	rBV	1116070	1488758	39.61%	4.111%
52	23.938	3520	3528	3545	rBV2	1786505	3758515	100.00%	10.378%
53	24.097	3548	3555	3567	rVB2	759273	1622191	43.16%	4.479%




Sum of corrected areas: 36216493

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037948.D
Acq On : 10 Dec 2022 23:57
Operator : CG/JU
Sample : N5927-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

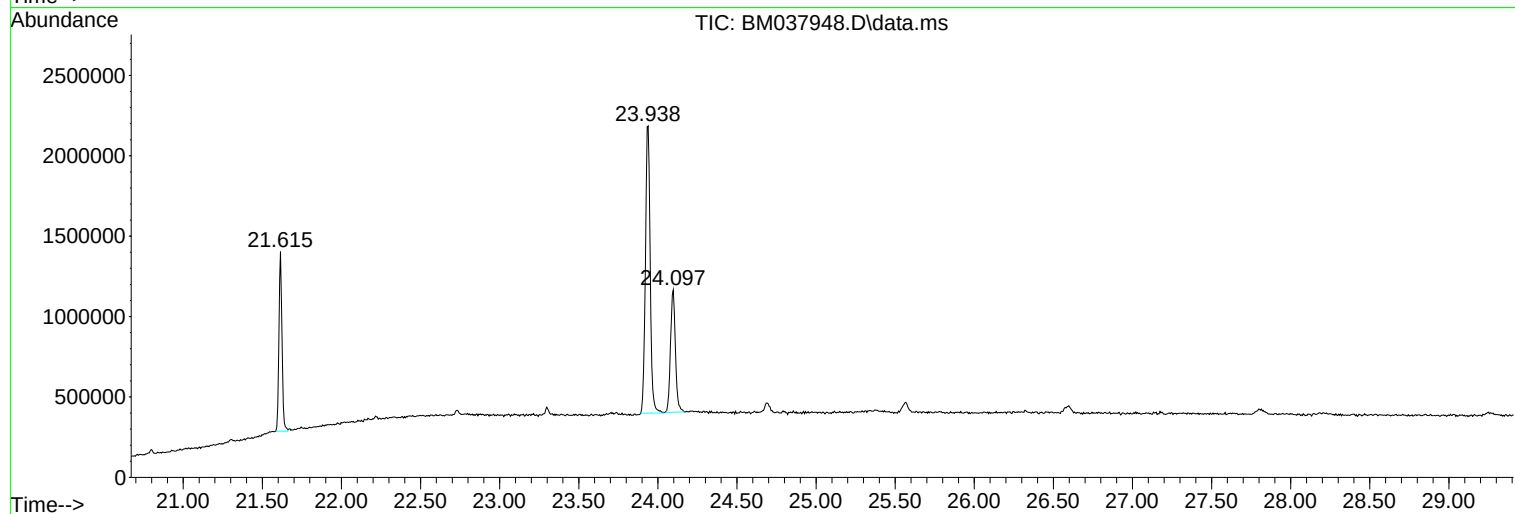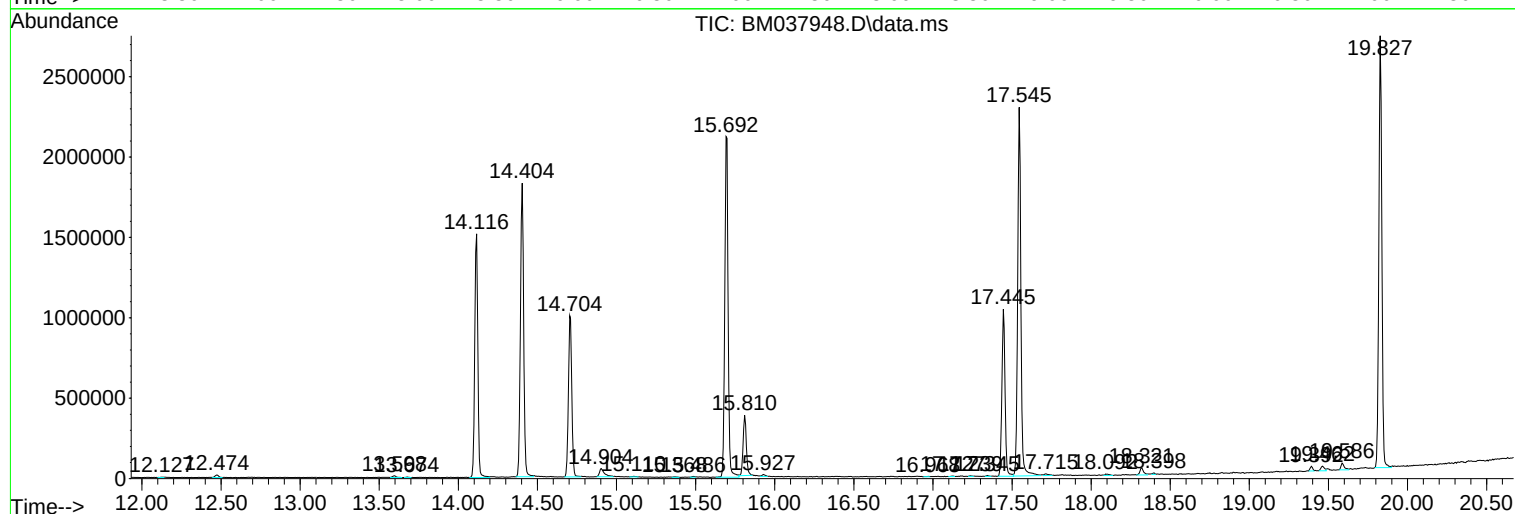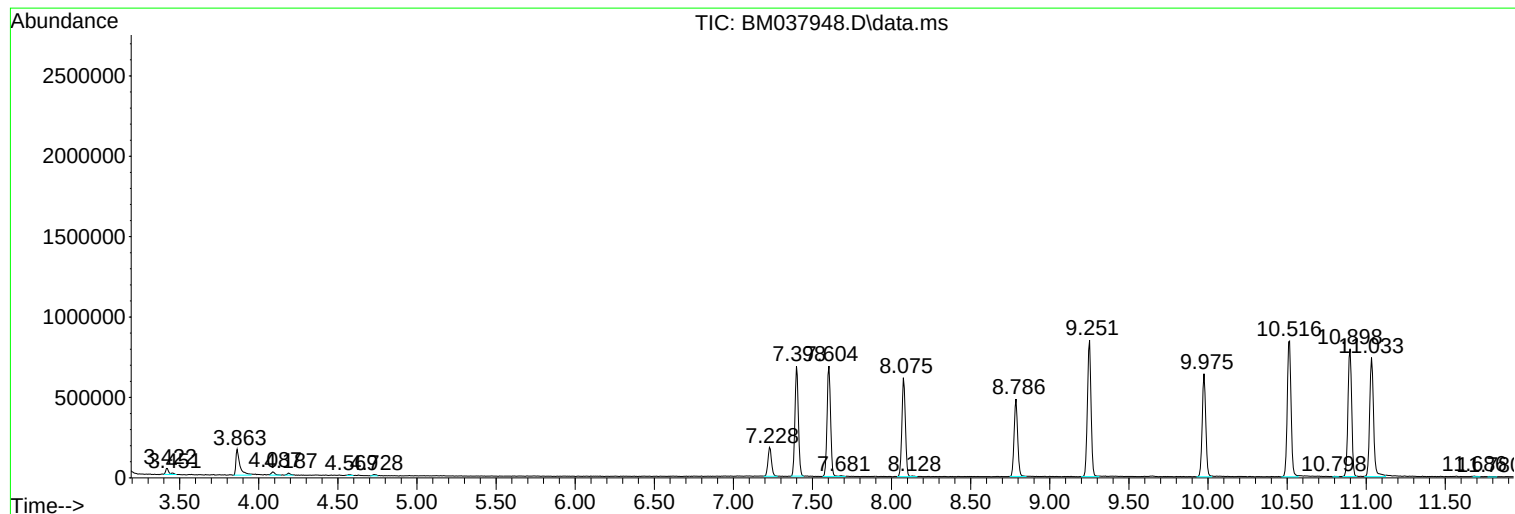

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037948.D
Acq On : 10 Dec 2022 23:57
Operator : CG/JU
Sample : N5927-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037948.D
Acq On : 10 Dec 2022 23:57
Operator : CG/JU
Sample : N5927-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
