

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037951.D
 Acq On : 11 Dec 2022 01:46
 Operator : CG/JU
 Sample : N5927-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	35	39	45	rBV	47441	66226	1.70%	0.171%
2	3.857	111	114	129	rBV	199619	347813	8.93%	0.897%
3	4.087	149	153	165	rVB	23611	40051	1.03%	0.103%
4	4.187	167	170	178	rVB2	16290	24575	0.63%	0.063%
5	4.569	231	235	238	rBV5	6801	9758	0.25%	0.025%
6	6.104	490	496	500	rVB8	2354	4314	0.11%	0.011%
7	6.716	594	600	601	rBV4	2304	4165	0.11%	0.011%
8	7.228	681	687	698	rVB	197879	323553	8.31%	0.835%
9	7.398	710	716	725	rBV	742462	1119831	28.76%	2.888%
10	7.604	744	751	760	rBV	731090	1107346	28.44%	2.856%
11	7.681	761	764	768	rVB6	3389	5492	0.14%	0.014%
12	8.075	825	831	838	rBV	780557	1200143	30.82%	3.095%
13	8.139	838	842	847	rVB6	3933	6204	0.16%	0.016%
14	8.786	943	952	960	rBV	513336	808665	20.77%	2.086%
15	9.086	999	1003	1007	rVB7	2690	4475	0.11%	0.012%
16	9.251	1022	1031	1040	rBV	867530	1424534	36.58%	3.674%
17	9.404	1052	1057	1062	rVB3	18157	29111	0.75%	0.075%
18	9.639	1094	1097	1102	rVB4	3195	4189	0.11%	0.011%
19	9.975	1146	1154	1164	rBV	590706	962640	24.72%	2.483%
20	10.510	1239	1245	1259	rBV	871958	1431971	36.77%	3.693%
21	10.898	1303	1311	1320	rBV	1002374	1623136	41.68%	4.186%
22	11.033	1327	1334	1356	rBV	779995	1365058	35.05%	3.521%
23	11.680	1438	1444	1448	rBV8	4683	9404	0.24%	0.024%
24	12.380	1559	1563	1567	rBV5	3296	5450	0.14%	0.014%
25	12.474	1574	1579	1584	rVB2	16722	25171	0.65%	0.065%
26	13.316	1717	1722	1724	rBV5	2313	4388	0.11%	0.011%
27	13.598	1764	1770	1773	rBV5	6707	9130	0.23%	0.024%
28	13.680	1779	1784	1790	rBV7	2959	5971	0.15%	0.015%
29	14.115	1851	1858	1870	rBV	1464734	2006268	51.52%	5.175%
30	14.404	1900	1907	1926	rBV	1805360	2652220	68.11%	6.841%
31	14.704	1952	1958	1968	rBV	1240275	1831615	47.04%	4.724%
32	14.904	1987	1992	2004	rBV2	46792	107238	2.75%	0.277%
33	15.115	2022	2028	2034	rVB10	7738	15217	0.39%	0.039%
34	15.480	2088	2090	2093	rVB3	4109	4033	0.10%	0.010%
35	15.692	2120	2126	2140	rBV	2126296	3050855	78.35%	7.869%
36	15.809	2140	2146	2155	rVB	308580	434413	11.16%	1.120%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037951.D
 Acq On : 11 Dec 2022 01:46
 Operator : CG/JU
 Sample : N5927-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	15.927	2161	2166	2171	rVB8	9642	19969	0.51%	0.052%
38	16.898	2328	2331	2334	rVB5	3747	4222	0.11%	0.011%
39	17.445	2417	2424	2435	rBV	1303868	1834307	47.11%	4.731%
40	17.545	2435	2441	2452	rVV	2257719	3150529	80.91%	8.126%
41	17.715	2467	2470	2475	rVB6	5832	7578	0.19%	0.020%
42	18.103	2533	2536	2541	rVB7	3854	5042	0.13%	0.013%
43	18.315	2568	2572	2580	rBV5	26923	49266	1.27%	0.127%
44	18.403	2583	2587	2592	rVB2	13482	18908	0.49%	0.049%
45	18.545	2608	2611	2613	rBV4	5159	6006	0.15%	0.015%
46	18.745	2642	2645	2648	rBV5	9605	12792	0.33%	0.033%
47	18.821	2656	2658	2662	rBV5	3973	5001	0.13%	0.013%
48	19.392	2751	2755	2761	rVB4	26527	36384	0.93%	0.094%
49	19.462	2763	2767	2771	rBV2	28491	41606	1.07%	0.107%
50	19.586	2785	2788	2794	rBV4	29370	42815	1.10%	0.110%
51	19.827	2823	2829	2841	rBV	2796124	3679508	94.49%	9.490%
52	21.615	3128	3133	3145	rVB	1511643	1901420	48.83%	4.904%
53	23.932	3520	3527	3540	rBV2	1832454	3894052	100.00%	10.044%
54	24.097	3548	3555	3565	rBV2	958902	1987486	51.04%	5.126%




Sum of corrected areas: 38771514

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037951.D
Acq On : 11 Dec 2022 01:46
Operator : CG/JU
Sample : N5927-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

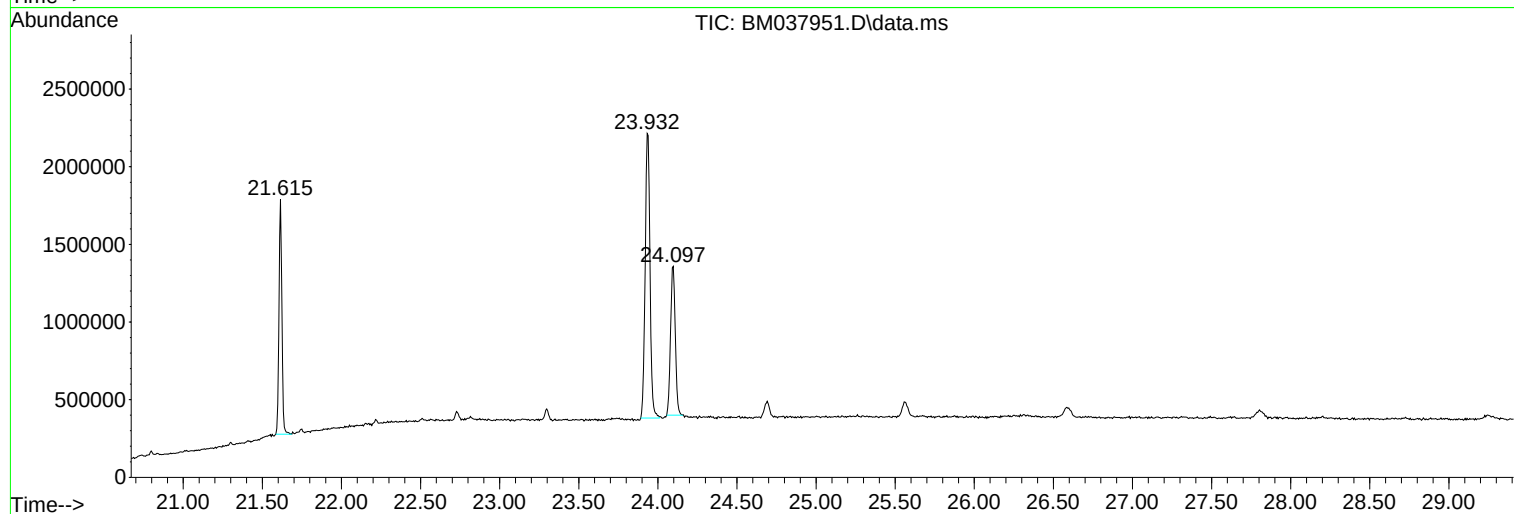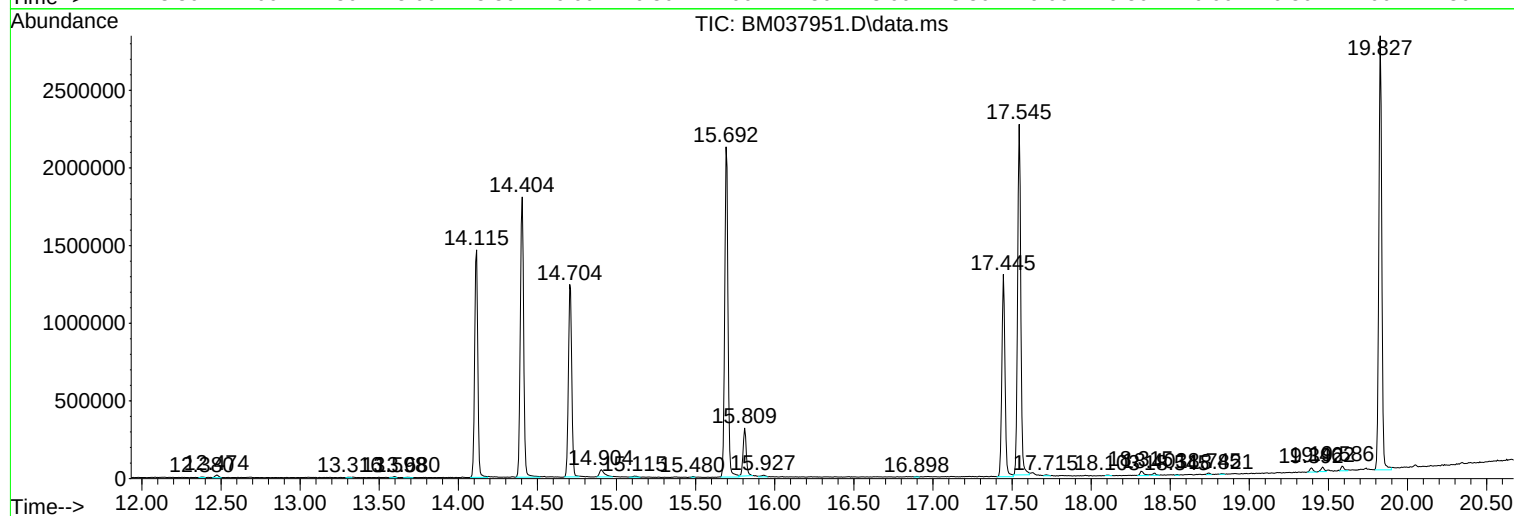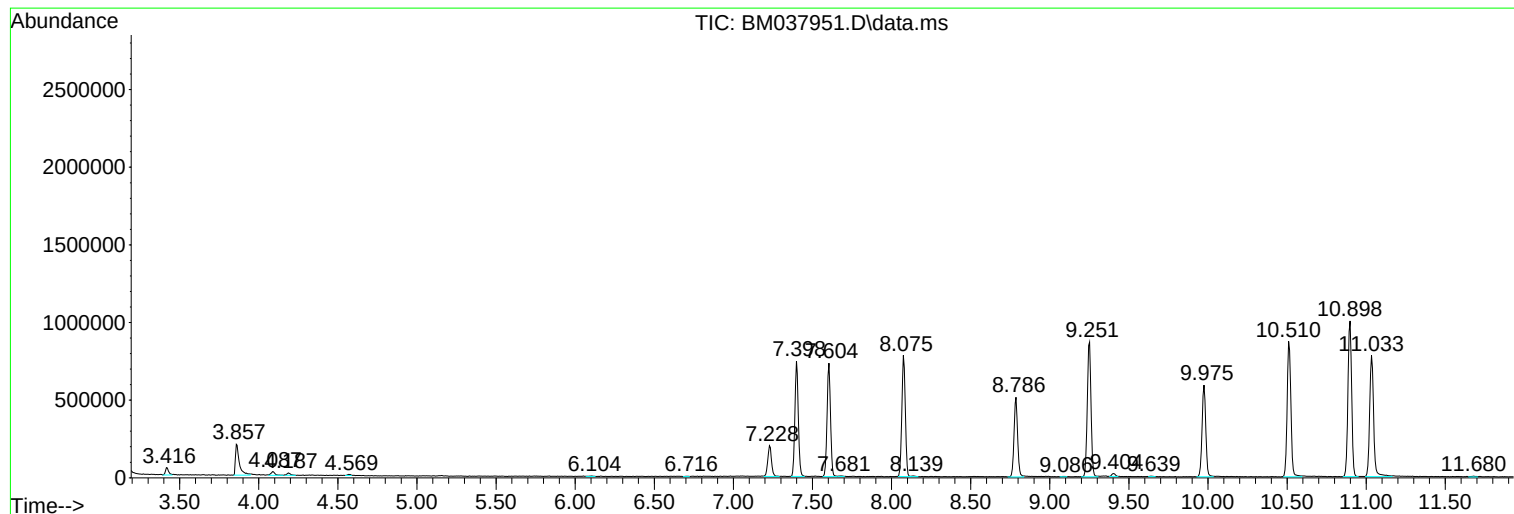

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037951.D
Acq On : 11 Dec 2022 01:46
Operator : CG/JU
Sample : N5927-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037951.D
Acq On : 11 Dec 2022 01:46
Operator : CG/JU
Sample : N5927-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc