

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037952.D
 Acq On : 11 Dec 2022 02:22
 Operator : CG/JU
 Sample : N5927-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	36	39	44	rBV	40251	53278	1.29%	0.135%
2	3.858	111	114	129	rBV	215426	359743	8.74%	0.910%
3	4.087	149	153	159	rVB4	18907	32142	0.78%	0.081%
4	4.187	167	170	175	rVB2	13775	17793	0.43%	0.045%
5	7.228	681	687	698	rVB	168950	267813	6.51%	0.678%
6	7.398	709	716	728	rVB	734879	1114934	27.09%	2.821%
7	7.604	743	751	761	rBV	696842	1091473	26.52%	2.762%
8	7.687	761	765	768	rVB5	3248	5604	0.14%	0.014%
9	8.075	820	831	838	rBV	756817	1167522	28.37%	2.954%
10	8.787	944	952	962	rBV	459818	739887	17.98%	1.872%
11	9.251	1023	1031	1040	rBV	893310	1428426	34.71%	3.614%
12	9.351	1045	1048	1053	rVB6	3124	5054	0.12%	0.013%
13	9.975	1146	1154	1166	rBV	637631	1048803	25.48%	2.654%
14	10.510	1238	1245	1257	rBV	870443	1435869	34.89%	3.633%
15	10.898	1302	1311	1319	rBV	970005	1588633	38.60%	4.019%
16	11.034	1327	1334	1350	rBV	778006	1320027	32.07%	3.340%
17	11.428	1396	1401	1405	rBV	12811	18169	0.44%	0.046%
18	11.486	1406	1411	1416	rVB2	10639	19643	0.48%	0.050%
19	11.675	1435	1443	1447	rBV9	4533	10324	0.25%	0.026%
20	12.475	1574	1579	1584	rVB2	16051	25078	0.61%	0.063%
21	13.069	1677	1680	1686	rVB5	4803	7460	0.18%	0.019%
22	13.316	1717	1722	1728	rVB4	6948	12110	0.29%	0.031%
23	13.592	1766	1769	1775	rBV5	3514	5174	0.13%	0.013%
24	14.110	1851	1857	1870	rBV	1457262	2065449	50.19%	5.226%
25	14.404	1900	1907	1918	rBV	1776542	2627654	63.85%	6.648%
26	14.704	1952	1958	1972	rBV	1237689	1824959	44.34%	4.617%
27	14.904	1986	1992	2003	rBV2	45892	101786	2.47%	0.258%
28	15.104	2022	2026	2035	rVV10	6027	13338	0.32%	0.034%
29	15.486	2085	2091	2100	rVB2	13291	21724	0.53%	0.055%
30	15.692	2120	2126	2139	rBV	2150557	3126921	75.98%	7.911%
31	15.810	2140	2146	2161	rVV	441637	634805	15.42%	1.606%
32	15.927	2163	2166	2170	rVB5	11126	16322	0.40%	0.041%
33	16.898	2327	2331	2333	rBV4	4421	6485	0.16%	0.016%
34	17.445	2418	2424	2435	rBV	1273747	1788622	43.46%	4.525%
35	17.545	2435	2441	2463	rVB	2467292	3396113	82.52%	8.593%
36	17.821	2484	2488	2492	rBV5	4565	7595	0.18%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037952.D
Acq On : 11 Dec 2022 02:22
Operator : CG/JU
Sample : N5927-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Title : SVOA CALIBRATION

37	18.104	2532	2536	2541	rBV8	6752	11030	0.27%	0.028%
38	18.321	2567	2573	2578	rBV4	40484	62493	1.52%	0.158%
39	18.745	2641	2645	2647	rBV5	7943	8246	0.20%	0.021%
40	19.392	2752	2755	2761	rVB3	26922	32397	0.79%	0.082%
41	19.462	2763	2767	2770	rBV	26793	31959	0.78%	0.081%
42	19.586	2785	2788	2794	rBV5	34369	48658	1.18%	0.123%
43	19.827	2823	2829	2838	rBV	3014428	3869842	94.03%	9.791%
44	21.615	3128	3133	3145	rVB	1454260	1912301	46.47%	4.838%
45	23.933	3520	3527	3541	rBV2	1987513	4115467	100.00%	10.413%
46	24.092	3548	3554	3567	rVB2	953712	2024988	49.20%	5.123%




Sum of corrected areas: 39524113

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037952.D
Acq On : 11 Dec 2022 02:22
Operator : CG/JU
Sample : N5927-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

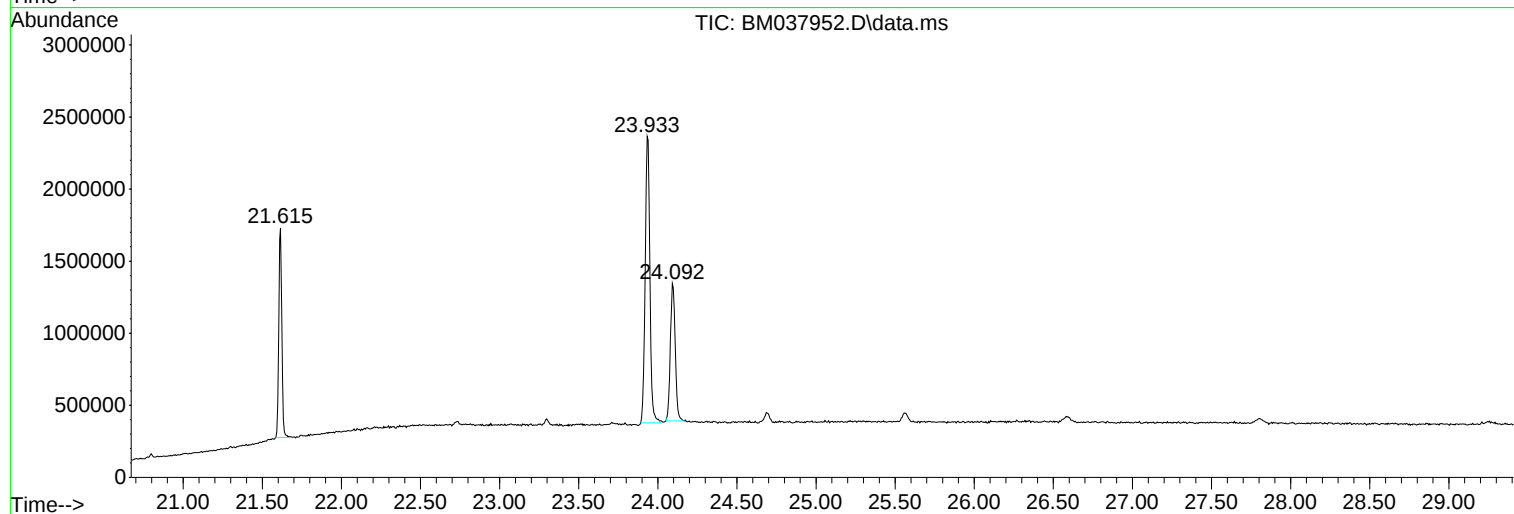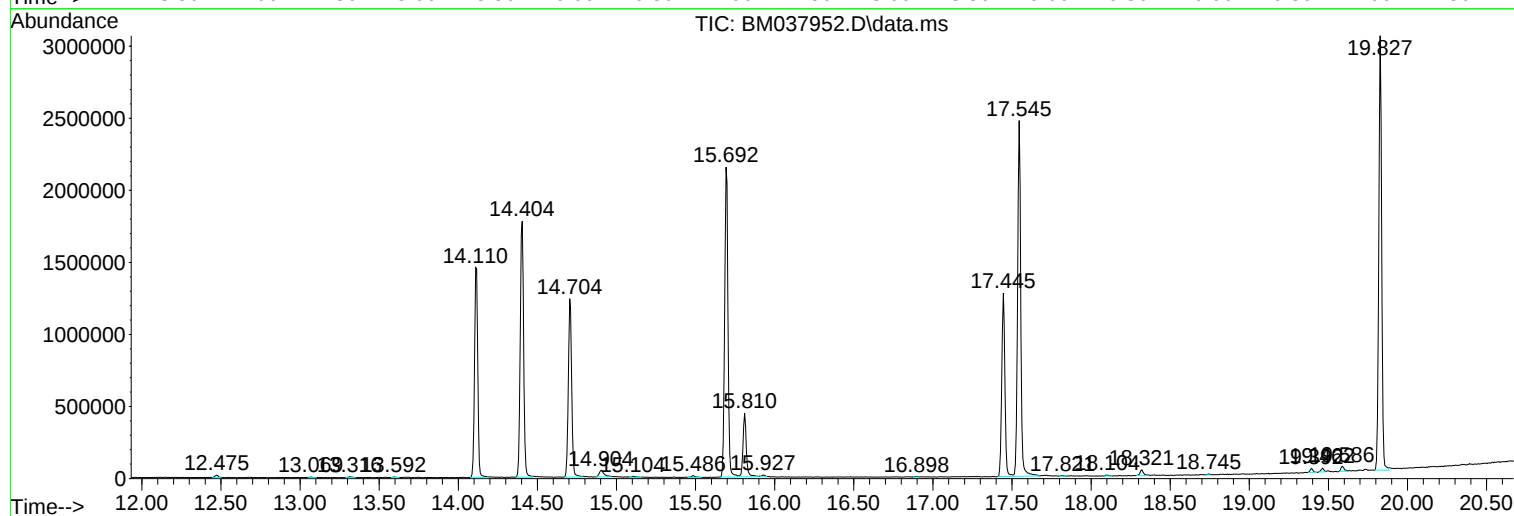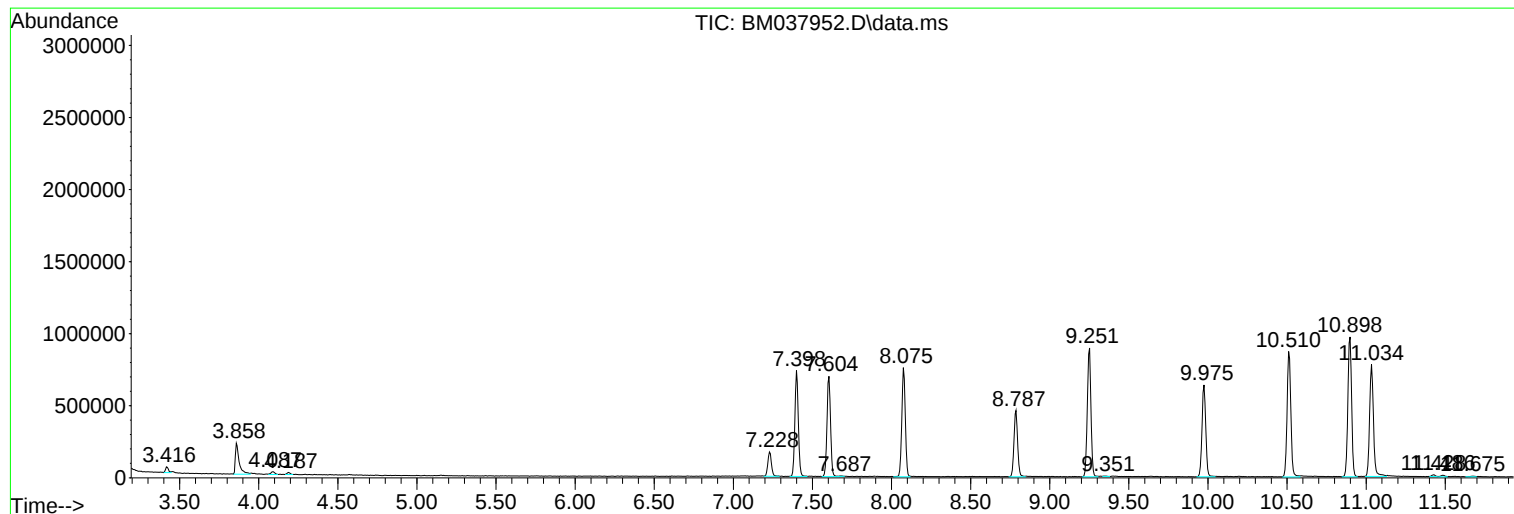

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037952.D
Acq On : 11 Dec 2022 02:22
Operator : CG/JU
Sample : N5927-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037952.D
Acq On : 11 Dec 2022 02:22
Operator : CG/JU
Sample : N5927-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
