

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037955.D
 Acq On : 11 Dec 2022 04:11
 Operator : CG/JU
 Sample : N5927-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037955.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	29	33	38	rBV	274312	402131	8.99%	1.022%
2	4.087	149	153	160	rVB	22975	35769	0.80%	0.091%
3	4.187	167	170	177	rVB3	15597	21232	0.47%	0.054%
4	4.293	185	188	196	rVB3	30343	44874	1.00%	0.114%
5	4.575	234	236	241	rVB6	4502	4889	0.11%	0.012%
6	4.734	257	263	274	rVB	1076864	1529738	34.21%	3.886%
7	5.481	388	390	393	rVB3	4364	4721	0.11%	0.012%
8	7.228	681	687	698	rVB	321977	497408	11.13%	1.264%
9	7.398	709	716	726	rBV	702525	1051154	23.51%	2.670%
10	7.604	744	751	759	rBV	845708	1320896	29.54%	3.355%
11	7.675	761	763	770	rVB7	5756	9329	0.21%	0.024%
12	8.075	824	831	838	rBV	632803	977088	21.85%	2.482%
13	8.133	838	841	845	rVB6	3526	4903	0.11%	0.012%
14	8.786	945	952	964	rBV	688141	1099389	24.59%	2.793%
15	9.251	1023	1031	1040	rBV	789119	1294515	28.95%	3.288%
16	9.645	1093	1098	1103	rVB5	3340	6563	0.15%	0.017%
17	9.975	1145	1154	1162	rBV	631081	1022173	22.86%	2.597%
18	10.510	1238	1245	1261	rBV	907548	1508806	33.75%	3.833%
19	10.898	1302	1311	1319	rBV	758631	1258916	28.16%	3.198%
20	11.033	1328	1334	1342	rBV	128445	229377	5.13%	0.583%
21	11.674	1440	1443	1447	rBV5	4352	7054	0.16%	0.018%
22	12.474	1572	1579	1583	rBV2	14267	23489	0.53%	0.060%
23	13.592	1765	1769	1773	rVB4	6495	9530	0.21%	0.024%
24	14.110	1851	1857	1872	rBV	1318225	1852377	41.43%	4.706%
25	14.404	1900	1907	1923	rBV	1630844	2395458	53.58%	6.085%
26	14.704	1951	1958	1973	rBV	966611	1410292	31.54%	3.583%
27	14.898	1985	1991	2006	rBV	136455	281035	6.29%	0.714%
28	15.110	2022	2027	2032	rVB8	6709	11835	0.26%	0.030%
29	15.439	2078	2083	2086	rVB6	3399	5525	0.12%	0.014%
30	15.692	2120	2126	2139	rVV	1966960	2841959	63.56%	7.219%
31	15.809	2140	2146	2163	rVV	498150	727452	16.27%	1.848%
32	15.933	2163	2167	2172	rVB4	11294	18272	0.41%	0.046%
33	16.468	2256	2258	2266	rBV8	4241	9410	0.21%	0.024%
34	16.968	2341	2343	2348	rVB6	3715	4955	0.11%	0.013%
35	17.180	2375	2379	2383	rBV5	4704	5338	0.12%	0.014%
36	17.227	2386	2387	2391	rBV4	3882	5016	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
 Data File : BM037955.D
 Acq On : 11 Dec 2022 04:11
 Operator : CG/JU
 Sample : N5927-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	17.445	2418	2424	2435	rBV	1093558	1547331	34.61%	3.931%
38	17.545	2435	2441	2457	rVV	2305164	3246803	72.62%	8.248%
39	17.651	2457	2459	2464	rVV4	11503	19087	0.43%	0.048%
40	17.709	2467	2469	2478	rVB7	8926	16908	0.38%	0.043%
41	17.927	2502	2506	2509	rVB4	3918	4842	0.11%	0.012%
42	18.068	2528	2530	2533	rBV4	3815	4872	0.11%	0.012%
43	18.103	2533	2536	2538	rVV4	5058	6513	0.15%	0.017%
44	18.203	2550	2553	2559	rBV9	5744	11058	0.25%	0.028%
45	18.315	2568	2572	2579	rBV2	89803	128352	2.87%	0.326%
46	18.398	2582	2586	2590	rVB	21868	26987	0.60%	0.069%
47	18.609	2619	2622	2625	rBV5	5142	5713	0.13%	0.015%
48	19.392	2751	2755	2760	rBV3	29443	43579	0.97%	0.111%
49	19.462	2762	2767	2770	rBV2	33031	47599	1.06%	0.121%
50	19.586	2785	2788	2795	rBV2	86550	118962	2.66%	0.302%
51	19.827	2823	2829	2838	rBV	3149483	3978590	88.99%	10.107%
52	21.615	3128	3133	3142	rBV	1385942	1801146	40.29%	4.575%
53	23.938	3520	3528	3539	rBV2	2165077	4471007	100.00%	11.358%
54	24.091	3548	3554	3564	rVB2	953691	1953349	43.69%	4.962%




Sum of corrected areas: 39365566

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037955.D
Acq On : 11 Dec 2022 04:11
Operator : CG/JU
Sample : N5927-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

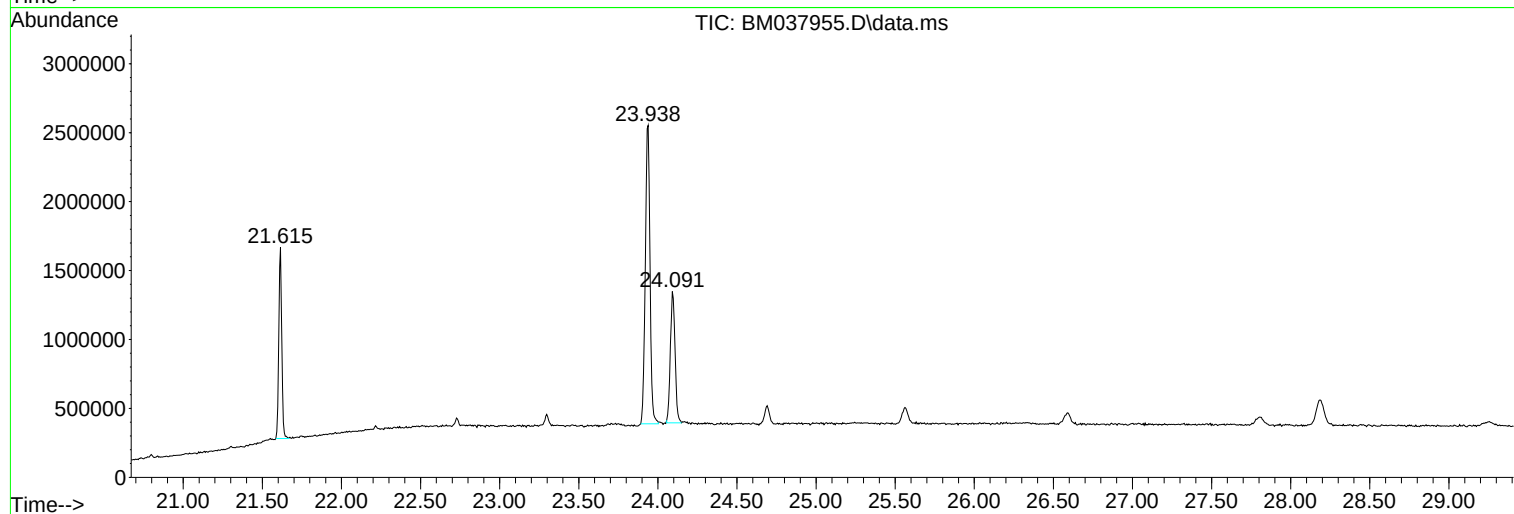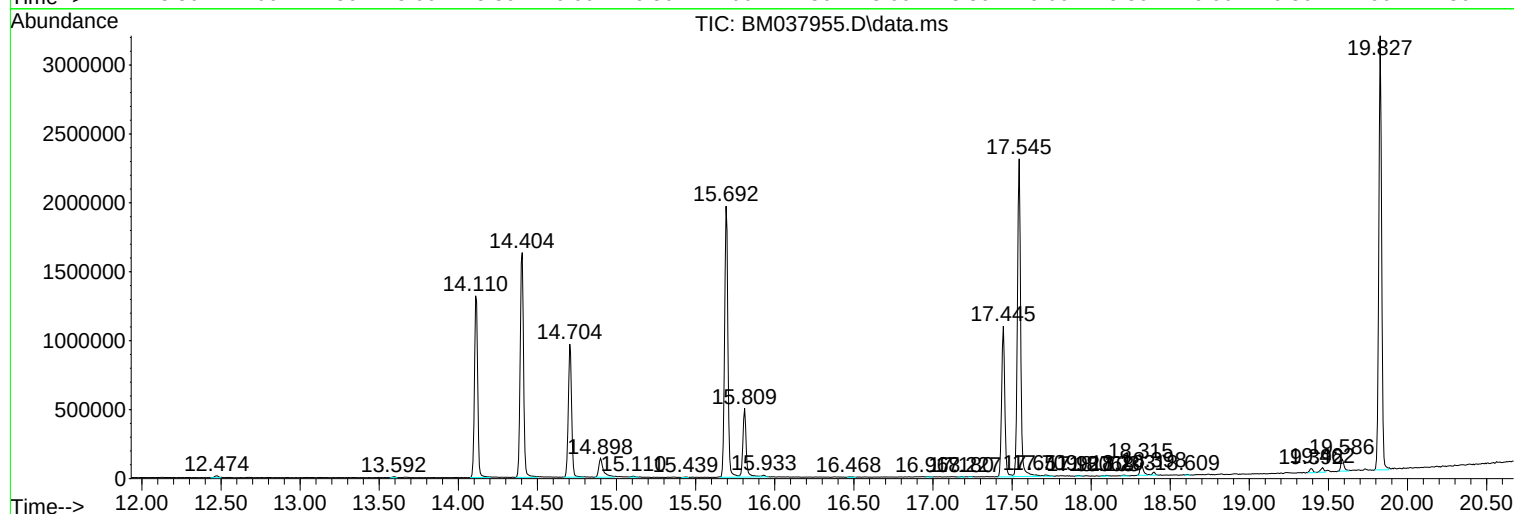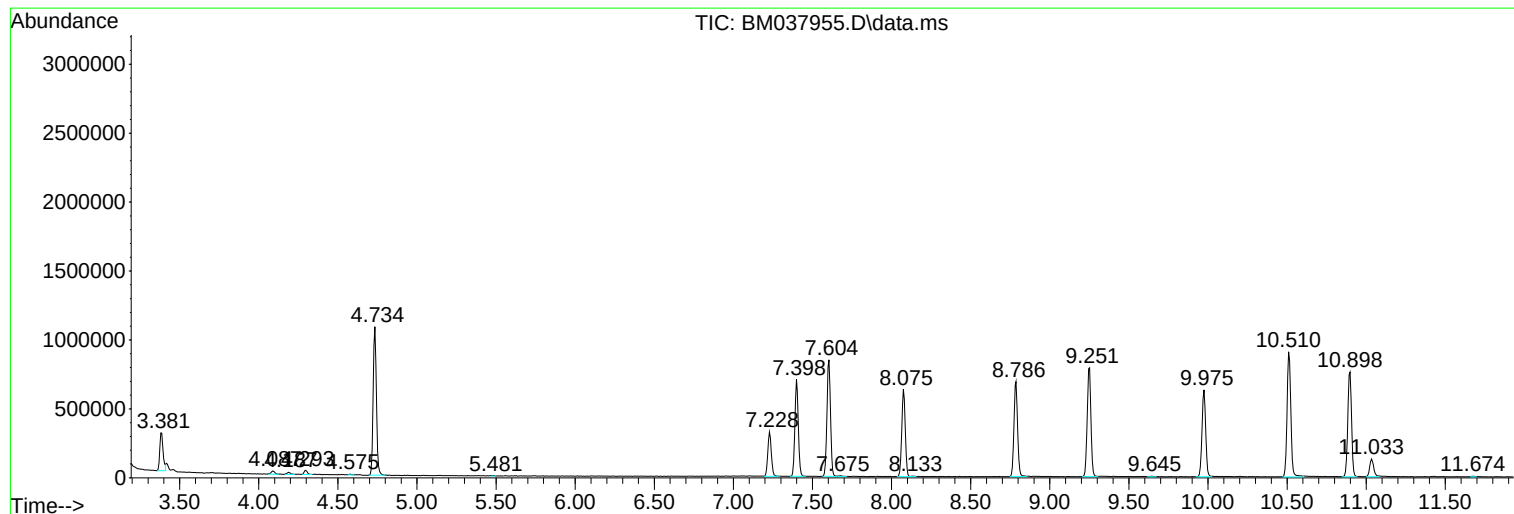

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037955.D
Acq On : 11 Dec 2022 04:11
Operator : CG/JU
Sample : N5927-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ91










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.734	31.31 ng/ul	1529740	1,4-Dichlorobenzene-d4	8.075

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HCl2FN2	002927-71-1	38

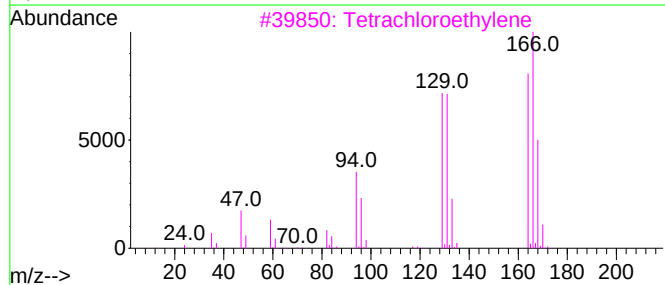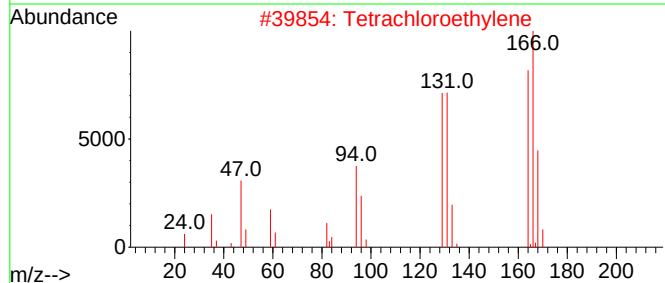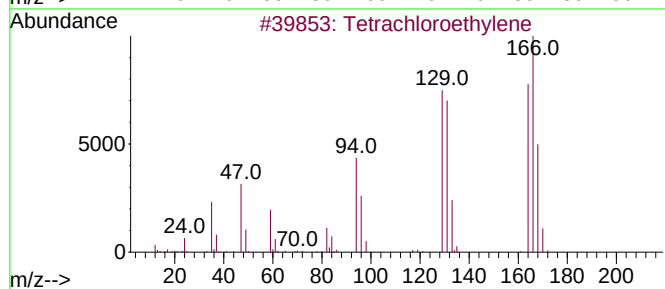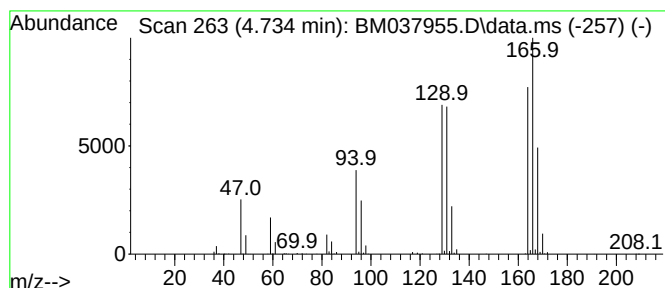

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121022\
Data File : BM037955.D
Acq On : 11 Dec 2022 04:11
Operator : CG/JU
Sample : N5927-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.734	31.3	ng/u1	1529740	1	8.075	977088	20.0