

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
 Data File : BM048928.D
 Acq On : 10 Dec 2024 17:57
 Operator : RC/JU
 Sample : P5109-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 10 22:50:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 09 17:52:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	3508	0.400	ng/ul	0.00
4) Naphthalene-d8	10.348	136	9688	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.215	164	5281	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.061	188	1164165	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.16
23) Perylene-d12	23.323	264	12169	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.159	96	20898	5.097	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.948	152	4622	0.374	ng/ul	0.00
18) Fluoranthene-d10	18.997	212	10904	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.214	166	2050	0.109	ng/ul#	15
26) Benzo(a)pyrene	23.188	252	4535	0.117	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048928.D
Acq On : 10 Dec 2024 17:57
Operator : RC/JU
Sample : P5109-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 10 22:50:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

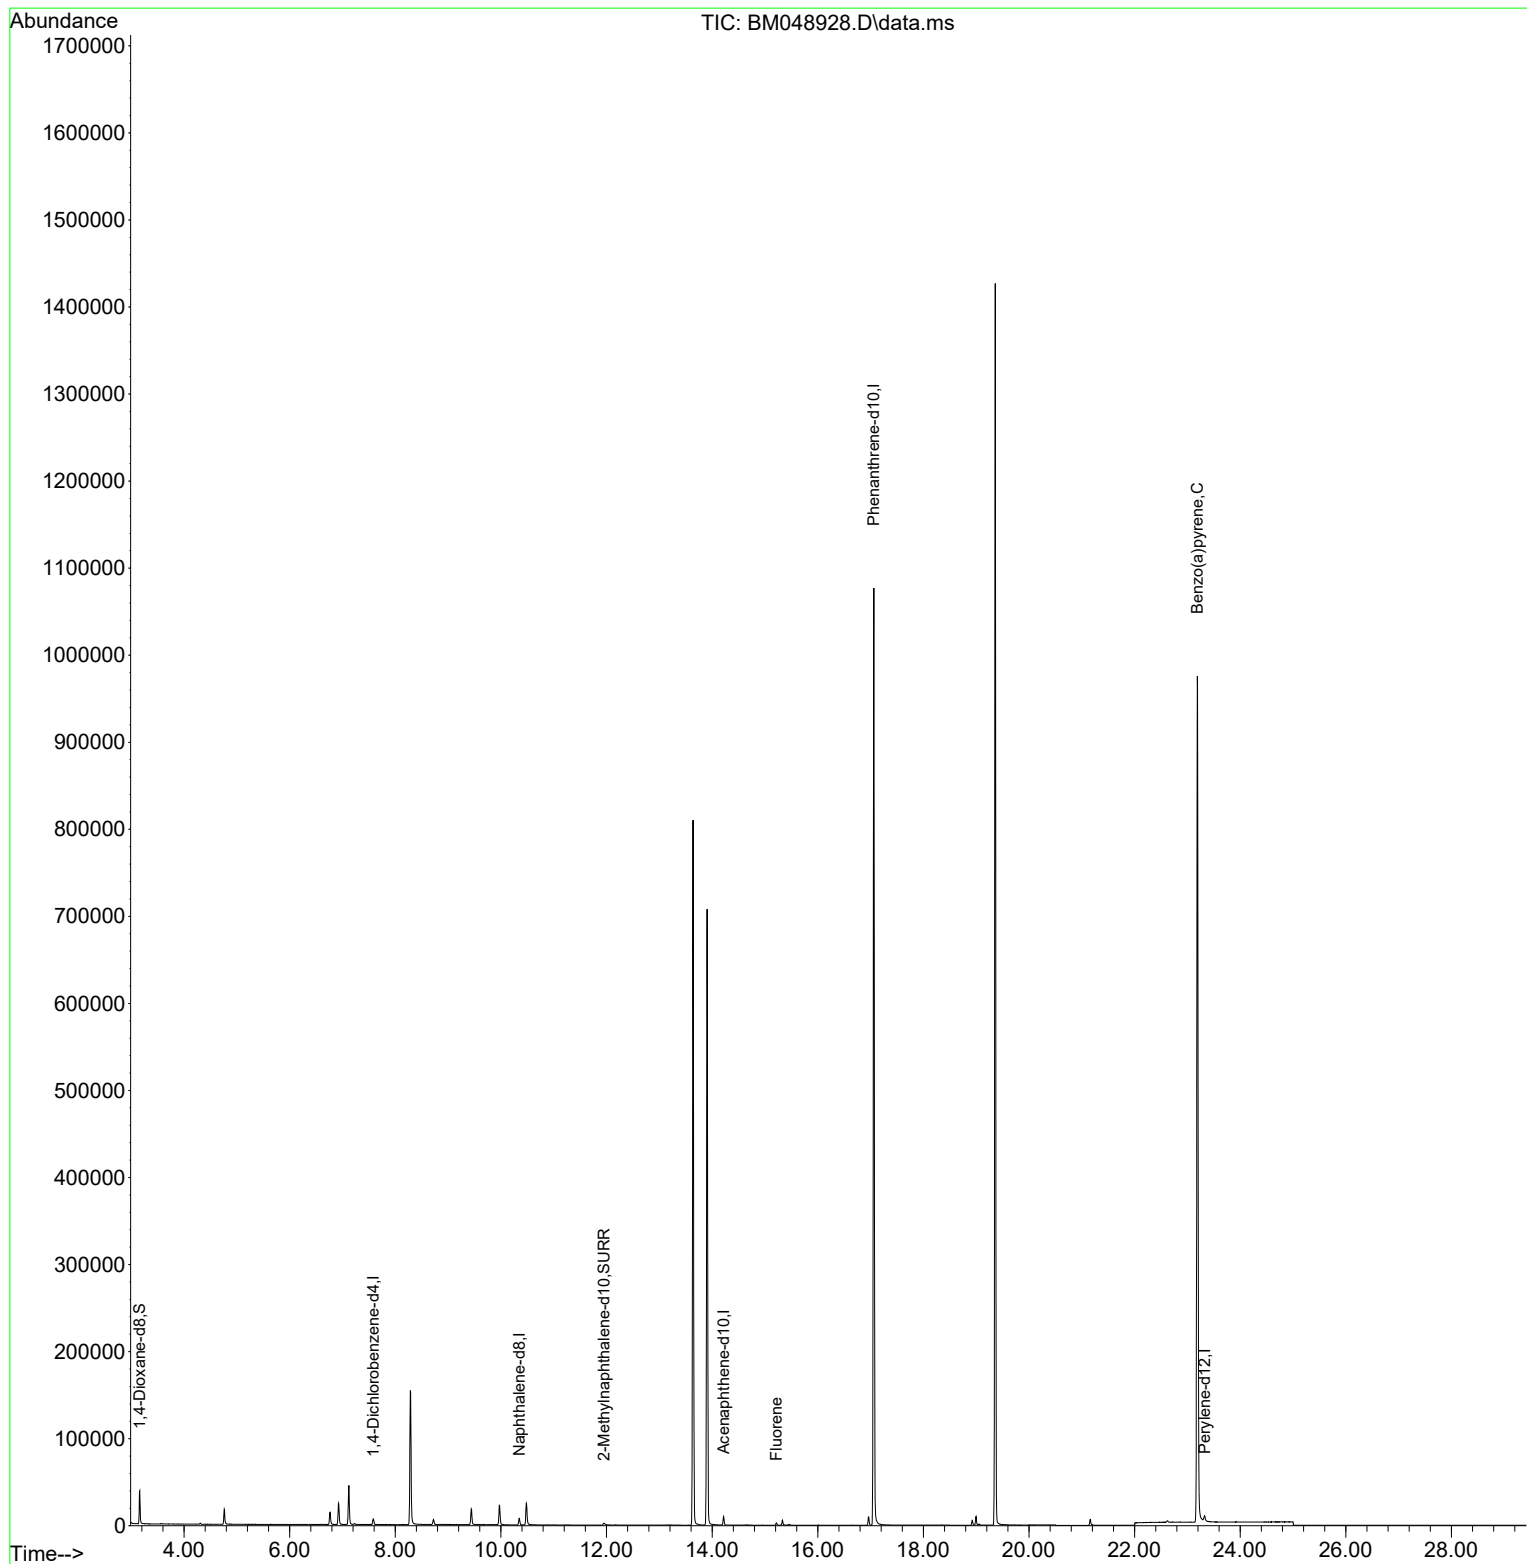

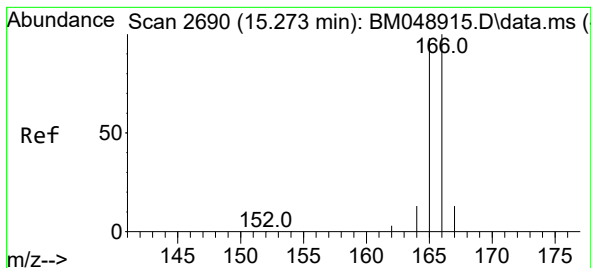

#12

Fluorene

Concen: 0.109 ng/ul

RT: 15.214 min Scan# 2

Delta R.T. -0.063 min

Lab File: BM048928.D





Acq: 10 Dec 2024 17:57

Instrument :

BNA_M

ClientSampleId :

Tgt Ion:166	Resp:	2050
Ion	Ratio	Lower Upper
166	100	
165	8.4	78.1 117.1#
167	34.5	11.6 17.4#

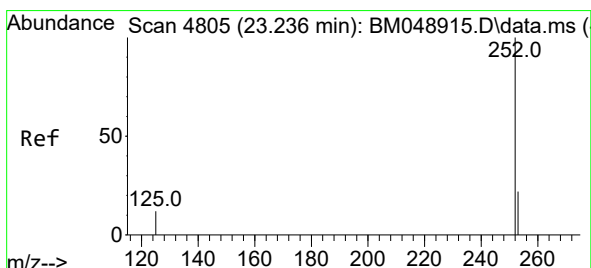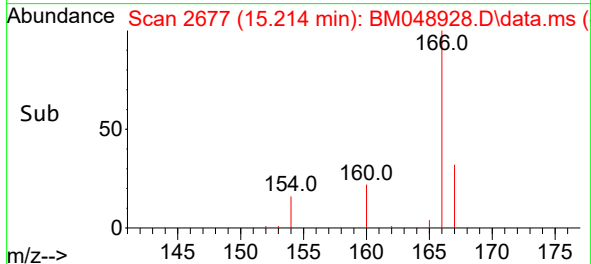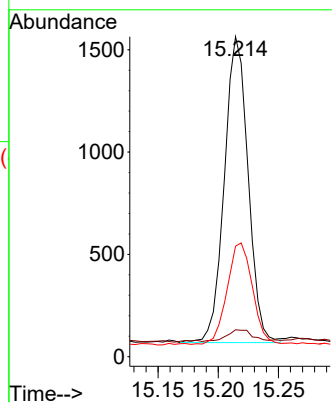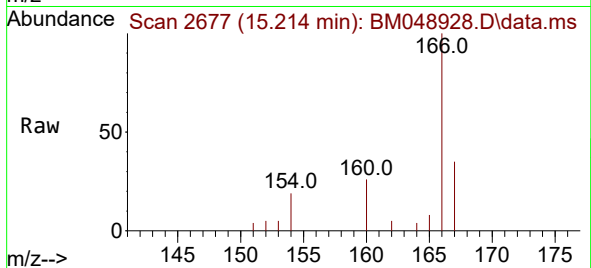

#26

Benzo(a)pyrene

Concen: 0.117 ng/ul

RT: 23.188 min Scan# 4789

Delta R.T. -0.053 min

Lab File: BM048928.D

Acq: 10 Dec 2024 17:57

Tgt Ion:252	Resp:	4535
Ion	Ratio	Lower Upper
252	100	
253	37.8	21.8 32.8#
125	36.2	18.6 27.8#

