

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
 Data File : BM048933.D
 Acq On : 10 Dec 2024 21:33
 Operator : RC/JU
 Sample : PB165509BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 10 22:50:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 09 17:52:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	3579	0.400	ng/ul	0.00
4) Naphthalene-d8	10.347	136	9232	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.218	164	4812	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.060	188	746681	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.16
23) Perylene-d12	23.323	264	10872	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.159	96	24548	5.869	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.952	152	3390	0.288	ng/ul	0.00
18) Fluoranthene-d10	18.996	212	6875	0.000	ng/ul	0.00
Target Compounds						
26) Benzo(a)pyrene	23.186	252	2961	0.085	ng/ul#	Qvalue 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048933.D
Acq On : 10 Dec 2024 21:33
Operator : RC/JU
Sample : PB165509BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Dec 10 22:50:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

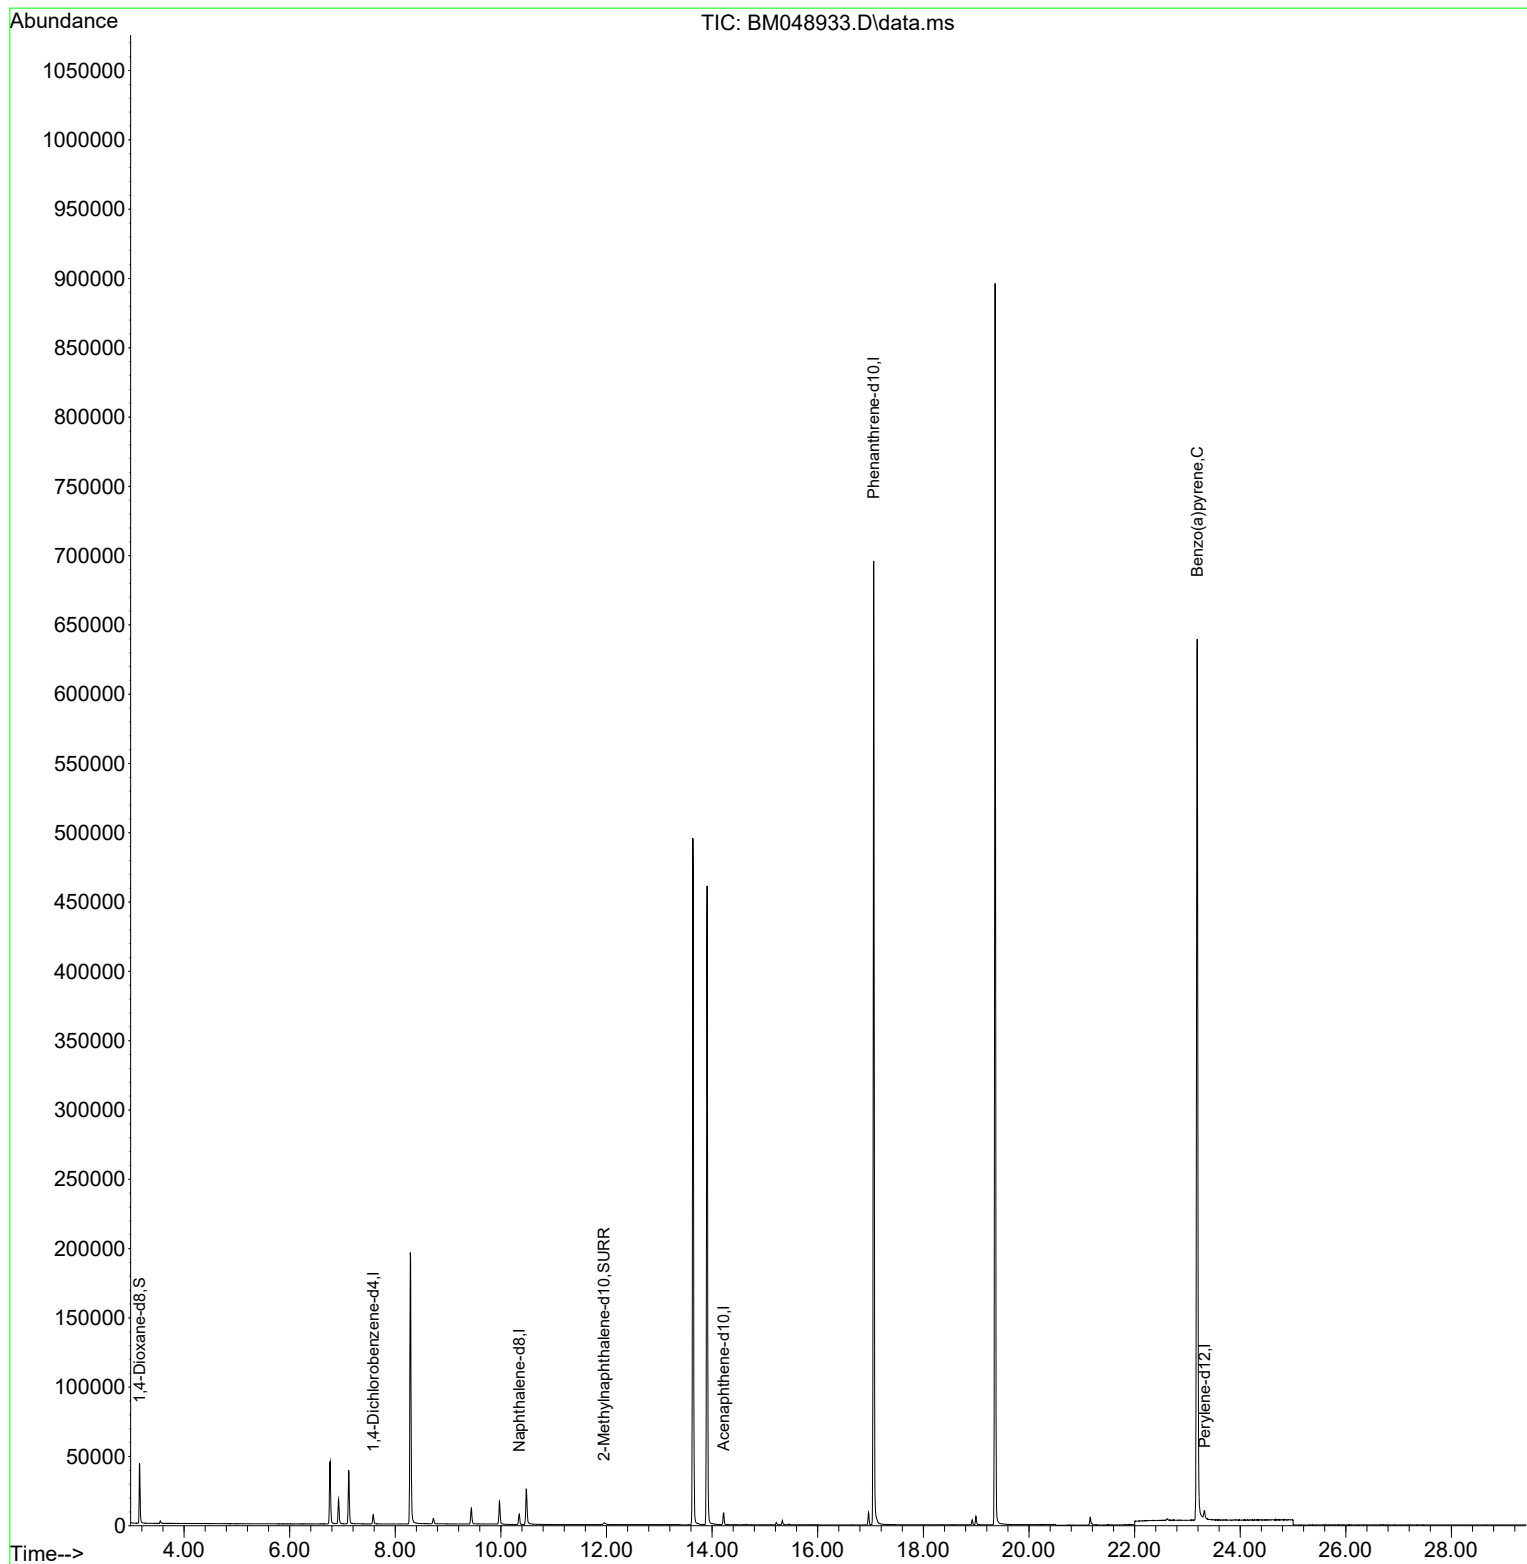

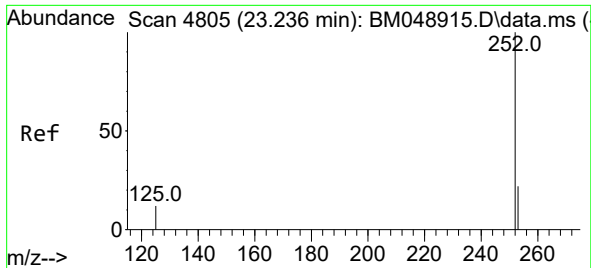

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.186 min Scan# 41
Delta R.T. -0.056 min
Lab File: BM048933.D
Acq: 10 Dec 2024 21:33

Instrument :
BNA_M
ClientSampleId :

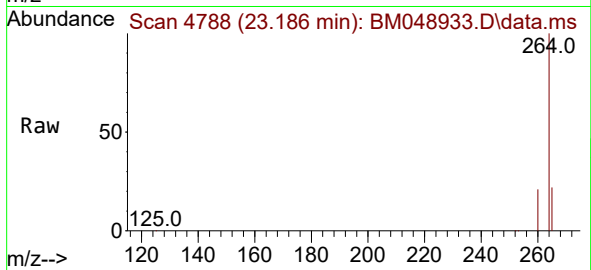

Tgt Ion:252 Resp: 2961
Ion Ratio Lower Upper
252 100
253 40.7 21.8 32.8#
125 41.7 18.6 27.8#

