




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048933.D
Acq On : 10 Dec 2024 21:33
Operator : RC/JU
Sample : PB165509BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK509

Manual IntegrationsAPPROVED

Quant Time: Dec 10 22:50:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/11/2024
Supervised By :mohammad ahmed 12/12/2024

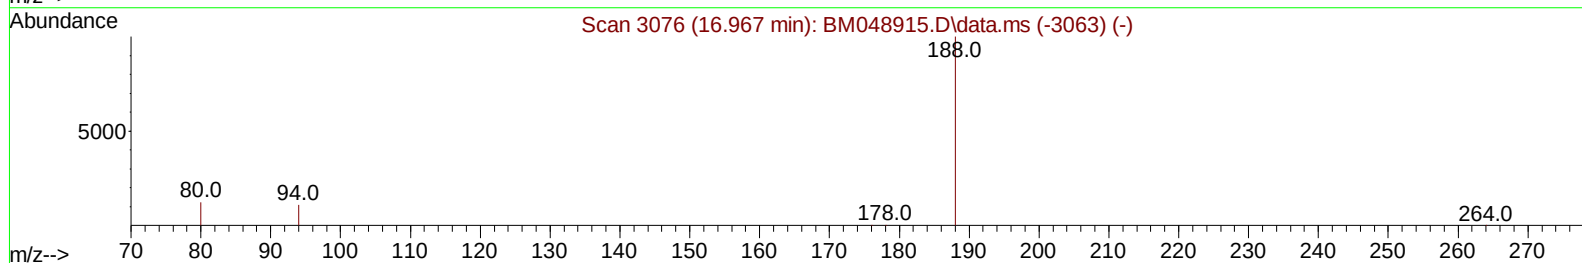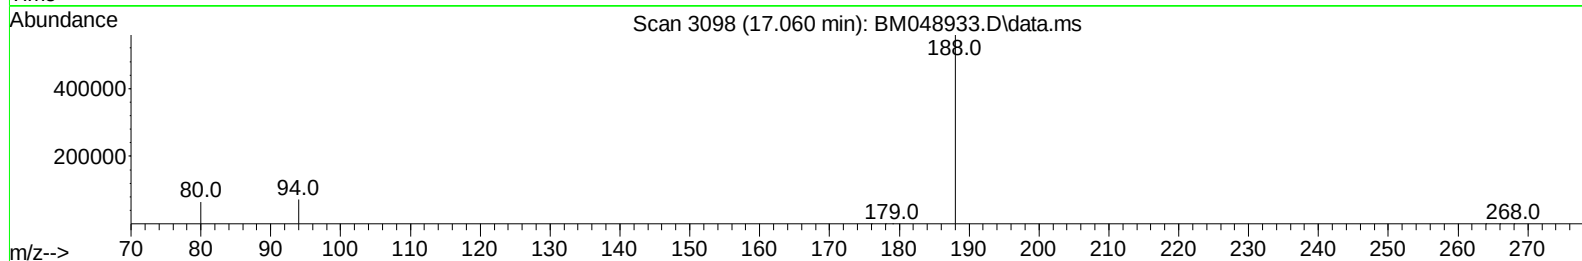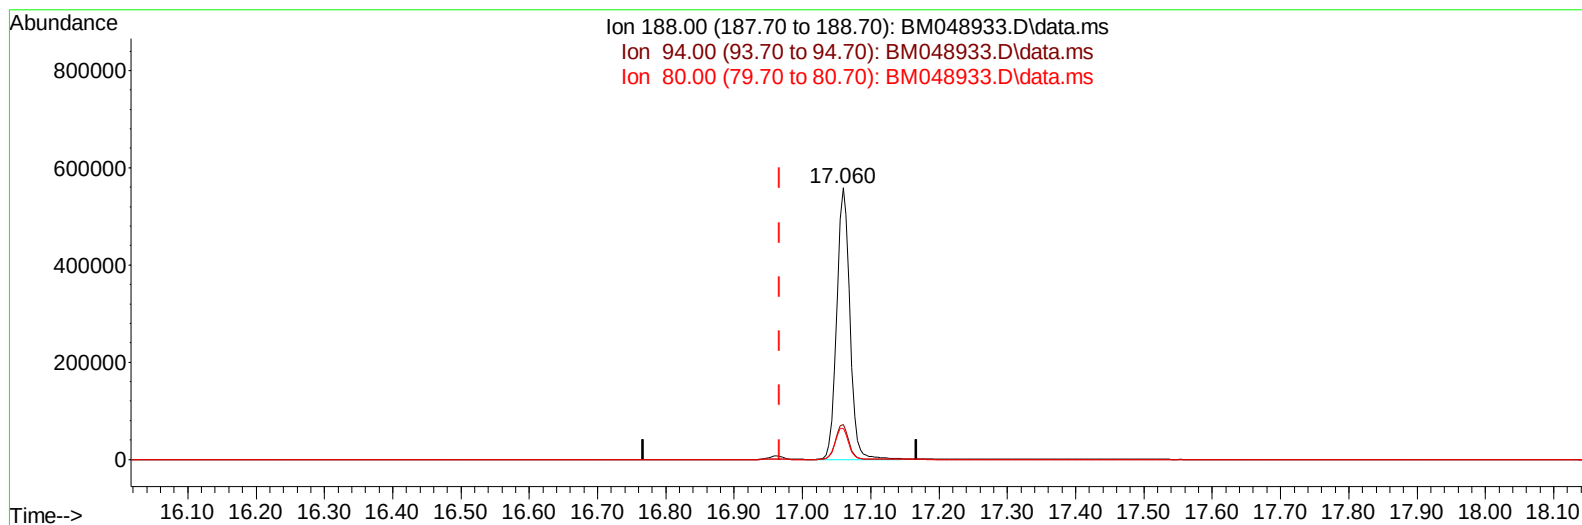

TIC: BM048933.D\data.ms

(13) Phenanthrene-d10 (I)

17.060min (+ 0.093) 0.40 ng/u1

response 746681

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	12.87
80.00	13.90	11.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048933.D
Acq On : 10 Dec 2024 21:33
Operator : RC/JU
Sample : PB165509BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK509

Manual IntegrationsAPPROVED

Quant Time: Dec 10 22:50:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/11/2024
Supervised By :mohammad ahmed 12/12/2024

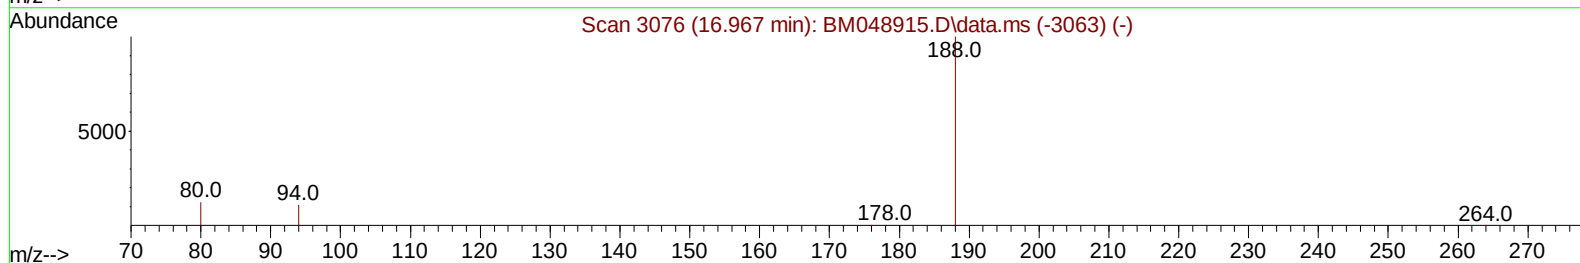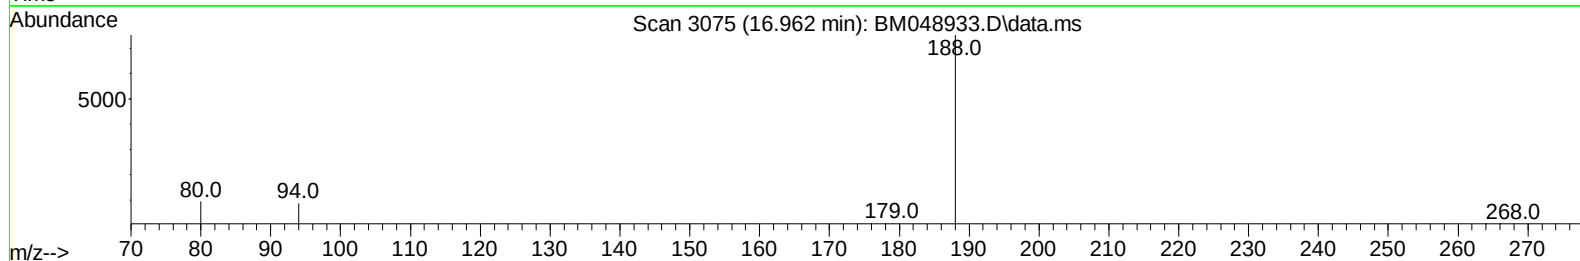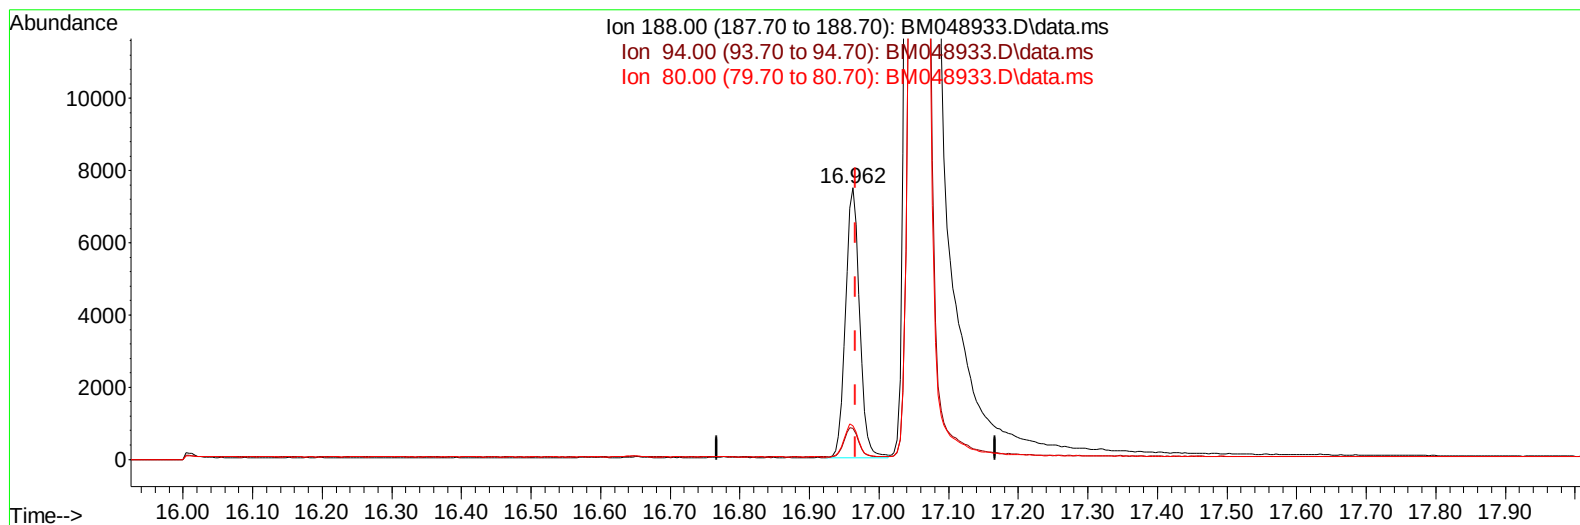

TIC: BM048933.D\data.ms

(13) Phenanthrene-d10 (I)

16.962min (-0.004) 0.40 ng/ul m

response 10510

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	11.48
80.00	13.90	12.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048933.D
Acq On : 10 Dec 2024 21:33
Operator : RC/JU
Sample : PB165509BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK509

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/11/2024
Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 10 22:50:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

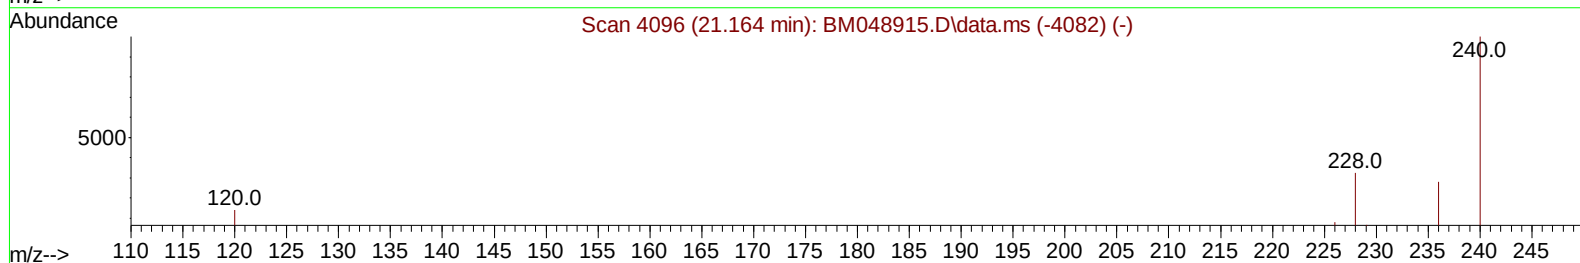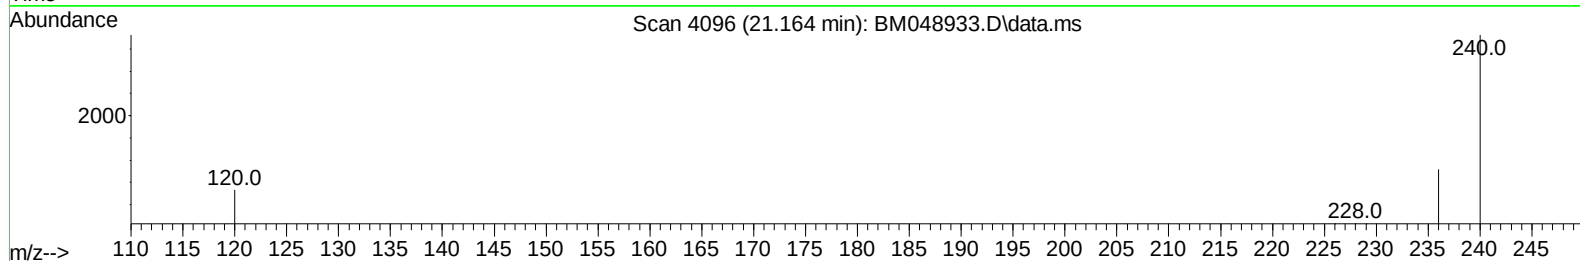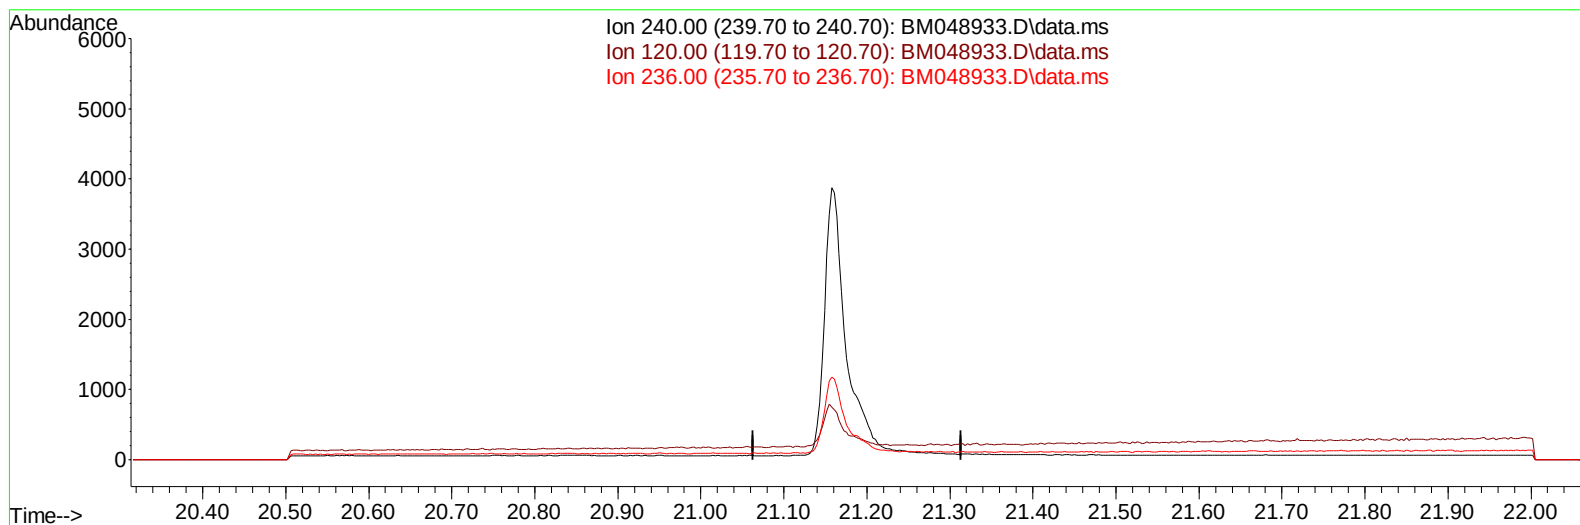

TIC: BM048933.D\data.ms

(17) Chrysene-d12

21.164min (-21.164) 0.00 ng/ul

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	18.30	0.00#
236.00	30.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048933.D
Acq On : 10 Dec 2024 21:33
Operator : RC/JU
Sample : PB165509BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK509

Manual IntegrationsAPPROVED

Quant Time: Dec 10 22:50:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/11/2024
Supervised By :mohammad ahmed 12/12/2024

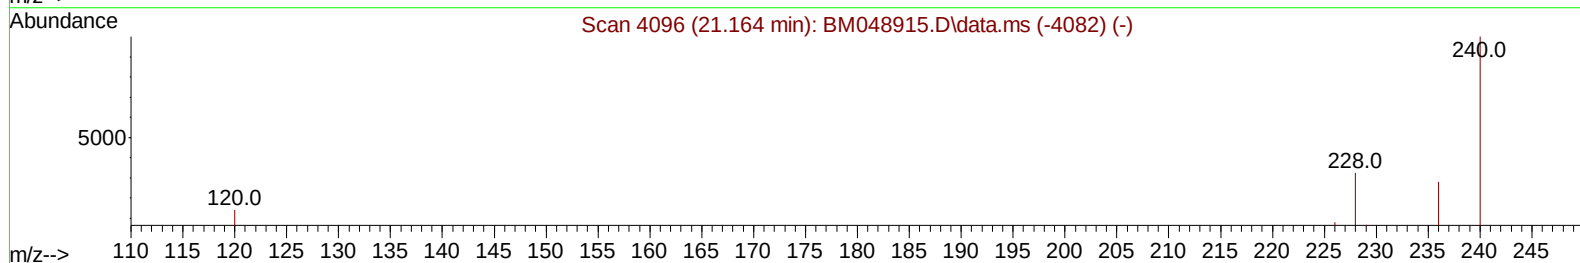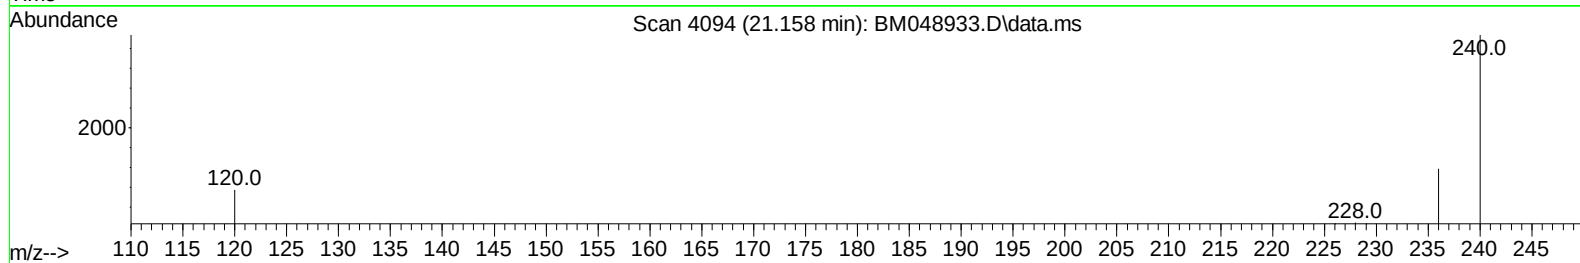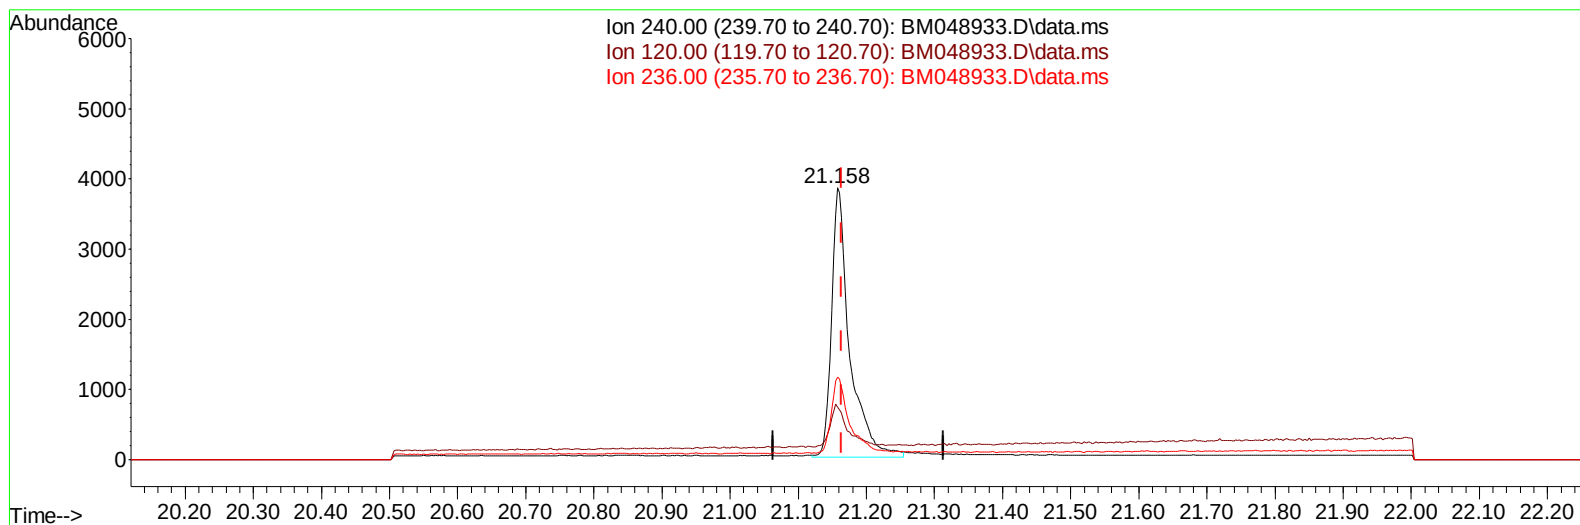

TIC: BM048933.D\data.ms

(17) Chrysene-d12

21.158min (-0.006) 0.40 ng/ul m

response 7140

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.30	19.14
236.00	30.50	30.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048933.D
Acq On : 10 Dec 2024 21:33
Operator : RC/JU
Sample : PB165509BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK509

Manual IntegrationsAPPROVED

Quant Time: Dec 10 22:50:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/11/2024
Supervised By :mohammad ahmed 12/12/2024

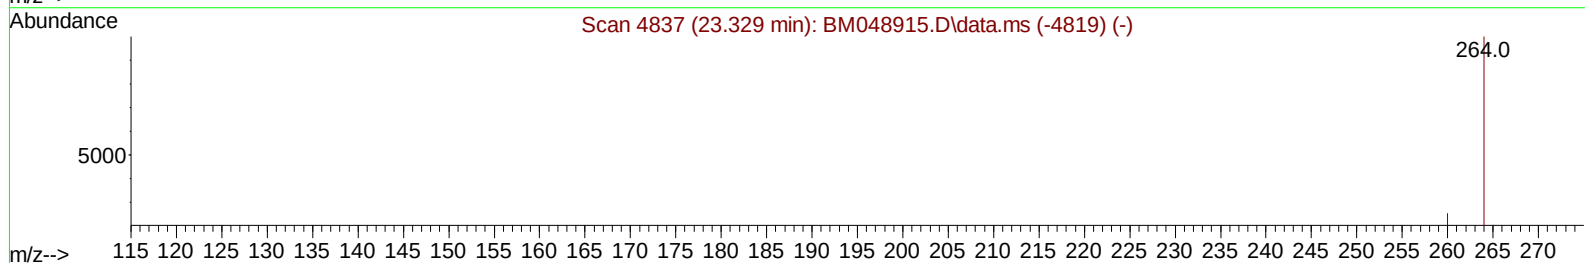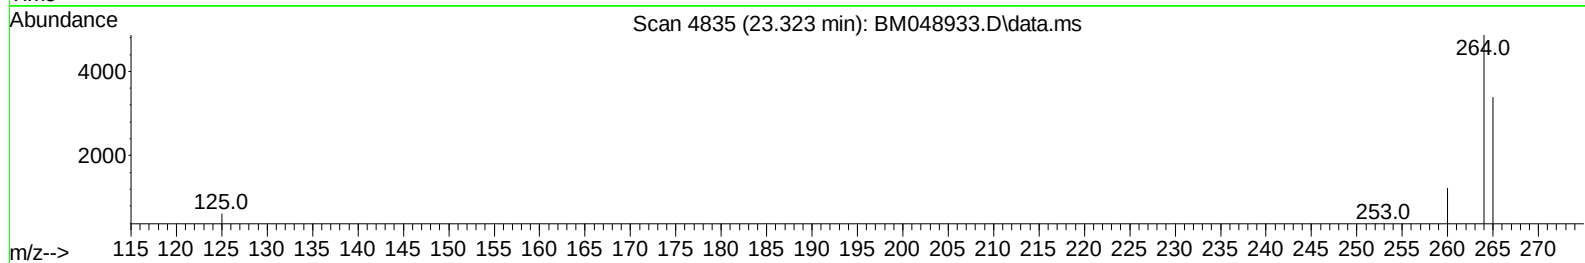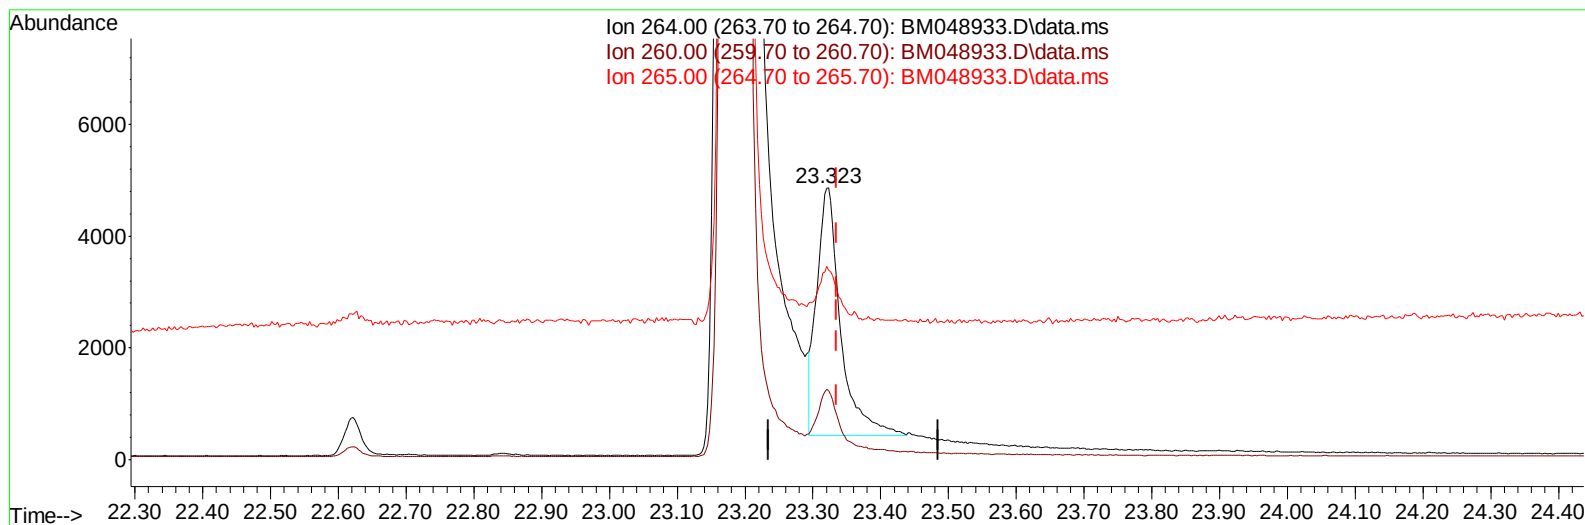

TIC: BM048933.D\data.ms

(23) Perylene-d12 (I)

23.323min (-0.012) 0.40 ng/u1

response 10872

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	25.31
265.00	82.60	69.68
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048933.D
Acq On : 10 Dec 2024 21:33
Operator : RC/JU
Sample : PB165509BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK509

Manual IntegrationsAPPROVED

Quant Time: Dec 10 22:50:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/11/2024
Supervised By :mohammad ahmed 12/12/2024

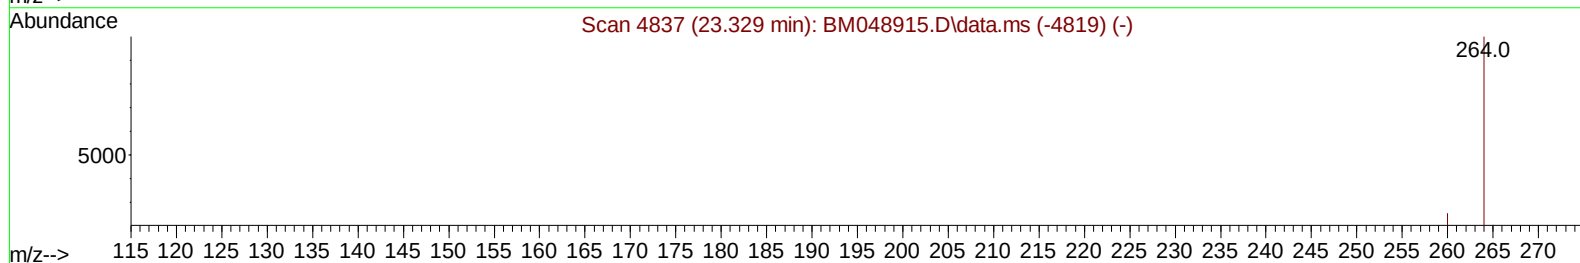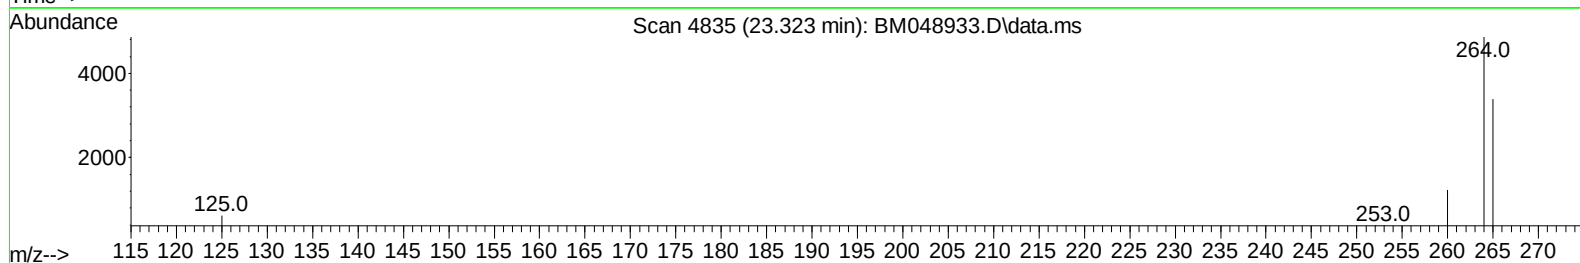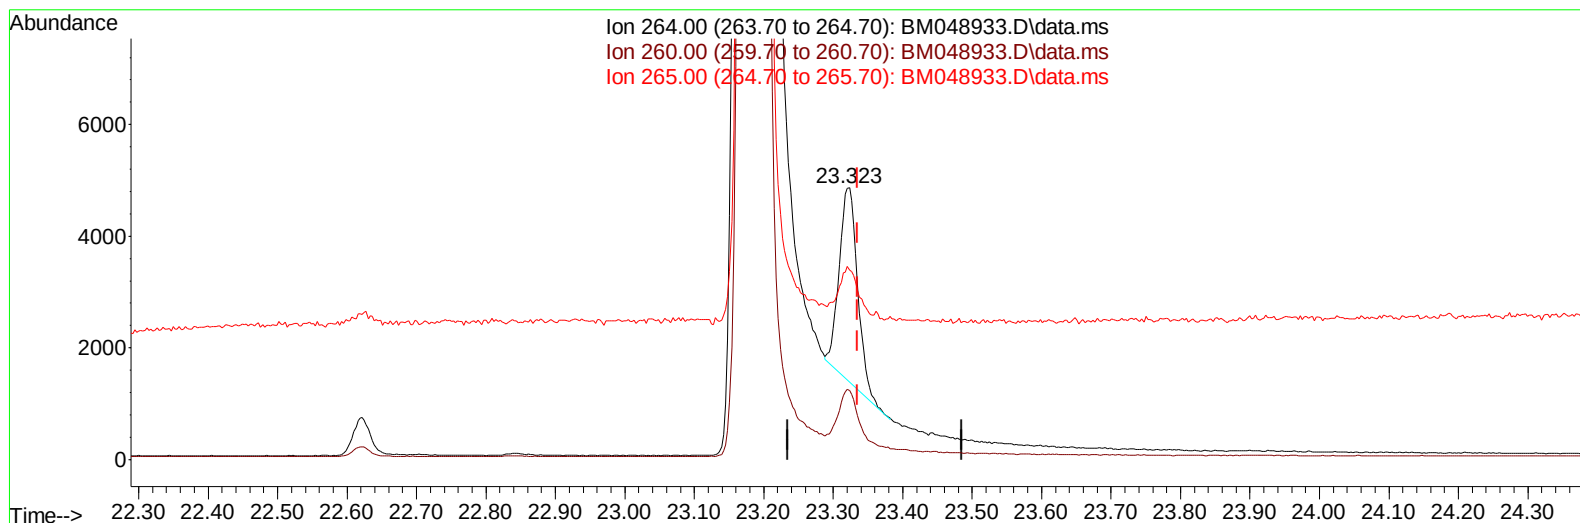

TIC: BM048933.D\data.ms

(23) Perylene-d12 (I)

23.323min (-0.012) 0.40 ng/ul m

response 6292

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	25.31
265.00	82.60	69.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
 Data File : BM048933.D
 Acq On : 10 Dec 2024 21:33
 Operator : RC/JU
 Sample : PB165509BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK509

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/11/2024
 Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 10 22:50:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 09 17:52:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	3579	0.400	ng/ul	0.00
4) Naphthalene-d8	10.347	136	9232	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.218	164	4812	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.962	188	10510m	0.400	ng/ul	0.00
17) Chrysene-d12	21.158	240	7140m	0.400	ng/ul	0.00
23) Perylene-d12	23.323	264	6292m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.159	96	24548	5.869	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.952	152	3390	0.288	ng/ul	0.00
18) Fluoranthene-d10	18.996	212	6875	0.322	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048933.D
Acq On : 10 Dec 2024 21:33
Operator : RC/JU
Sample : PB165509BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK509

Manual IntegrationsAPPROVED

Quant Time: Dec 10 22:50:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/11/2024
Supervised By :mohammad ahmed 12/12/2024

