




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048938.D
Acq On : 11 Dec 2024 00:33
Operator : RC/JU
Sample : P5109-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHPE1

Manual IntegrationsAPPROVED

Quant Time: Dec 11 01:09:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

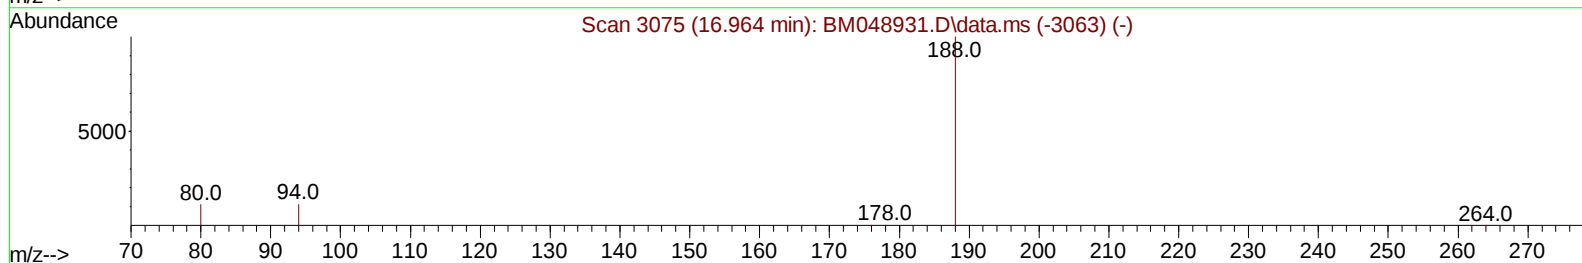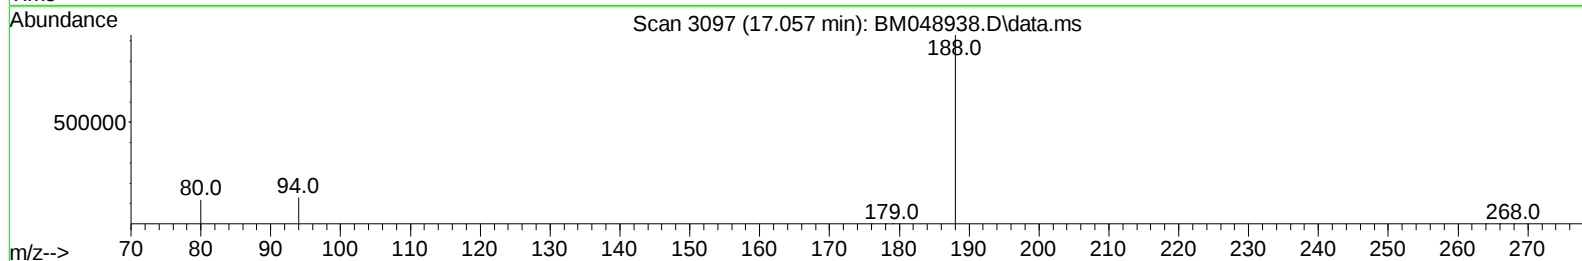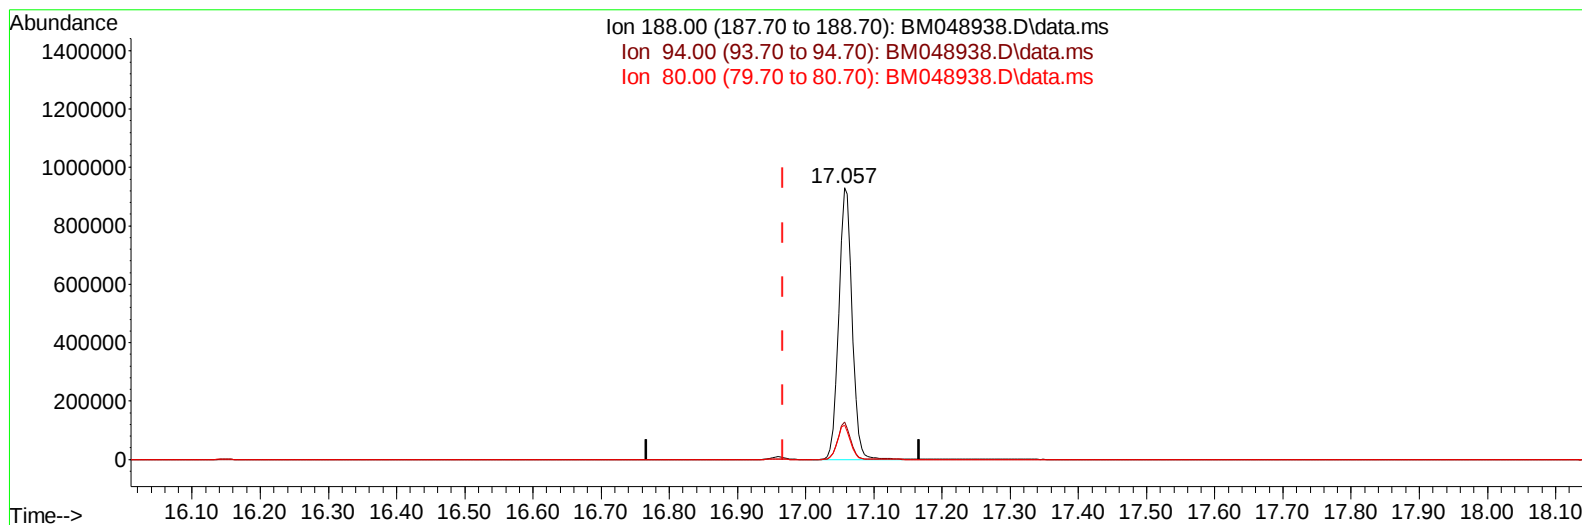

TIC: BM048938.D\data.ms

(13) Phenanthrene-d10 (I)

17.057min (+ 0.090) 0.40 ng/u1

response 1256529

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	13.79
80.00	13.90	12.58
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048938.D
Acq On : 11 Dec 2024 00:33
Operator : RC/JU
Sample : P5109-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHPE1

Manual IntegrationsAPPROVED

Quant Time: Dec 11 01:09:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

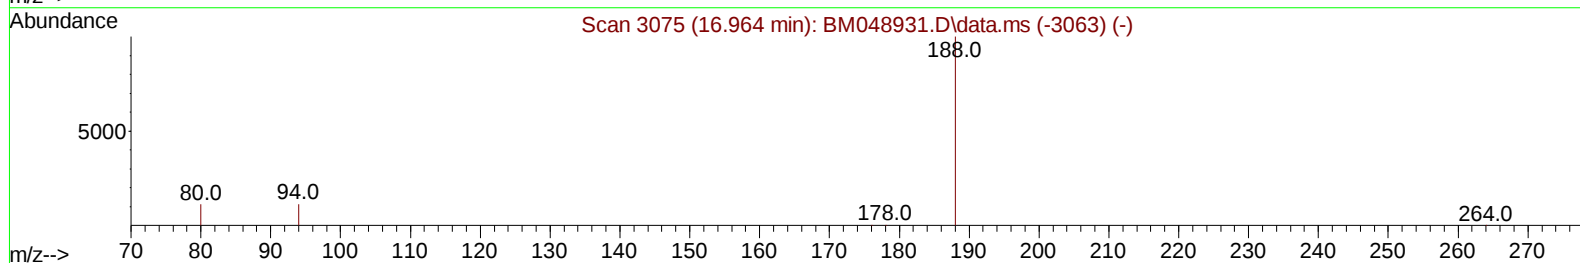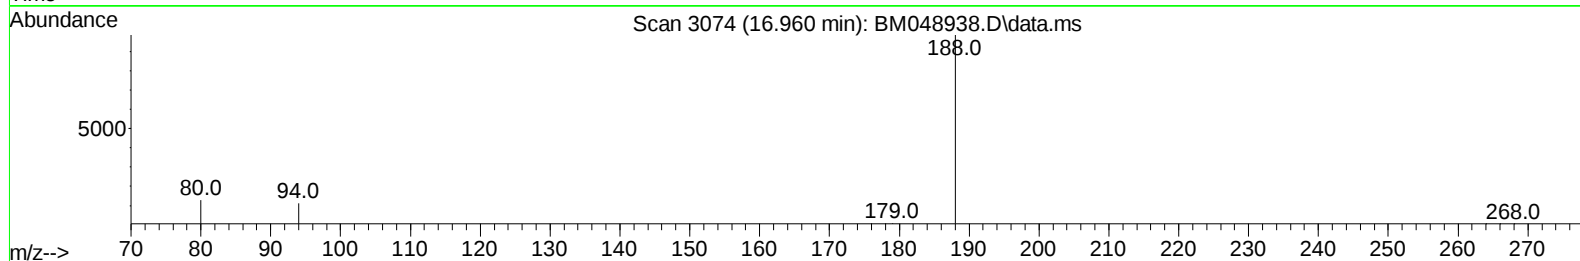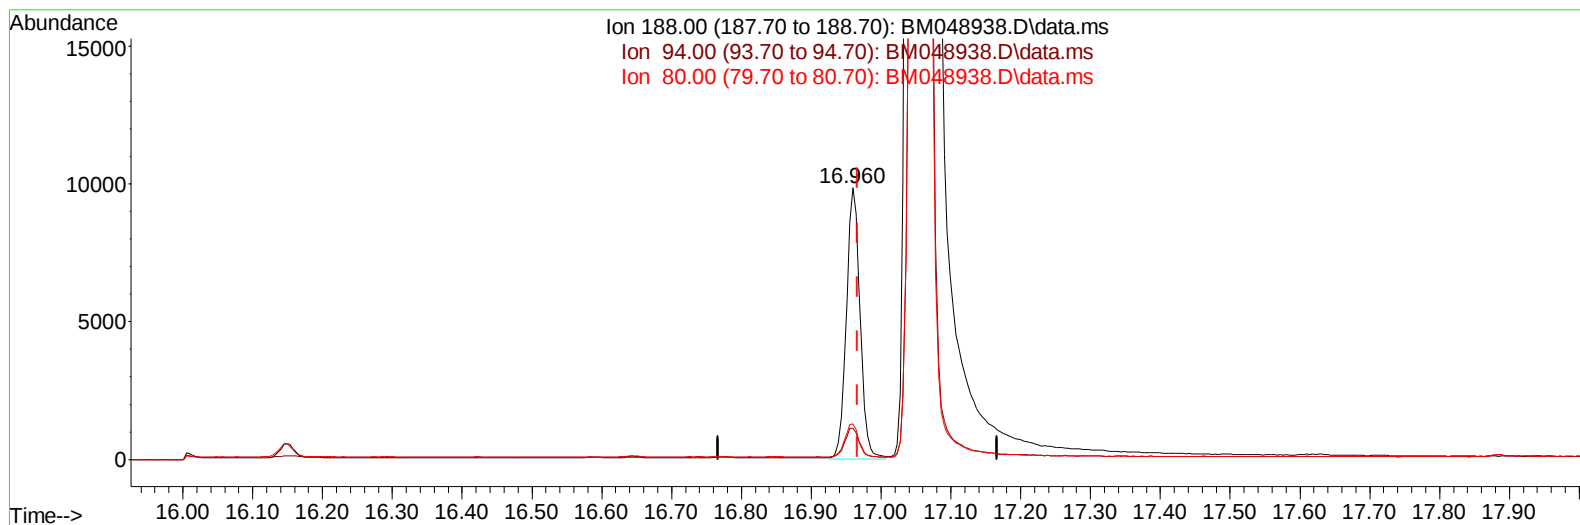

TIC: BM048938.D\data.ms

(13) Phenanthrene-d10 (I)

16.960min (-0.007) 0.40 ng/ul m

response 13331

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	11.34
80.00	13.90	13.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048938.D
Acq On : 11 Dec 2024 00:33
Operator : RC/JU
Sample : P5109-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHPE1

Manual IntegrationsAPPROVED

Quant Time: Dec 11 01:09:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

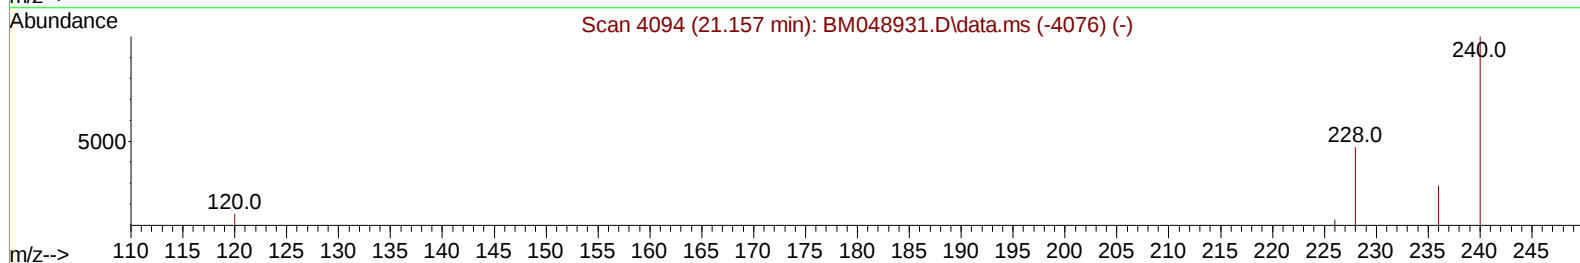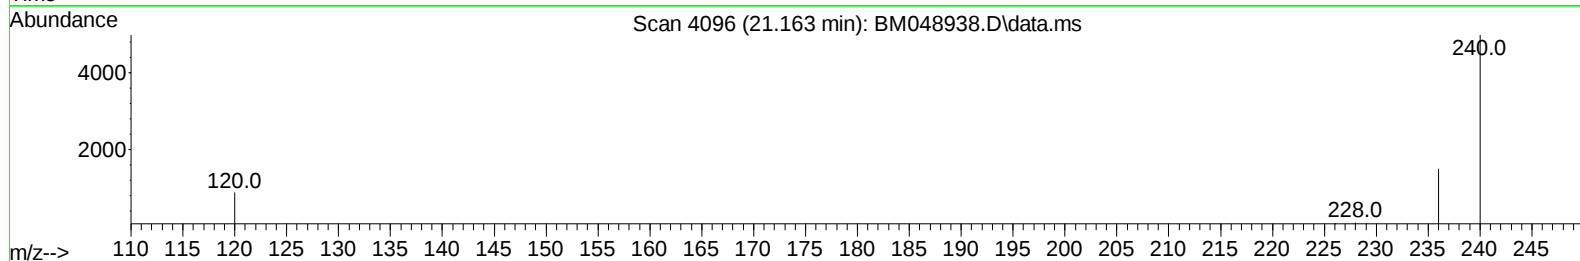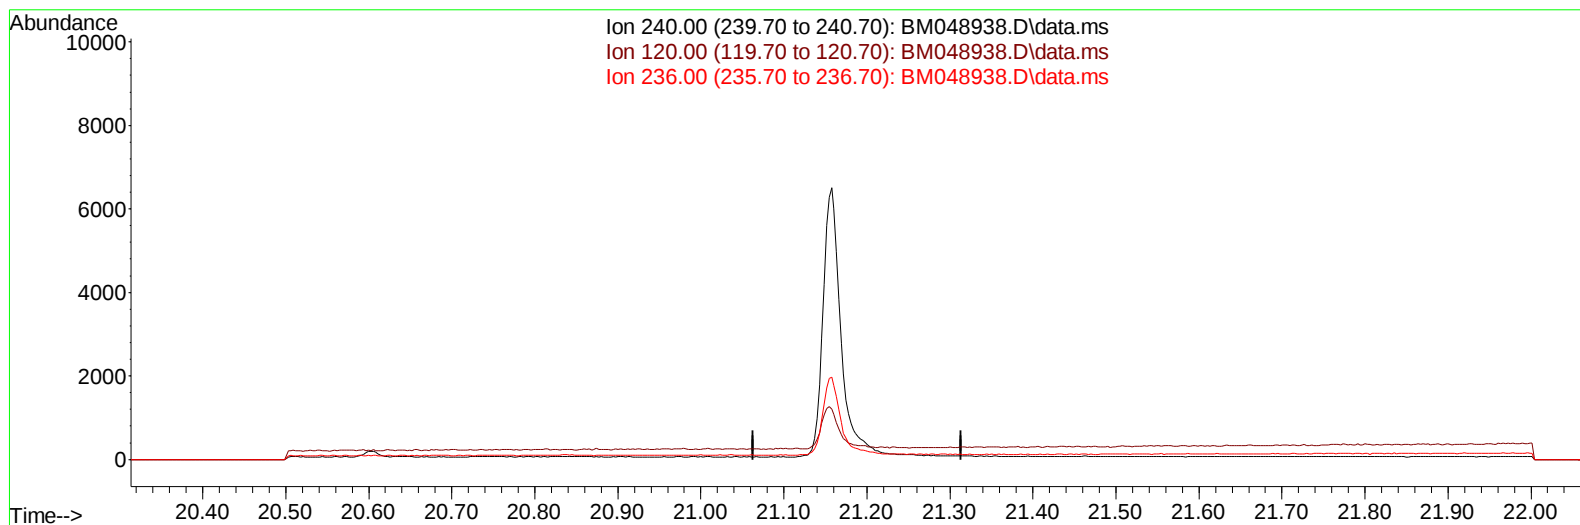

TIC: BM048938.D\data.ms

(17) Chrysene-d12

21.164min (-21.164) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	18.30	0.00#
236.00	30.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048938.D
Acq On : 11 Dec 2024 00:33
Operator : RC/JU
Sample : P5109-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHPE1

Manual IntegrationsAPPROVED

Quant Time: Dec 11 01:09:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

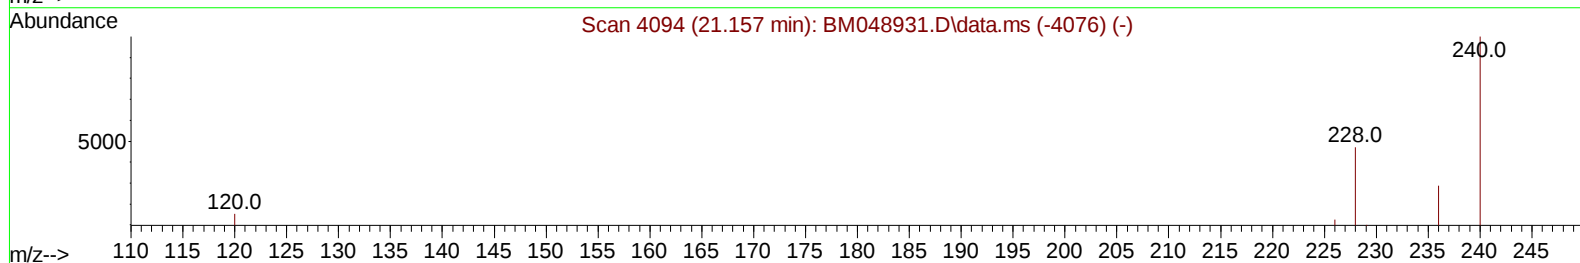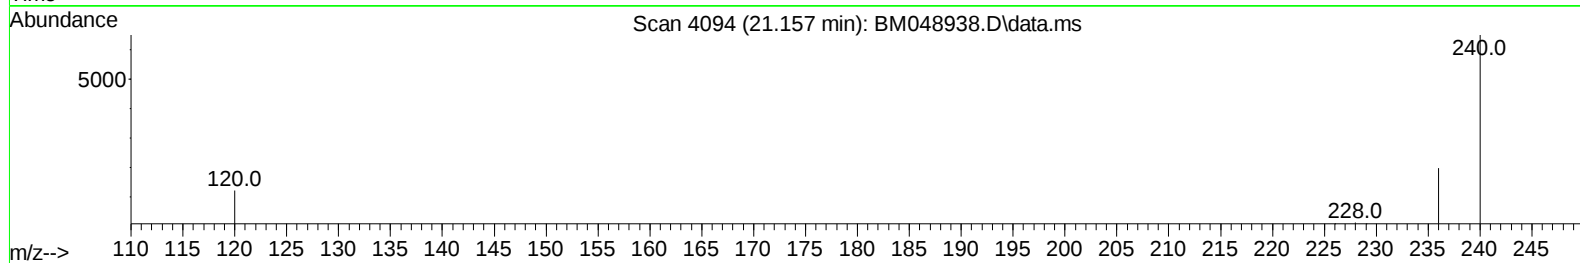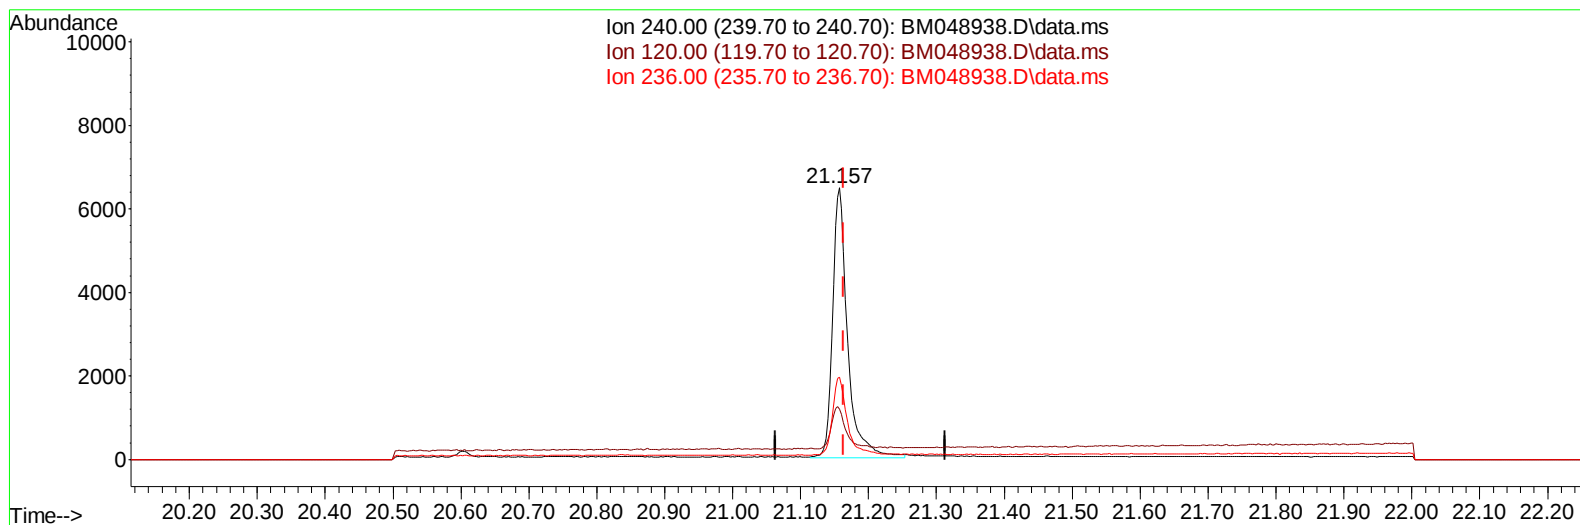

TIC: BM048938.D\data.ms

(17) Chrysene-d12

21.157min (-0.006) 0.40 ng/u1 m

response 9938

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.30	18.50
236.00	30.50	30.36
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048938.D
Acq On : 11 Dec 2024 00:33
Operator : RC/JU
Sample : P5109-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHPE1

Manual IntegrationsAPPROVED

Quant Time: Dec 11 01:09:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

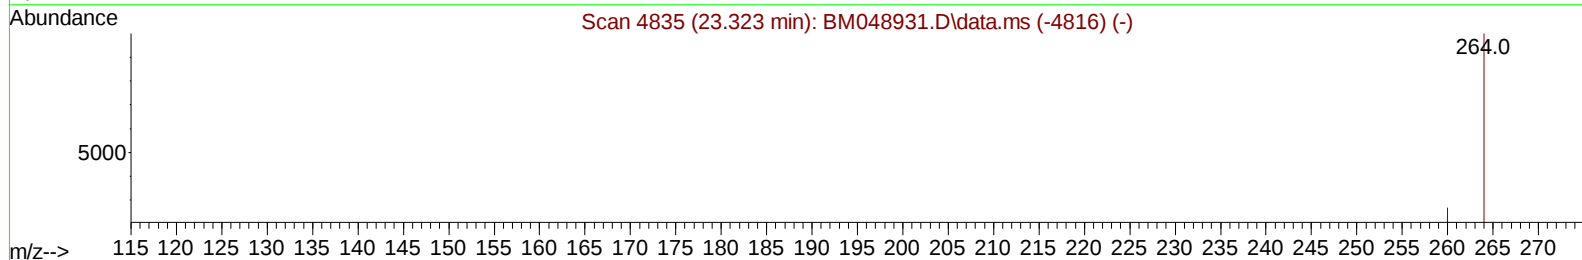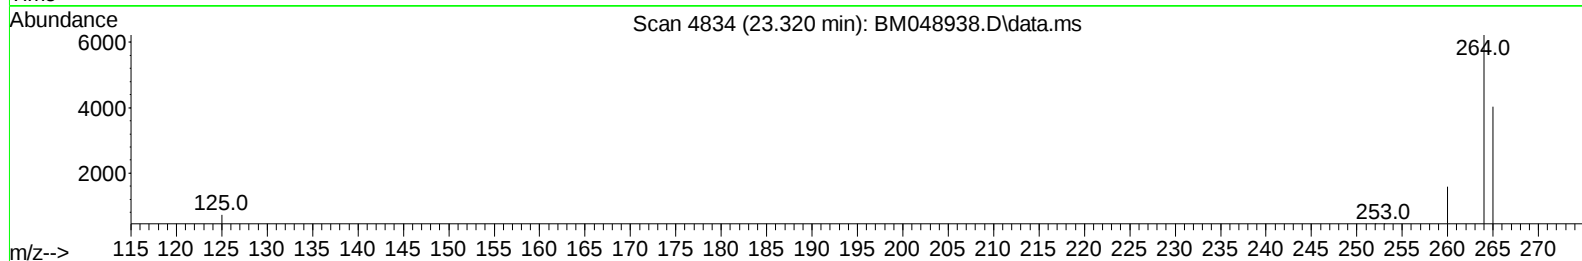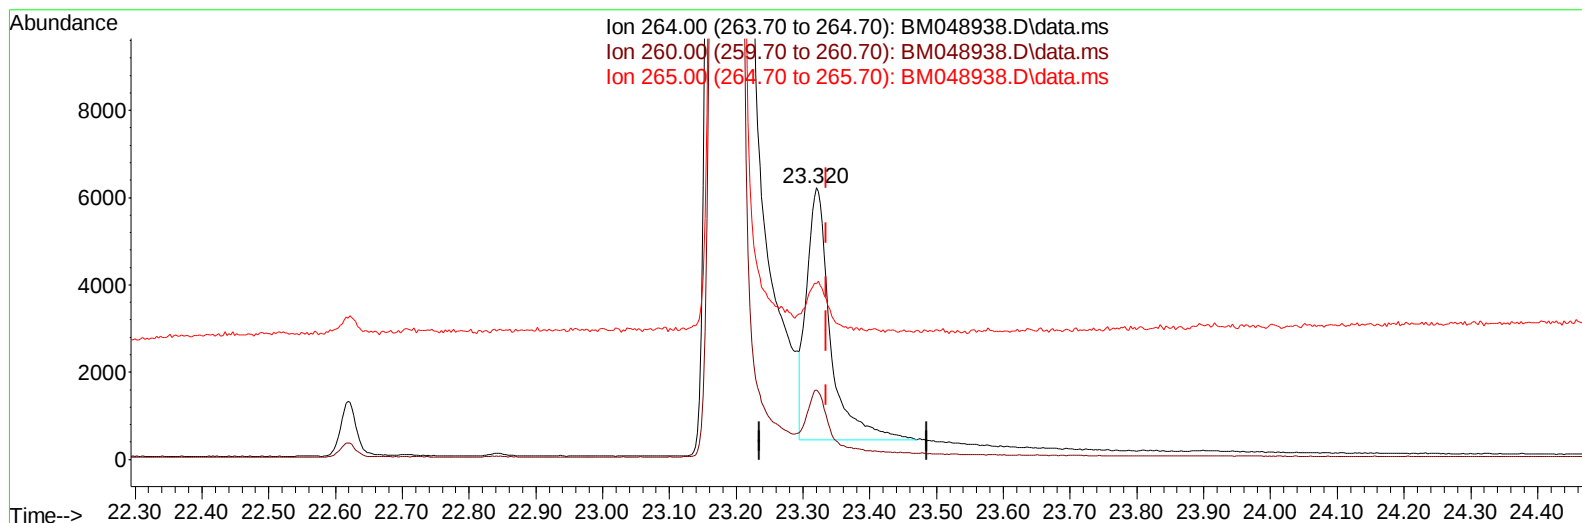

TIC: BM048938.D\data.ms

(23) Perylene-d12 (I)

23.320min (-0.015) 0.40 ng/u1

response 14529

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	25.57
265.00	82.60	64.83#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048938.D
Acq On : 11 Dec 2024 00:33
Operator : RC/JU
Sample : P5109-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHPE1

Manual IntegrationsAPPROVED

Quant Time: Dec 11 01:09:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

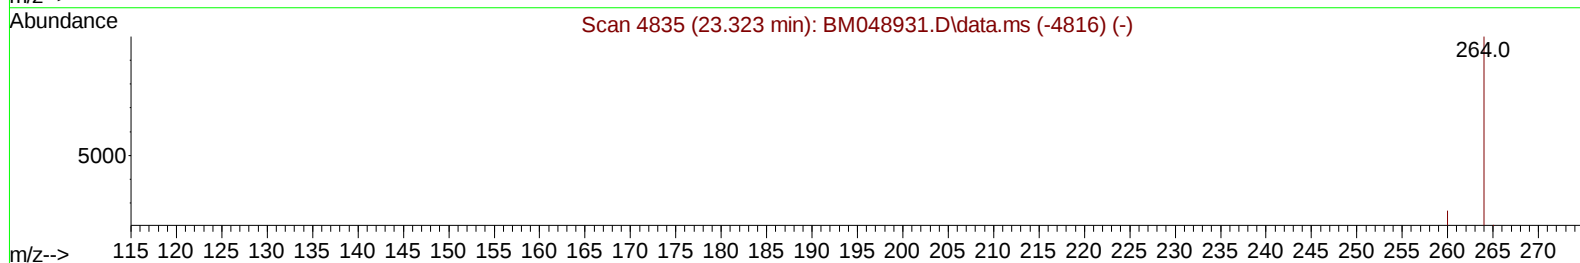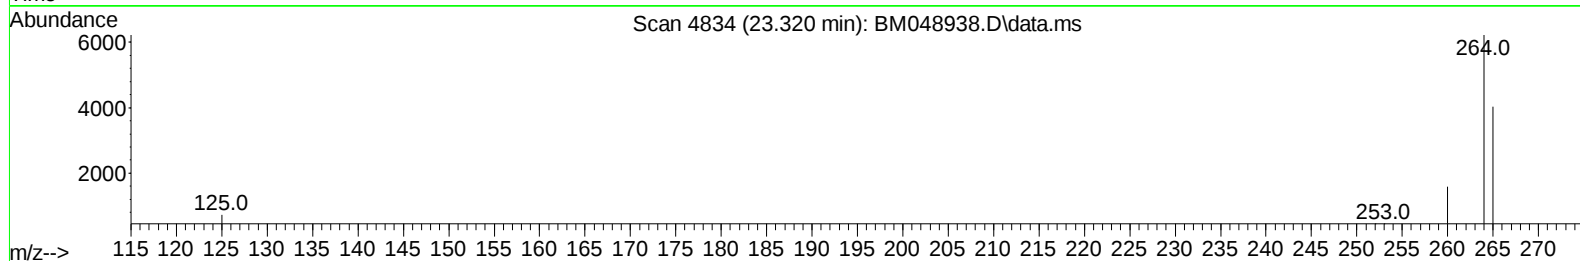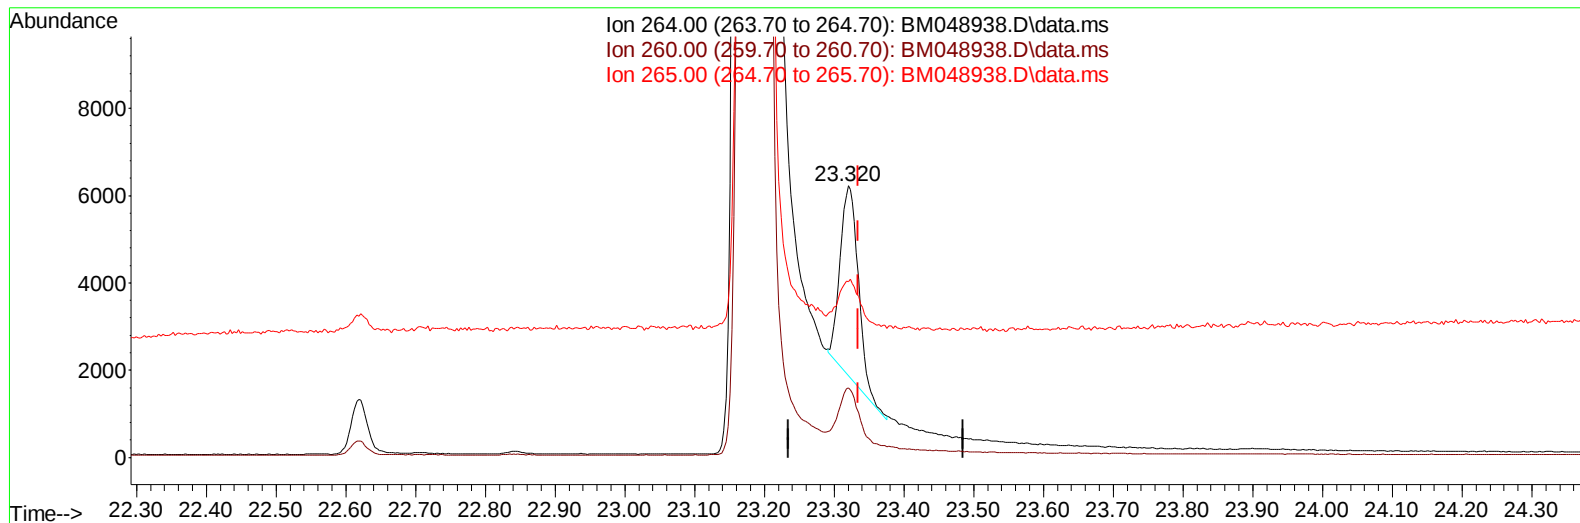

TIC: BM048938.D\data.ms

(23) Perylene-d12 (I)

23.320min (-0.015) 0.40 ng/ul m

response 7807

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	25.57
265.00	82.60	64.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
 Data File : BM048938.D
 Acq On : 11 Dec 2024 00:33
 Operator : RC/JU
 Sample : P5109-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHPE1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/12/2024
 Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 01:09:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 09 17:52:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	4436	0.400	ng/ul	0.00
4) Naphthalene-d8	10.343	136	12344	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.215	164	6227	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.960	188	13331m	0.400	ng/ul	0.00
17) Chrysene-d12	21.157	240	9938m	0.400	ng/ul	0.00
23) Perylene-d12	23.320	264	7807m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	30396	5.863	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.943	152	5577	0.354	ng/ul	0.00
18) Fluoranthene-d10	18.993	212	12248	0.413	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048938.D
Acq On : 11 Dec 2024 00:33
Operator : RC/JU
Sample : P5109-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHPE1

Manual IntegrationsAPPROVED

Quant Time: Dec 11 01:09:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

