
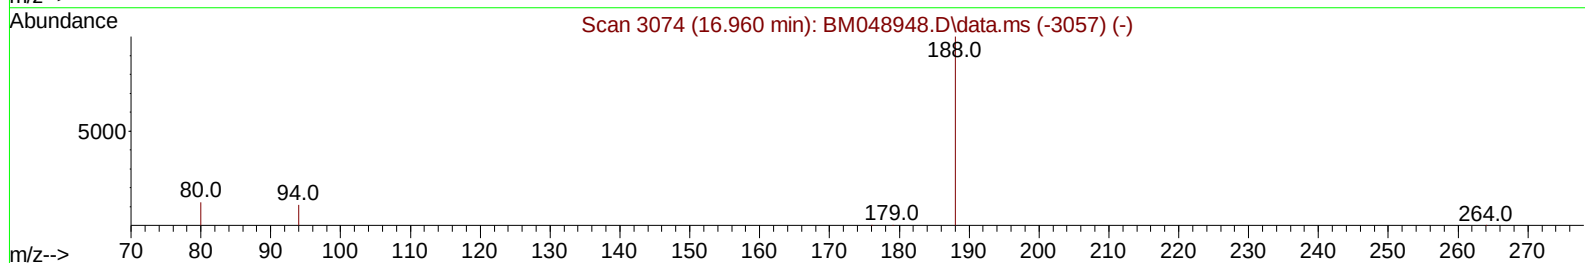
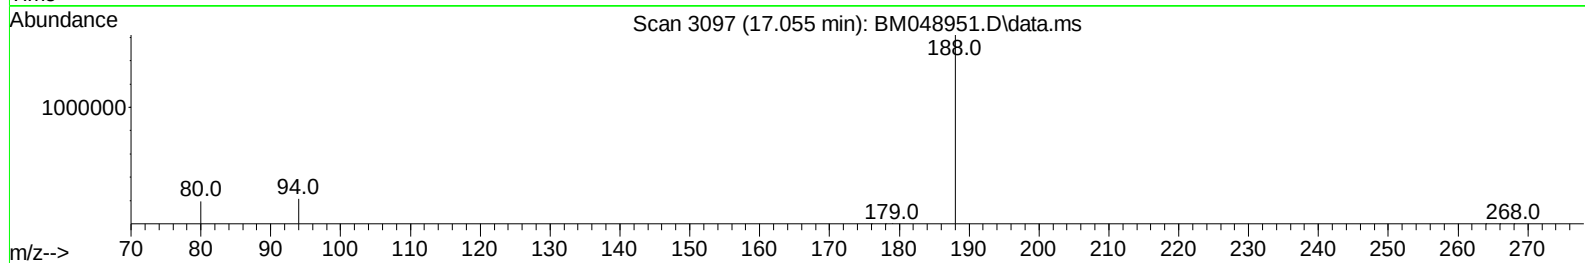


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

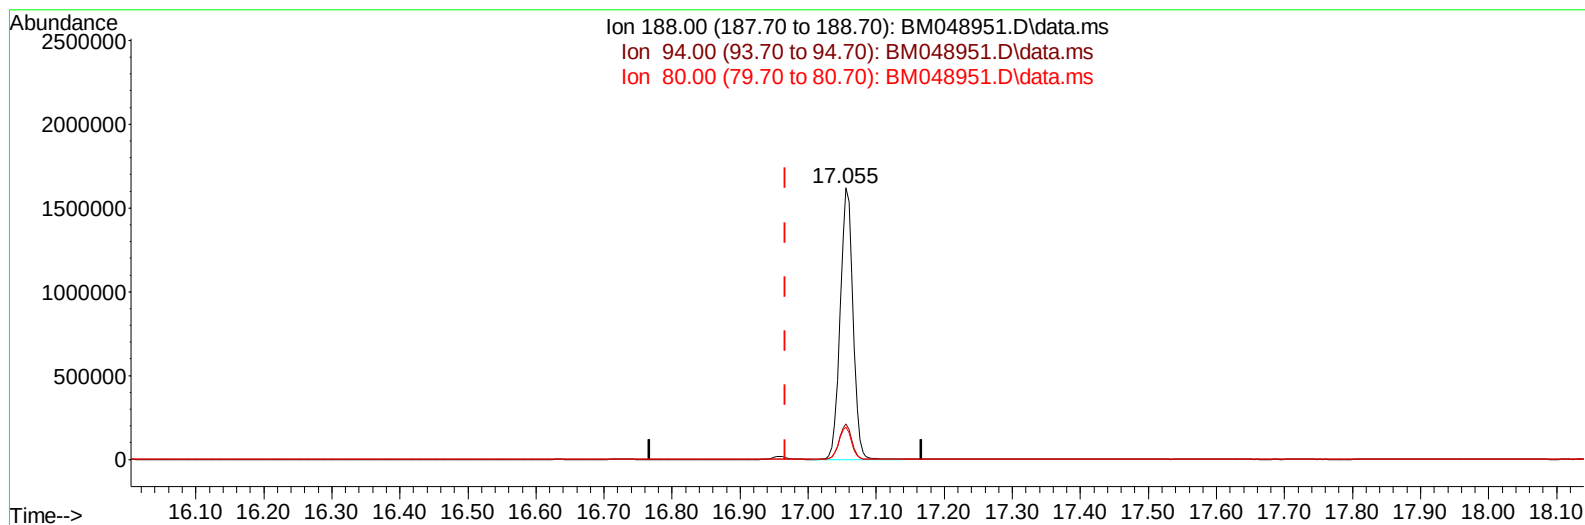

TIC: BM048951.D\data.ms

(13) Phenanthrene-d10 (I)




17.055min (+ 0.089) 0.40 ng/u1

response 2138424

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	13.09
80.00	13.90	11.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

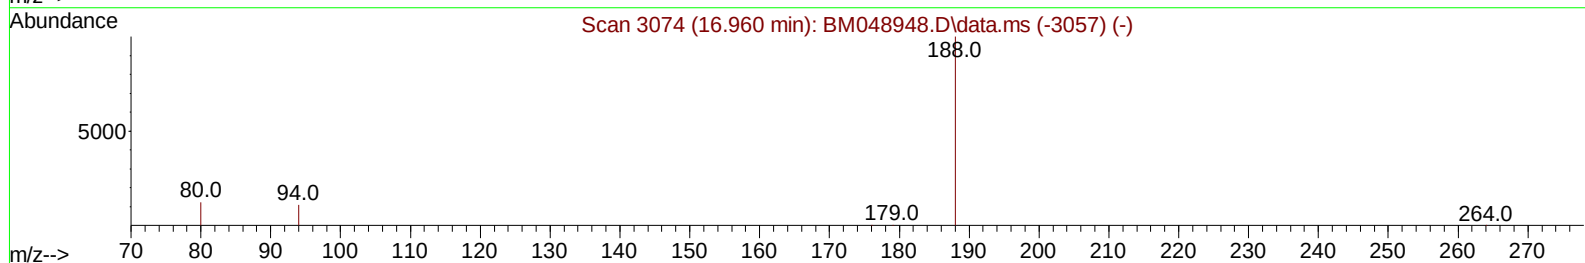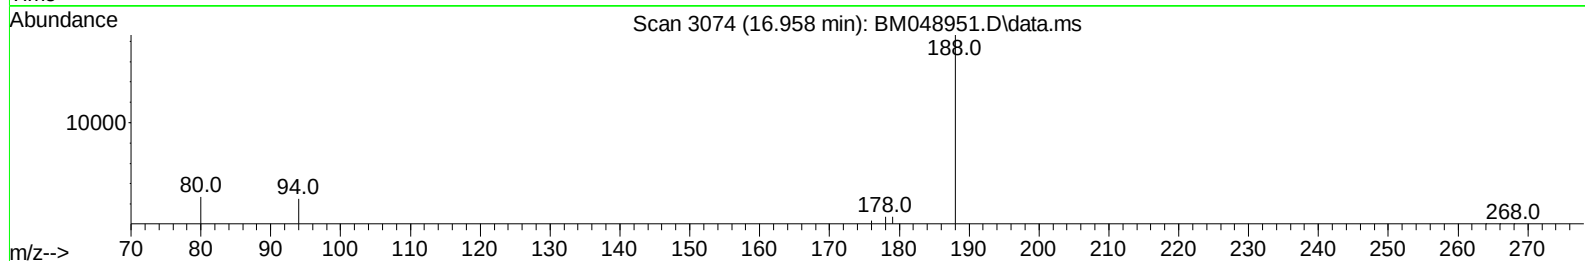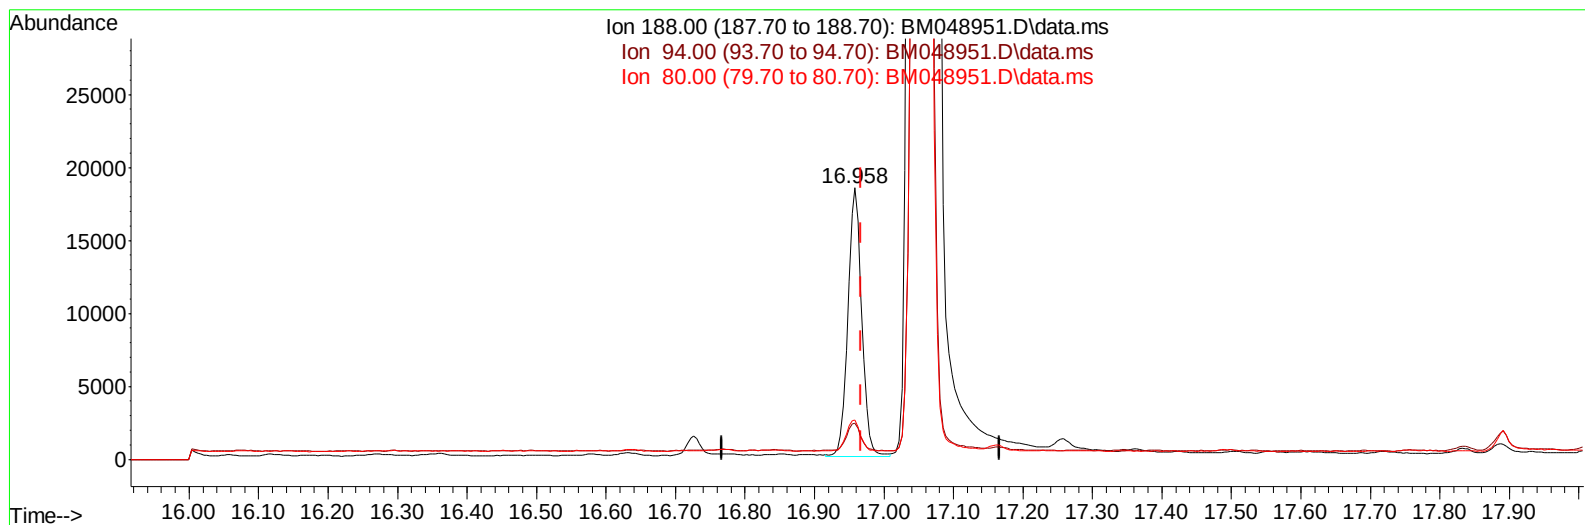

TIC: BM048951.D\data.ms

(13) Phenanthrene-d10 (I)




16.958min (-0.008) 0.40 ng/ul m

response 25441

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	13.41
80.00	13.90	14.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

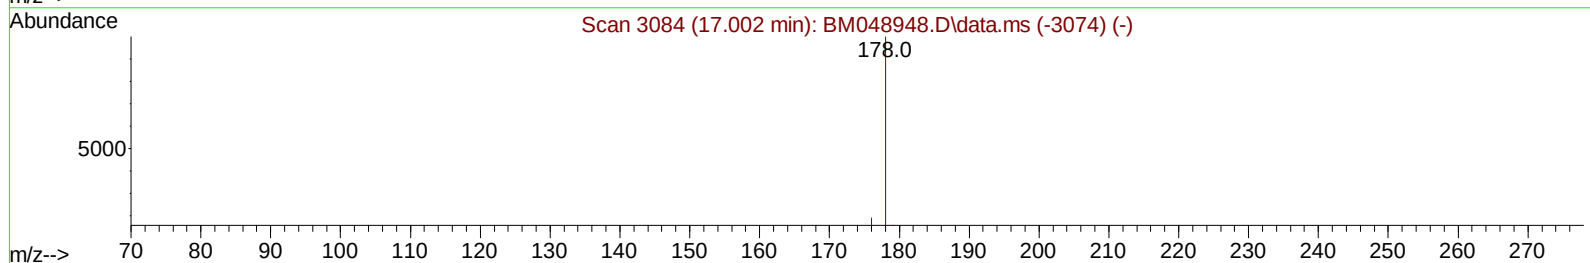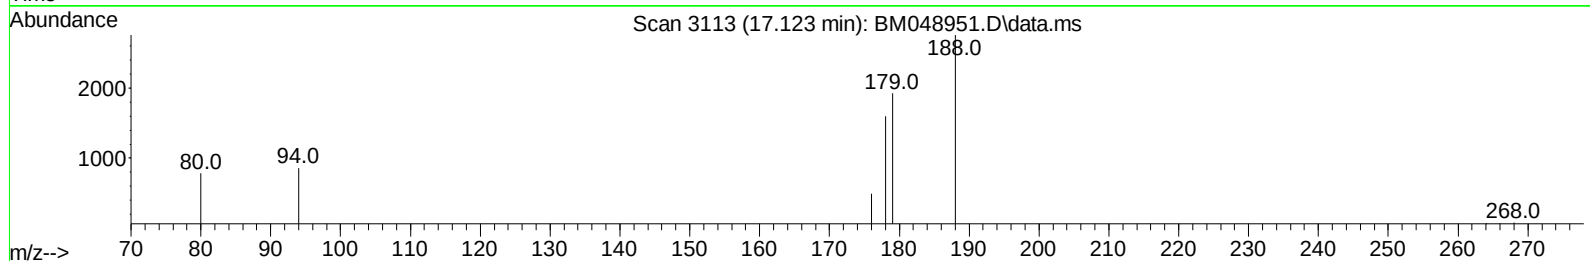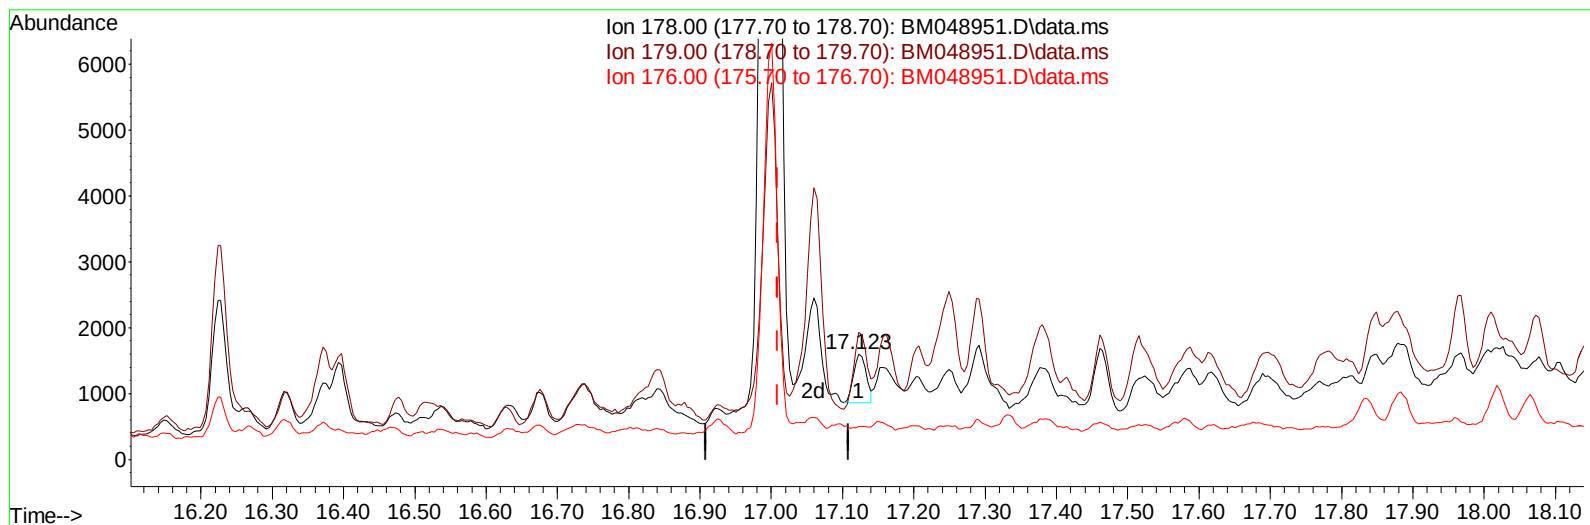

TIC: BM048951.D\data.ms

(15) Phenanthrene




17.123min (+ 0.114) 0.01 ng/u1

response 915

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.30	120.24#
176.00	19.80	31.04#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

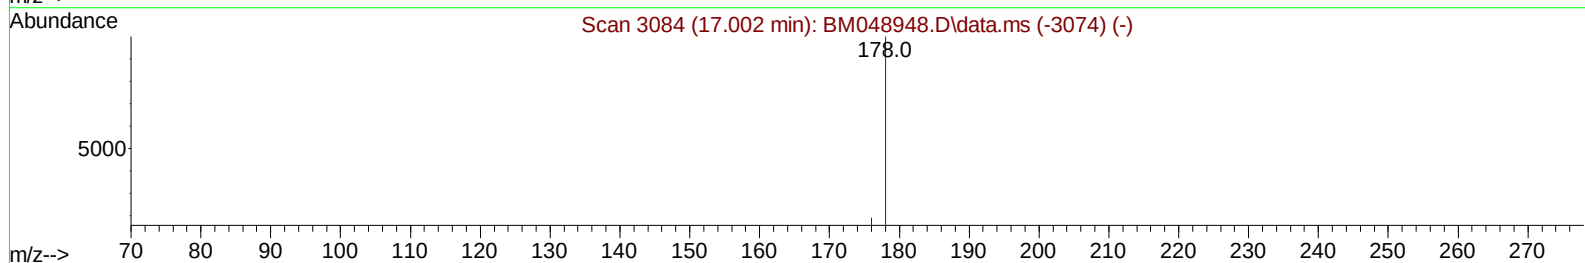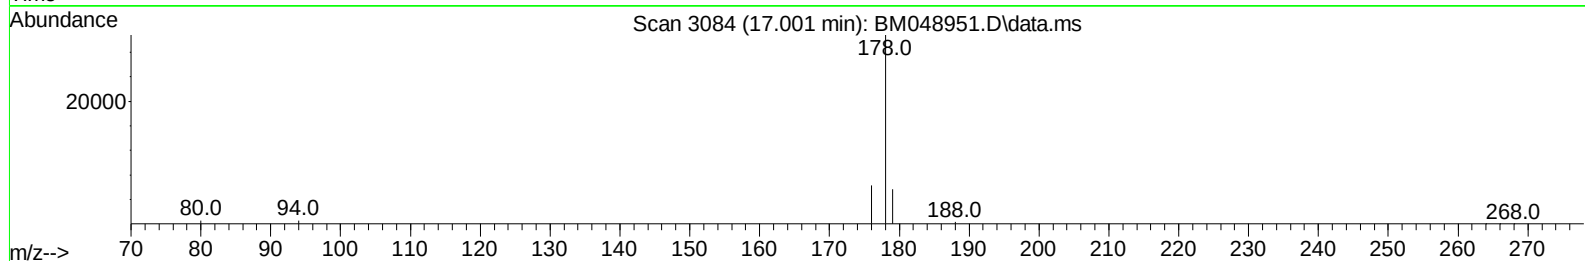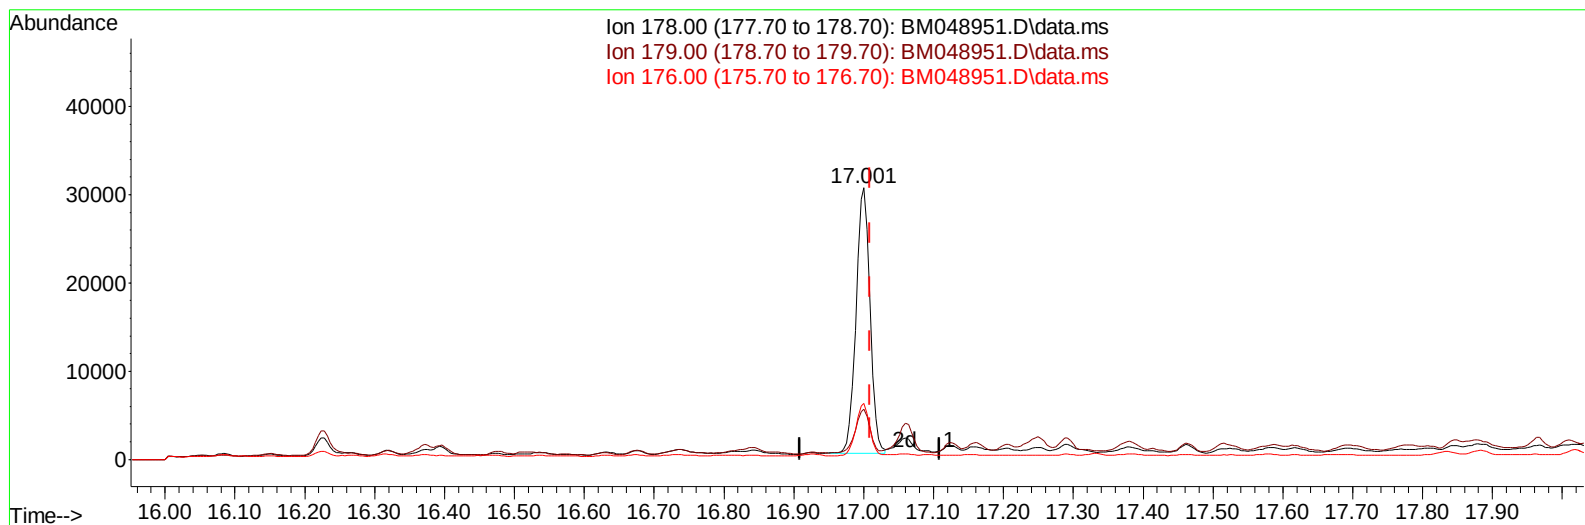

TIC: BM048951.D\data.ms

(15) Phenanthrene




17.001min (-0.008) 0.60 ng/ul m

response 41725

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.30	18.59
176.00	19.80	20.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

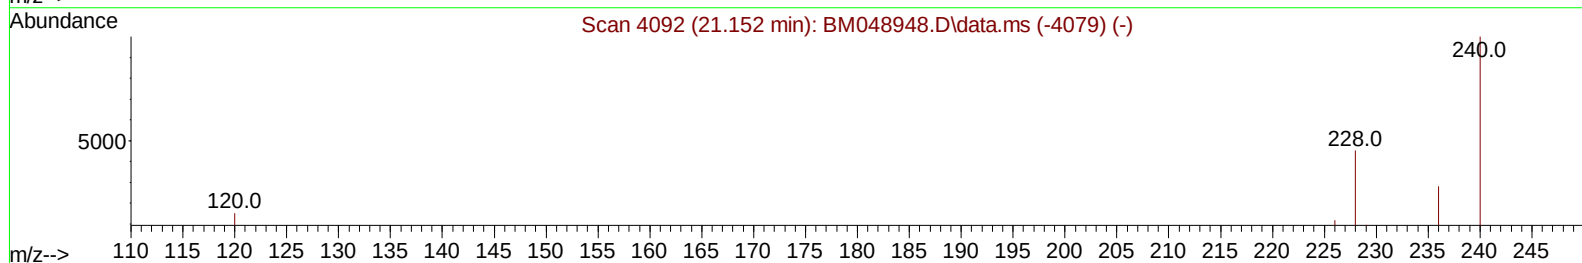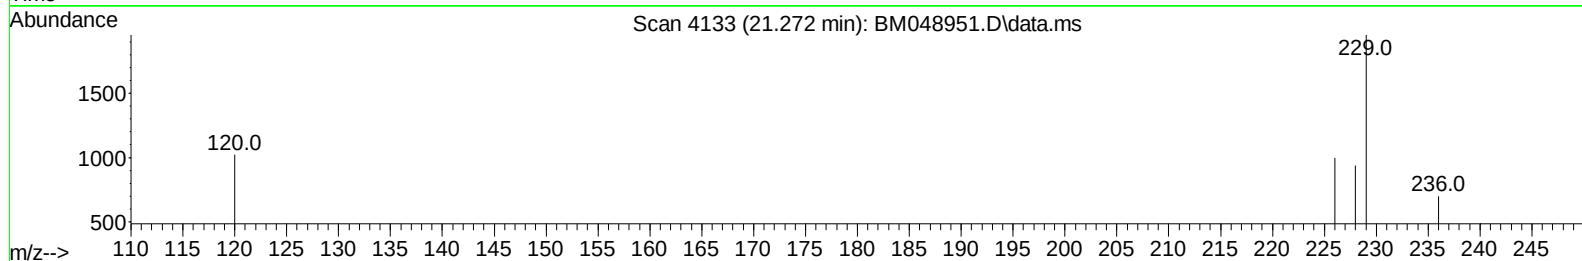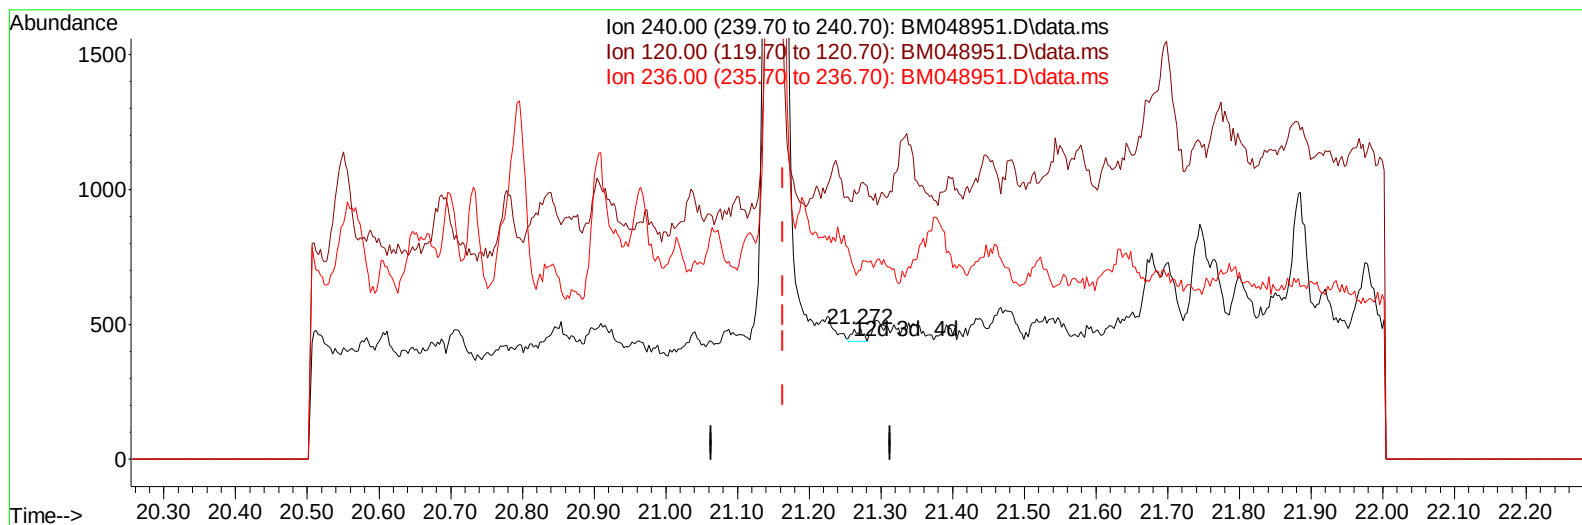

TIC: BM048951.D\data.ms

(17) Chrysene-d12




21.272min (+ 0.108) 0.40 ng/u1

response 43

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.30	210.95#
236.00	30.50	144.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

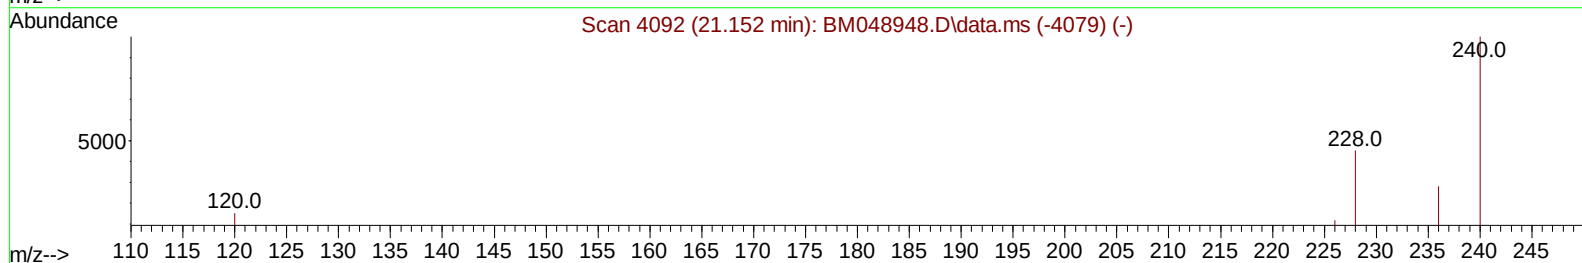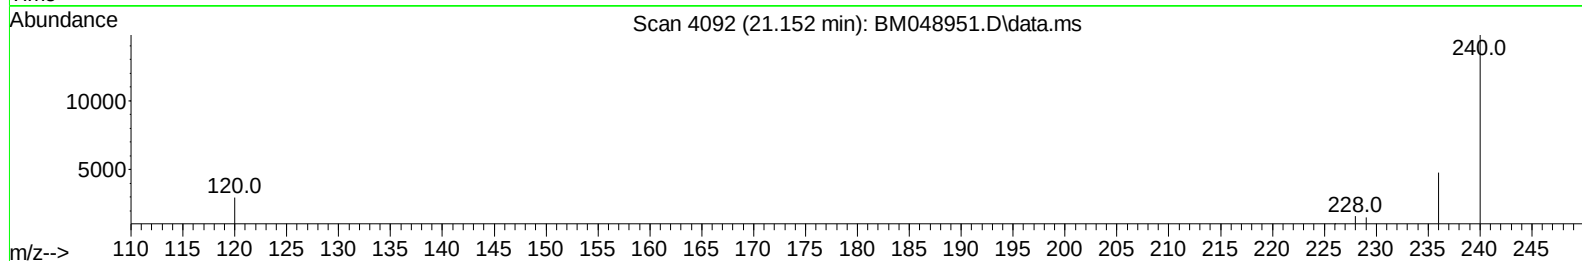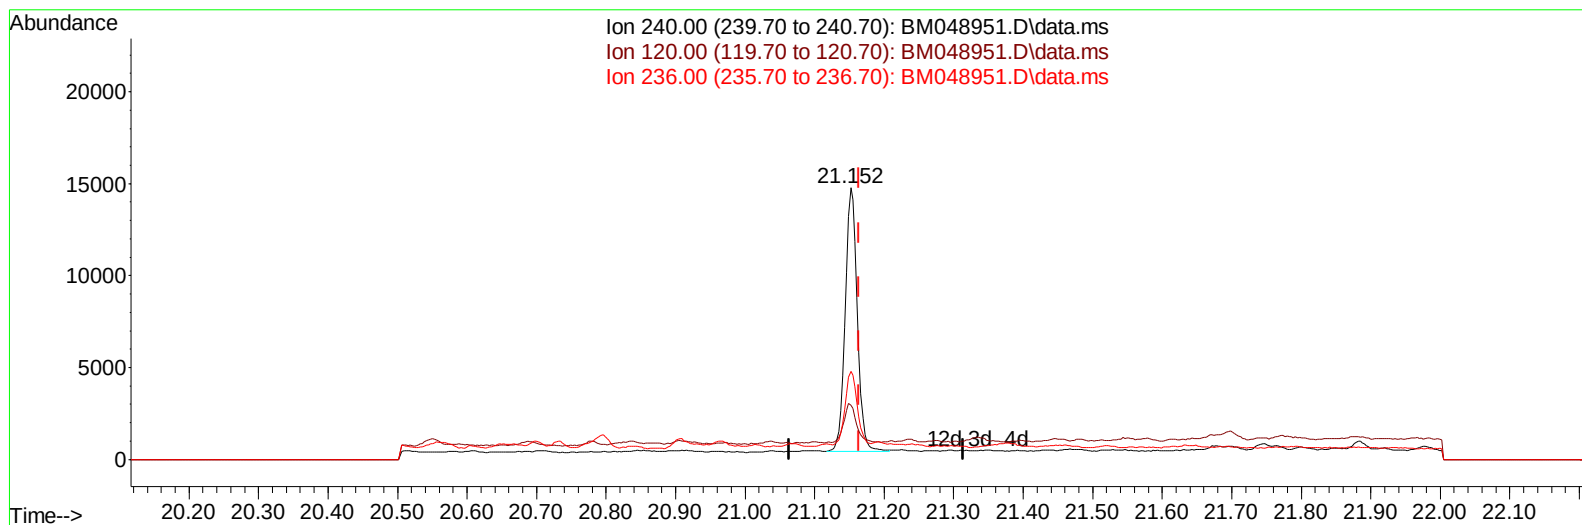

TIC: BM048951.D\data.ms

(17) Chrysene-d12




21.152min (-0.012) 0.40 ng/ul m

response 17269

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.30	19.98
236.00	30.50	32.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

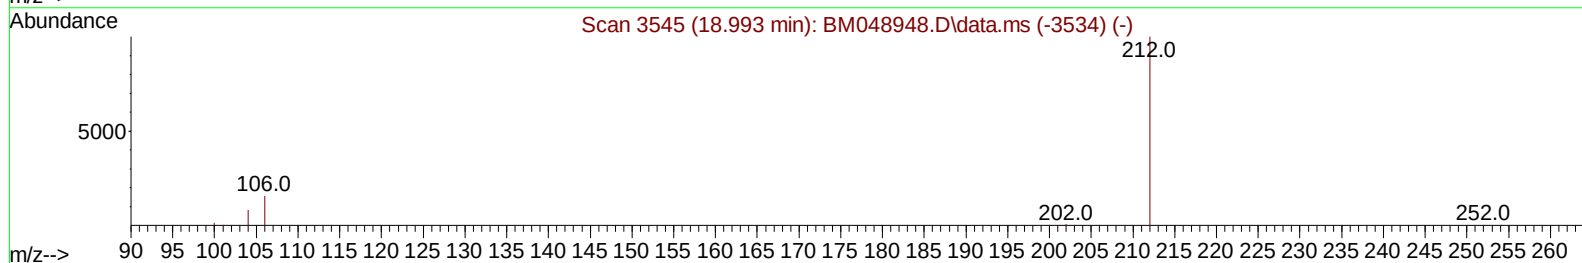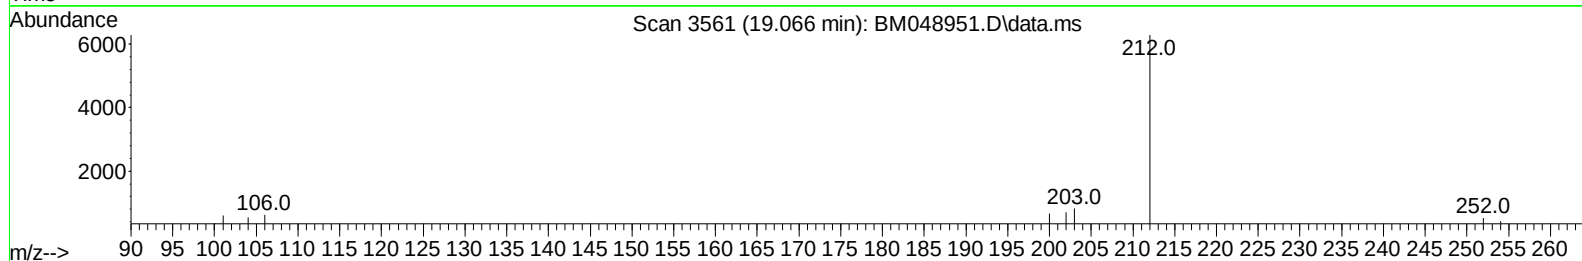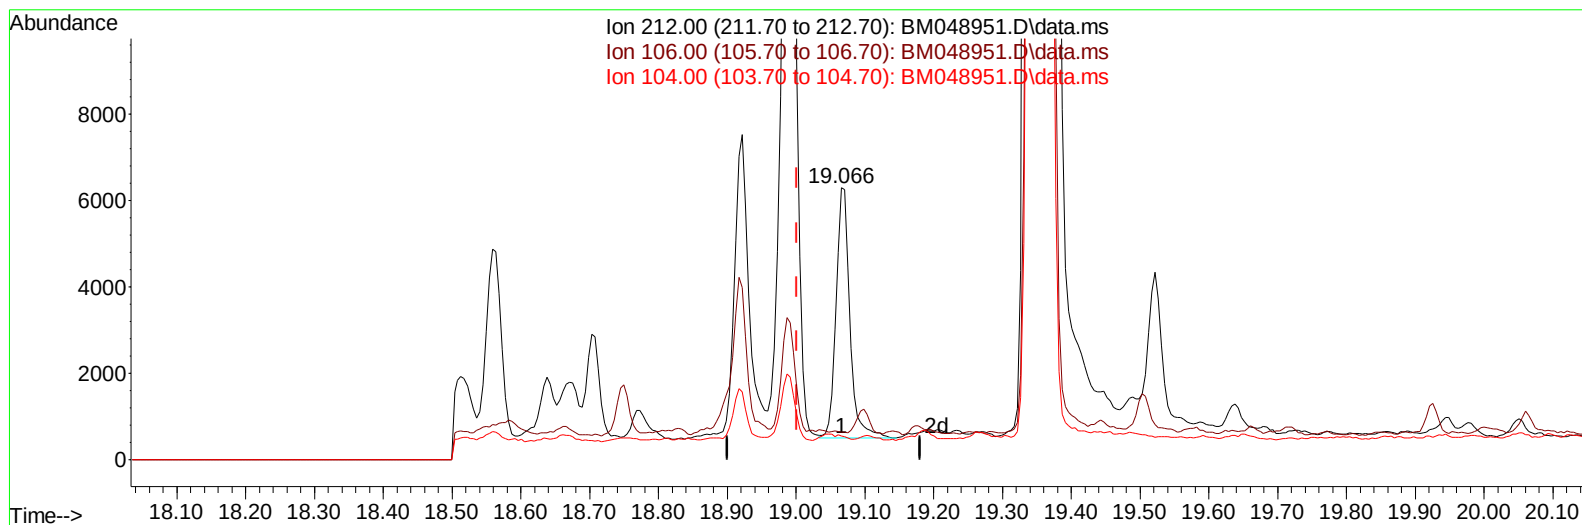

TIC: BM048951.D\data.ms

(18) Fluoranthene-d10 (SURR)




19.066min (+ 0.065) 0.16 ng/u1

response 8061

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	15.90	0.00#
104.00	8.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

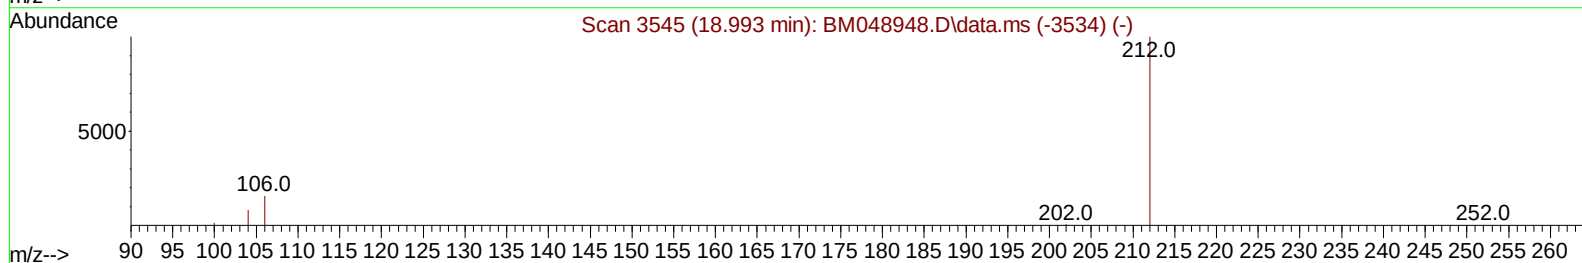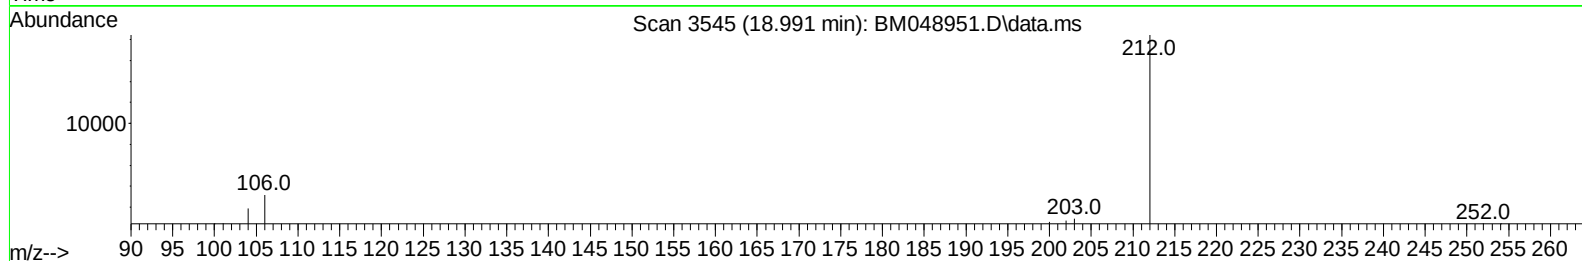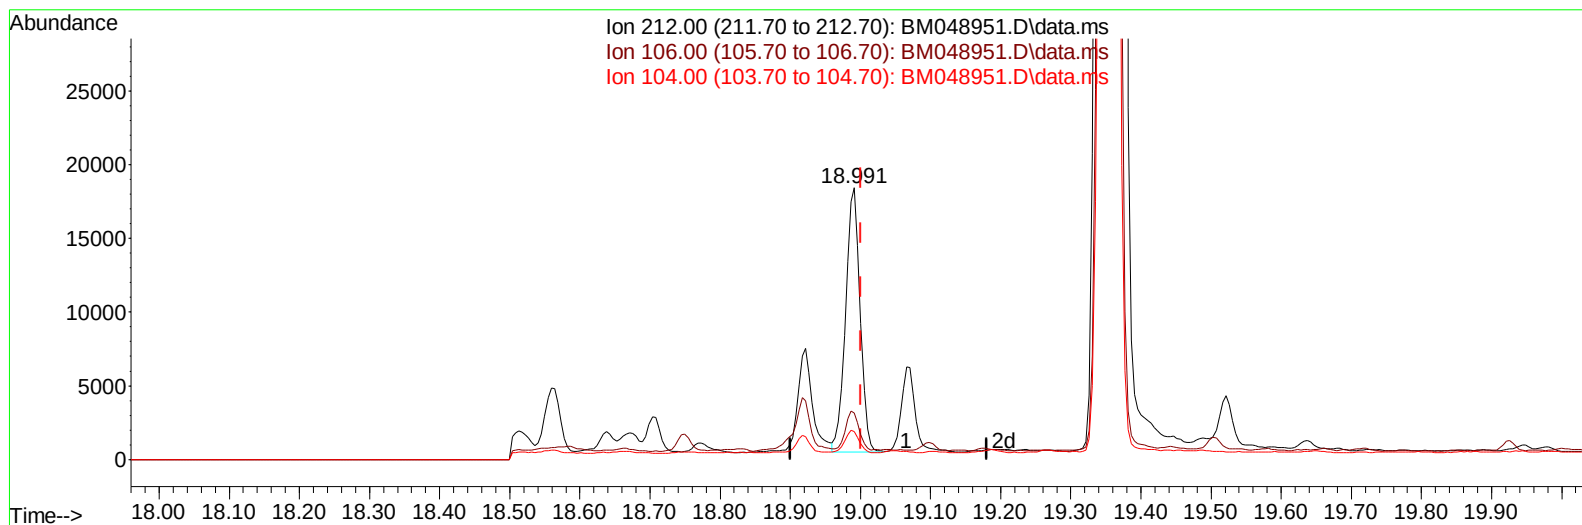

TIC: BM048951.D\data.ms

(18) Fluoranthene-d10 (SURR)




18.991min (-0.009) 0.50 ng/ul m

response 25740

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	15.90	0.00#
104.00	8.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

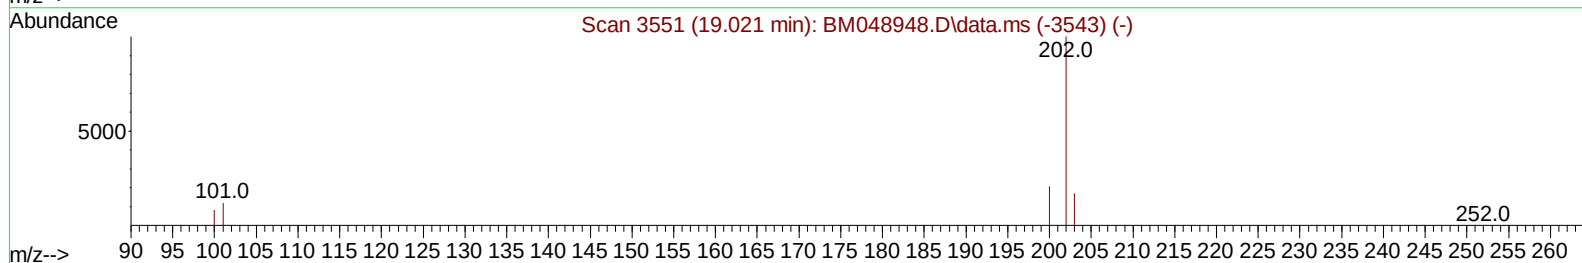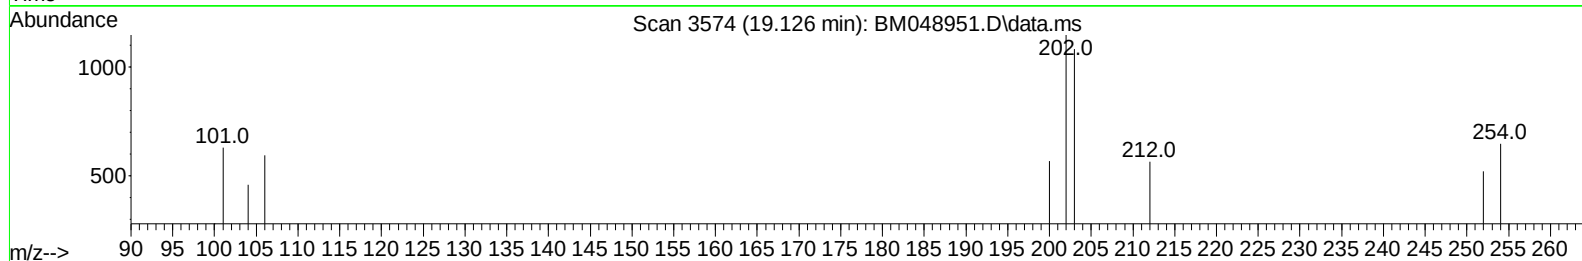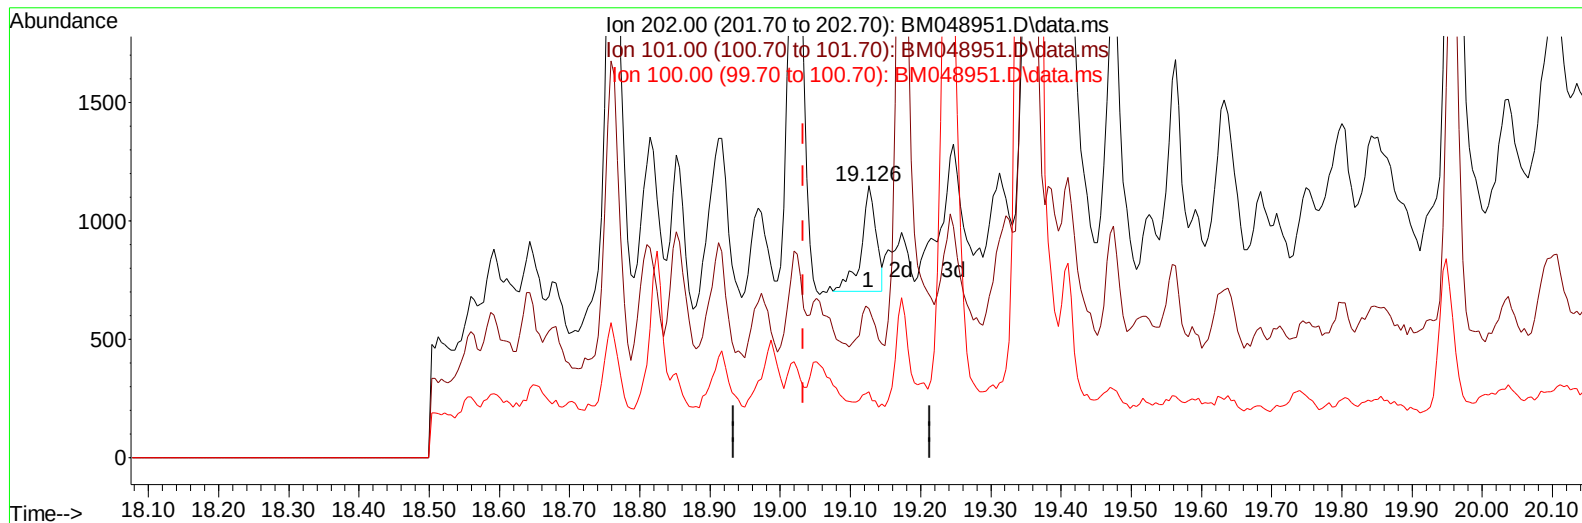

TIC: BM048951.D\data.ms

(19) Fluoranthene (C)




19.126min (+ 0.093) 0.01 ng/ul

response 666

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.10	54.93#
100.00	9.10	24.24#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

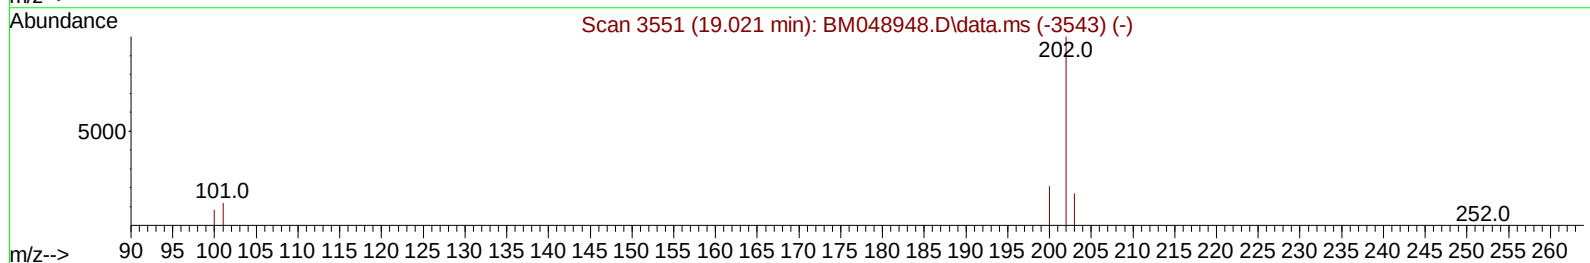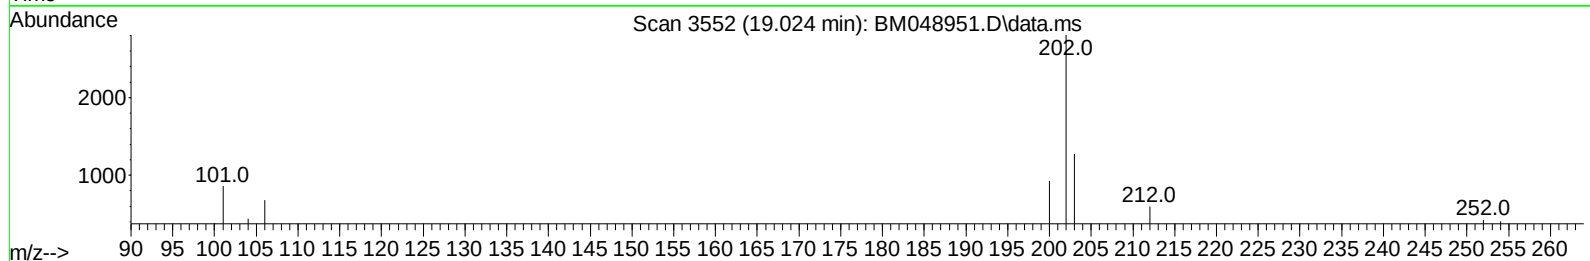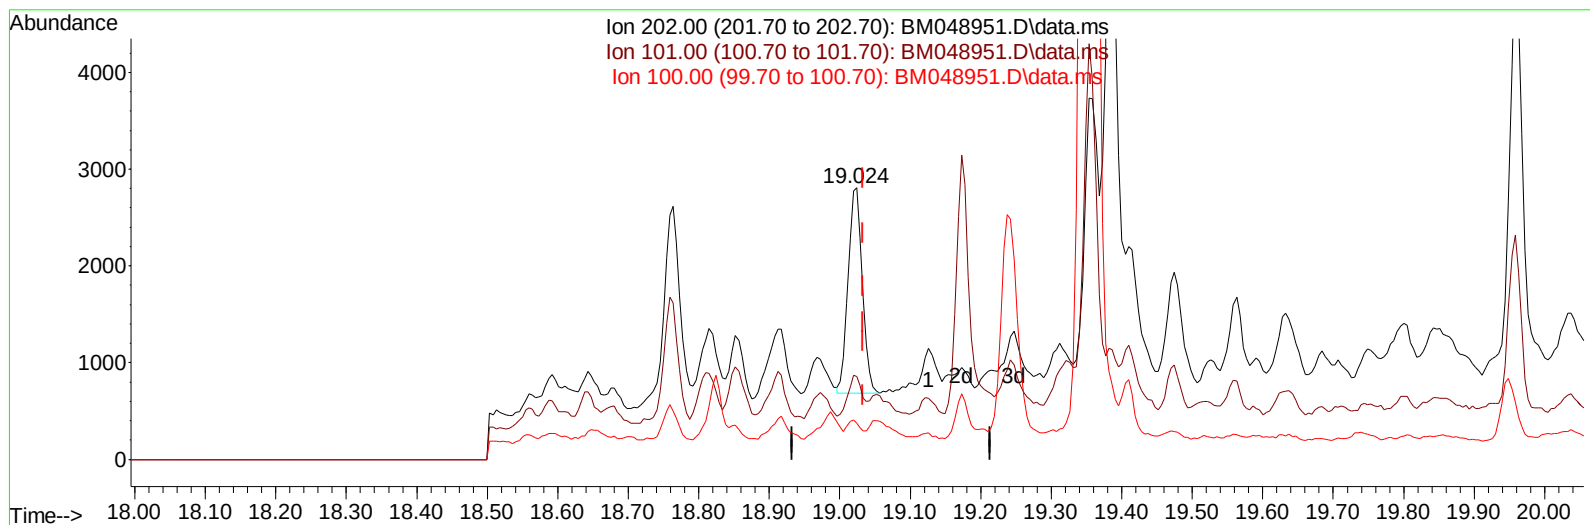

TIC: BM048951.D\data.ms

(19) Fluoranthene (C)




19.024min (-0.009) 0.04 ng/ul m

response 2952

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.10	30.61#
100.00	9.10	13.36#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

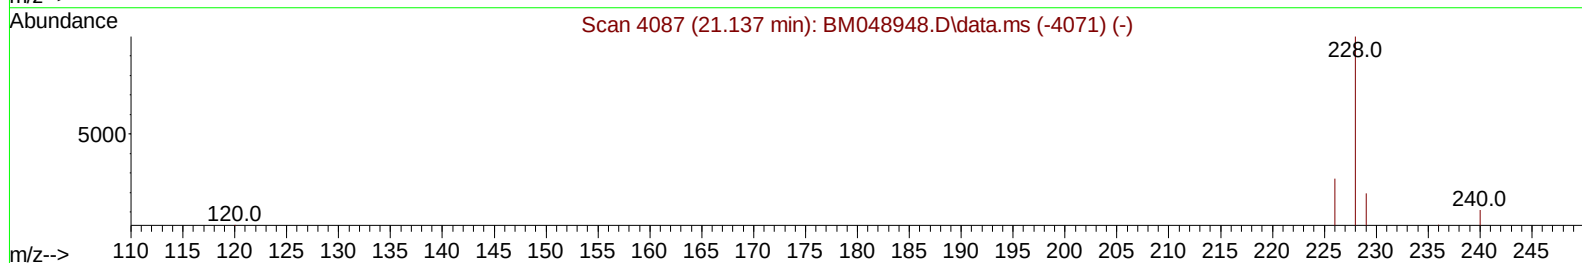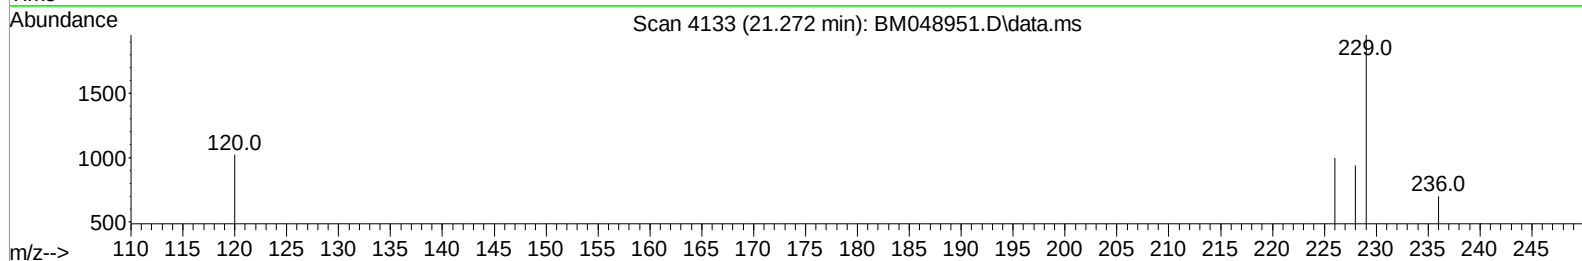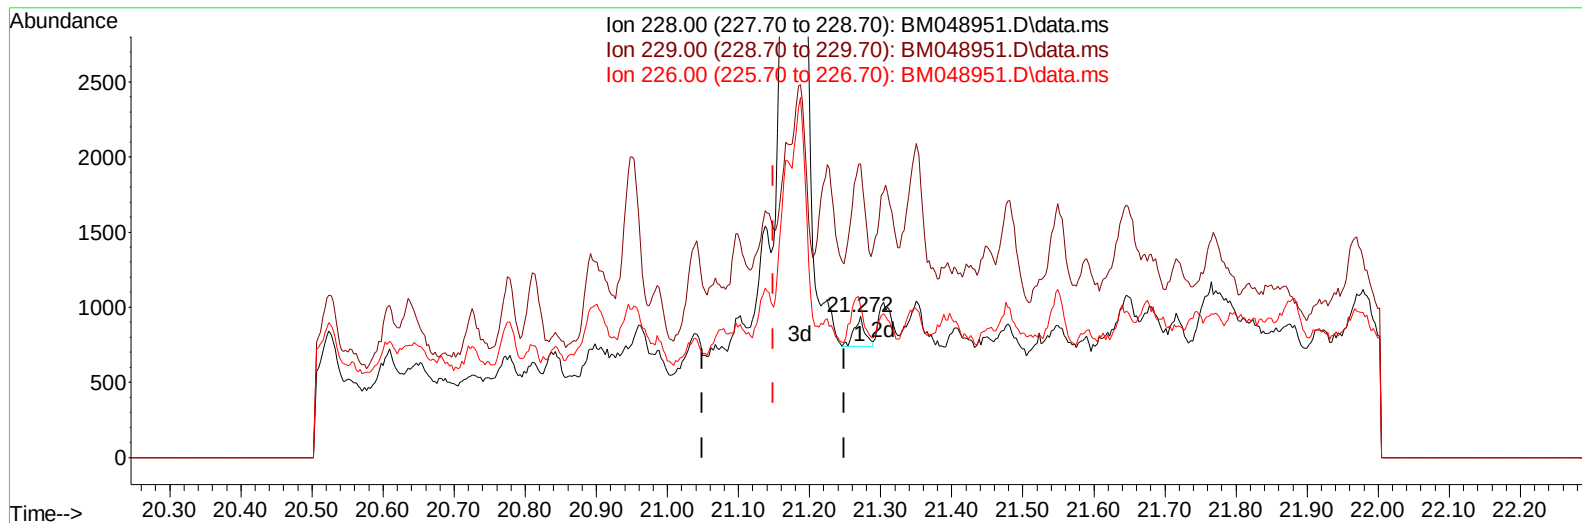

TIC: BM048951.D\data.ms

(21) Benzo(a)anthracene




21.272min (+ 0.123) 0.00 ng/u1

response 212

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.60	208.20#
226.00	28.70	106.39#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

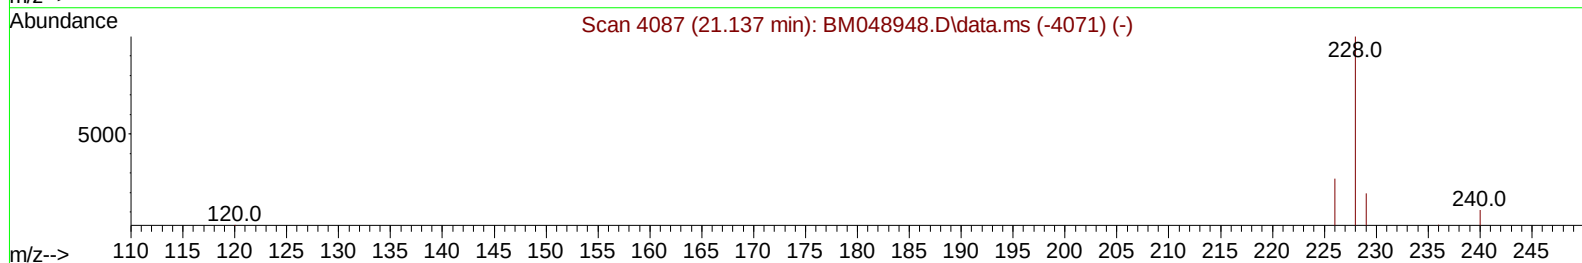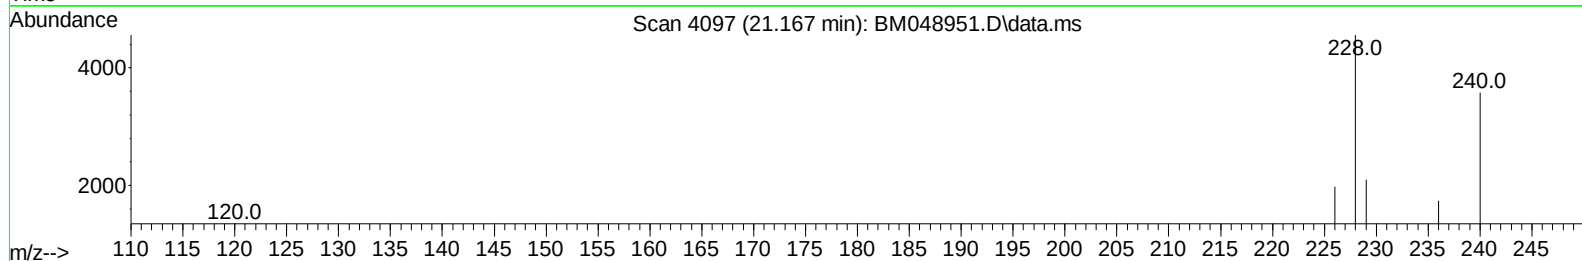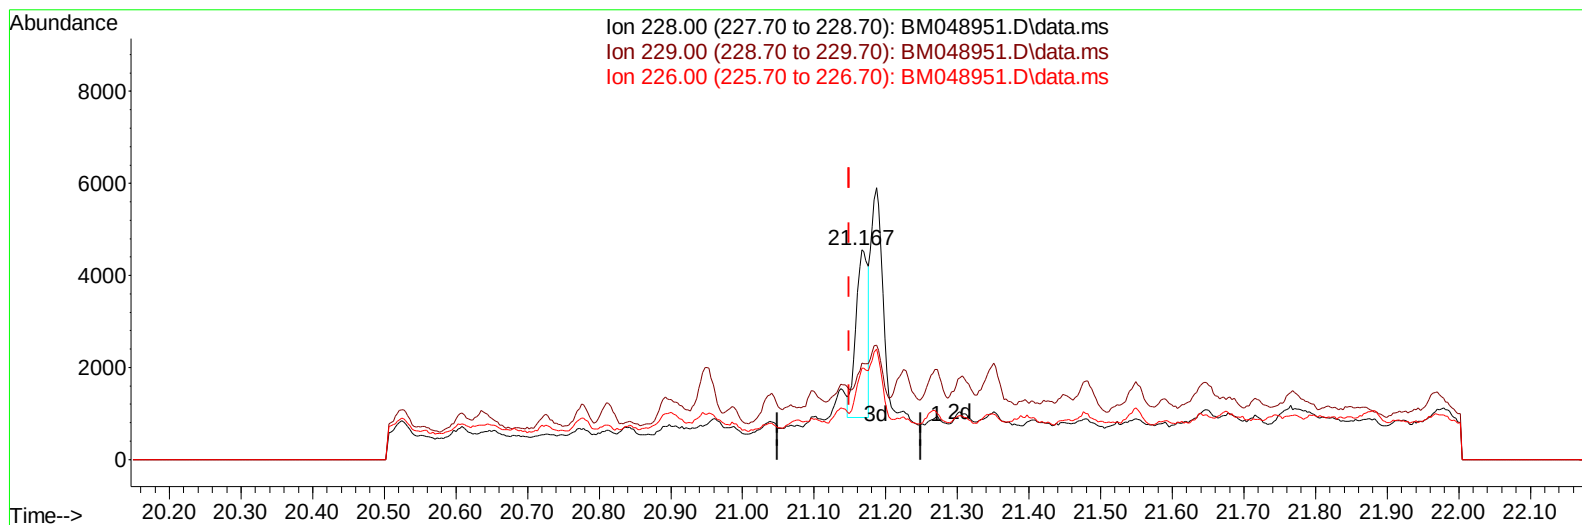

TIC: BM048951.D\data.ms

(21) Benzo(a)anthracene




21.167min (+ 0.018) 0.07 ng/u1 m

response 4268

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.60	46.03#
226.00	28.70	43.42#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

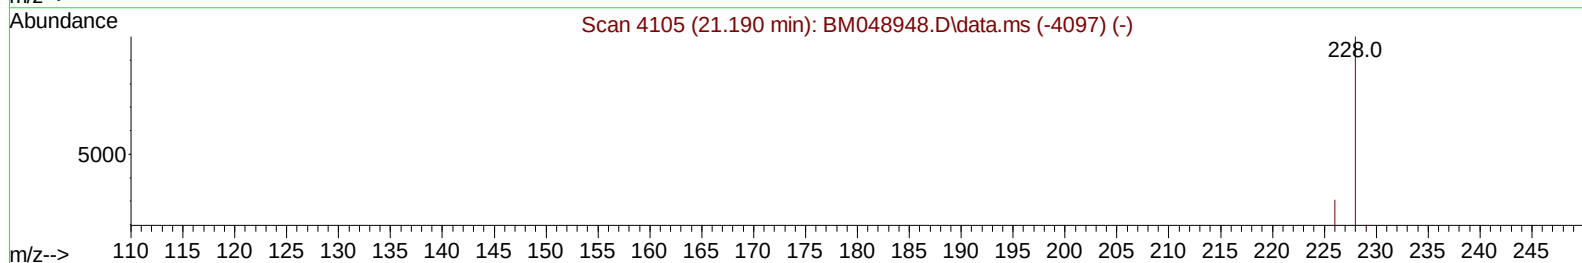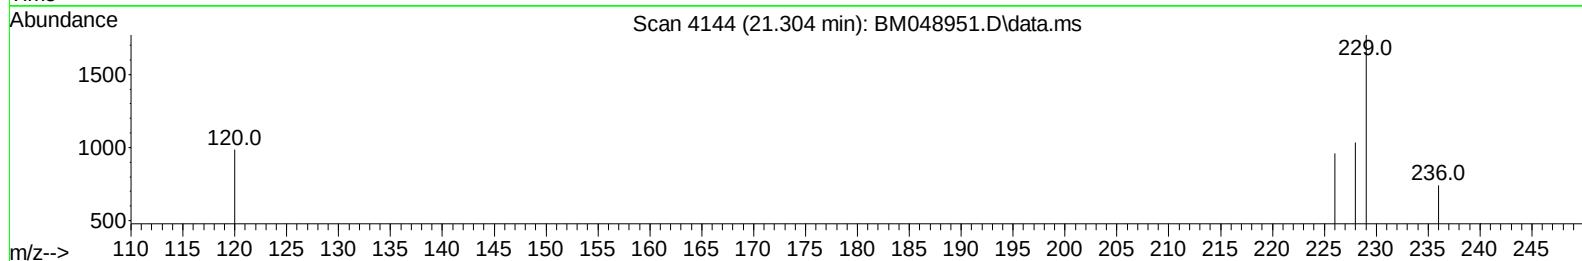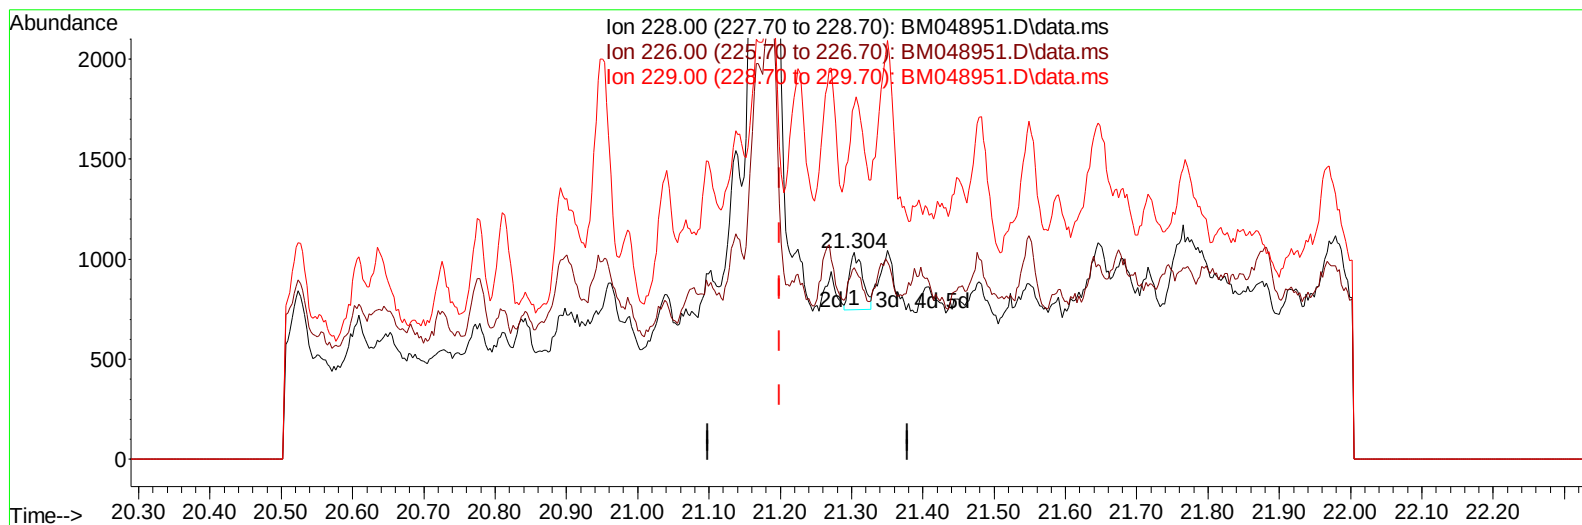

TIC: BM048951.D\data.ms

(22) Chrysene




21.304min (+ 0.105) 0.01 ng/u1

response 372

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	31.00	92.75#
229.00	20.00	171.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

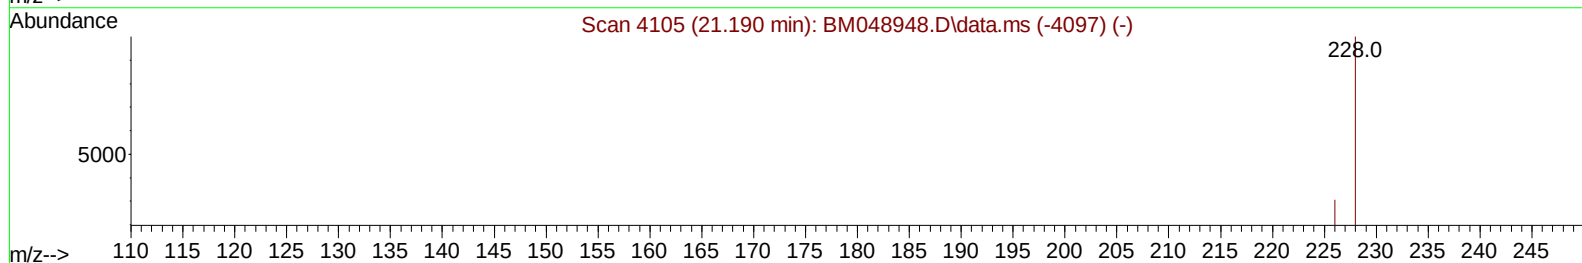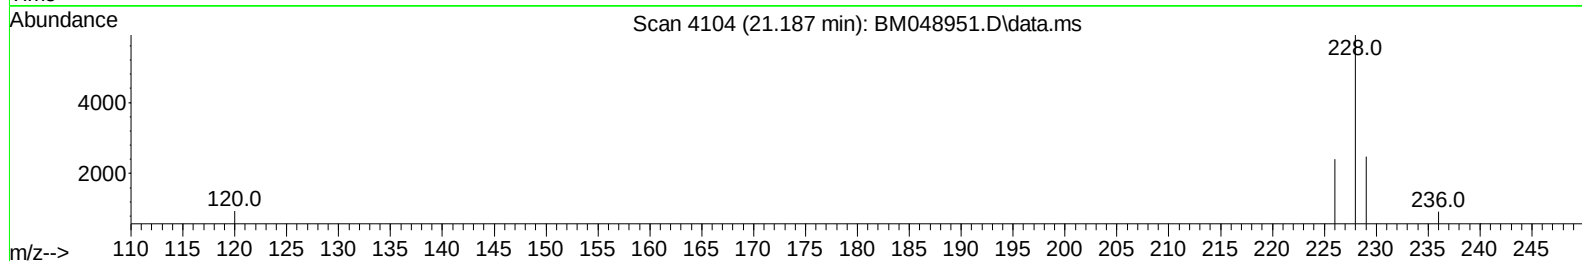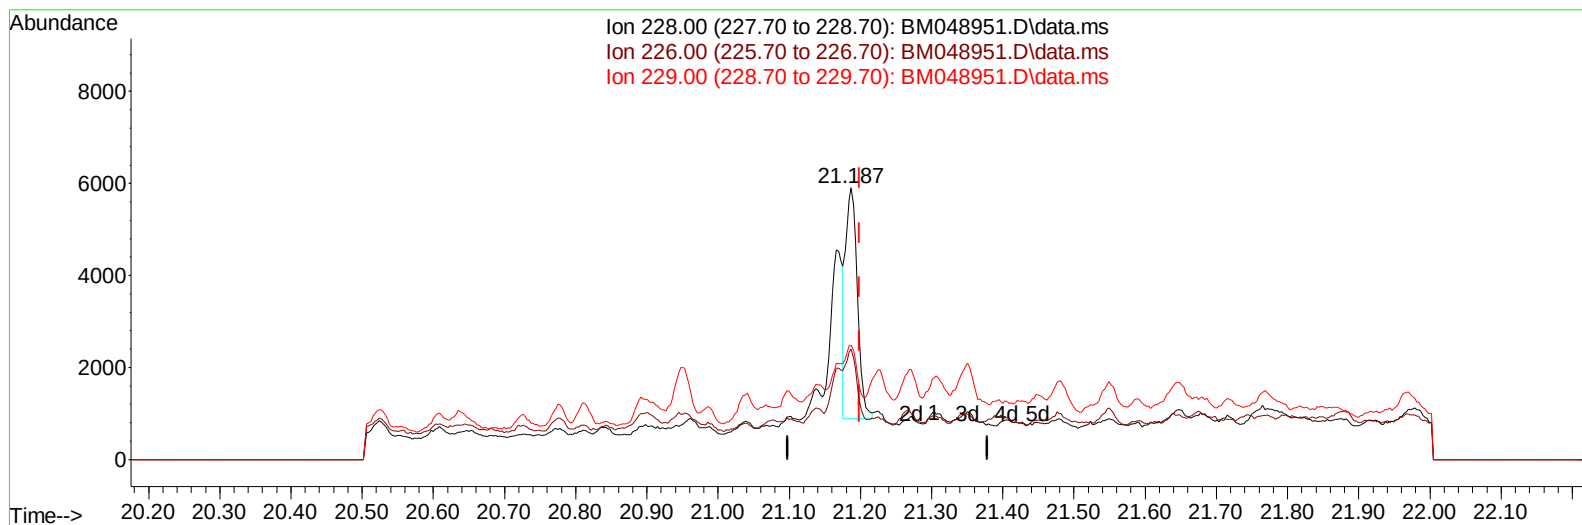

TIC: BM048951.D\data.ms

(22) Chrysene




21.187min (-0.012) 0.08 ng/ul m

response 5748

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	31.00	40.64#
229.00	20.00	42.06#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

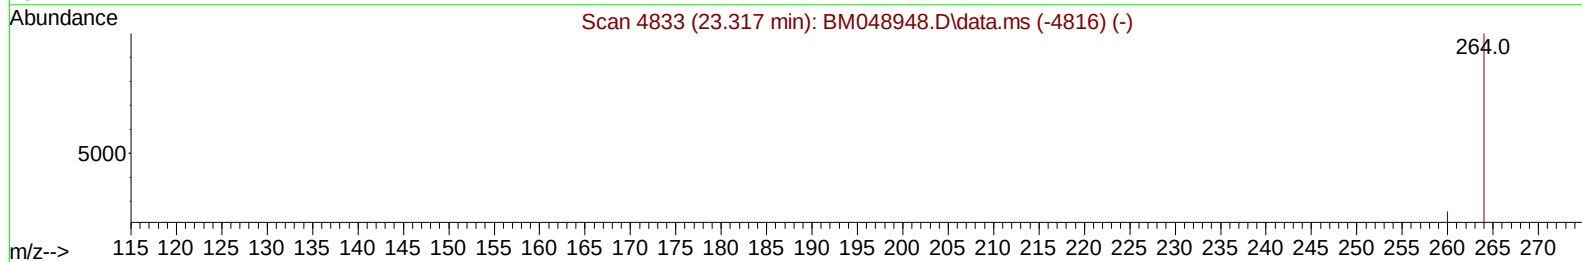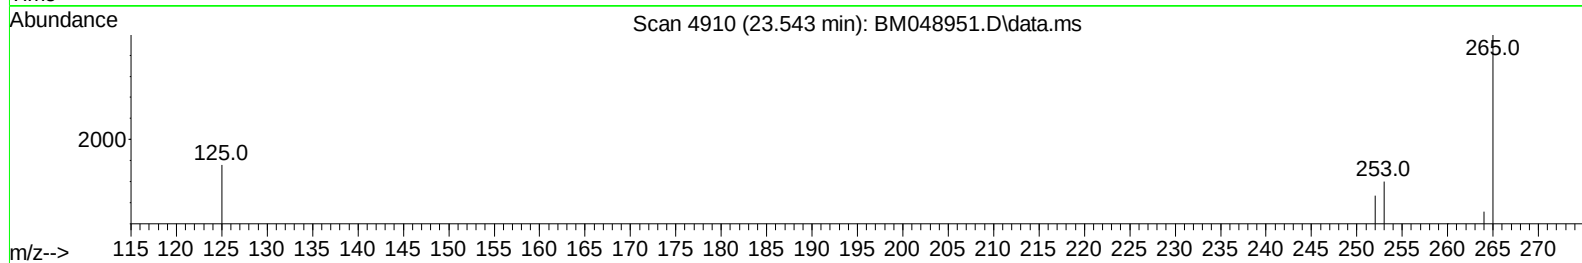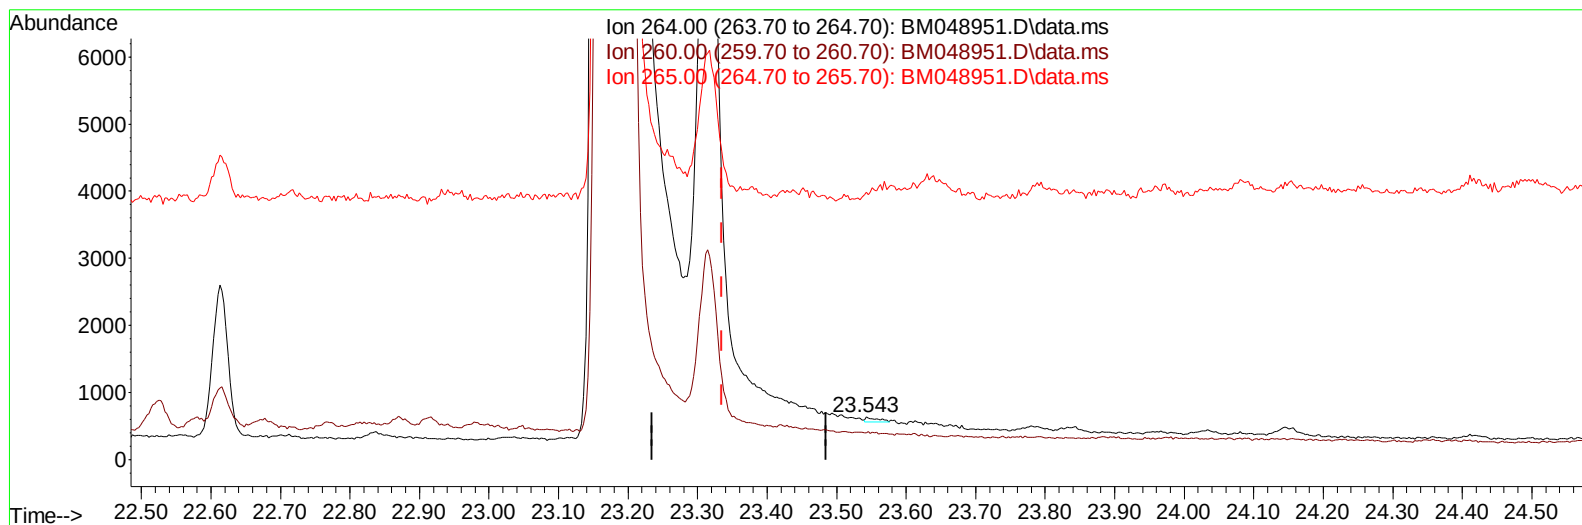

TIC: BM048951.D\data.ms

(23) Perylene-d12 (I)




23.543min (+ 0.208) 0.40 ng/ul

response 80

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	62.99#
265.00	82.60	627.40#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

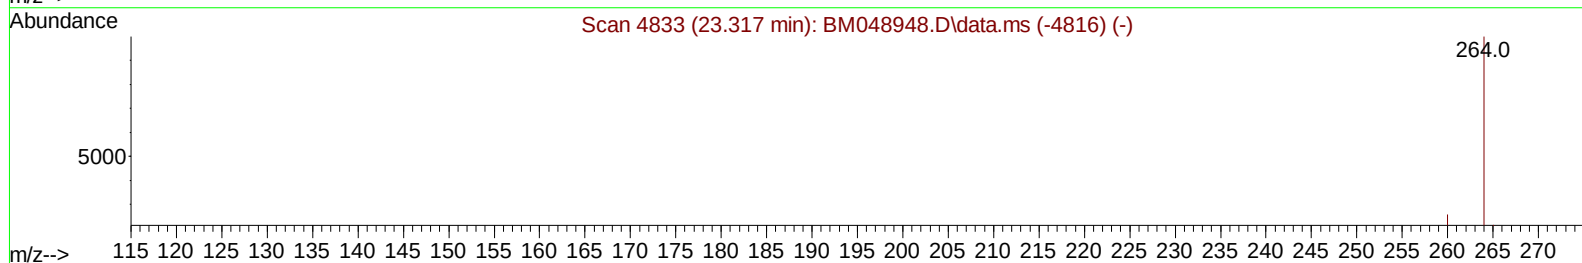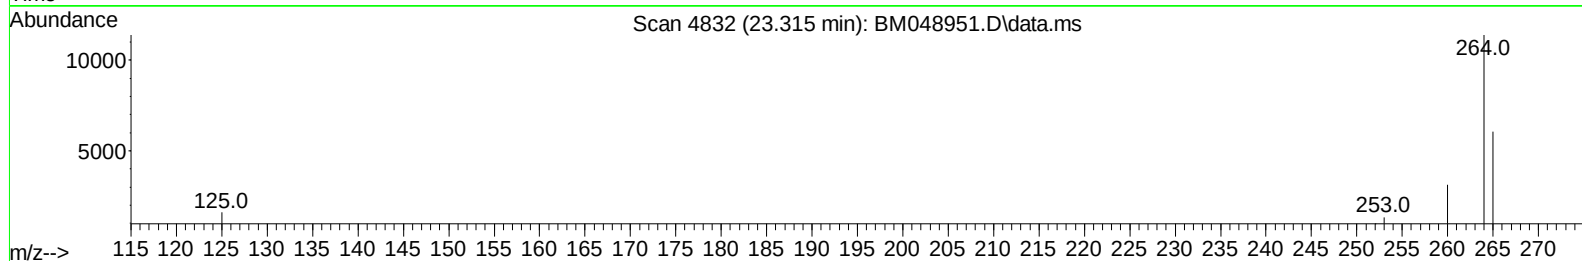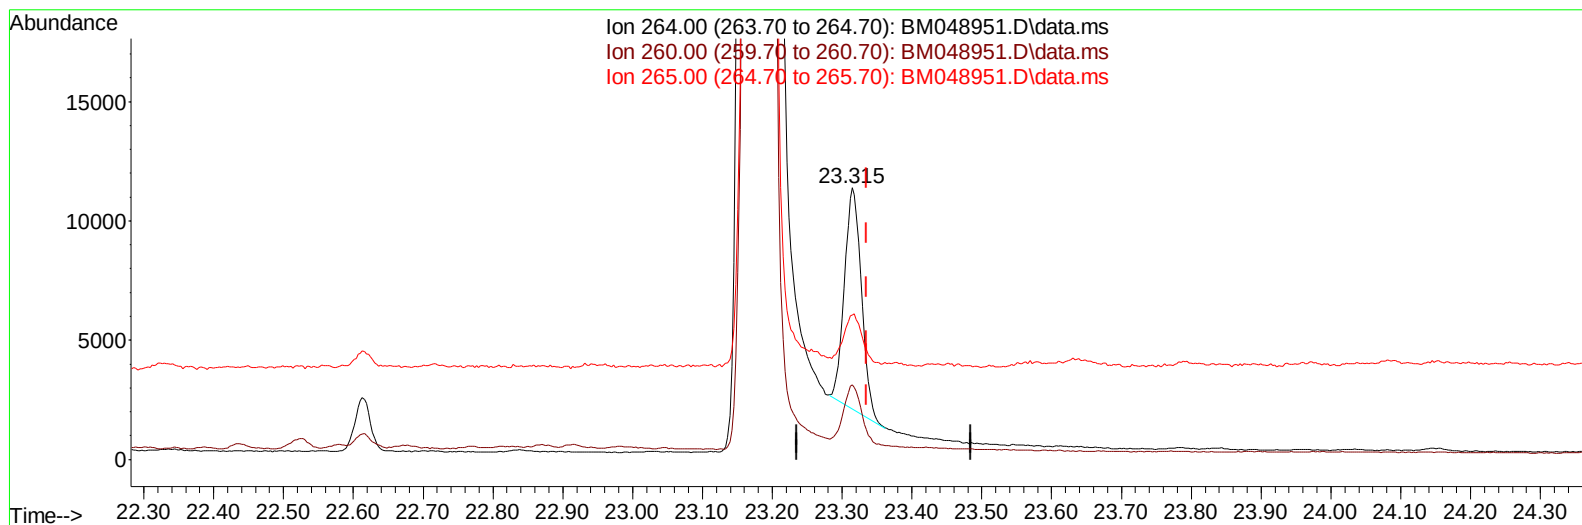

TIC: BM048951.D\data.ms

(23) Perylene-d12 (I)




23.315min (-0.020) 0.40 ng/ul m

response 15619

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.50	27.47
265.00	82.60	53.23#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

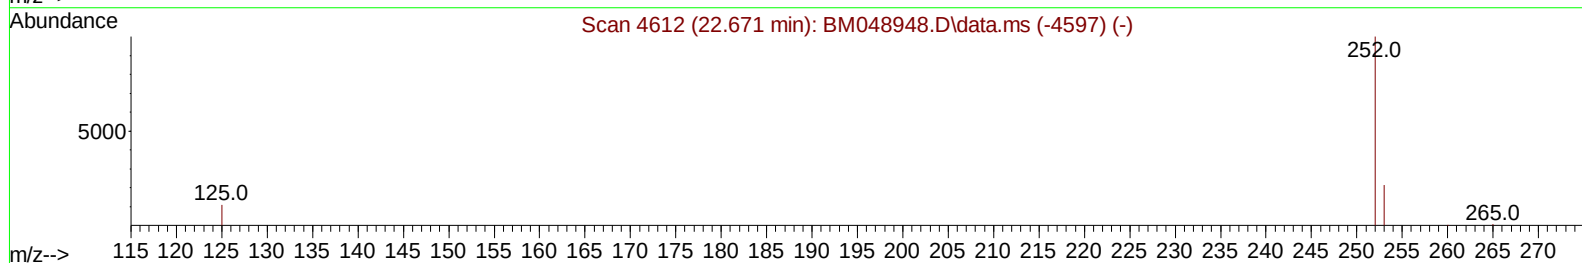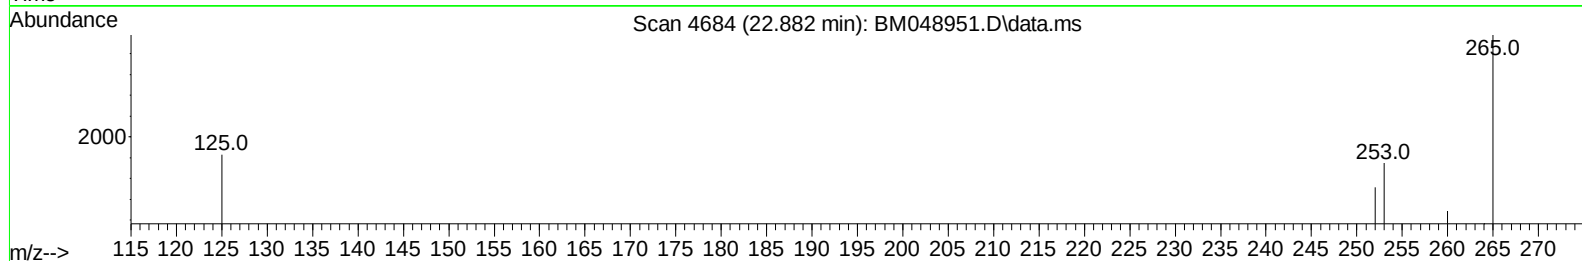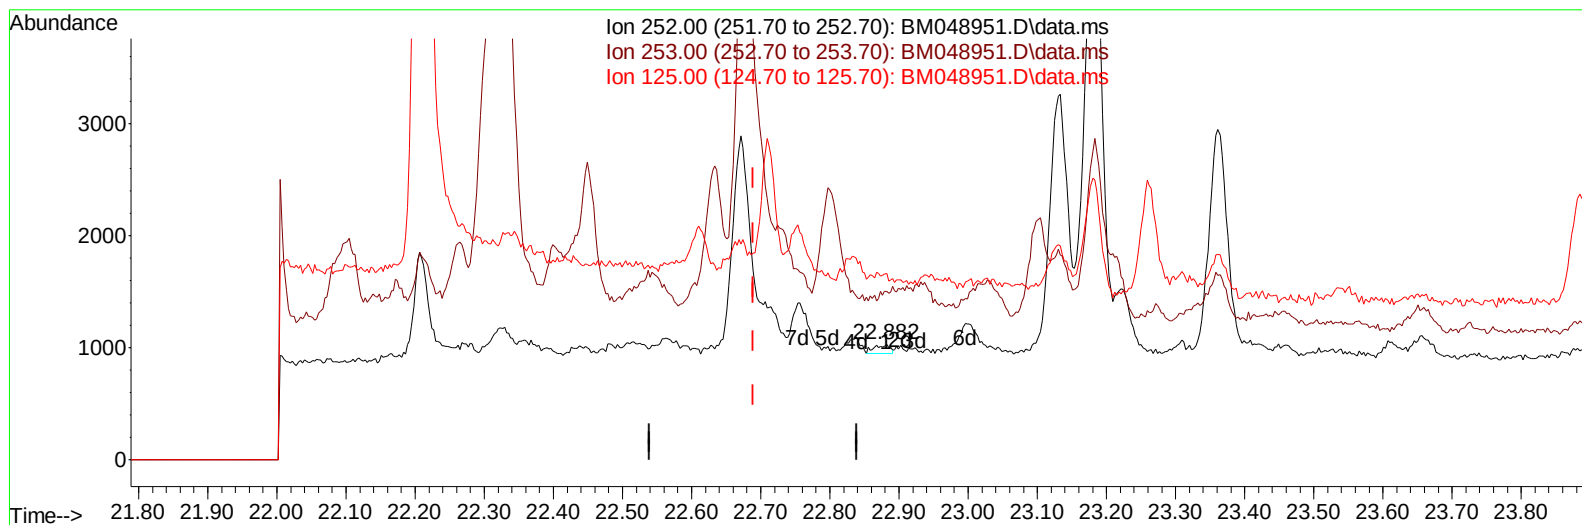

TIC: BM048951.D\data.ms




(24) Benzo(b)fluoranthene

22.882min (+ 0.193) 0.00 ng/u^l

response 127

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.50	145.82#
125.00	18.30	161.58#
0.00	0.00	0.00

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

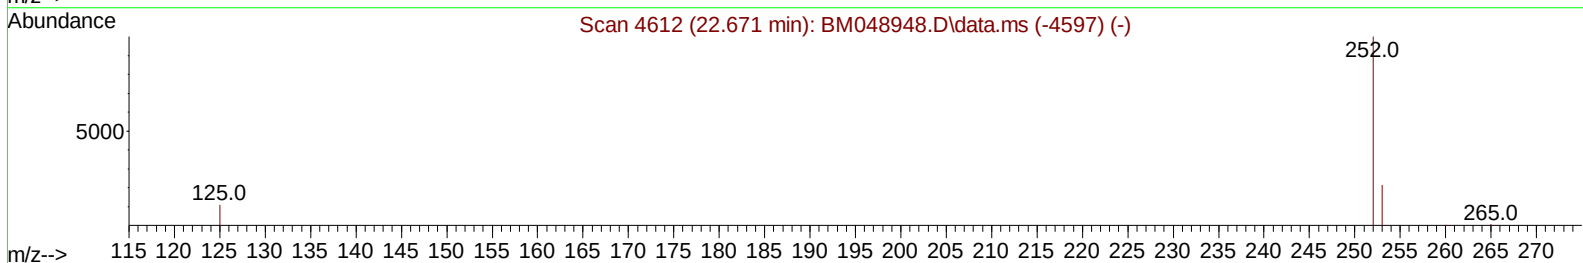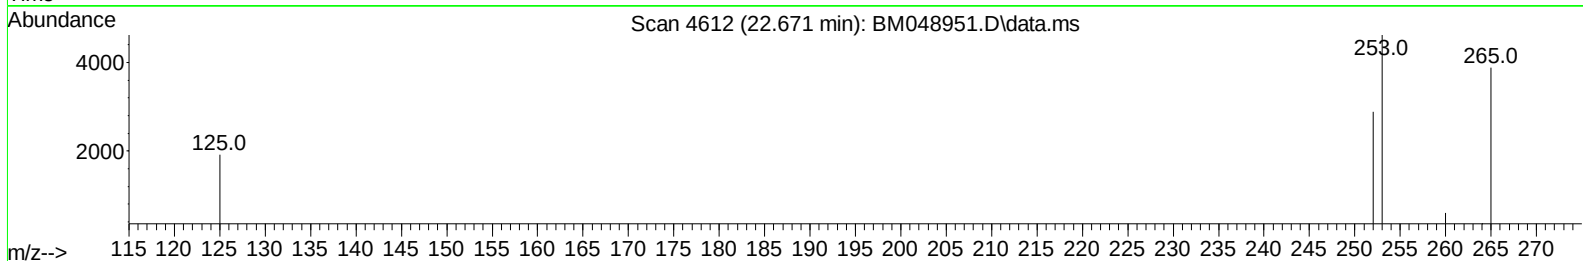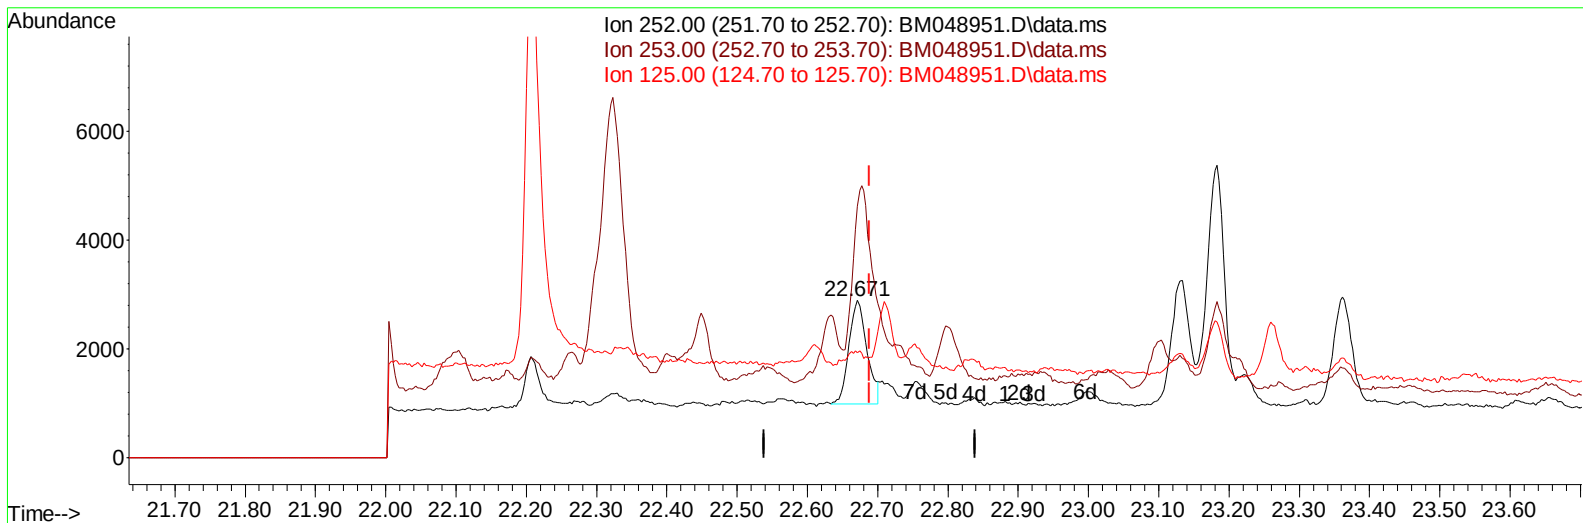

TIC: BM048951.D\data.ms

(24) Benzo(b)fluoranthene




22.671min (-0.018) 0.06 ng/ul m

response **3408**

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.50	159.90#
125.00	18.30	66.47#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

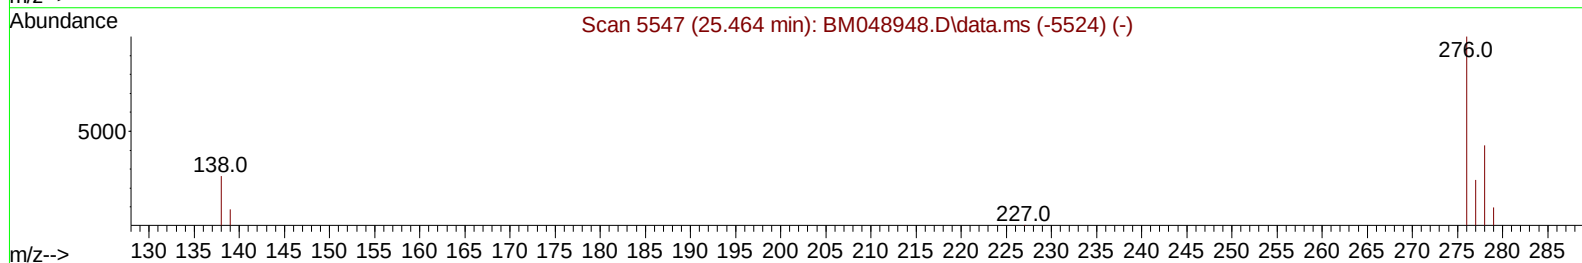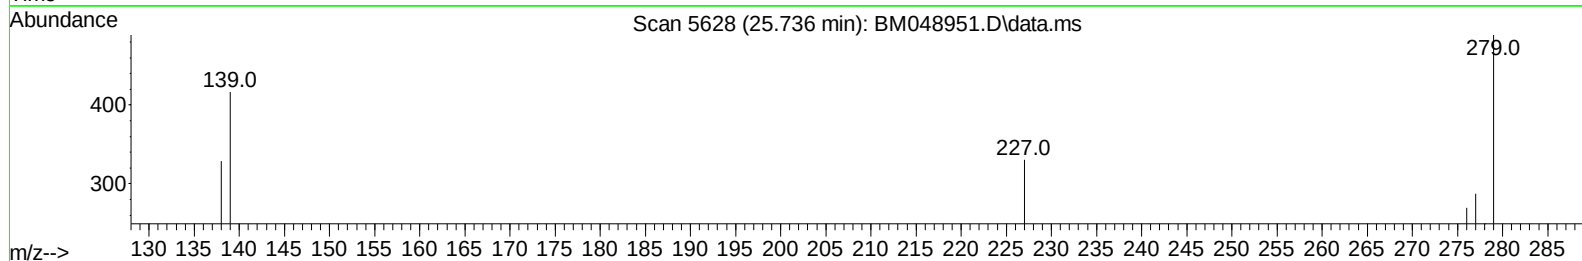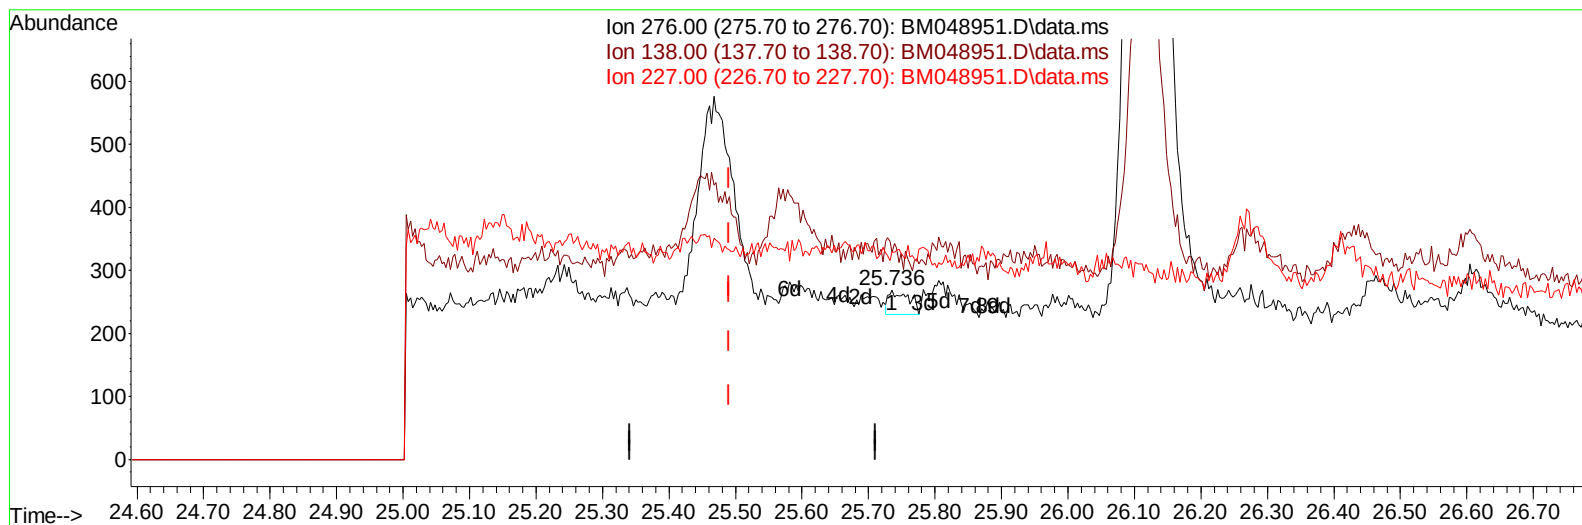

TIC: BM048951.D\data.ms

(27) Indeno(1,2,3-cd)pyrene




25.736min (+ 0.245) 0.00 ng/u^l

response 81

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	27.60	0.00#
227.00	0.20	25.93#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

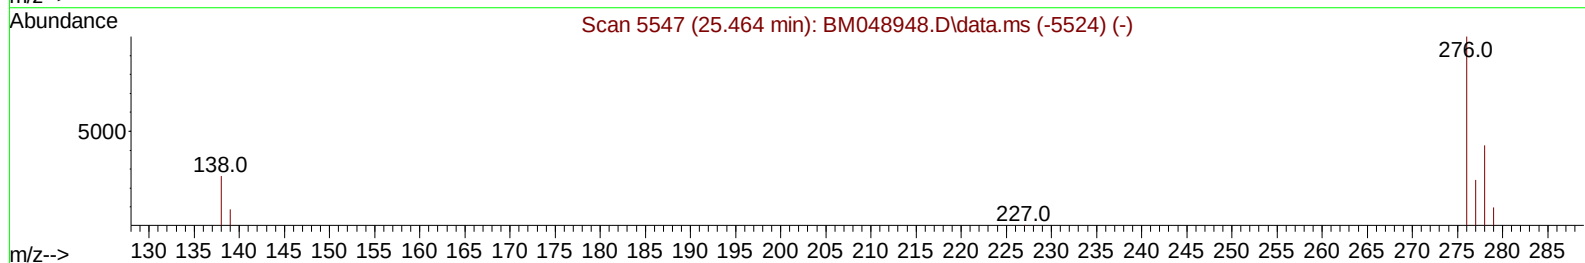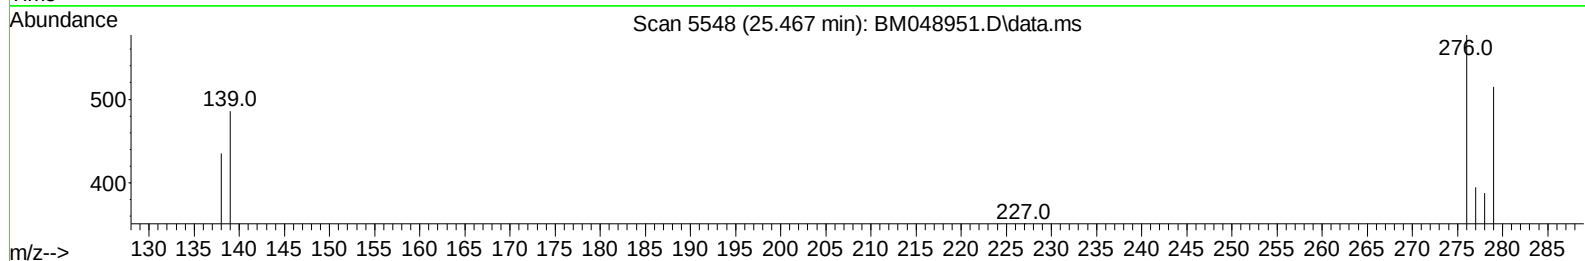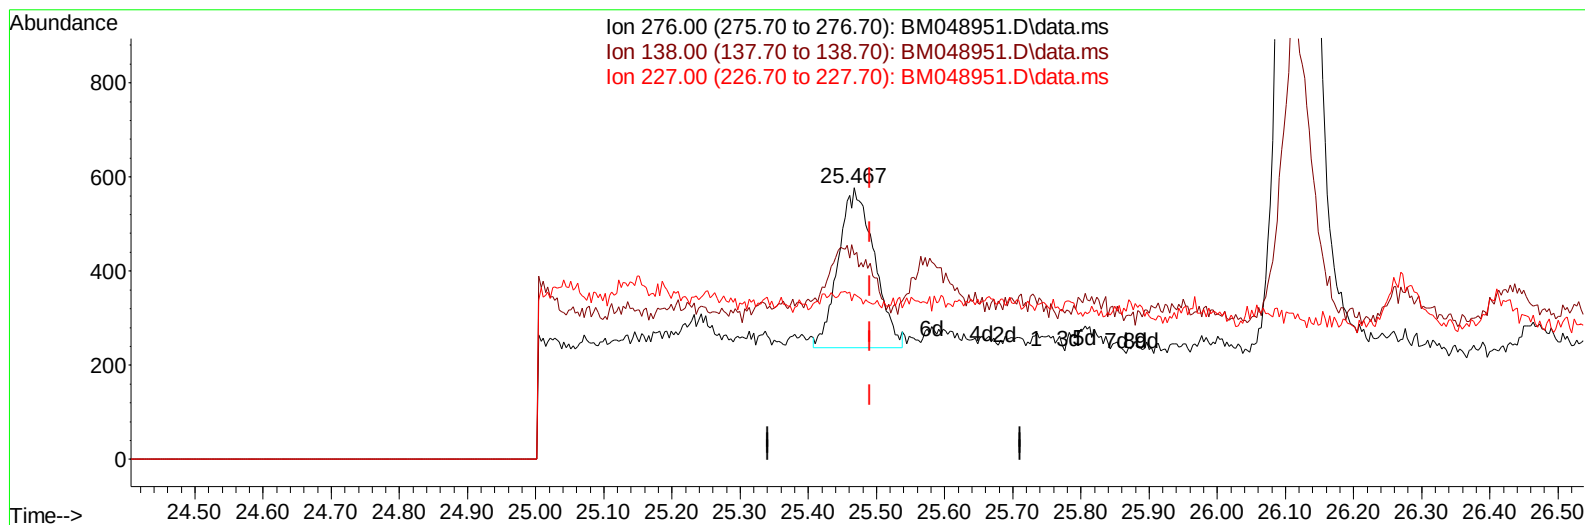

TIC: BM048951.D\data.ms

(27) Indeno(1,2,3-cd)pyrene




25.467min (-0.023) 0.02 ng/ul m

response 1243

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	27.60	0.00#
227.00	0.20	1.69#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

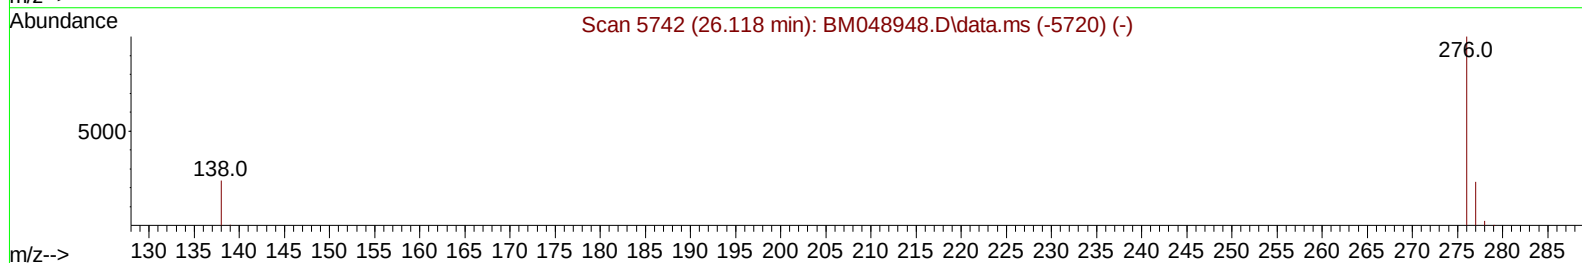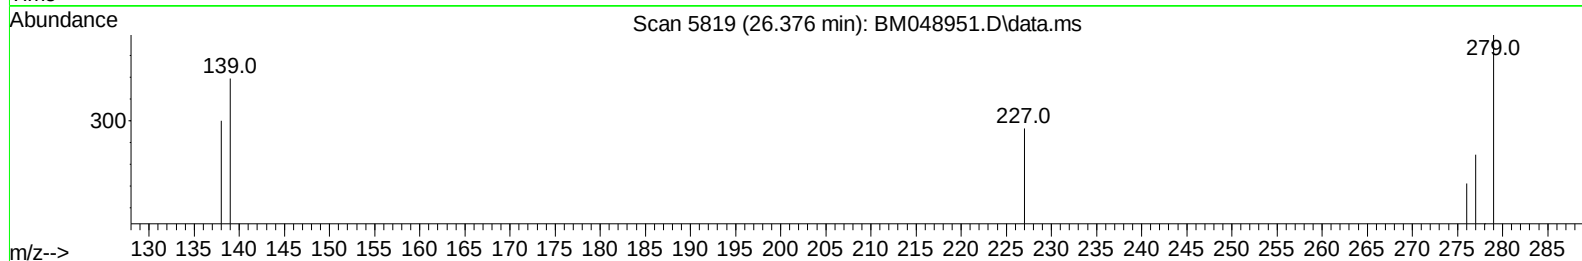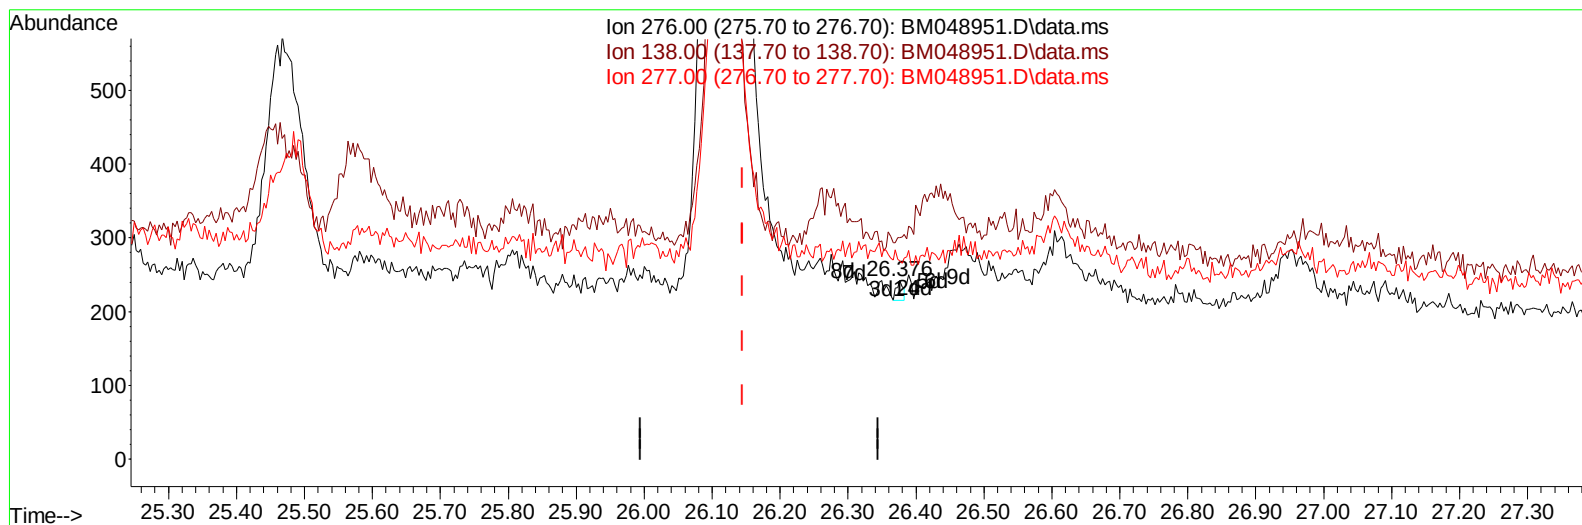

TIC: BM048951.D\data.ms

(29) Benzo(g,h,i)perylene




26.376min (+ 0.231) 0.00 ng/u1

response 20

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	24.70	123.97#
277.00	24.50	111.16#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

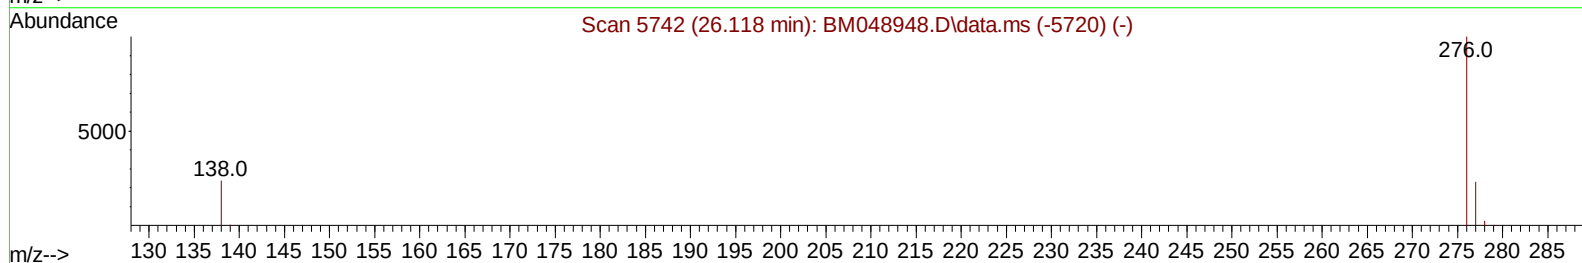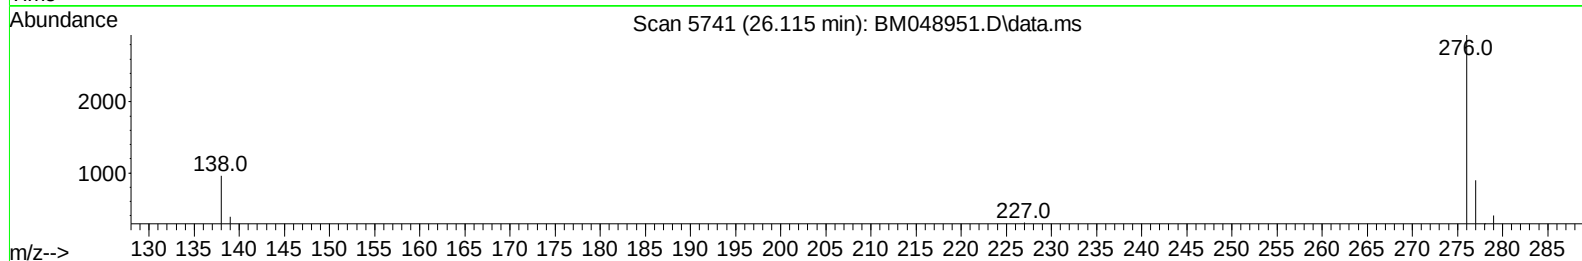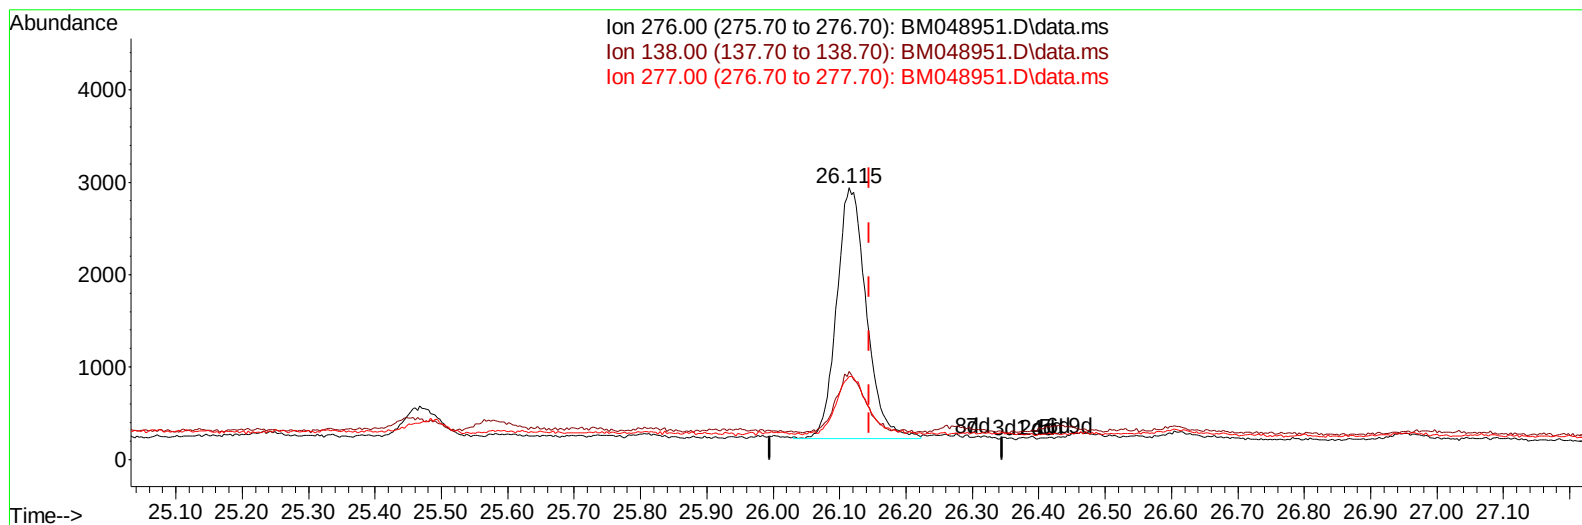

TIC: BM048951.D\data.ms

(29) Benzo(g,h,i)perylene

26.115min (-0.030) 0.15 ng/ul m

response 8436

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	24.70	32.53#
277.00	24.50	30.49#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
 Data File : BM048951.D
 Acq On : 11 Dec 2024 10:48
 Operator : RC/JU
 Sample : P5066-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 09 17:52:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.577	152	7071	0.400	ng/ul	0.00
4) Naphthalene-d8	10.341	136	20848	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.214	164	11865	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.958	188	25441m	0.400	ng/ul	0.00
17) Chrysene-d12	21.152	240	17269m	0.400	ng/ul	-0.01
23) Perylene-d12	23.315	264	15619m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	38391	4.645	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.941	152	11910	0.448	ng/ul	0.00
18) Fluoranthene-d10	18.991	212	25740m	0.499	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.391	128	5709	0.107	ng/ul#	79
7) 2-Methylnaphthalene	12.013	142	17505	0.536	ng/ul	97
8) 1-Methylnaphthalene	12.233	142	14448	0.435	ng/ul	94
10) Acenaphthylene	13.936	152	1291	0.026	ng/ul#	1
11) Acenaphthene	14.269	153	971	0.026	ng/ul#	68
12) Fluorene	15.264	166	1671	0.040	ng/ul#	38
15) Phenanthrene	17.001	178	41725m	0.598	ng/ul	
19) Fluoranthene	19.024	202	2952m	0.041	ng/ul	
21) Benzo(a)anthracene	21.167	228	4268m	0.070	ng/ul	
22) Chrysene	21.187	228	5748m	0.084	ng/ul	
24) Benzo(b)fluoranthene	22.671	252	3408m	0.063	ng/ul	
29) Benzo(g,h,i)perylene	26.115	276	8436m	0.150	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121024\
Data File : BM048951.D
Acq On : 11 Dec 2024 10:48
Operator : RC/JU
Sample : P5066-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Dec 11 11:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM120924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:52:26 2024
Response via : Initial Calibration

